

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080922\
 Data File : PP050374.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2022 13:31
 Operator : YP\AJ
 Sample : N3980-07
 Misc : AR1248 LOD 25 PPB
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 01:37:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 09 11:38:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.347	3.593	27291608	51452529	16.955	16.427
2) SA Decachlor...	10.097	8.559	30284750	26092910	17.198	16.954
Target Compounds						
21) L5 AR-1248-1	5.524	4.665	927715	1314429	22.976m	19.667
22) L5 AR-1248-2	5.795	4.900	1105648	1820285	19.791m	21.072
23) L5 AR-1248-3	6.003	4.941	1262082	1851011	19.729m	20.418
24) L5 AR-1248-4	6.410	5.112	1771079	2701537	22.389	25.632
25) L5 AR-1248-5	6.449	5.502	1656572	2203543	21.822	22.193m



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080922\
Data File : PP050374.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2022 13:31
Operator : YP\AJ
Sample : N3980-07
Misc : AR1248 LOD 25 PPB
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 01:37:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 09 11:38:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

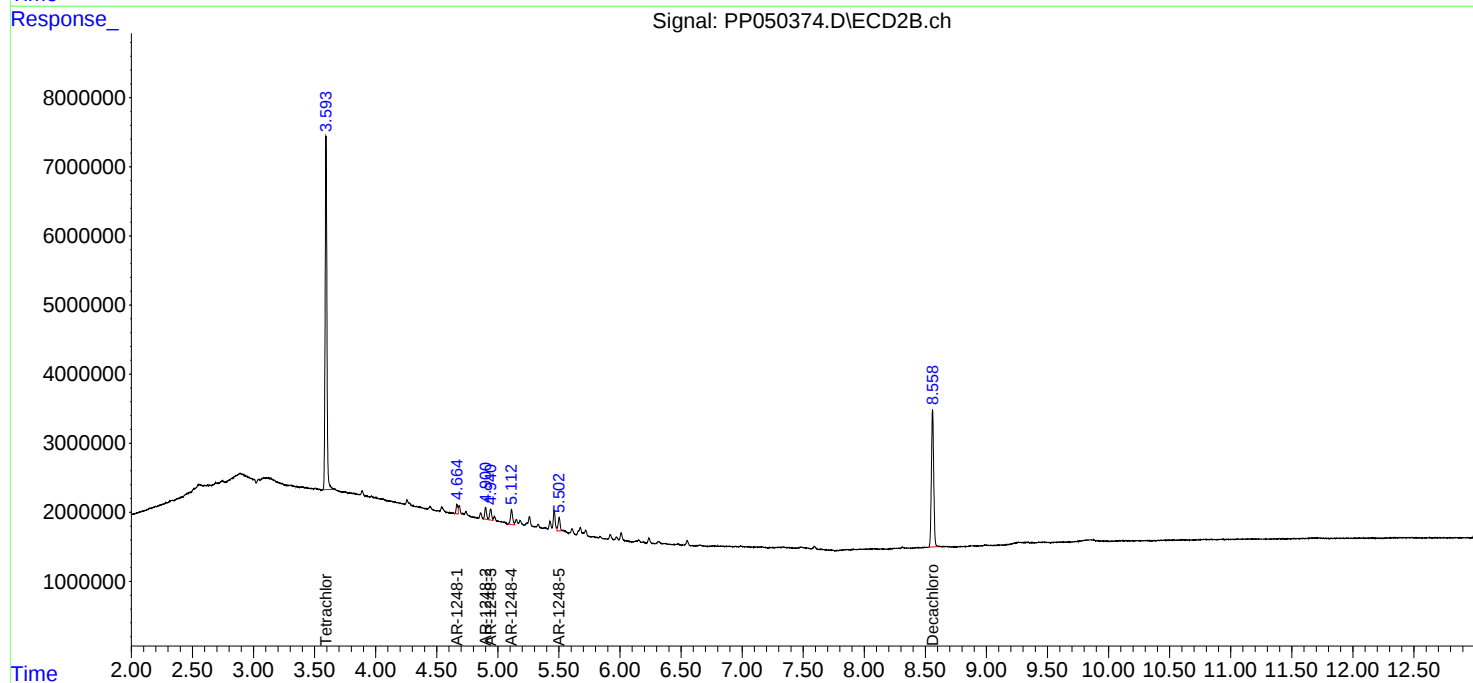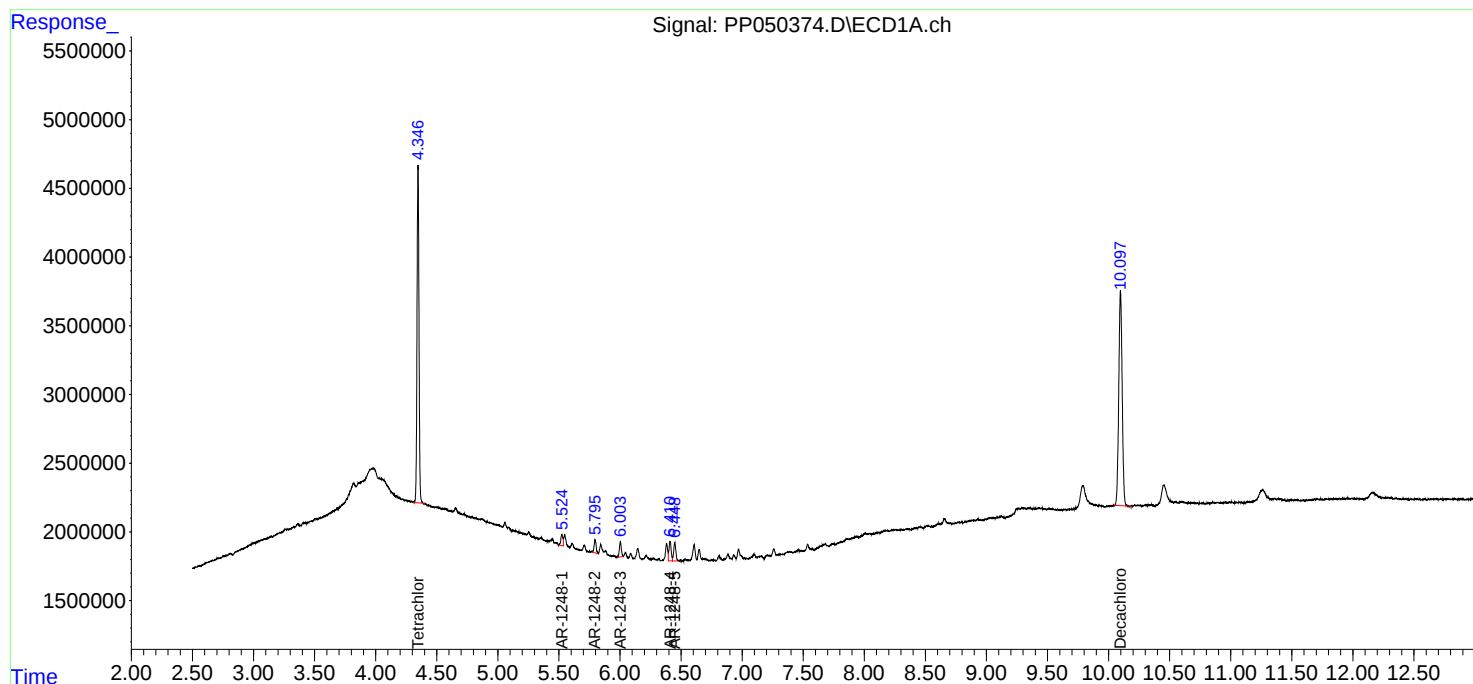


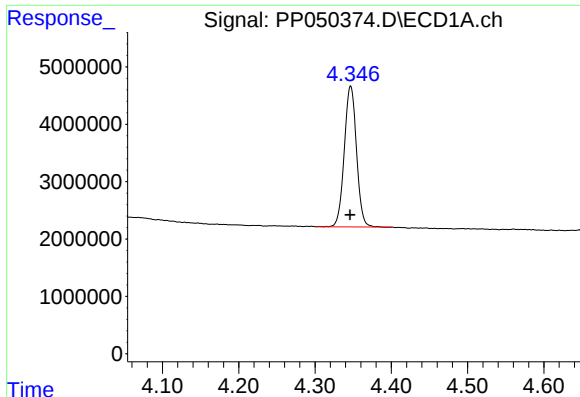

#1 Tetrachloro-m-xylene


R.T.: 4.347 min
Delta R.T.: 0.000 min
Response: 27291608
Conc: 16.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

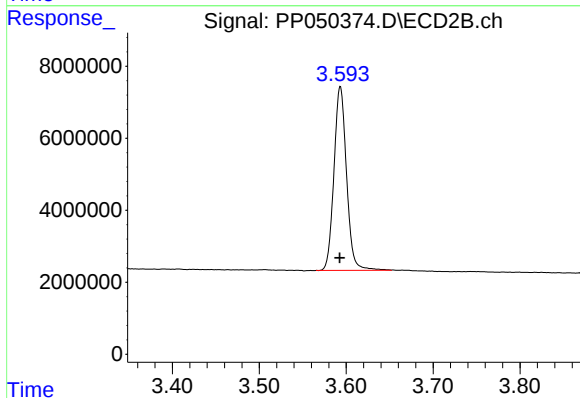


#1 Tetrachloro-m-xylene

R.T.: 3.593 min
Delta R.T.: 0.000 min
Response: 51452529
Conc: 16.43 ng/ml

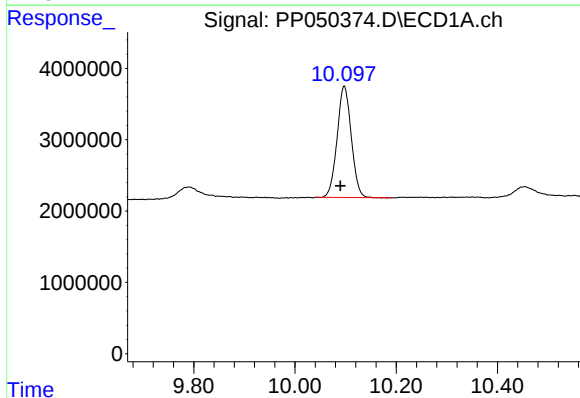


#2 Decachlorobiphenyl

R.T.: 10.097 min
Delta R.T.: 0.008 min
Response: 30284750
Conc: 17.20 ng/ml

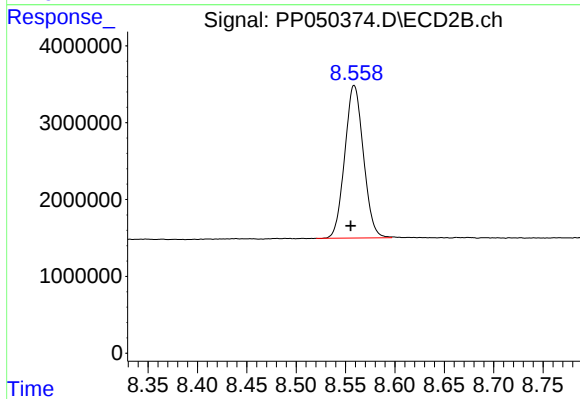

#2 Decachlorobiphenyl


R.T.: 8.559 min
Delta R.T.: 0.003 min
Response: 26092910
Conc: 16.95 ng/ml

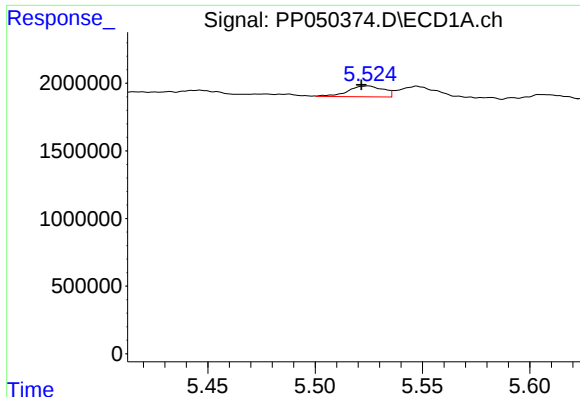

#21 AR-1248-1


R.T.: 5.524 min
Delta R.T.: 0.003 min
Response: 927715
Conc: 22.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

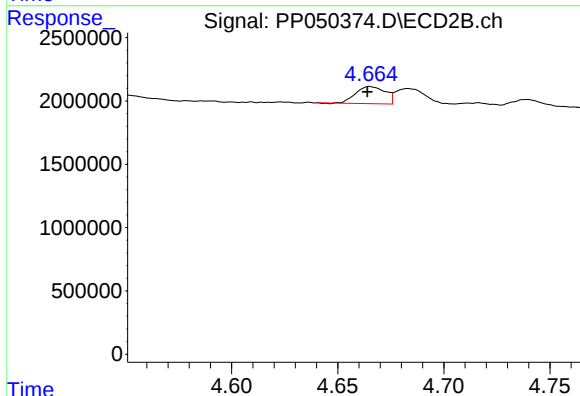


#21 AR-1248-1

R.T.: 4.665 min
Delta R.T.: 0.000 min
Response: 1314429
Conc: 19.67 ng/ml

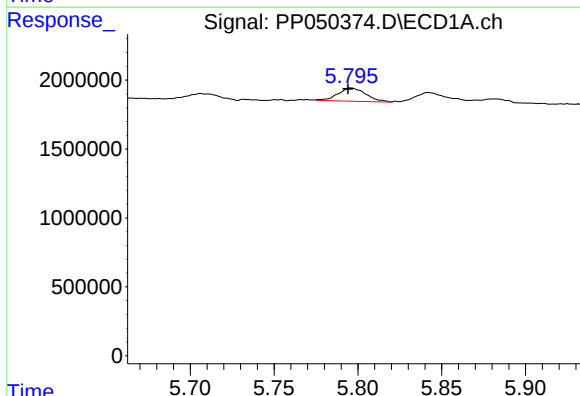


#22 AR-1248-2

R.T.: 5.795 min
Delta R.T.: 0.000 min
Response: 1105648
Conc: 19.79 ng/ml m

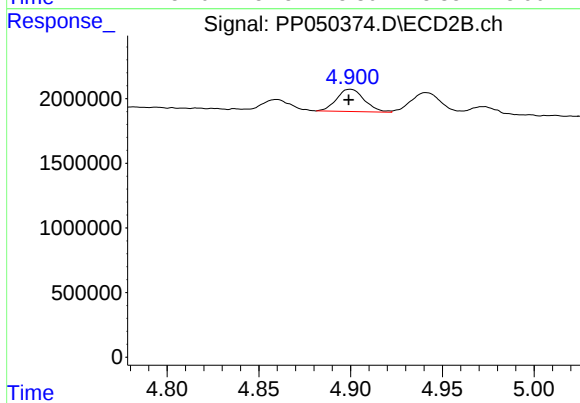

#22 AR-1248-2


R.T.: 4.900 min
Delta R.T.: 0.001 min
Response: 1820285
Conc: 21.07 ng/ml

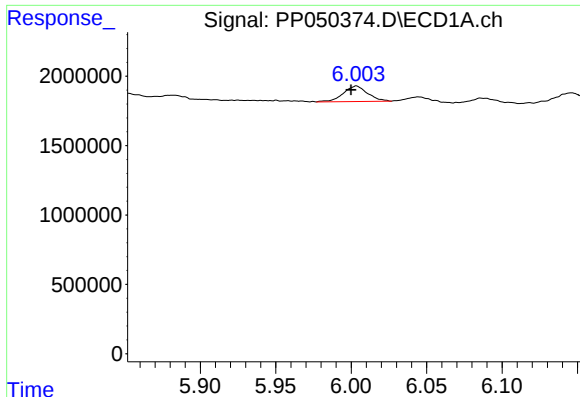

#23 AR-1248-3


R.T.: 6.003 min
Delta R.T.: 0.003 min
Response: 1262082
Conc: 19.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

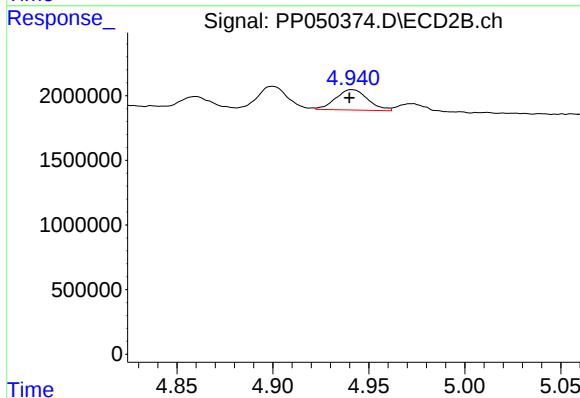


#23 AR-1248-3

R.T.: 4.941 min
Delta R.T.: 0.001 min
Response: 1851011
Conc: 20.42 ng/ml

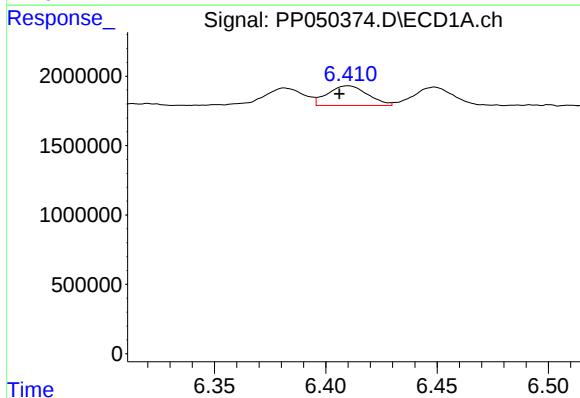


#24 AR-1248-4

R.T.: 6.410 min
Delta R.T.: 0.004 min
Response: 1771079
Conc: 22.39 ng/ml

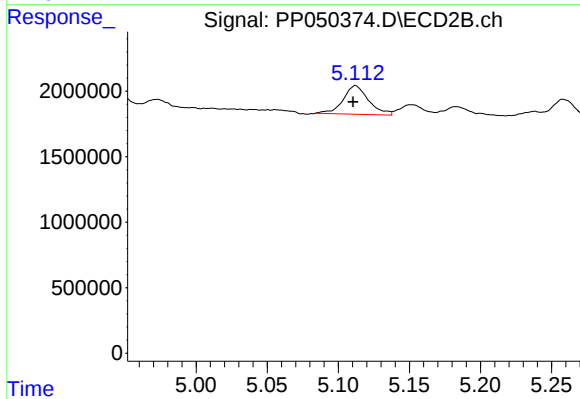

#24 AR-1248-4


R.T.: 5.112 min
Delta R.T.: 0.002 min
Response: 2701537
Conc: 25.63 ng/ml

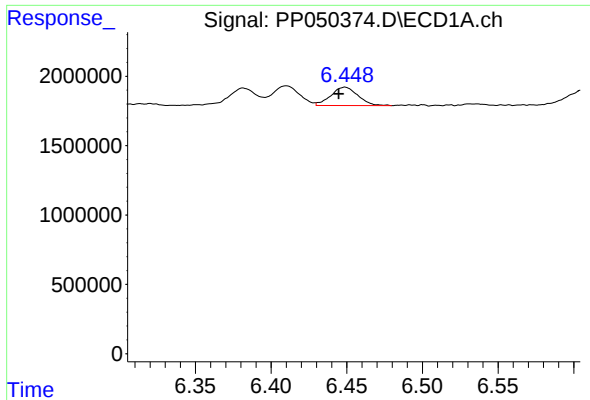

#25 AR-1248-5

R.T.: 6.449 min
Delta R.T.: 0.004 min
Response: 1656572
Conc: 21.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

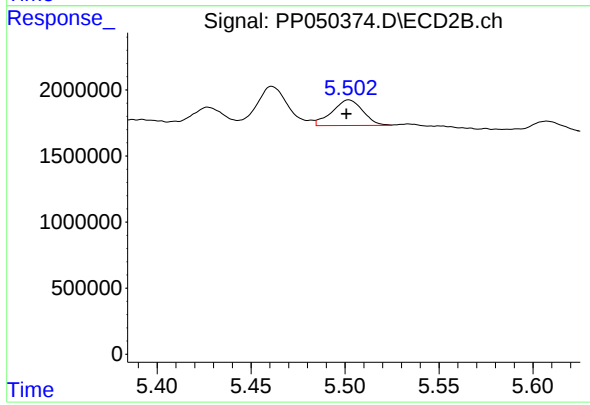

#25 AR-1248-5

R.T.: 5.502 min
Delta R.T.: 0.000 min
Response: 2203543
Conc: 22.19 ng/ml m