

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080922\
 Data File : PP050375.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2022 13:48
 Operator : YP\AJ
 Sample : N3980-07
 Misc : AR1254 LOD 25 PPB
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 01:38:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 09 11:38:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.348	3.595	24030026	46285865	14.929	14.777
2) SA Decachlor...	10.100	8.561	26940984	23067984	15.300	14.988
Target Compounds						
26) L6 AR-1254-1	6.385	5.462	1768106	3382933	23.898m	23.803m
27) L6 AR-1254-2	6.601	5.609	2528982	2955232	21.769	24.971
28) L6 AR-1254-3	6.973	6.011	2800584	4085807	22.601	23.745
29) L6 AR-1254-4	7.259	6.240	1975421	2478567	20.189m	23.492
30) L6 AR-1254-5	7.679	6.655	1861694	3056669	18.557m	22.956



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080922\
Data File : PP050375.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2022 13:48
Operator : YP\AJ
Sample : N3980-07
Misc : AR1254 LOD 25 PPB
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 01:38:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 09 11:38:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

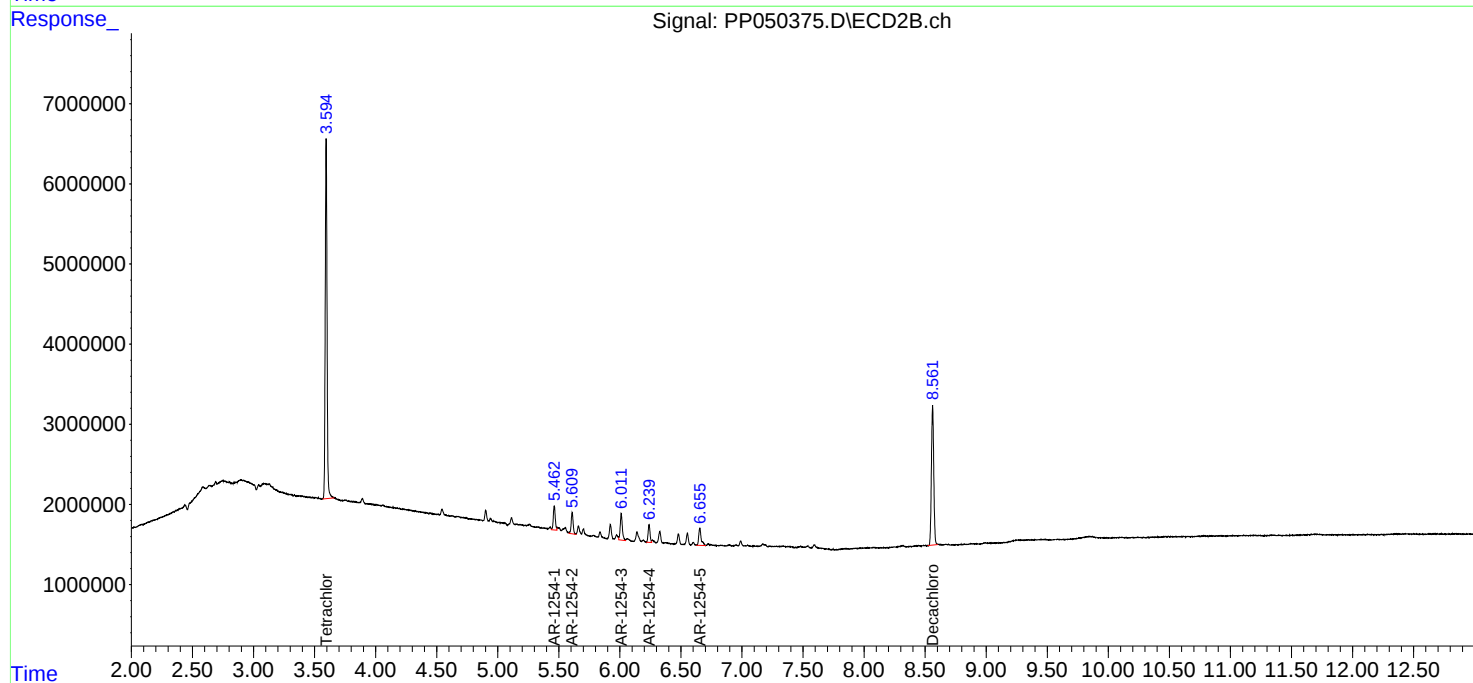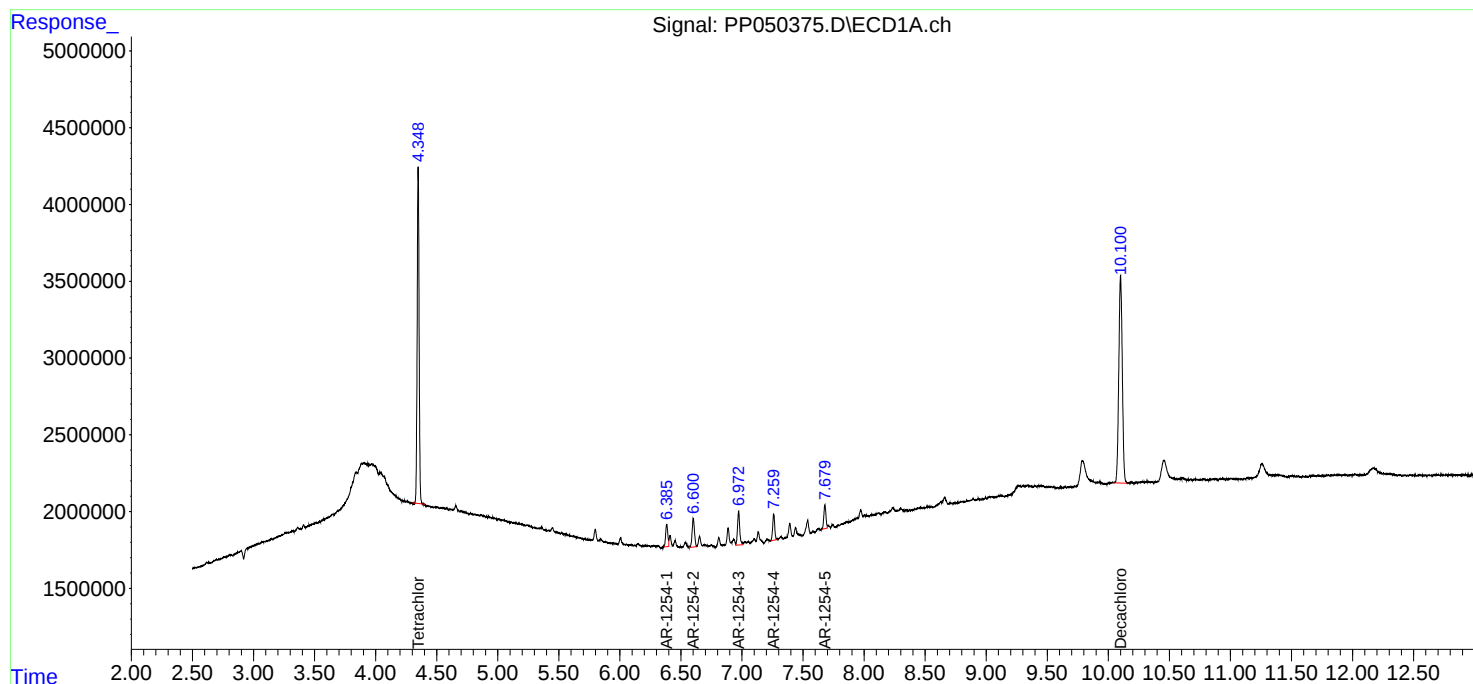


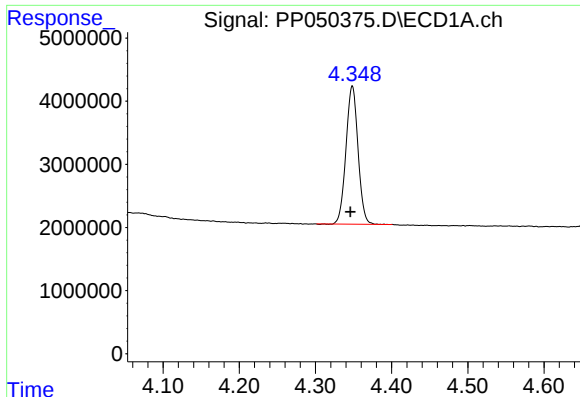

#1 Tetrachloro-m-xylene


R.T.: 4.348 min
Delta R.T.: 0.002 min
Response: 24030026
Conc: 14.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

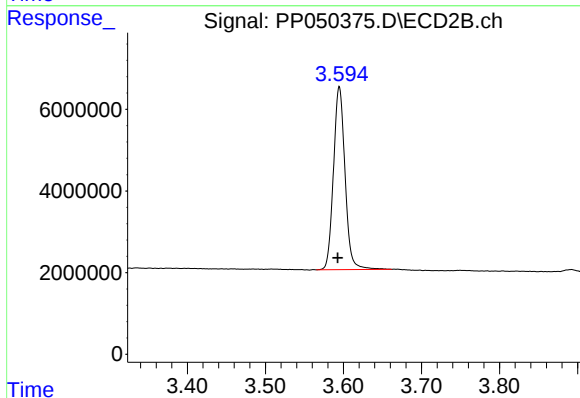


#1 Tetrachloro-m-xylene

R.T.: 3.595 min
Delta R.T.: 0.002 min
Response: 46285865
Conc: 14.78 ng/ml

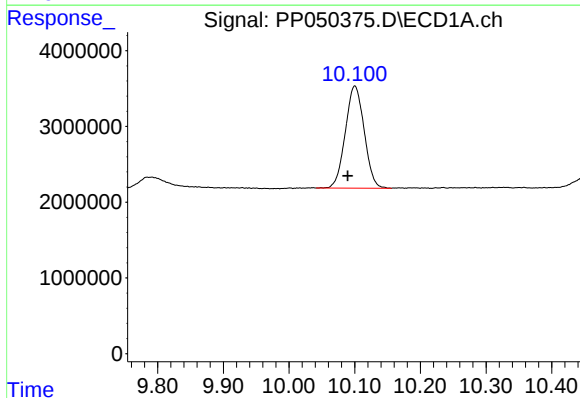


#2 Decachlorobiphenyl

R.T.: 10.100 min
Delta R.T.: 0.011 min
Response: 26940984
Conc: 15.30 ng/ml

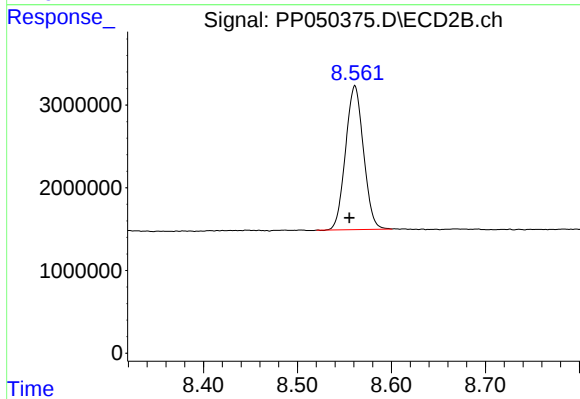

#2 Decachlorobiphenyl


R.T.: 8.561 min
Delta R.T.: 0.006 min
Response: 23067984
Conc: 14.99 ng/ml

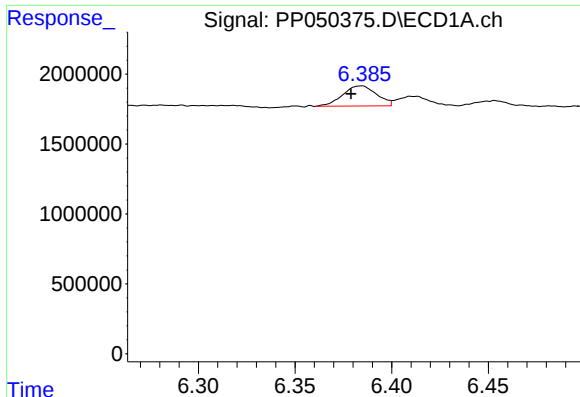

#26 AR-1254-1


R.T.: 6.385 min
Delta R.T.: 0.006 min
Response: 1768106
Conc: 23.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

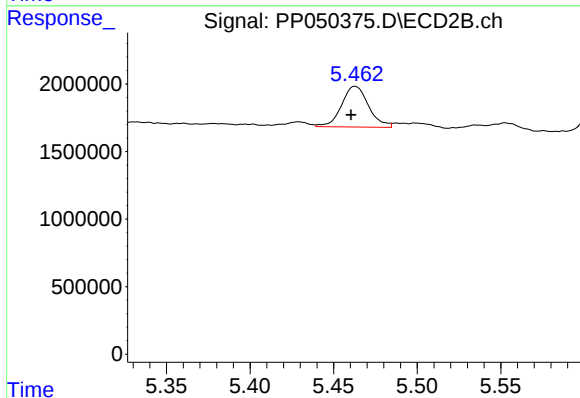


#26 AR-1254-1

R.T.: 5.462 min
Delta R.T.: 0.002 min
Response: 3382933
Conc: 23.80 ng/ml m

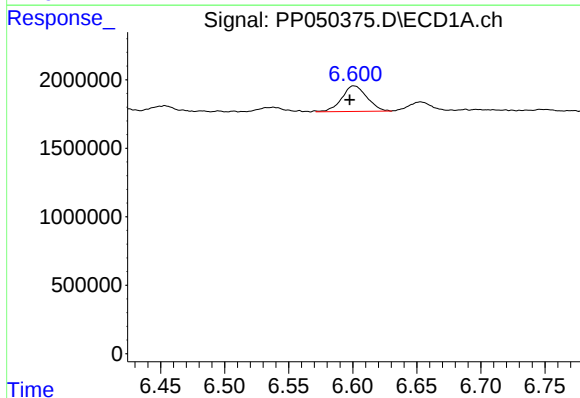


#27 AR-1254-2

R.T.: 6.601 min
Delta R.T.: 0.004 min
Response: 2528982
Conc: 21.77 ng/ml

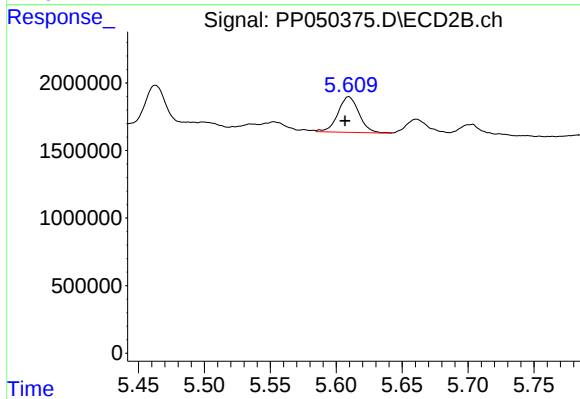

#27 AR-1254-2


R.T.: 5.609 min
Delta R.T.: 0.003 min
Response: 2955232
Conc: 24.97 ng/ml

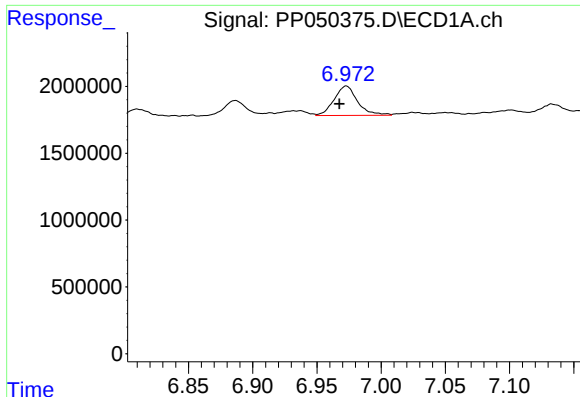

#28 AR-1254-3


R.T.: 6.973 min
Delta R.T.: 0.005 min
Response: 2800584
Conc: 22.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

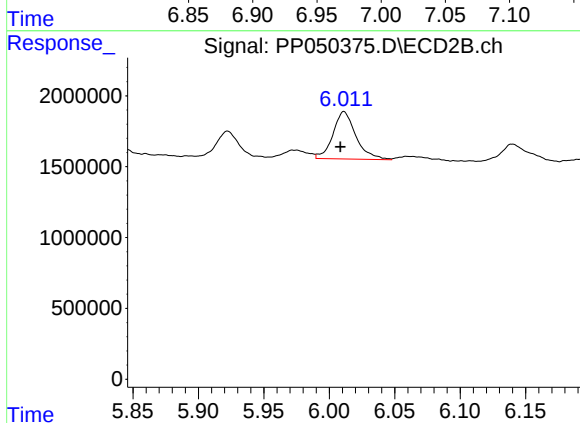


#28 AR-1254-3

R.T.: 6.011 min
Delta R.T.: 0.003 min
Response: 4085807
Conc: 23.74 ng/ml

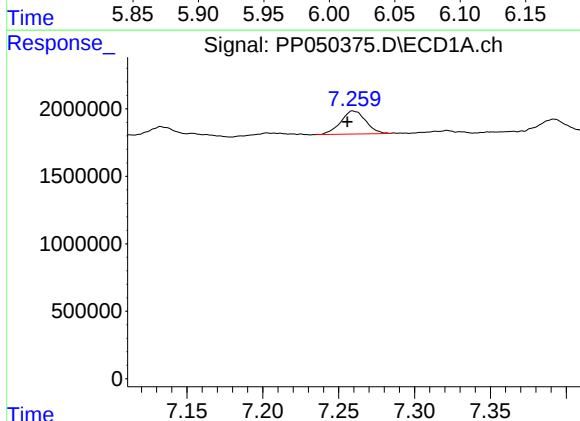


#29 AR-1254-4

R.T.: 7.259 min
Delta R.T.: 0.003 min
Response: 1975421
Conc: 20.19 ng/ml m

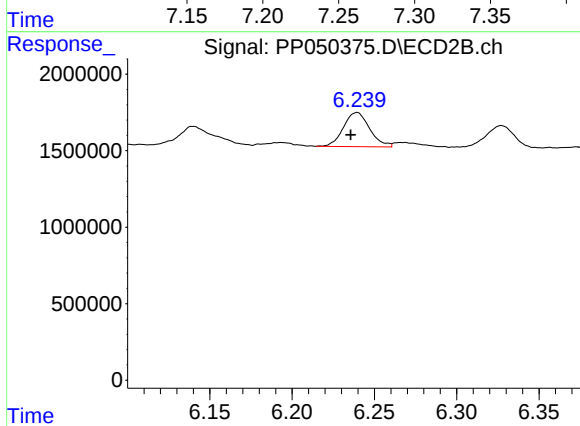

#29 AR-1254-4


R.T.: 6.240 min
Delta R.T.: 0.004 min
Response: 2478567
Conc: 23.49 ng/ml

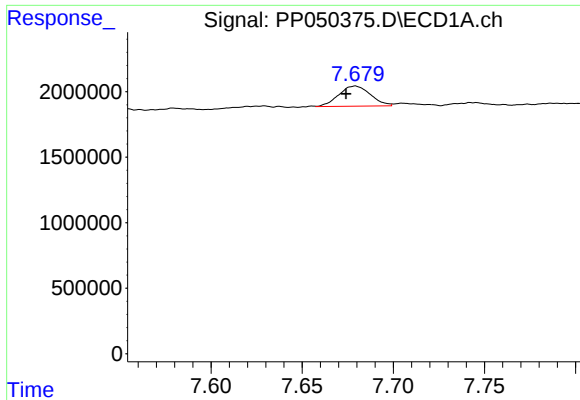

#30 AR-1254-5

R.T.: 7.679 min
Delta R.T.: 0.005 min
Response: 1861694
Conc: 18.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

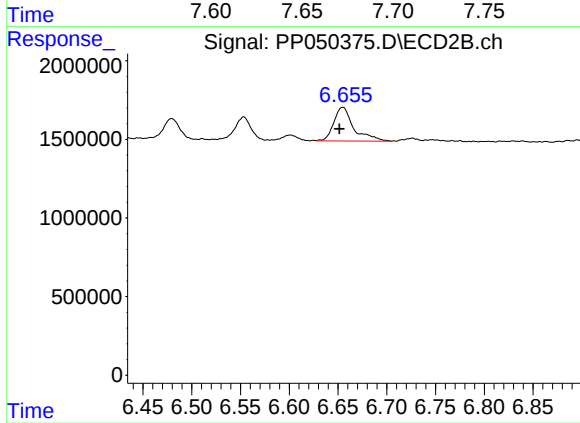

#30 AR-1254-5

R.T.: 6.655 min
Delta R.T.: 0.004 min
Response: 3056669
Conc: 22.96 ng/ml