

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080922\
 Data File : PP050377.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2022 14:21
 Operator : YP\AJ
 Sample : N3980-07
 Misc : AR1268 LOD 25 PPB
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 01:39:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 09 11:38:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.348	3.594	28217162	53922619	17.530	17.215
2) SA Decachlor...	10.100	8.560	34288696	29452355	19.472	19.136
Target Compounds						
41) L9 AR-1268-1	8.603	7.473	5987304	5740643	23.581	26.125
42) L9 AR-1268-2	8.701	7.538	5543656	4939159	22.727	24.798
43) L9 AR-1268-3	8.923	7.743	5049952	4112592	25.429	24.293
44) L9 AR-1268-4	9.358	8.031	1933235	1535314	22.430	21.608
45) L9 AR-1268-5	9.768	8.314	19210576	12398968	28.804	22.519



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080922\
Data File : PP050377.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2022 14:21
Operator : YP\AJ
Sample : N3980-07
Misc : AR1268 LOD 25 PPB
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 01:39:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 09 11:38:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

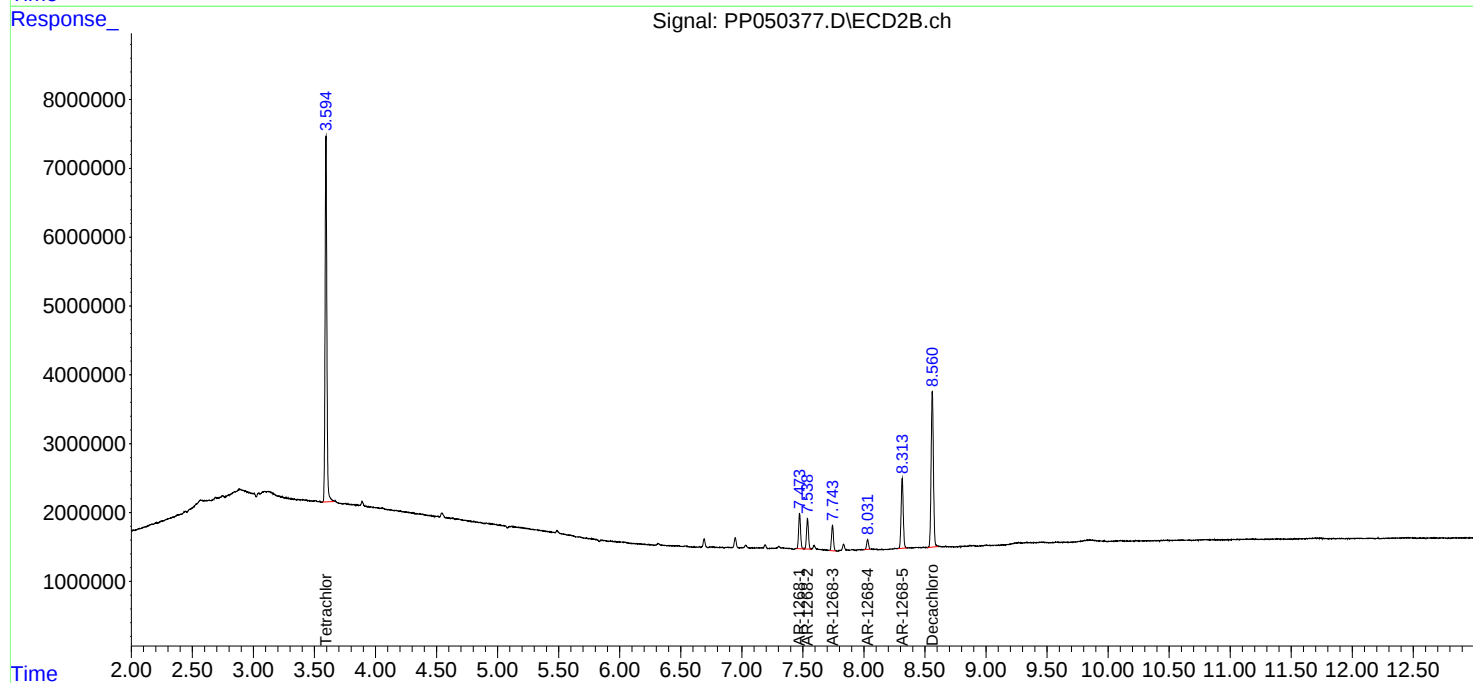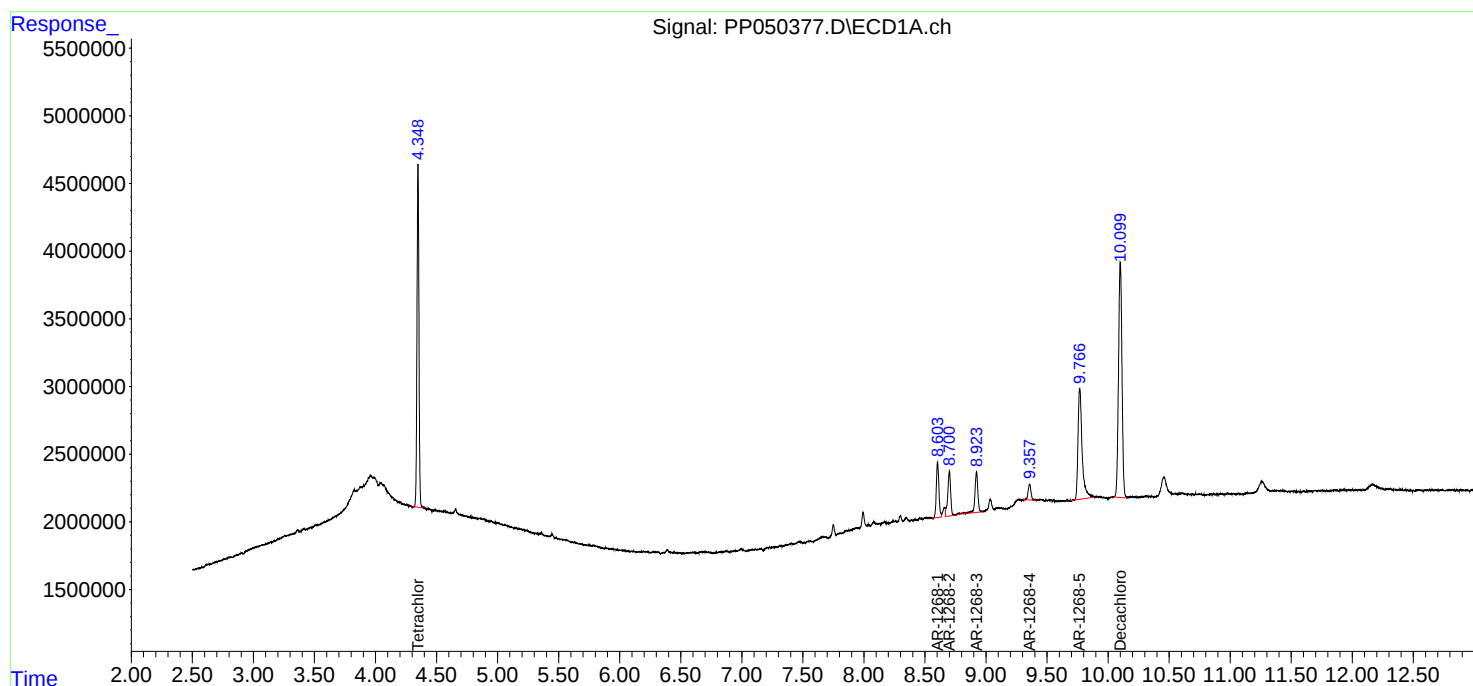


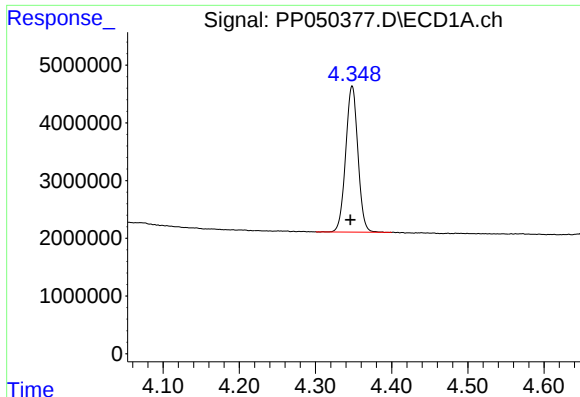

#1 Tetrachloro-m-xylene


R.T.: 4.348 min
Delta R.T.: 0.002 min
Response: 28217162
Conc: 17.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

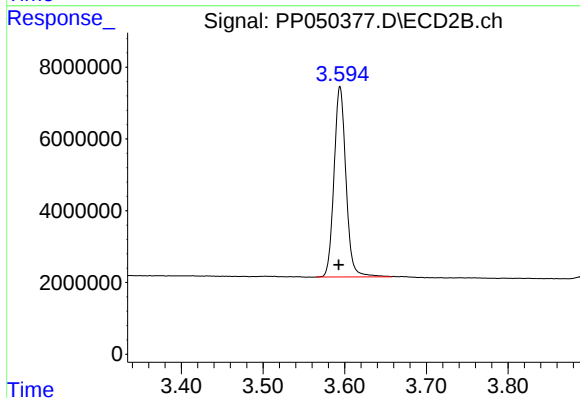


#1 Tetrachloro-m-xylene

R.T.: 3.594 min
Delta R.T.: 0.002 min
Response: 53922619
Conc: 17.22 ng/ml

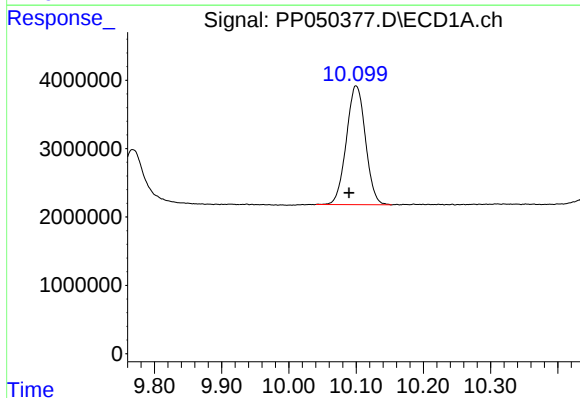


#2 Decachlorobiphenyl

R.T.: 10.100 min
Delta R.T.: 0.010 min
Response: 34288696
Conc: 19.47 ng/ml

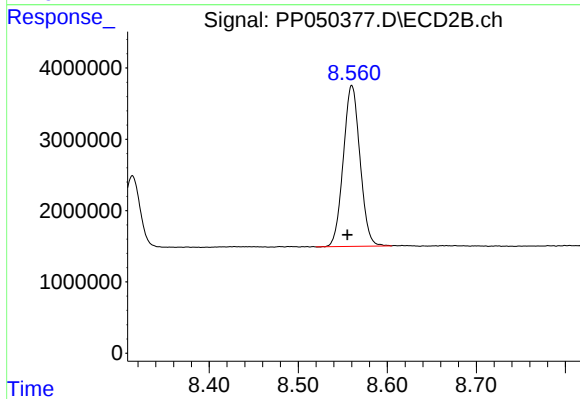

#2 Decachlorobiphenyl


R.T.: 8.560 min
Delta R.T.: 0.005 min
Response: 29452355
Conc: 19.14 ng/ml

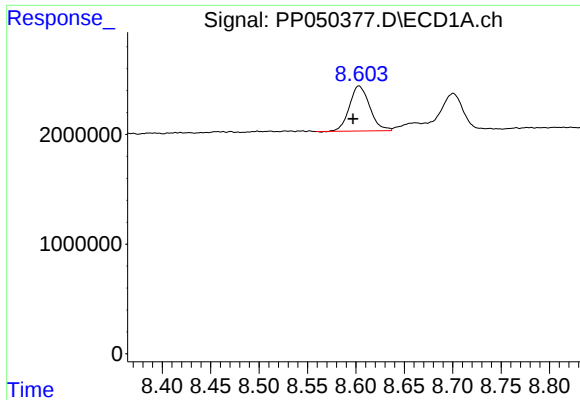

#41 AR-1268-1


R.T.: 8.603 min
Delta R.T.: 0.006 min
Response: 5987304
Conc: 23.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

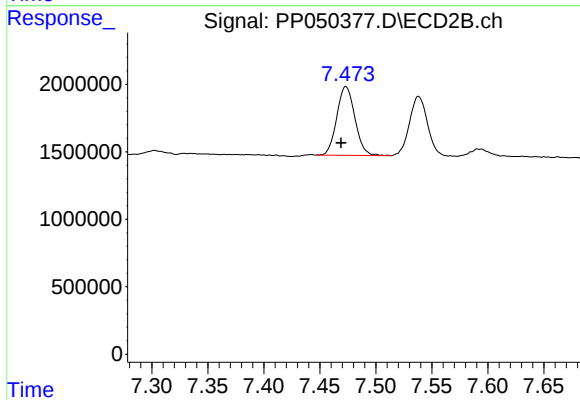


#41 AR-1268-1

R.T.: 7.473 min
Delta R.T.: 0.004 min
Response: 5740643
Conc: 26.13 ng/ml

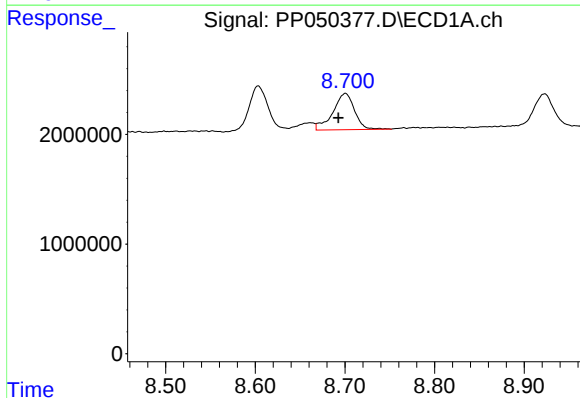


#42 AR-1268-2

R.T.: 8.701 min
Delta R.T.: 0.008 min
Response: 5543656
Conc: 22.73 ng/ml

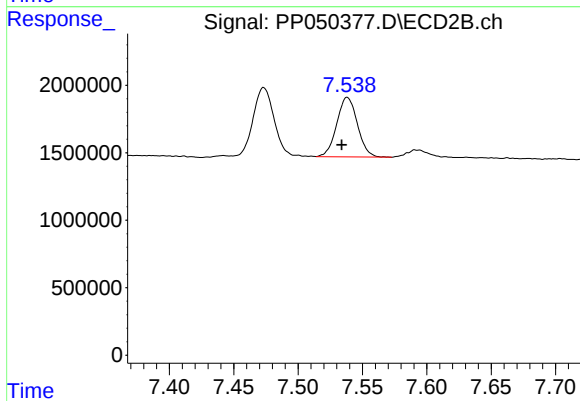

#42 AR-1268-2


R.T.: 7.538 min
Delta R.T.: 0.004 min
Response: 4939159
Conc: 24.80 ng/ml

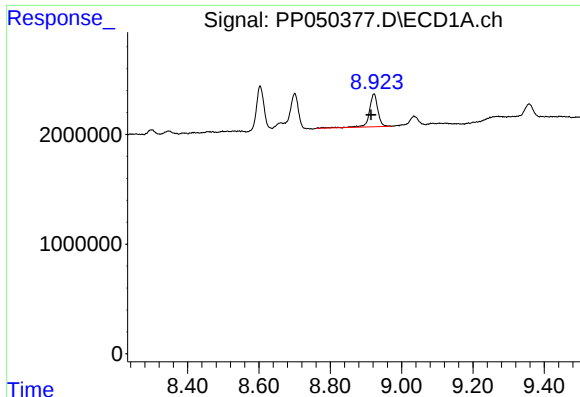

#43 AR-1268-3


R.T.: 8.923 min
Delta R.T.: 0.008 min
Response: 5049952
Conc: 25.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

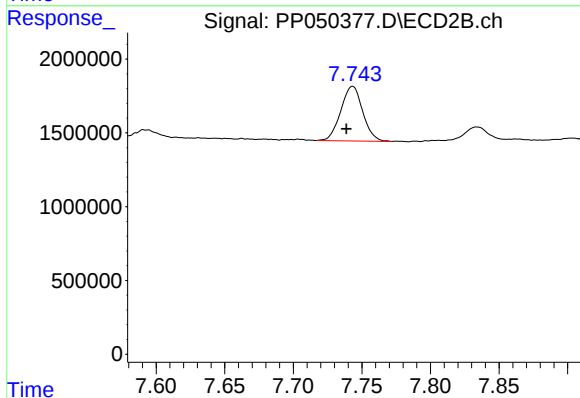


#43 AR-1268-3

R.T.: 7.743 min
Delta R.T.: 0.005 min
Response: 4112592
Conc: 24.29 ng/ml

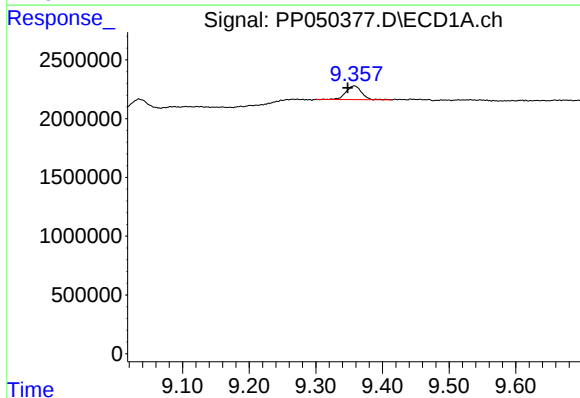


#44 AR-1268-4

R.T.: 9.358 min
Delta R.T.: 0.010 min
Response: 1933235
Conc: 22.43 ng/ml

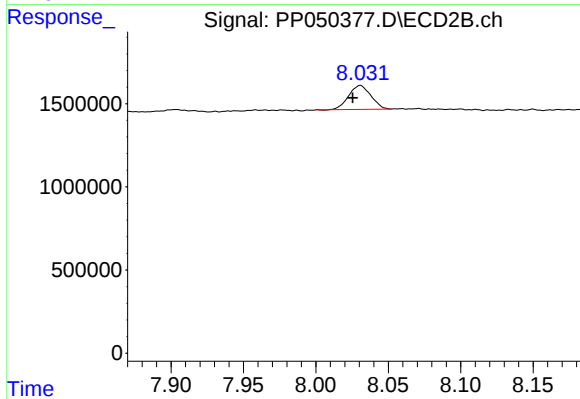

#44 AR-1268-4


R.T.: 8.031 min
Delta R.T.: 0.005 min
Response: 1535314
Conc: 21.61 ng/ml

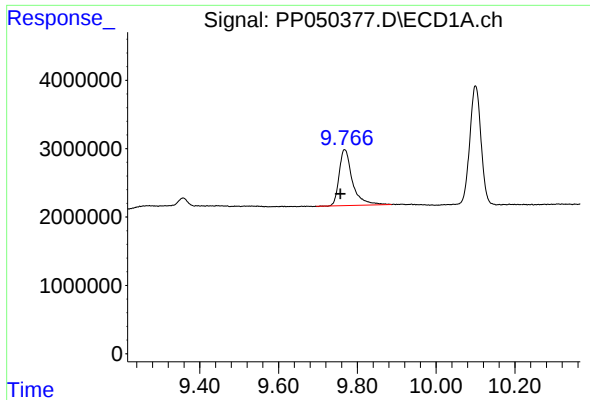

#45 AR-1268-5

R.T.: 9.768 min
Delta R.T.: 0.010 min
Response: 19210576
Conc: 28.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2022

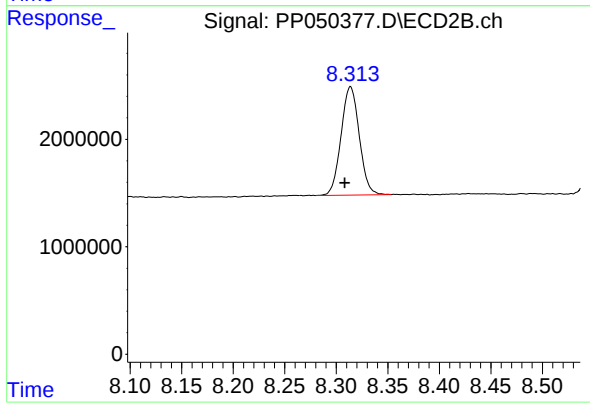

#45 AR-1268-5

R.T.: 8.314 min
Delta R.T.: 0.006 min
Response: 12398968
Conc: 22.52 ng/ml