

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081021\
 Data File : PP038214.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Aug 2021 21:51
 Operator : AJ\MA
 Sample : M3338-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 VNJ-202

Manual Integrations
 APPROVED

mohammad
 8/11/2021 2:47:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 02:43:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 06 03:08:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.895	3.885	601498	341904	13.535	13.275m
2) SA Decachlor...	10.879	9.143	440997	473518	19.386	18.302

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081021\
Data File : PP038214.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Aug 2021 21:51
Operator : AJ\MA
Sample : M3338-01
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
VNJ-202


Manual Integrations
APPROVED

mohammad
8/11/2021 2:47:48 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 02:43:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 06 03:08:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

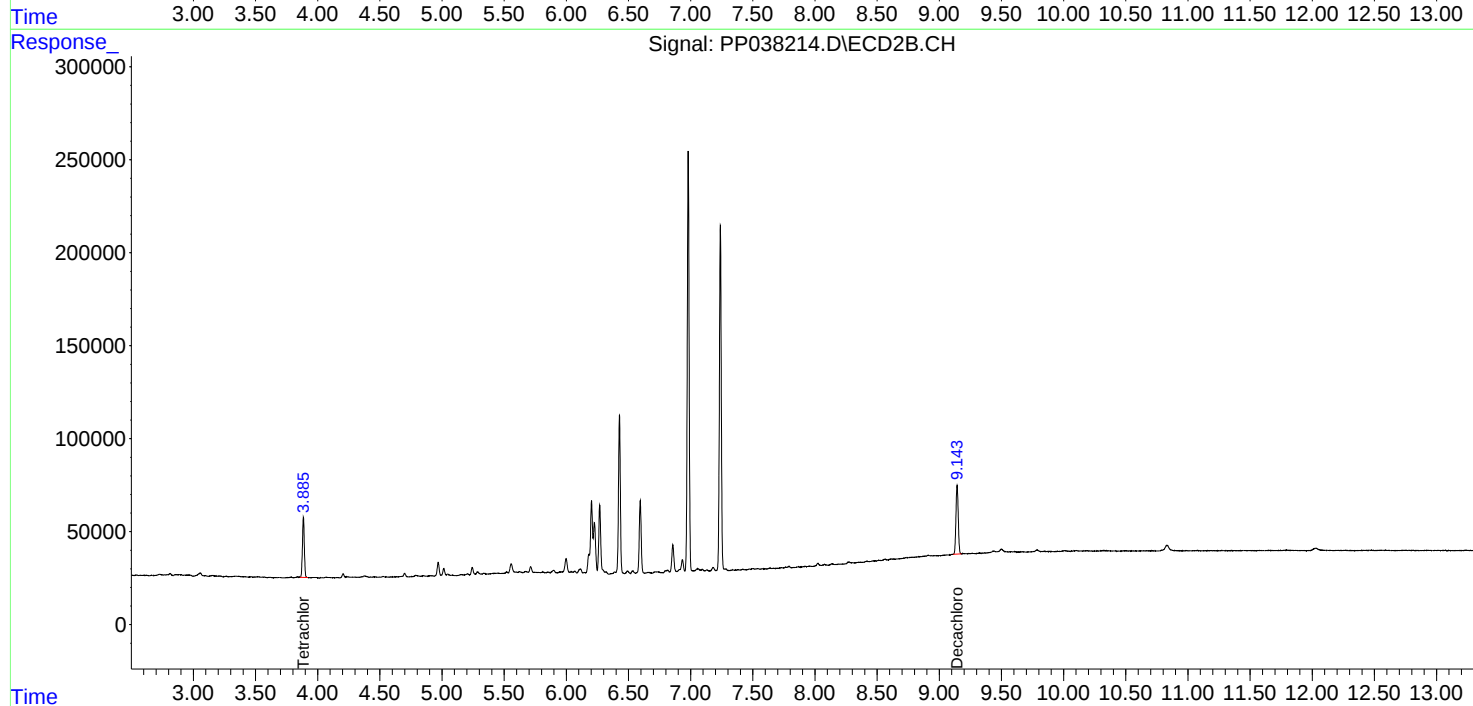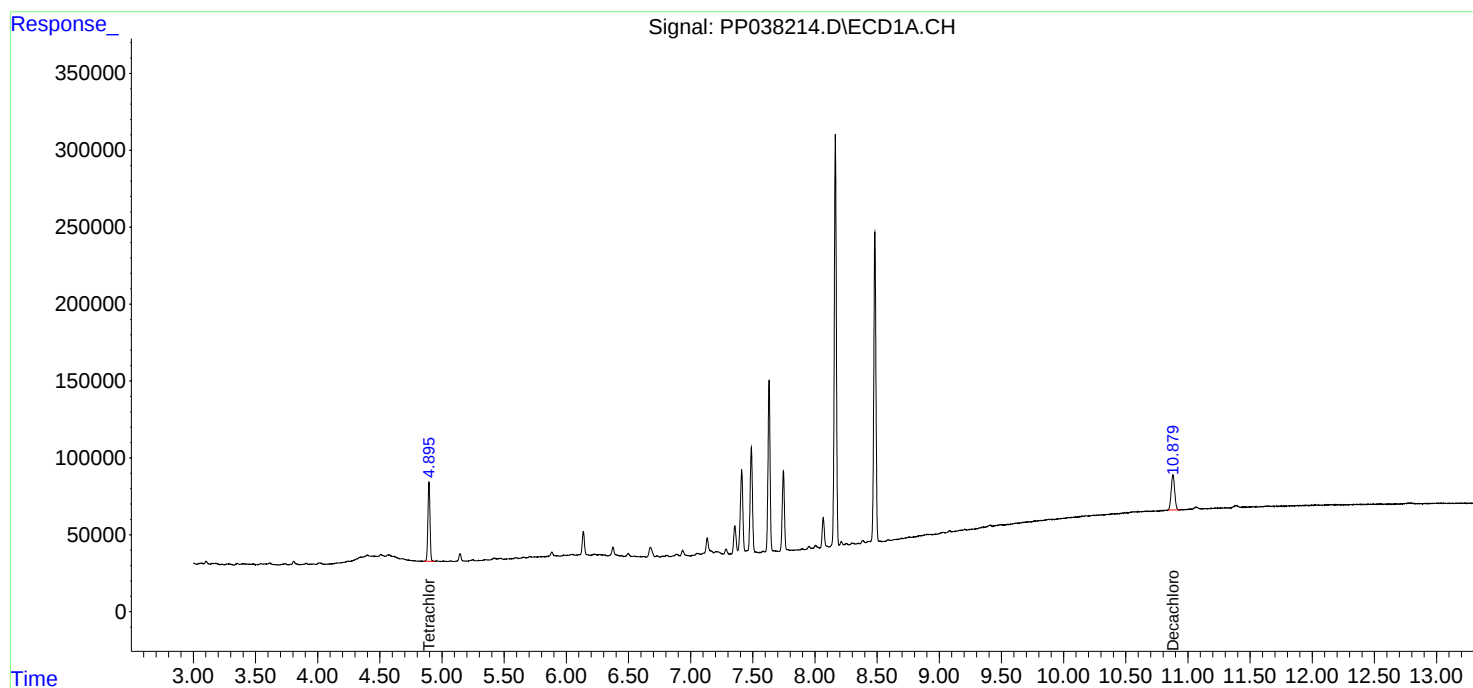

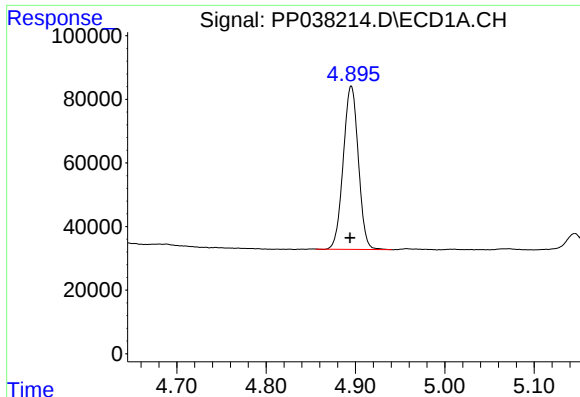


#1 Tetrachloro-m-xylene

R.T.: 4.895 min
Delta R.T.: 0.001 min
Response: 601498
Conc: 13.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
VNJ-202


Manual Integrations
APPROVED

mohammad
8/11/2021 2:47:48 PM

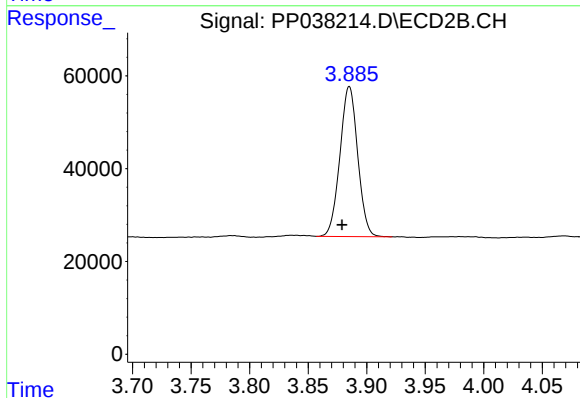


#1 Tetrachloro-m-xylene

R.T.: 3.885 min
Delta R.T.: 0.006 min
Response: 341904
Conc: 13.27 ng/ml m

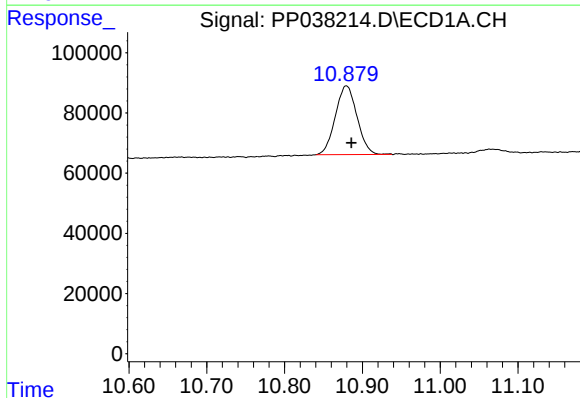

#2 Decachlorobiphenyl

R.T.: 10.879 min
Delta R.T.: -0.007 min
Response: 440997
Conc: 19.39 ng/ml

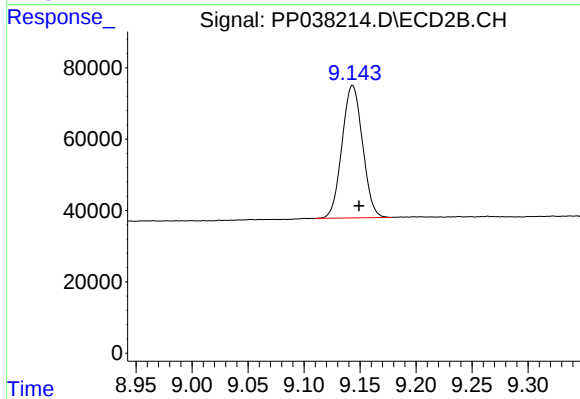

#2 Decachlorobiphenyl

R.T.: 9.143 min
Delta R.T.: -0.006 min
Response: 473518
Conc: 18.30 ng/ml