

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081023\
 Data File : PP059291.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2023 10:53
 Operator : YP\AJ
 Sample : 03572-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 21:39:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.415	3.646	21576439	36916373	17.584	18.220
2)	SA Decachlor...	10.209	8.681	16269911	31628791	21.317	22.483
Target Compounds							
26)	L6 AR-1254-1	6.452	5.545	1260165	2737362	26.976	27.018
27)	L6 AR-1254-2	6.672	5.694	1899230	2369533	27.602	26.842
28)	L6 AR-1254-3	7.039	6.098	2137311	3500869	30.966	25.324
29)	L6 AR-1254-4	7.326	6.329	1170026	2026968	25.992	25.217
30)	L6 AR-1254-5	7.746	6.748	1228268	2921861	26.141	24.433



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081023\
Data File : PP059291.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2023 10:53
Operator : YP\AJ
Sample : 03572-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 21:39:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 09 02:30:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

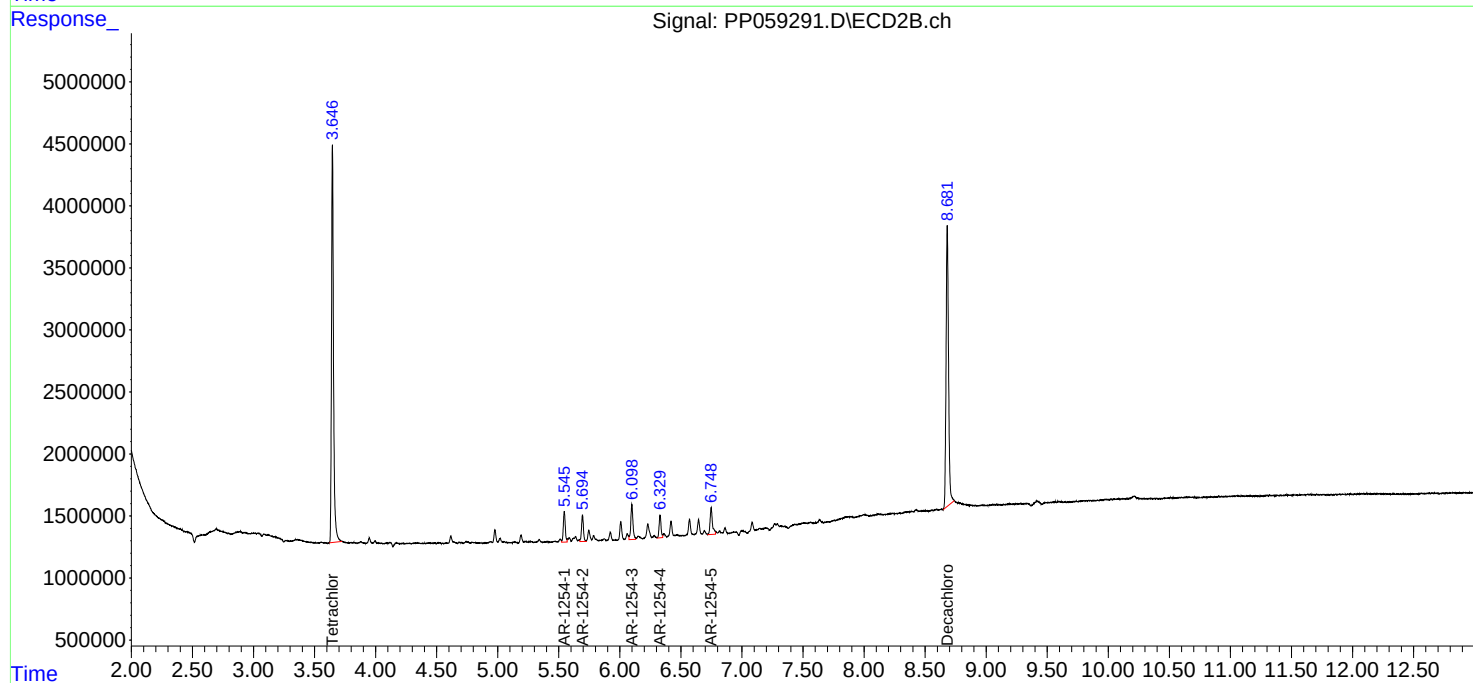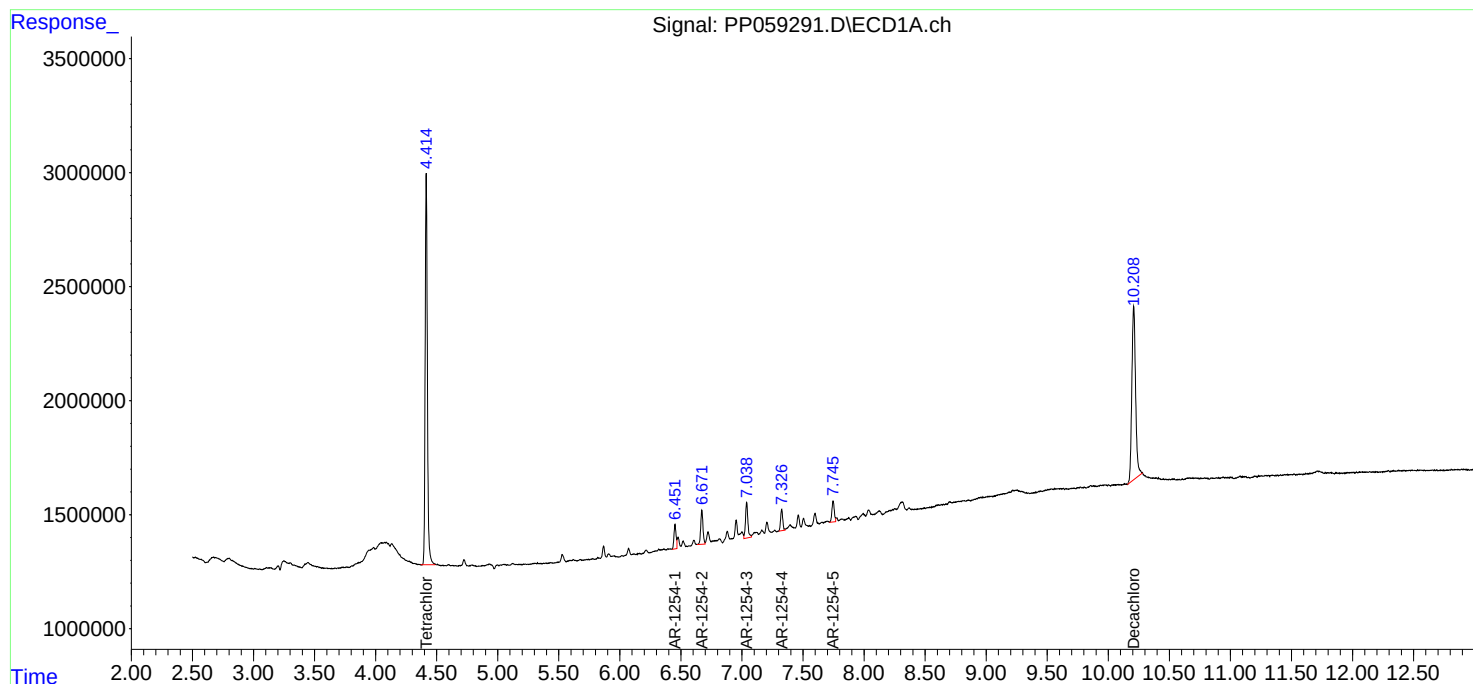


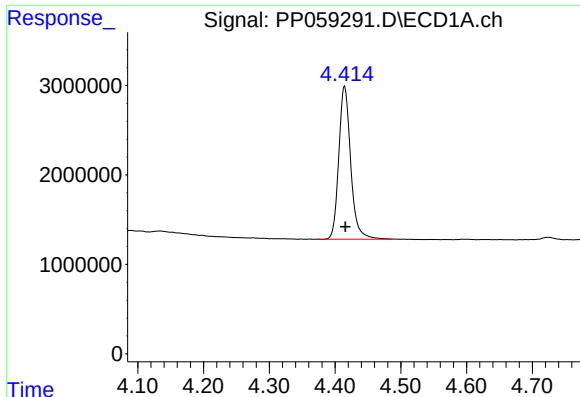

#1 Tetrachloro-m-xylene


R.T.: 4.415 min
Delta R.T.: -0.001 min
Response: 21576439
Conc: 17.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

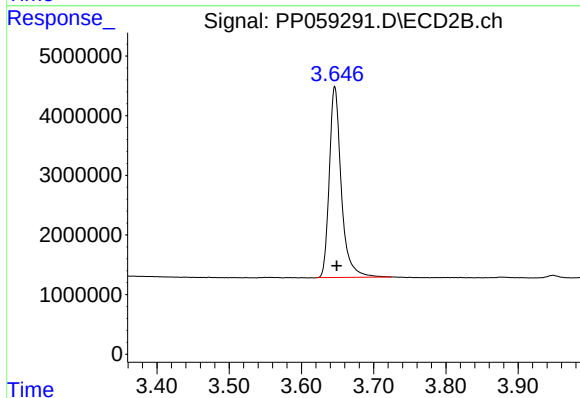


#1 Tetrachloro-m-xylene

R.T.: 3.646 min
Delta R.T.: -0.003 min
Response: 36916373
Conc: 18.22 ng/ml

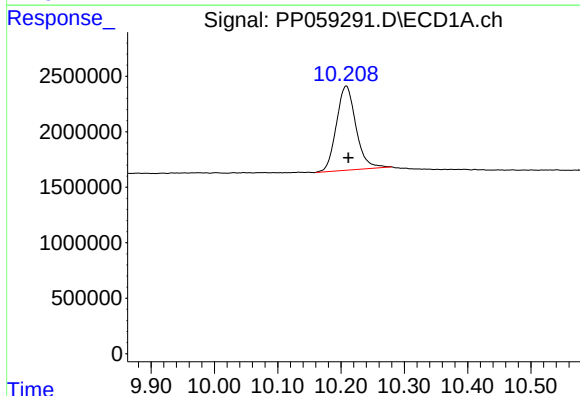


#2 Decachlorobiphenyl

R.T.: 10.209 min
Delta R.T.: -0.003 min
Response: 16269911
Conc: 21.32 ng/ml

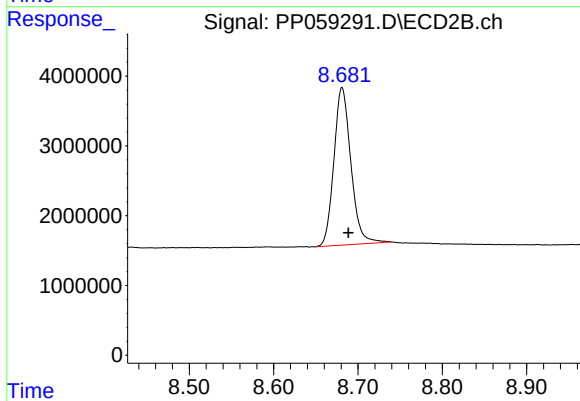

#2 Decachlorobiphenyl


R.T.: 8.681 min
Delta R.T.: -0.007 min
Response: 31628791
Conc: 22.48 ng/ml

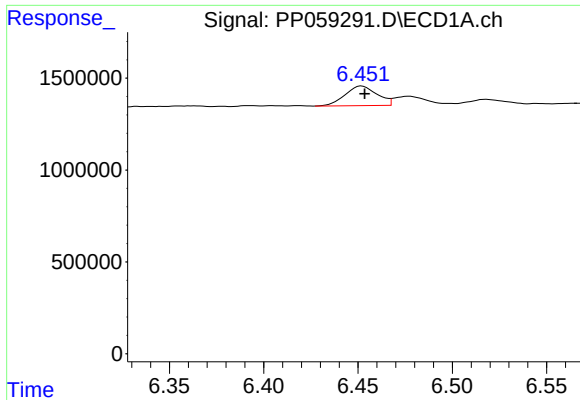

#26 AR-1254-1


R.T.: 6.452 min
Delta R.T.: -0.002 min
Response: 1260165
Conc: 26.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

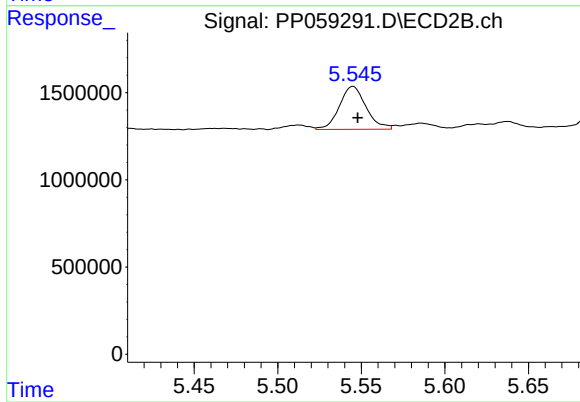


#26 AR-1254-1

R.T.: 5.545 min
Delta R.T.: -0.003 min
Response: 2737362
Conc: 27.02 ng/ml

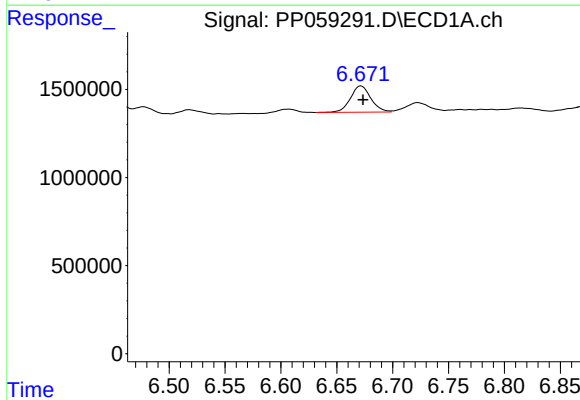


#27 AR-1254-2

R.T.: 6.672 min
Delta R.T.: -0.002 min
Response: 1899230
Conc: 27.60 ng/ml

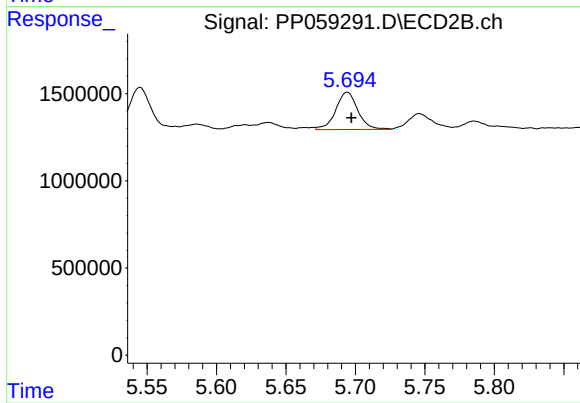

#27 AR-1254-2


R.T.: 5.694 min
Delta R.T.: -0.003 min
Response: 2369533
Conc: 26.84 ng/ml

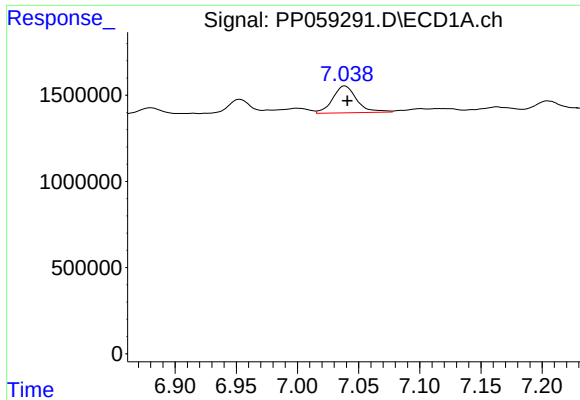

#28 AR-1254-3


R.T.: 7.039 min
Delta R.T.: -0.002 min
Response: 2137311
Conc: 30.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

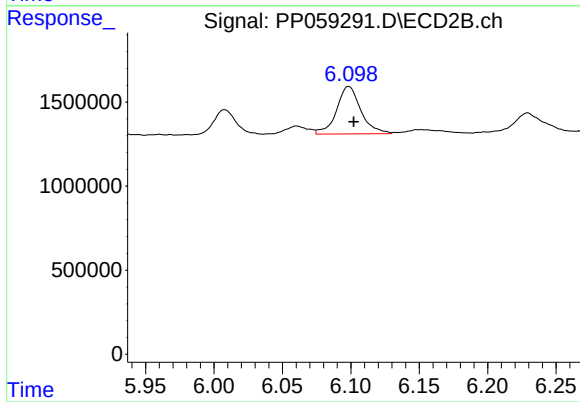


#28 AR-1254-3

R.T.: 6.098 min
Delta R.T.: -0.004 min
Response: 3500869
Conc: 25.32 ng/ml

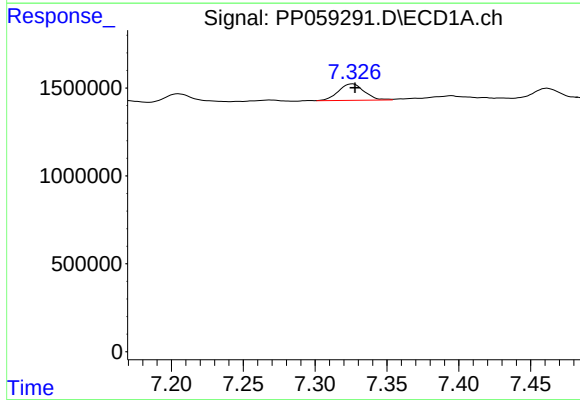


#29 AR-1254-4

R.T.: 7.326 min
Delta R.T.: -0.002 min
Response: 1170026
Conc: 25.99 ng/ml

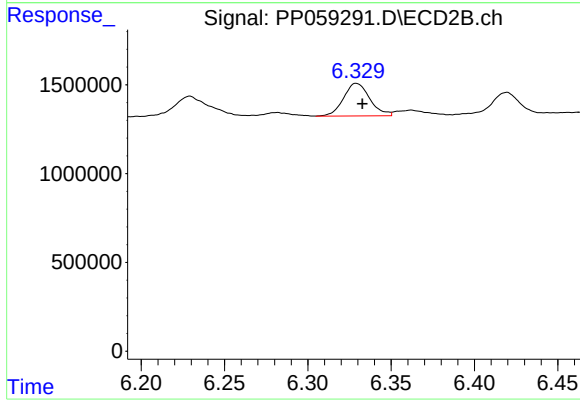

#29 AR-1254-4


R.T.: 6.329 min
Delta R.T.: -0.004 min
Response: 2026968
Conc: 25.22 ng/ml

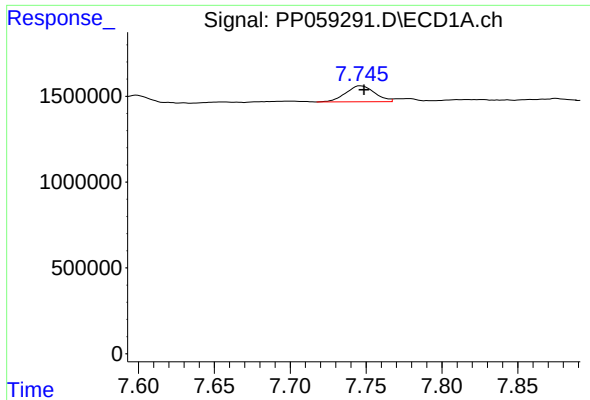

#30 AR-1254-5

R.T.: 7.746 min
Delta R.T.: -0.002 min
Response: 1228268
Conc: 26.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

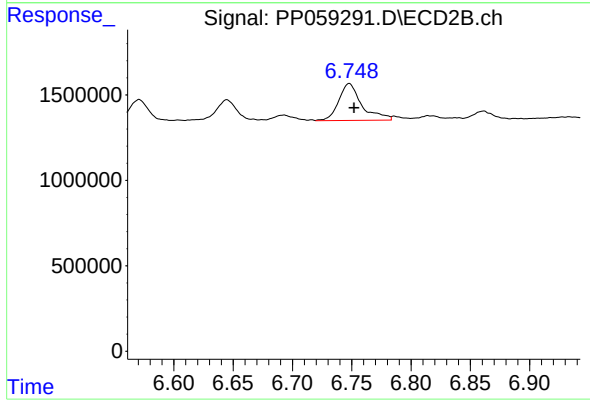

#30 AR-1254-5

R.T.: 6.748 min
Delta R.T.: -0.004 min
Response: 2921861
Conc: 24.43 ng/ml