

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081023\
 Data File : PP059292.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2023 11:09
 Operator : YP\AJ
 Sample : 03572-09
 Misc : AR1262 MDL 25 PPB
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 21:40:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.414	3.646	20324185	34747896	16.564	17.150
2) SA Decachlor...	10.207	8.682	15061158	29182368	19.733	20.744
Target Compounds						
36) L8 AR-1262-1	7.822	6.840	1548294	1207270	24.309	20.983
37) L8 AR-1262-2	8.370	7.046	1993611	2471971	21.708	20.949
38) L8 AR-1262-3	8.685	7.574	1394521	2048571	21.670	24.073
39) L8 AR-1262-4	8.778	7.638	654509	3427700	19.710	22.691
40) L8 AR-1262-5	9.440	8.136	626238	1594261	20.986	24.998



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081023\
Data File : PP059292.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2023 11:09
Operator : YP\AJ
Sample : 03572-09
Misc : AR1262 MDL 25 PPB
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 21:40:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 09 02:30:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

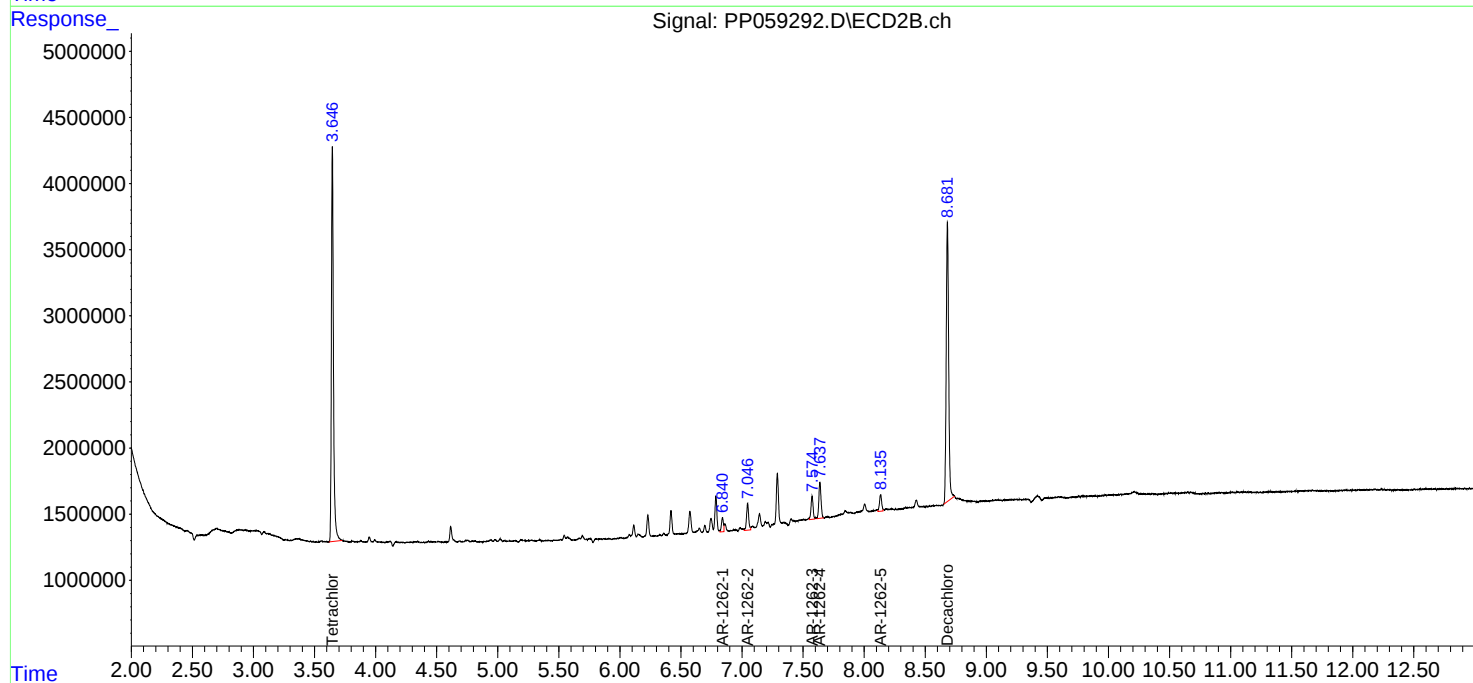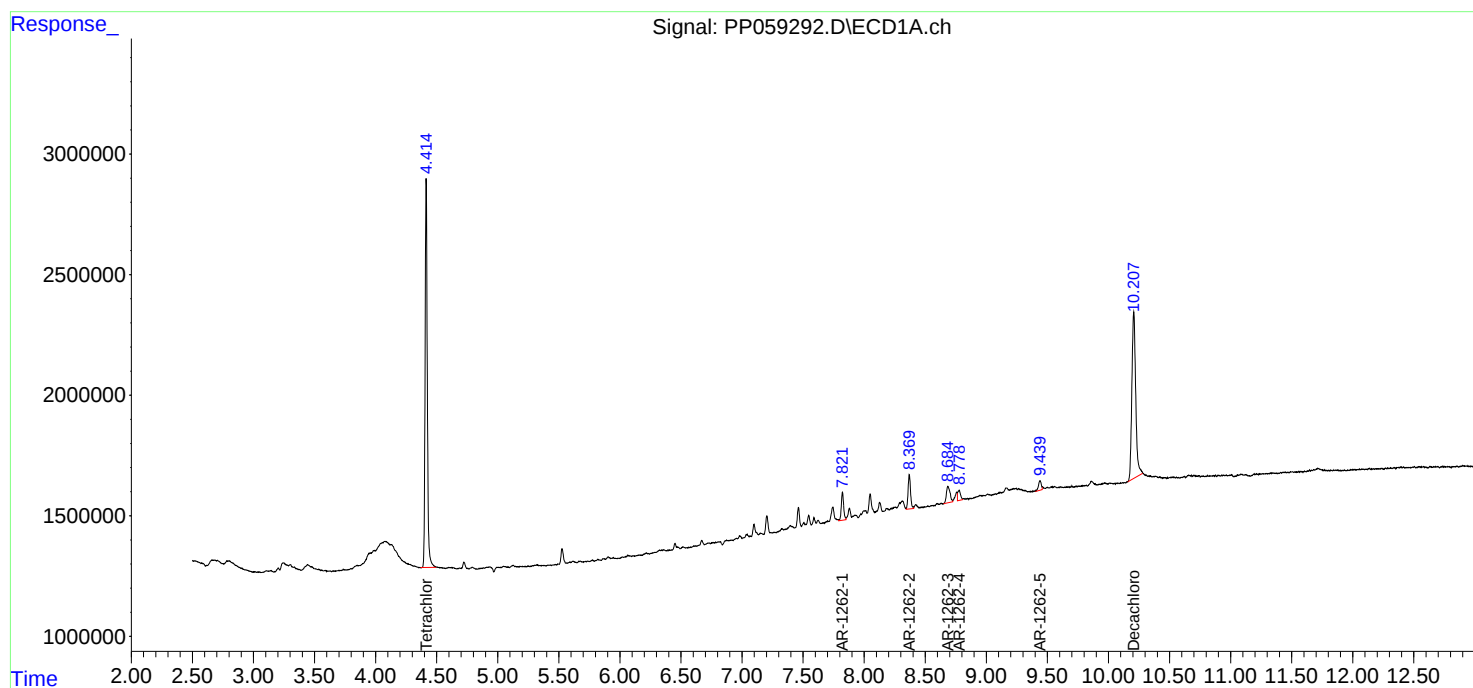


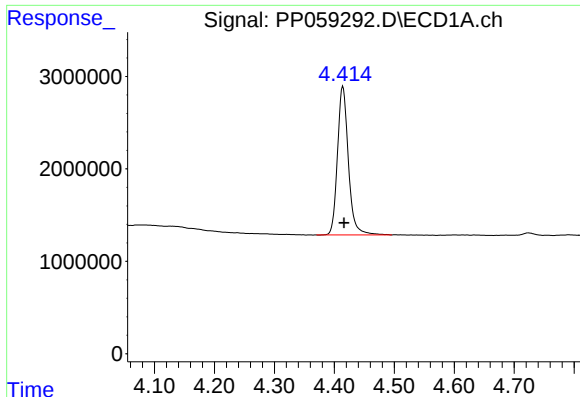

#1 Tetrachloro-m-xylene


R.T.: 4.414 min
Delta R.T.: -0.002 min
Response: 20324185
Conc: 16.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

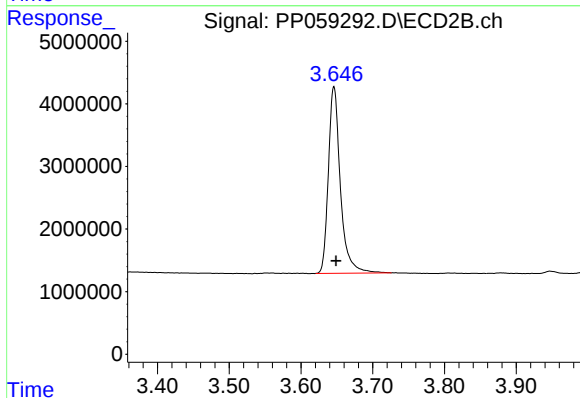


#1 Tetrachloro-m-xylene

R.T.: 3.646 min
Delta R.T.: -0.003 min
Response: 34747896
Conc: 17.15 ng/ml

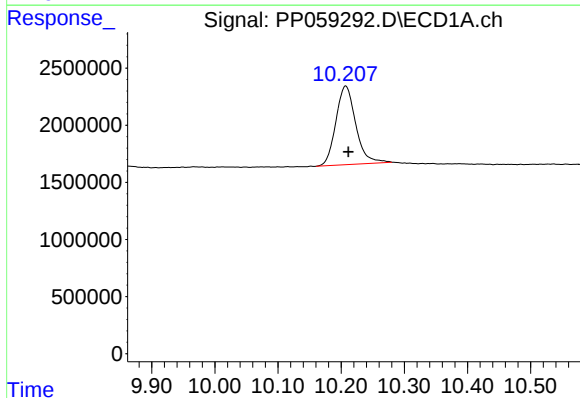


#2 Decachlorobiphenyl

R.T.: 10.207 min
Delta R.T.: -0.004 min
Response: 15061158
Conc: 19.73 ng/ml

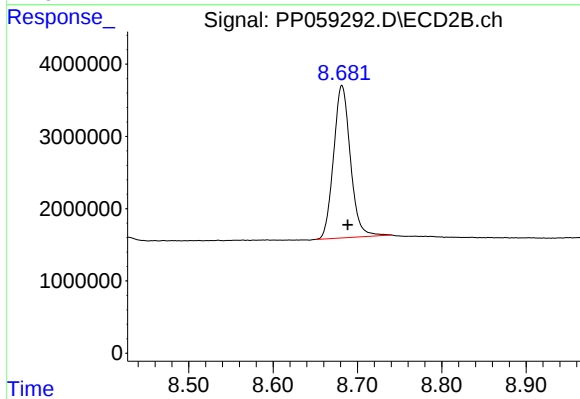

#2 Decachlorobiphenyl


R.T.: 8.682 min
Delta R.T.: -0.007 min
Response: 29182368
Conc: 20.74 ng/ml

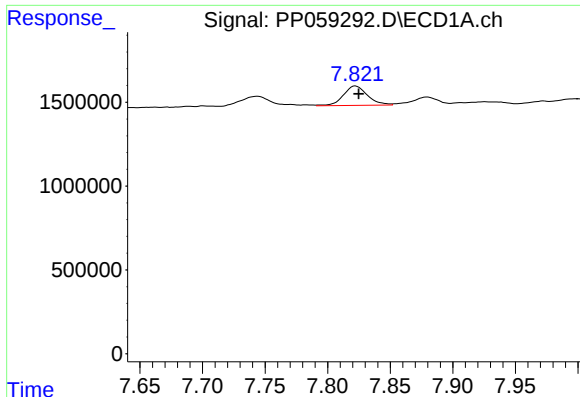

#36 AR-1262-1


R.T.: 7.822 min
Delta R.T.: -0.003 min
Response: 1548294
Conc: 24.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

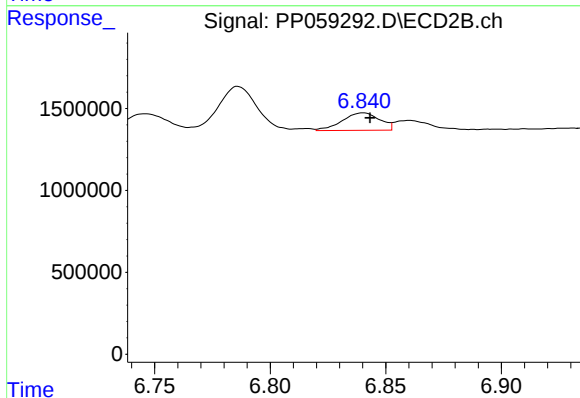


#36 AR-1262-1

R.T.: 6.840 min
Delta R.T.: -0.003 min
Response: 1207270
Conc: 20.98 ng/ml

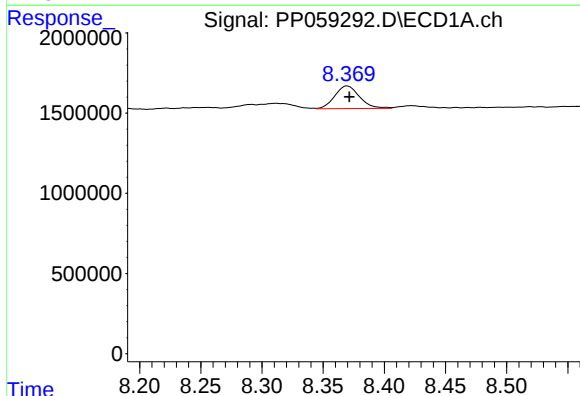


#37 AR-1262-2

R.T.: 8.370 min
Delta R.T.: -0.002 min
Response: 1993611
Conc: 21.71 ng/ml

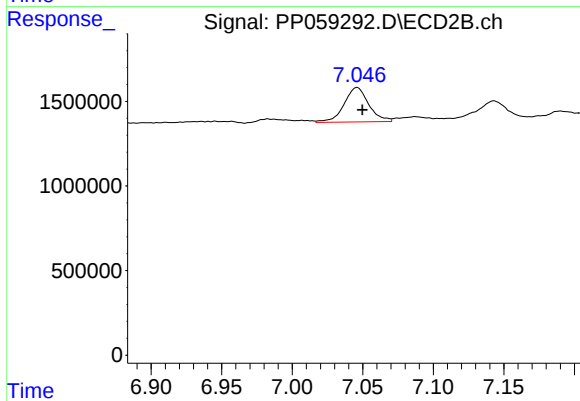

#37 AR-1262-2


R.T.: 7.046 min
Delta R.T.: -0.004 min
Response: 2471971
Conc: 20.95 ng/ml

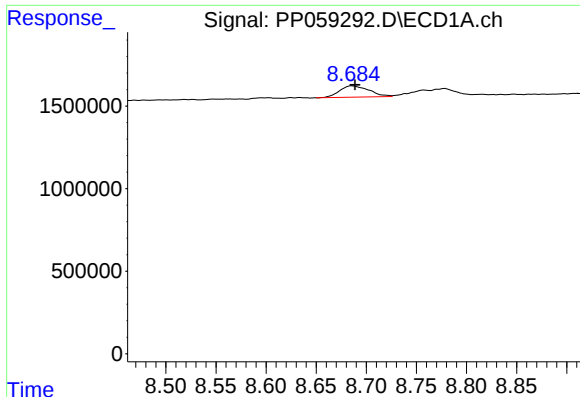

#38 AR-1262-3


R.T.: 8.685 min
Delta R.T.: -0.003 min
Response: 1394521
Conc: 21.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

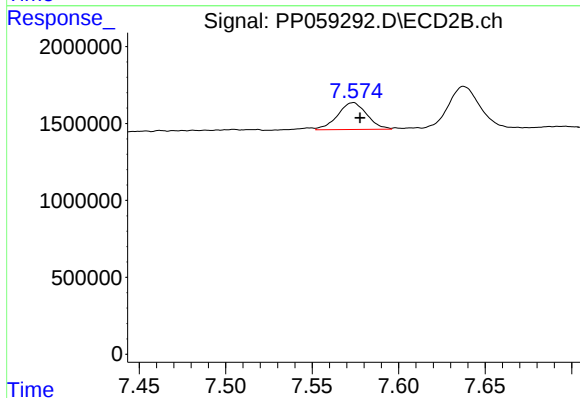


#38 AR-1262-3

R.T.: 7.574 min
Delta R.T.: -0.004 min
Response: 2048571
Conc: 24.07 ng/ml

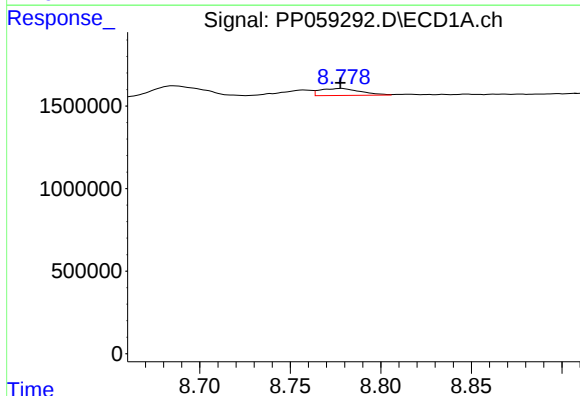


#39 AR-1262-4

R.T.: 8.778 min
Delta R.T.: 0.000 min
Response: 654509
Conc: 19.71 ng/ml

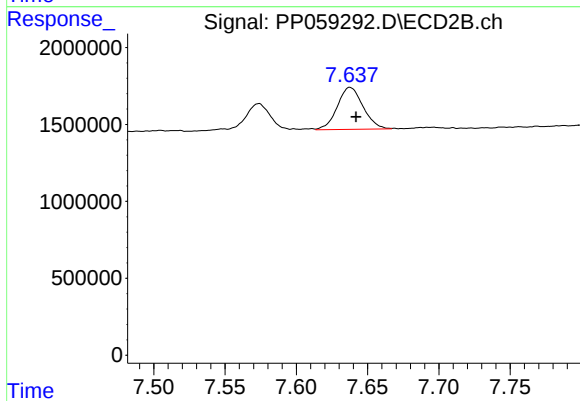

#39 AR-1262-4


R.T.: 7.638 min
Delta R.T.: -0.004 min
Response: 3427700
Conc: 22.69 ng/ml

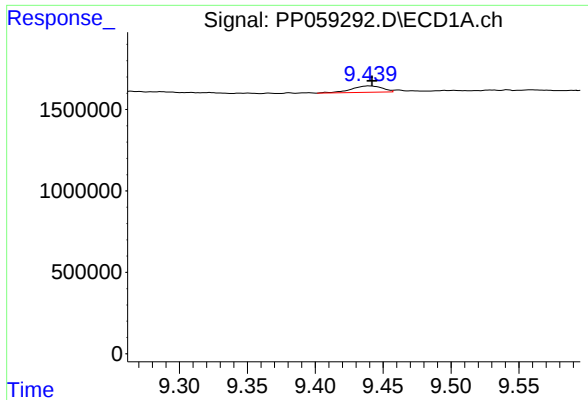

#40 AR-1262-5

R.T.: 9.440 min
Delta R.T.: -0.002 min
Response: 626238
Conc: 20.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2023

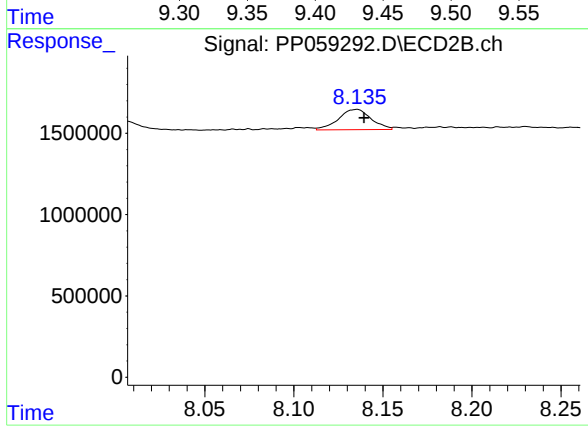

#40 AR-1262-5

R.T.: 8.136 min
Delta R.T.: -0.004 min
Response: 1594261
Conc: 25.00 ng/ml