

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081023\
 Data File : PP059312.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2023 16:37
 Operator : YP\AJ
 Sample : 03936-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TRADE-67-PAINT-CHIPS

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/11/2023
 Supervised By :Ankita Jodhani 08/11/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 21:57:12 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.415	3.647	26936202	39662218	21.952	19.575
2) SA Decachlor...	10.209	8.682	21546640	49506294	28.231	35.190
Target Compounds						
26) L6 AR-1254-1	6.458	5.548	51839808	74888466	1109.709	739.162 #
27) L6 AR-1254-2	6.675	5.695	52743429	43423065	766.530	491.888 #
28) L6 AR-1254-3	7.041	6.100	59589835	120.1E6	863.369	868.514
29) L6 AR-1254-4	7.328	6.330	49570219	77331218	1101.177m	962.061
30) L6 AR-1254-5	7.748	6.747	80906654	343.7E6	1721.893m	2874.061 #
31) L7 AR-1260-1	7.206	6.230	36714117	73048071	671.077	737.571
32) L7 AR-1260-2	7.457	6.423	111.2E6	187.1E6	1866.871	1616.676
33) L7 AR-1260-3	7.826	6.573	31904396	120.1E6	810.683	1080.029 #
34) L7 AR-1260-4	8.049	7.046	44911579	67656856	1011.209m	780.400
35) L7 AR-1260-5	8.372	7.290	44624711	165.8E6	558.020	899.578 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081023\
Data File : PP059312.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2023 16:37
Operator : YP\AJ
Sample : 03936-02
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TRADE-67-PAINT-CHIPS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/11/2023
Supervised By :Ankita Jodhani 08/11/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 21:57:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 09 02:30:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

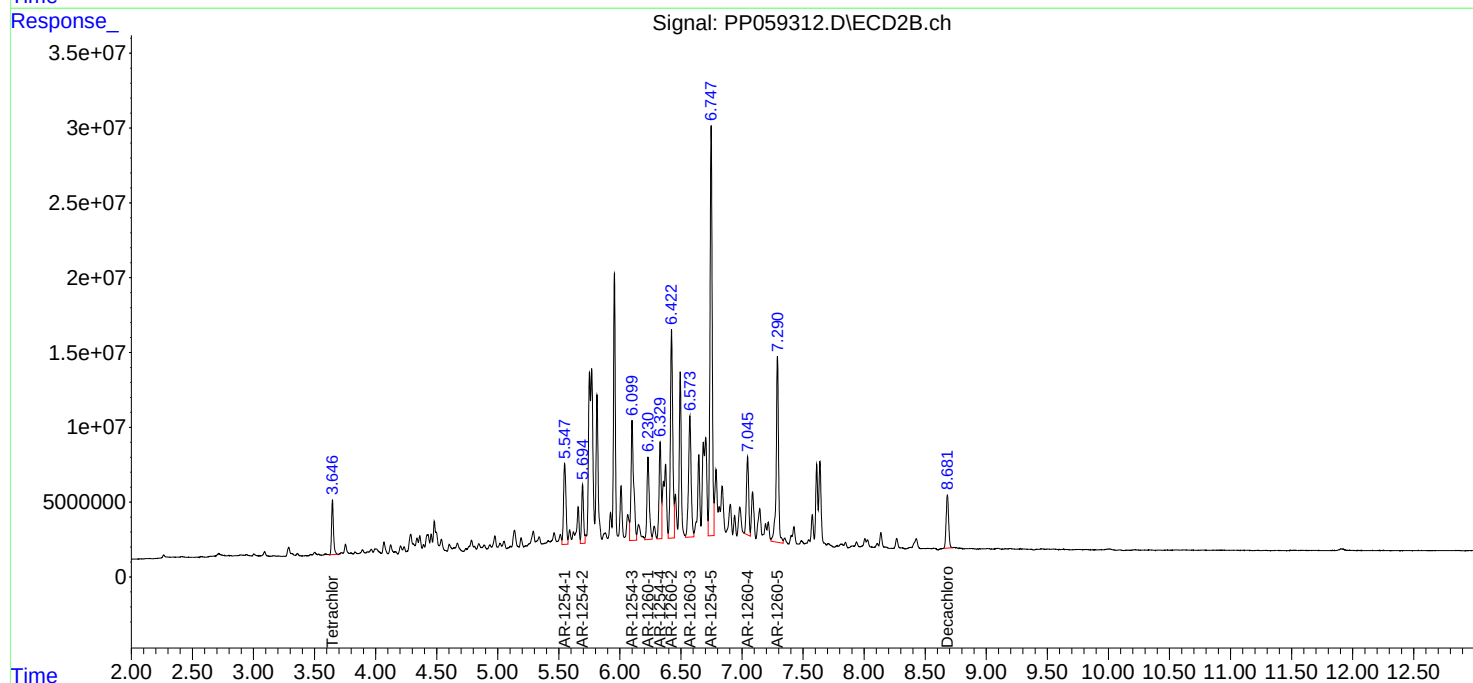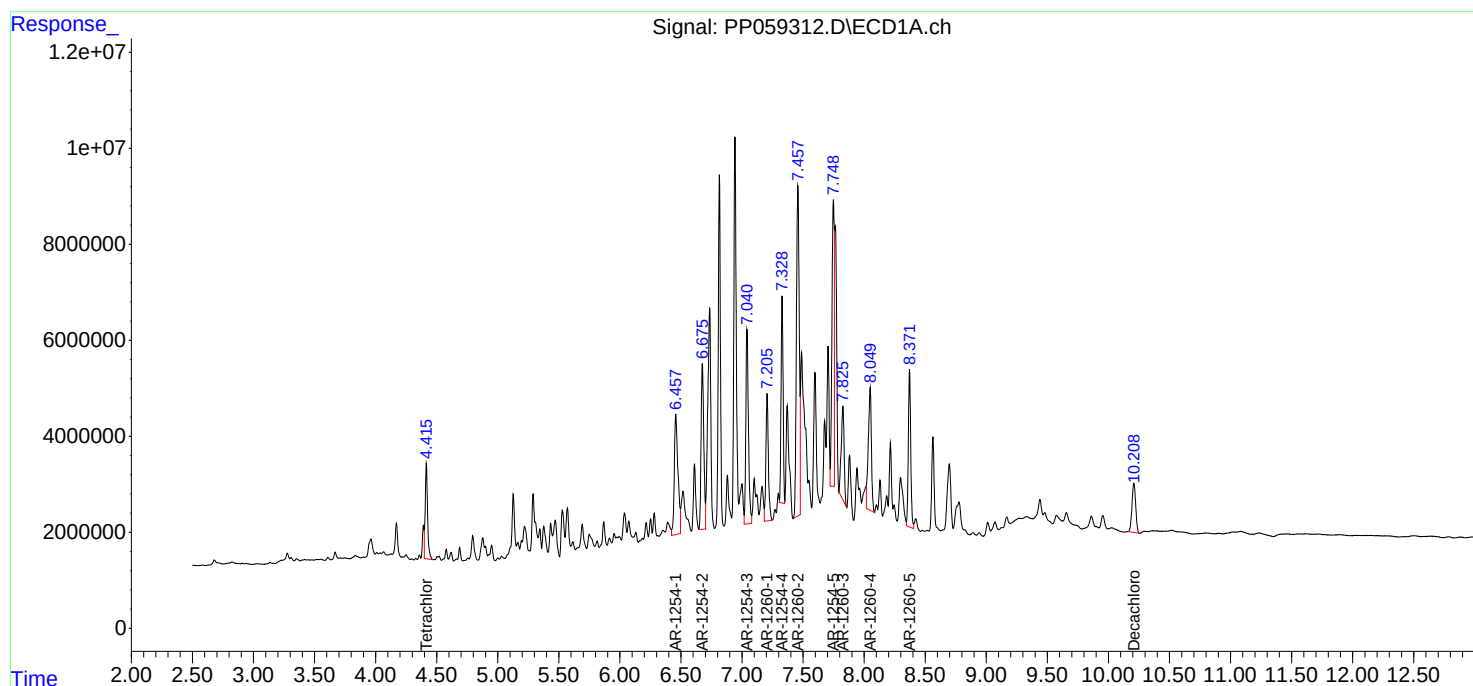

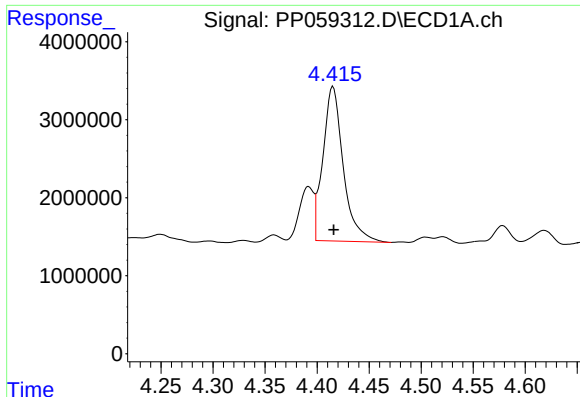


#1 Tetrachloro-m-xylene

R.T.: 4.415 min
Delta R.T.: 0.000 min
Response: 26936202
Conc: 21.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRADE-67-PAINT-CHIPS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/11/2023
Supervised By :Ankita Jodhani 08/11/2023

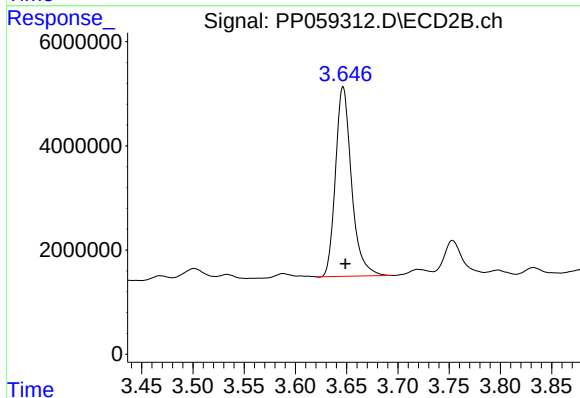


#1 Tetrachloro-m-xylene

R.T.: 3.647 min
Delta R.T.: -0.002 min
Response: 39662218
Conc: 19.58 ng/ml

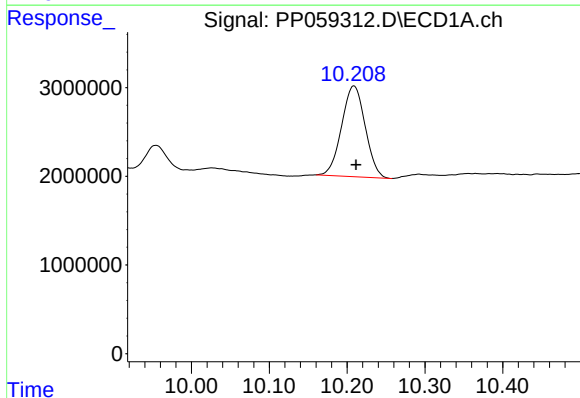


#2 Decachlorobiphenyl

R.T.: 10.209 min
Delta R.T.: -0.003 min
Response: 21546640
Conc: 28.23 ng/ml

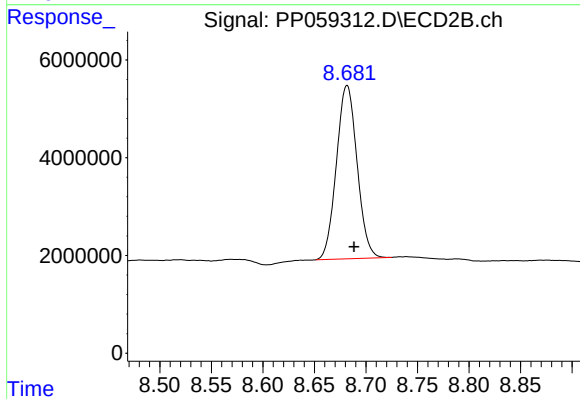

#2 Decachlorobiphenyl

R.T.: 8.682 min
Delta R.T.: -0.007 min
Response: 49506294
Conc: 35.19 ng/ml

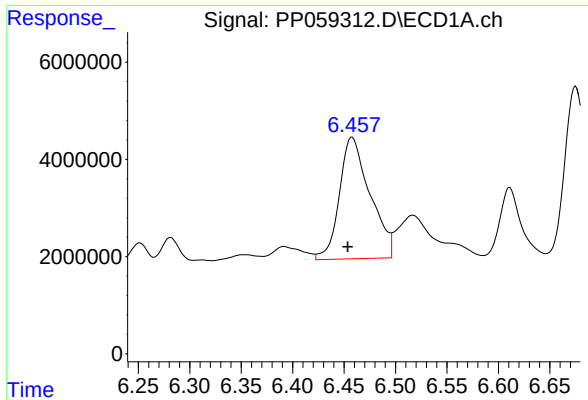


#26 AR-1254-1

R.T.: 6.458 min
Delta R.T.: 0.004 min
Response: 51839808
Conc: 1109.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRADE-67-PAINT-CHIPS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/11/2023
Supervised By :Ankita Jodhani 08/11/2023

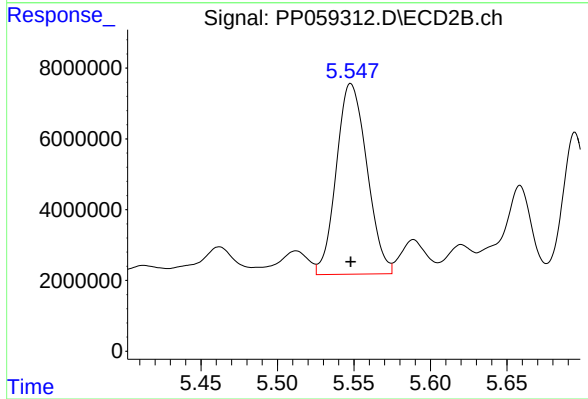


#26 AR-1254-1

R.T.: 5.548 min
Delta R.T.: 0.000 min
Response: 74888466
Conc: 739.16 ng/ml

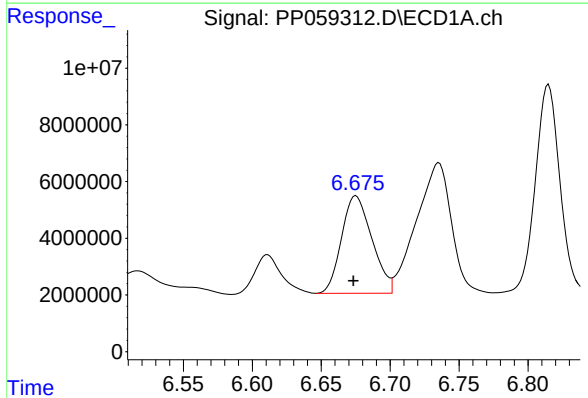


#27 AR-1254-2

R.T.: 6.675 min
Delta R.T.: 0.002 min
Response: 52743429
Conc: 766.53 ng/ml

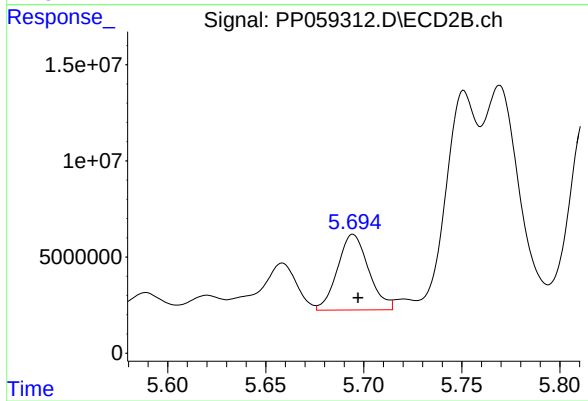

#27 AR-1254-2

R.T.: 5.695 min
Delta R.T.: -0.003 min
Response: 43423065
Conc: 491.89 ng/ml

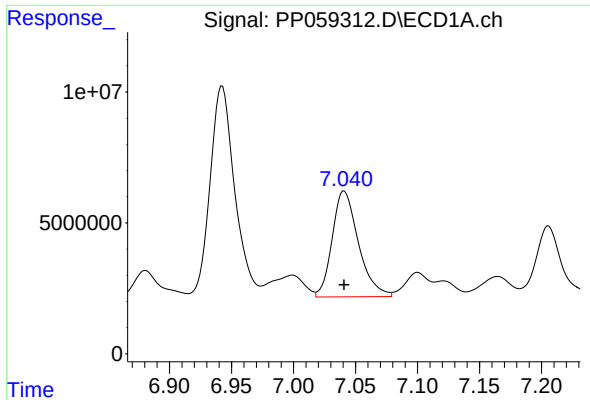


#28 AR-1254-3

R.T.: 7.041 min
Delta R.T.: 0.000 min
Response: 59589835
Conc: 863.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRADE-67-PAINT-CHIPS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/11/2023
Supervised By :Ankita Jodhani 08/11/2023

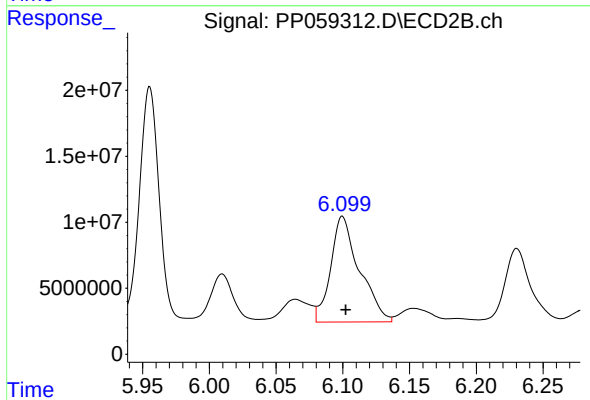


#28 AR-1254-3

R.T.: 6.100 min
Delta R.T.: -0.002 min
Response: 120068309
Conc: 868.51 ng/ml

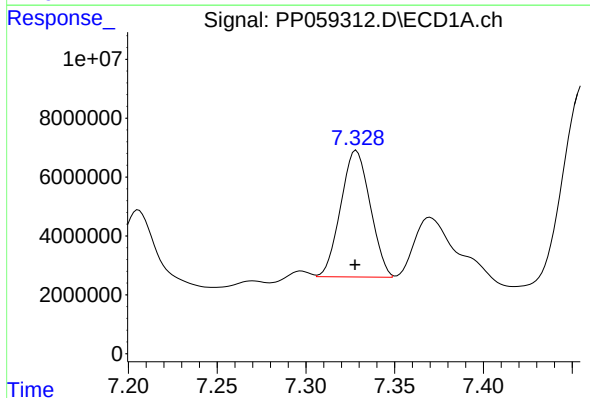


#29 AR-1254-4

R.T.: 7.328 min
Delta R.T.: 0.000 min
Response: 49570219
Conc: 1101.18 ng/ml m

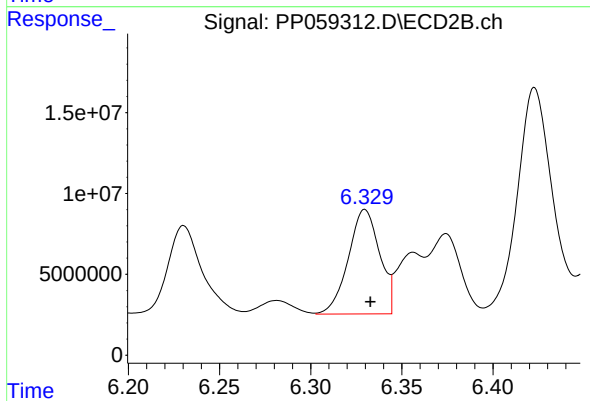

#29 AR-1254-4

R.T.: 6.330 min
Delta R.T.: -0.003 min
Response: 77331218
Conc: 962.06 ng/ml

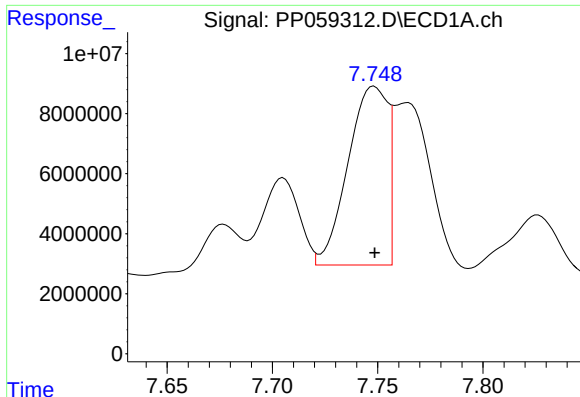


#30 AR-1254-5

R.T.: 7.748 min
Delta R.T.: -0.001 min
Response: 80906654
Conc: 1721.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRADE-67-PAINT-CHIPS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/11/2023
Supervised By :Ankita Jodhani 08/11/2023

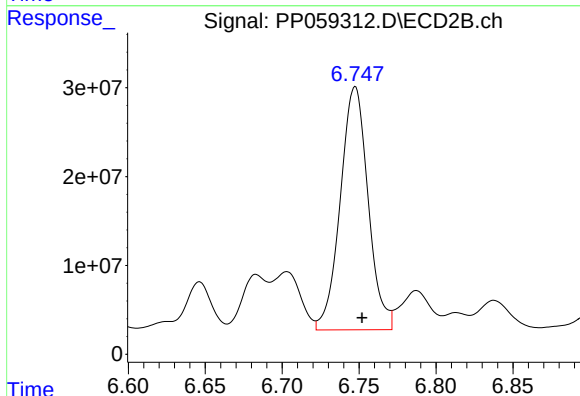


#30 AR-1254-5

R.T.: 6.747 min
Delta R.T.: -0.004 min
Response: 343700114
Conc: 2874.06 ng/ml

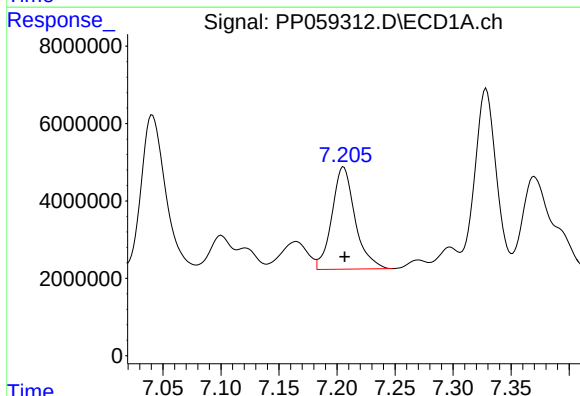


#31 AR-1260-1

R.T.: 7.206 min
Delta R.T.: 0.000 min
Response: 36714117
Conc: 671.08 ng/ml

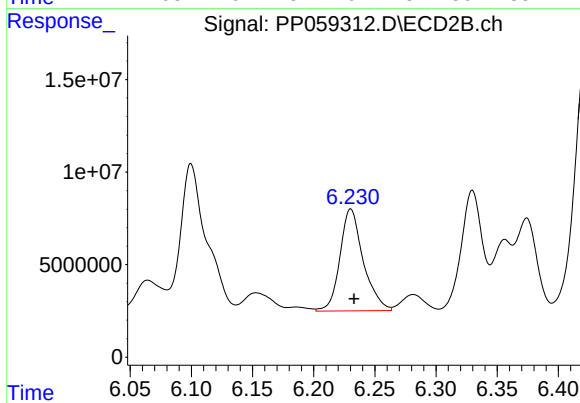

#31 AR-1260-1

R.T.: 6.230 min
Delta R.T.: -0.003 min
Response: 73048071
Conc: 737.57 ng/ml

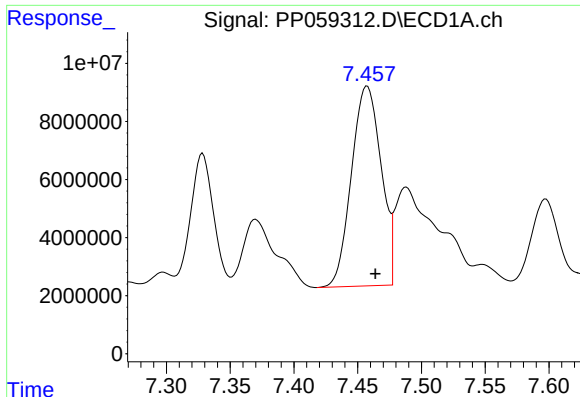


#32 AR-1260-2

R.T.: 7.457 min
Delta R.T.: -0.006 min
Response: 111151151
Conc: 1866.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRADE-67-PAINT-CHIPS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/11/2023
Supervised By :Ankita Jodhani 08/11/2023

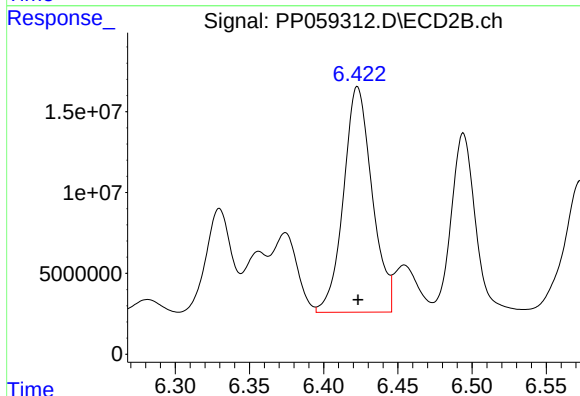


#32 AR-1260-2

R.T.: 6.423 min
Delta R.T.: 0.000 min
Response: 187064274
Conc: 1616.68 ng/ml

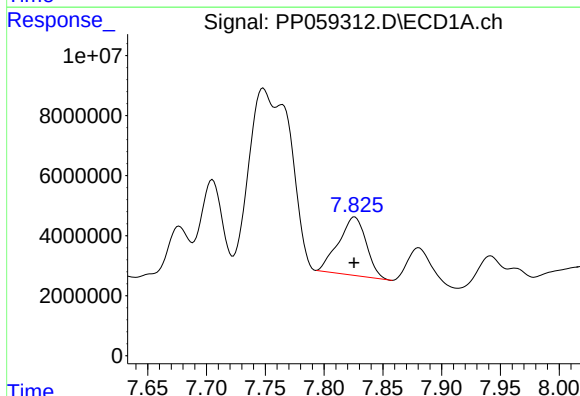


#33 AR-1260-3

R.T.: 7.826 min
Delta R.T.: 0.000 min
Response: 31904396
Conc: 810.68 ng/ml

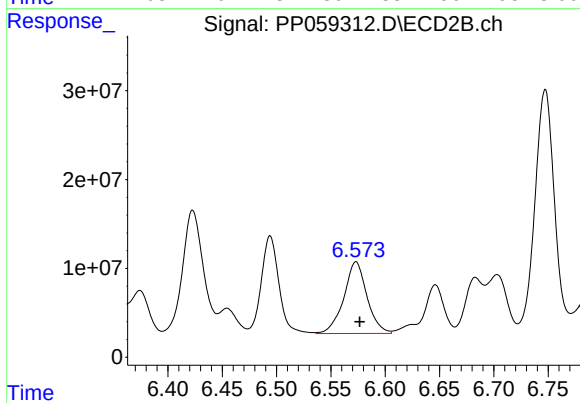

#33 AR-1260-3

R.T.: 6.573 min
Delta R.T.: -0.003 min
Response: 120135539
Conc: 1080.03 ng/ml

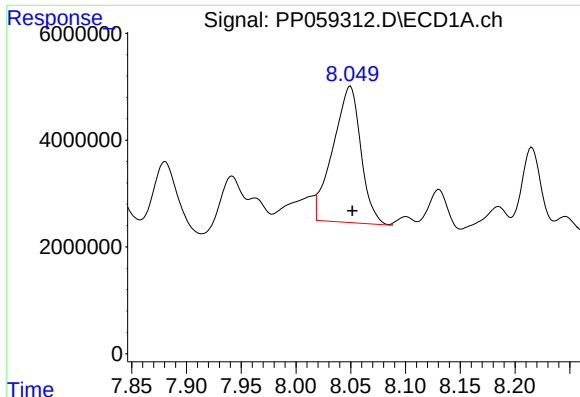


#34 AR-1260-4

R.T.: 8.049 min
Delta R.T.: -0.002 min
Response: 44911579
Conc: 1011.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRADE-67-PAINT-CHIPS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/11/2023
Supervised By :Ankita Jodhani 08/11/2023

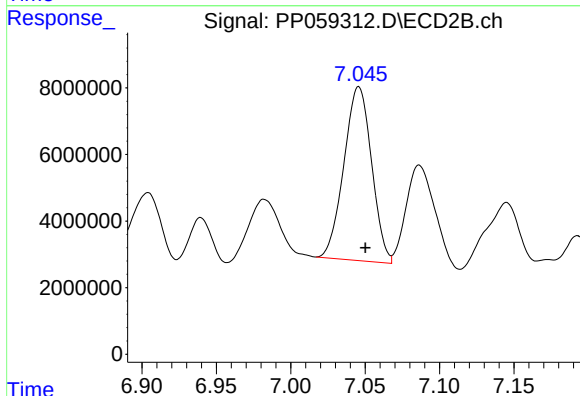


#34 AR-1260-4

R.T.: 7.046 min
Delta R.T.: -0.004 min
Response: 67656856
Conc: 780.40 ng/ml

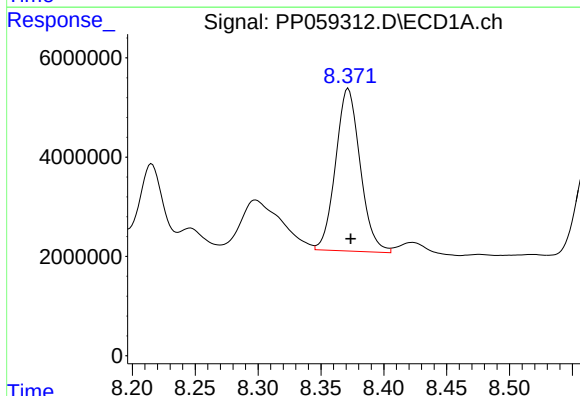

#35 AR-1260-5

R.T.: 8.372 min
Delta R.T.: -0.002 min
Response: 44624711
Conc: 558.02 ng/ml

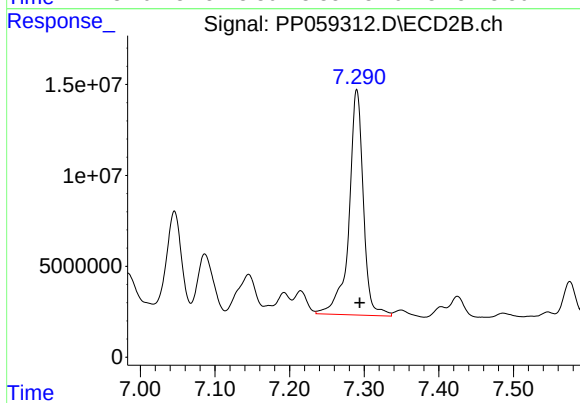

#35 AR-1260-5

R.T.: 7.290 min
Delta R.T.: -0.004 min
Response: 165814009
Conc: 899.58 ng/ml