

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081023\
 Data File : PP059313.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2023 16:53
 Operator : YP\AJ
 Sample : 03936-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TRDAE-68-PPE-TARP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/11/2023
 Supervised By :Ankita Jodhani 08/11/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 21:57:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.415	3.667	22297759	35491897	18.172	17.517m
2) SA Decachlor...	10.207	8.704	15210811	31182922	19.929	22.166

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081023\
Data File : PP059313.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2023 16:53
Operator : YP\AJ
Sample : 03936-03
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TRDAE-68-PPE-TARP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/11/2023
Supervised By :Ankita Jodhani 08/11/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 21:57:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 09 02:30:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

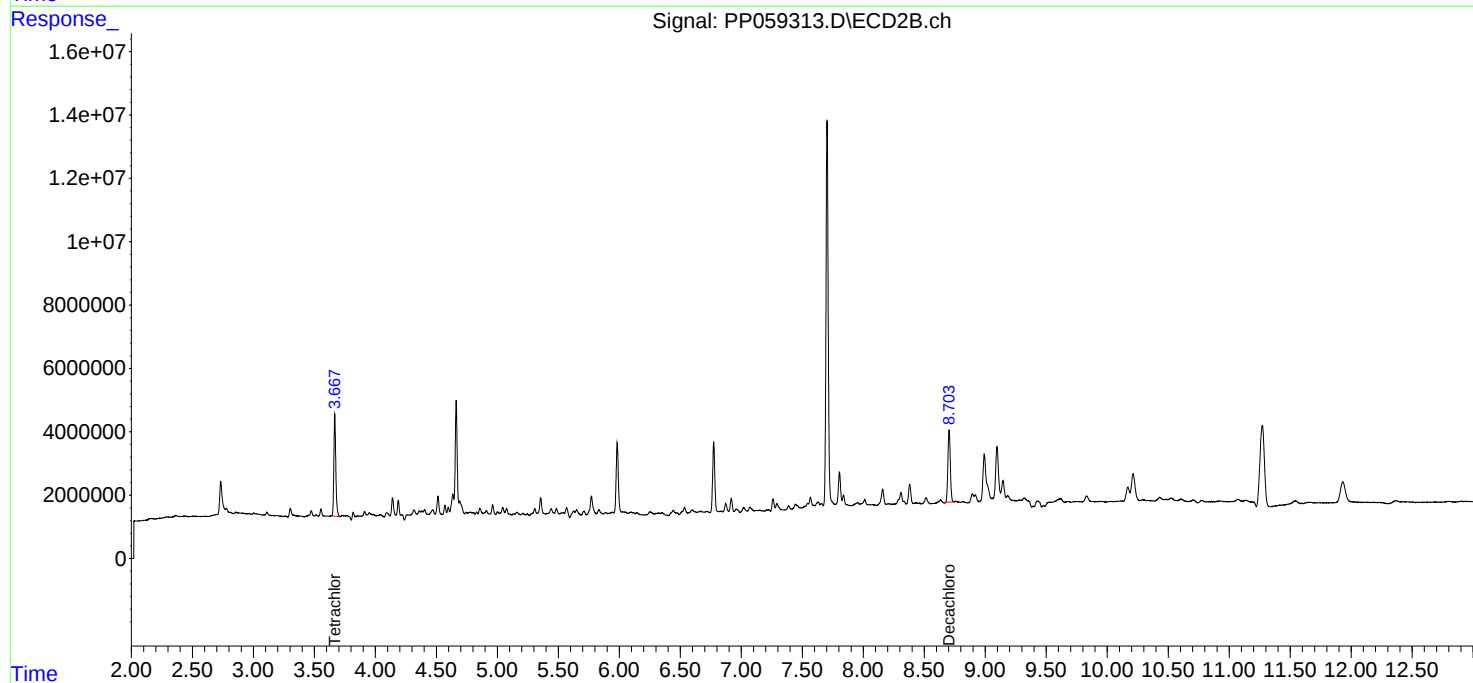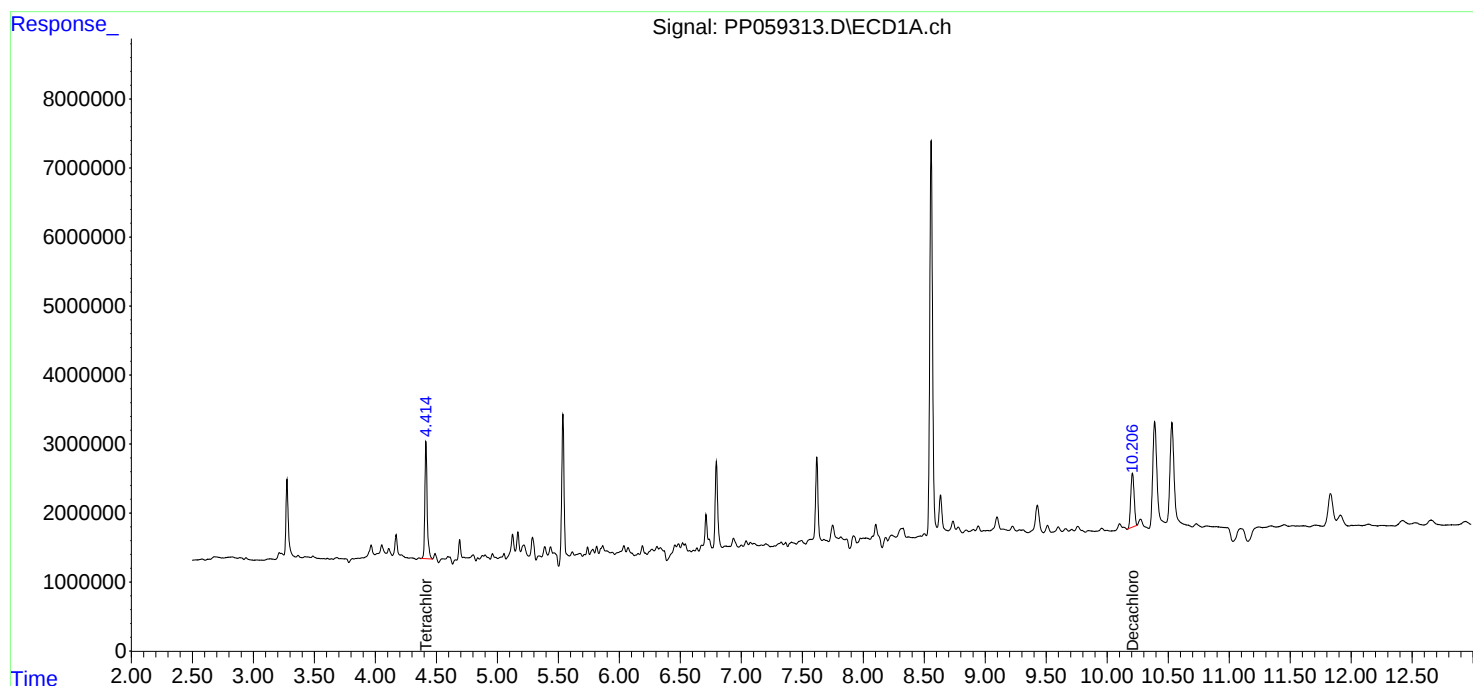

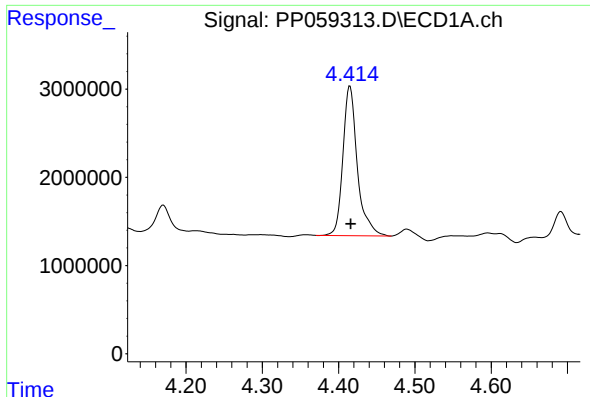


#1 Tetrachloro-m-xylene

R.T.: 4.415 min
Delta R.T.: -0.001 min
Response: 22297759
Conc: 18.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRDAE-68-PPE-TARP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/11/2023
Supervised By :Ankita Jodhani 08/11/2023

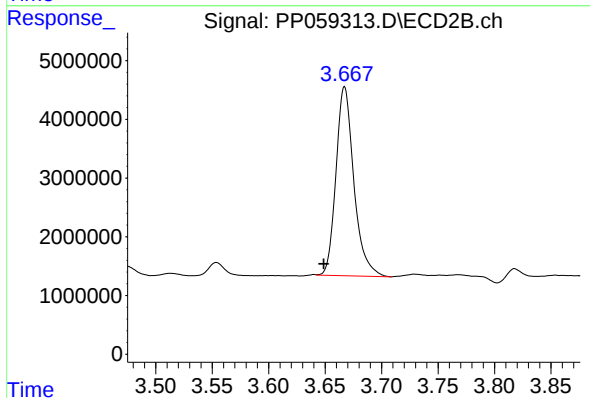


#1 Tetrachloro-m-xylene

R.T.: 3.667 min
Delta R.T.: 0.018 min
Response: 35491897
Conc: 17.52 ng/ml m

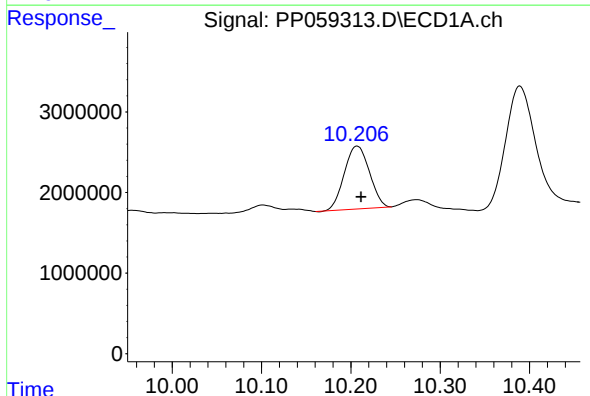

#2 Decachlorobiphenyl

R.T.: 10.207 min
Delta R.T.: -0.004 min
Response: 15210811
Conc: 19.93 ng/ml

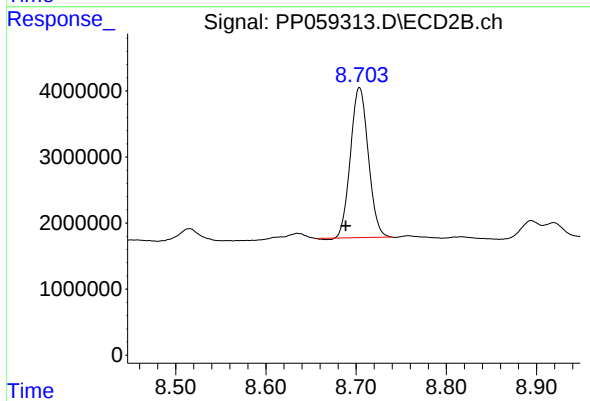

#2 Decachlorobiphenyl

R.T.: 8.704 min
Delta R.T.: 0.015 min
Response: 31182922
Conc: 22.17 ng/ml