

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081023\
 Data File : PP059314.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2023 17:10
 Operator : YP\AJ
 Sample : 03936-04
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TRADE-69-PAINT-CHIPS

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/11/2023
 Supervised By :Ankita Jodhani 08/11/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 21:58:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.415	3.646	27578147	40546900	22.475	20.012
2)	SA Decachlor...	10.208	8.682	19190105	37261241	25.143	26.486
Target Compounds							
26)	L6 AR-1254-1	6.453	5.546	10080989	24684512	215.799	243.640
27)	L6 AR-1254-2	6.673	5.695	17767958	21927510	258.225	248.390
28)	L6 AR-1254-3	7.039	6.099	23286396	49907330	337.386m	361.005m
29)	L6 AR-1254-4	7.326	6.330	21507327	42015045	477.774	522.700m
30)	L6 AR-1254-5	7.748	6.748	29600872	99068284	629.979	828.421 #
31)	L7 AR-1260-1	7.204	6.229	15188418	28465868	277.621m	287.422m
32)	L7 AR-1260-2	7.462	6.420	22204089	39280062	372.935	339.472m
33)	L7 AR-1260-3	7.822	6.572	7694587	37547135	195.518	337.552m#
34)	L7 AR-1260-4	8.040	7.046	14288063	13507416	321.703	155.804 #
35)	L7 AR-1260-5	8.371	7.290	12294389	36256606	153.738	196.700 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081023\
Data File : PP059314.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2023 17:10
Operator : YP\AJ
Sample : 03936-04
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TRADE-69-PAINT-CHIPS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/11/2023
Supervised By :Ankita Jodhani 08/11/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 21:58:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 09 02:30:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

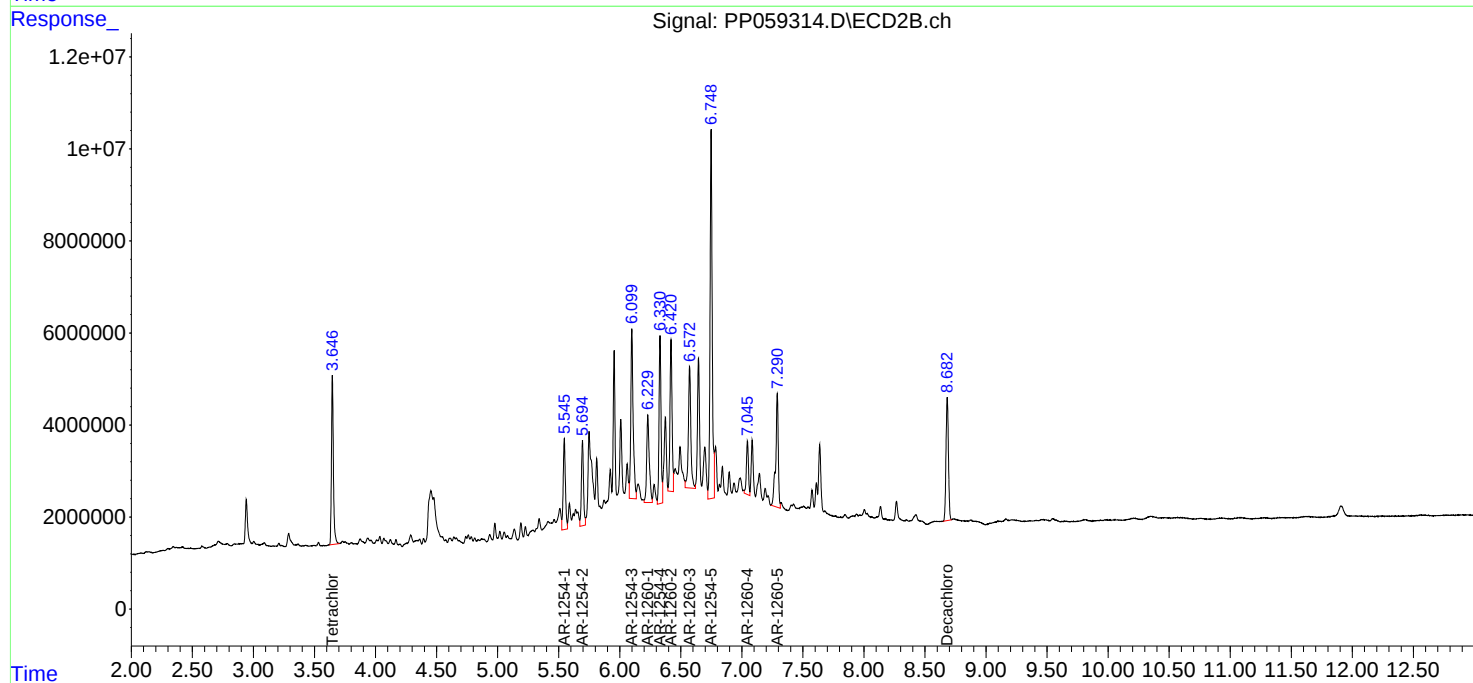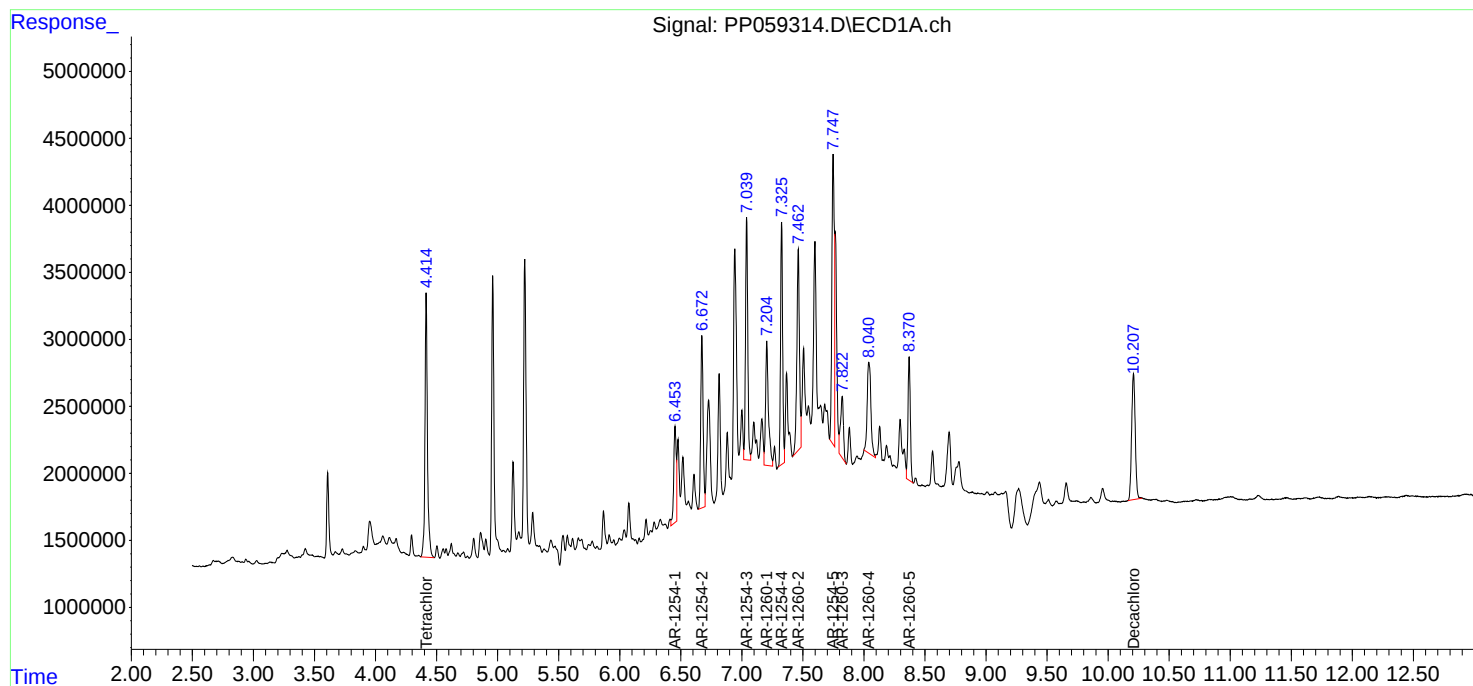

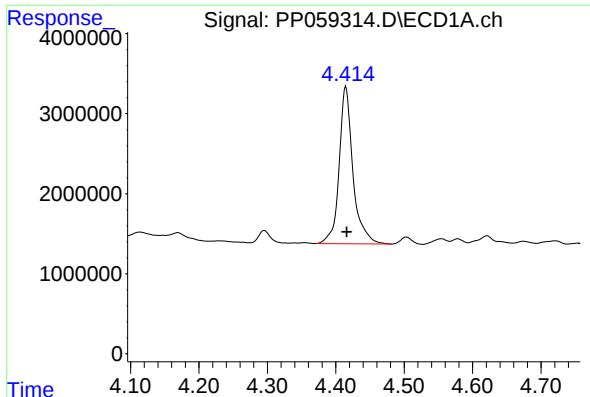


#1 Tetrachloro-m-xylene

R.T.: 4.415 min
Delta R.T.: -0.001 min
Response: 27578147
Conc: 22.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRADE-69-PAINT-CHIPS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/11/2023
Supervised By :Ankita Jodhani 08/11/2023

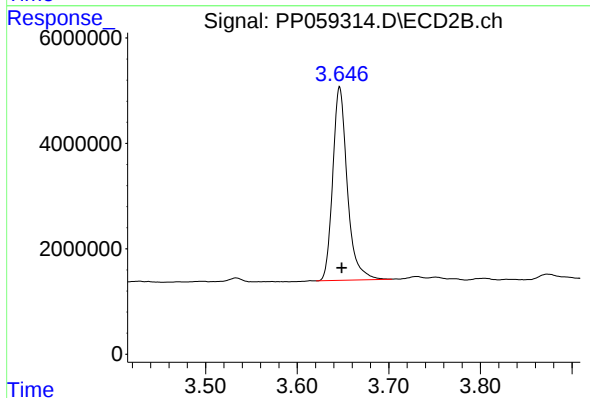


#1 Tetrachloro-m-xylene

R.T.: 3.646 min
Delta R.T.: -0.003 min
Response: 40546900
Conc: 20.01 ng/ml

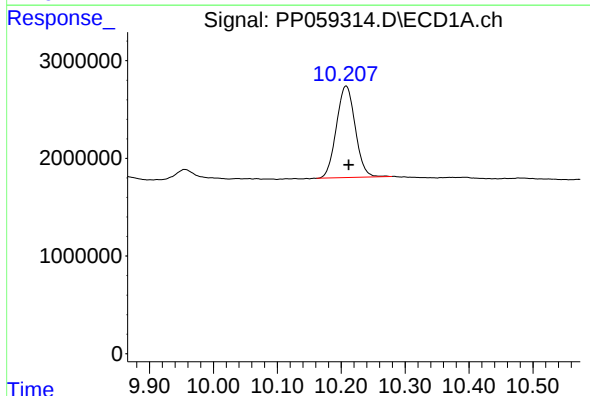


#2 Decachlorobiphenyl

R.T.: 10.208 min
Delta R.T.: -0.004 min
Response: 19190105
Conc: 25.14 ng/ml

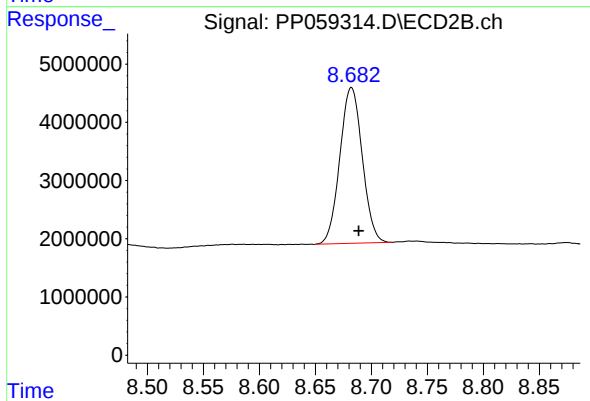

#2 Decachlorobiphenyl

R.T.: 8.682 min
Delta R.T.: -0.006 min
Response: 37261241
Conc: 26.49 ng/ml

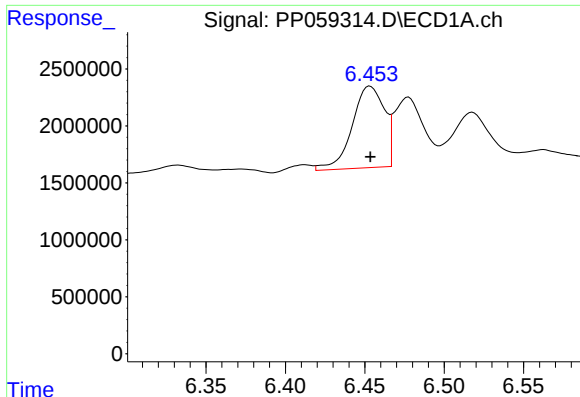


#26 AR-1254-1

R.T.: 6.453 min
Delta R.T.: 0.000 min
Response: 10080989
Conc: 215.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRADE-69-PAINT-CHIPS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/11/2023
Supervised By :Ankita Jodhani 08/11/2023

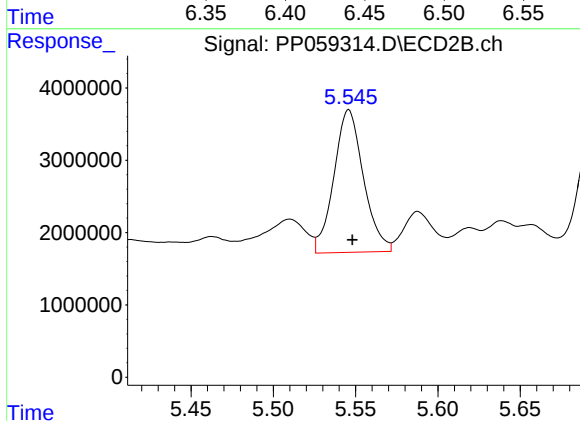


#26 AR-1254-1

R.T.: 5.546 min
Delta R.T.: -0.002 min
Response: 24684512
Conc: 243.64 ng/ml

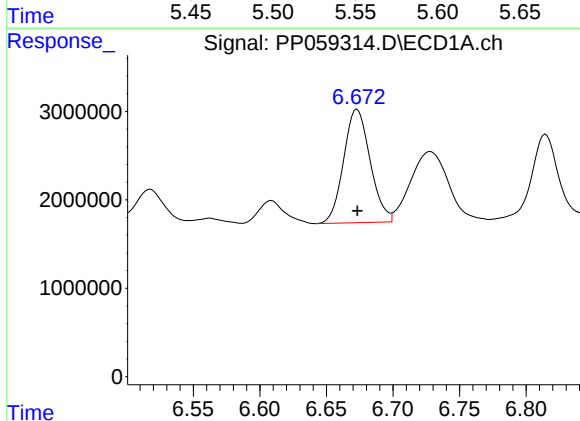


#27 AR-1254-2

R.T.: 6.673 min
Delta R.T.: 0.000 min
Response: 17767958
Conc: 258.23 ng/ml

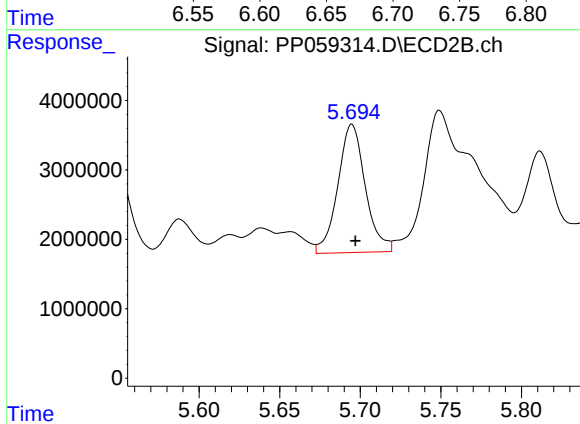

#27 AR-1254-2

R.T.: 5.695 min
Delta R.T.: -0.002 min
Response: 21927510
Conc: 248.39 ng/ml

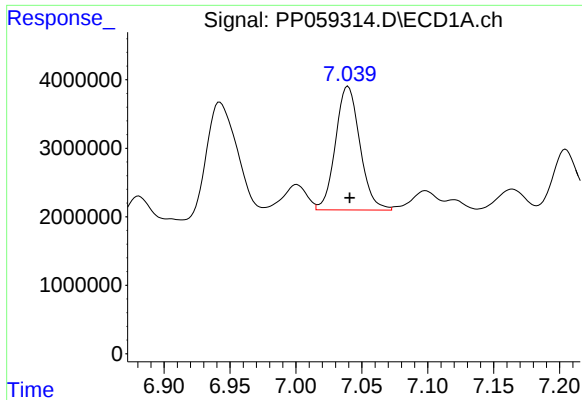


#28 AR-1254-3

R.T.: 7.039 min
Delta R.T.: -0.002 min
Response: 23286396
Conc: 337.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRADE-69-PAINT-CHIPS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/11/2023
Supervised By :Ankita Jodhani 08/11/2023

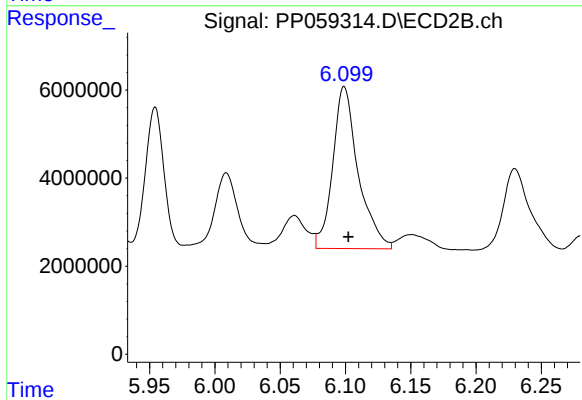


#28 AR-1254-3

R.T.: 6.099 min
Delta R.T.: -0.004 min
Response: 49907330
Conc: 361.00 ng/ml m

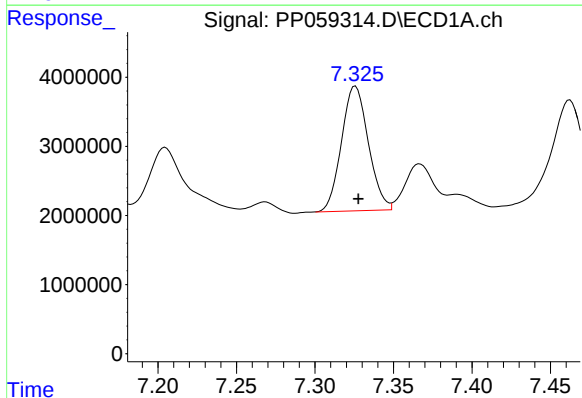


#29 AR-1254-4

R.T.: 7.326 min
Delta R.T.: -0.002 min
Response: 21507327
Conc: 477.77 ng/ml

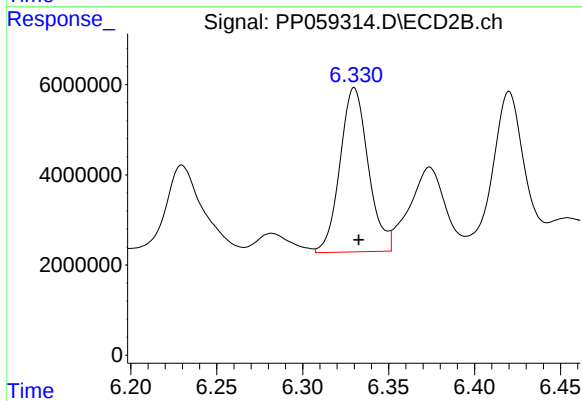

#29 AR-1254-4

R.T.: 6.330 min
Delta R.T.: -0.003 min
Response: 42015045
Conc: 522.70 ng/ml m

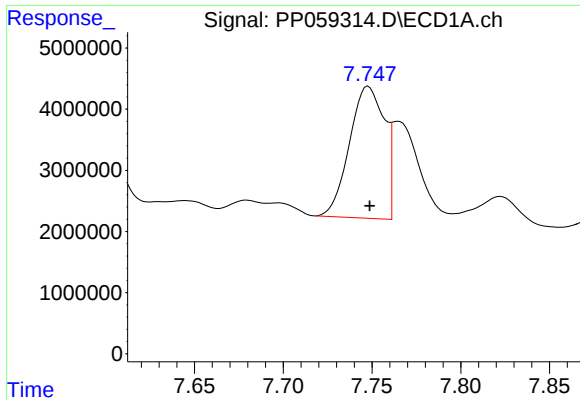


#30 AR-1254-5

R.T.: 7.748 min
Delta R.T.: 0.000 min
Response: 29600872
Conc: 629.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRADE-69-PAINT-CHIPS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/11/2023
Supervised By :Ankita Jodhani 08/11/2023

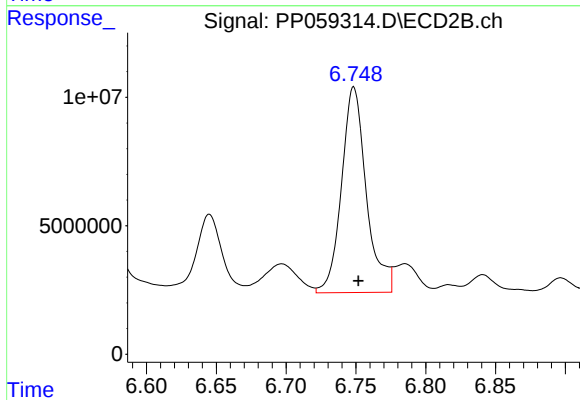


#30 AR-1254-5

R.T.: 6.748 min
Delta R.T.: -0.003 min
Response: 99068284
Conc: 828.42 ng/ml

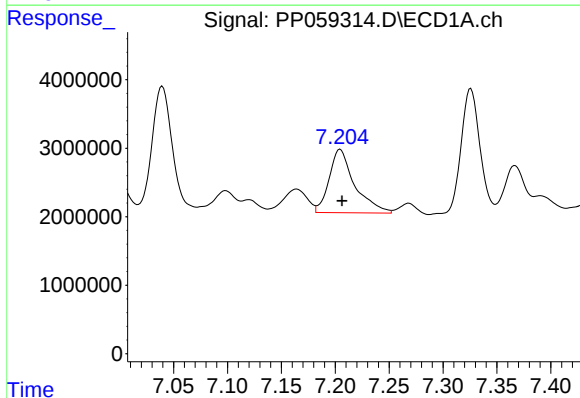


#31 AR-1260-1

R.T.: 7.204 min
Delta R.T.: -0.003 min
Response: 15188418
Conc: 277.62 ng/ml m

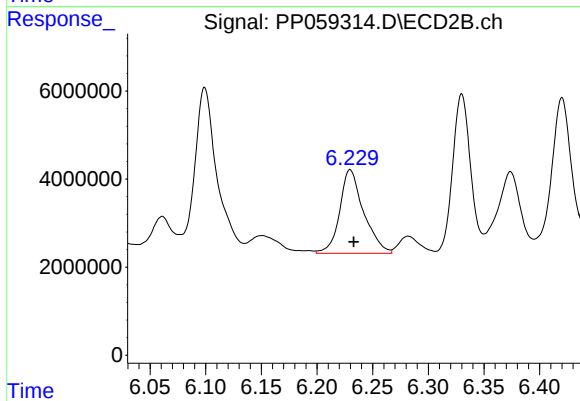

#31 AR-1260-1

R.T.: 6.229 min
Delta R.T.: -0.004 min
Response: 28465868
Conc: 287.42 ng/ml m

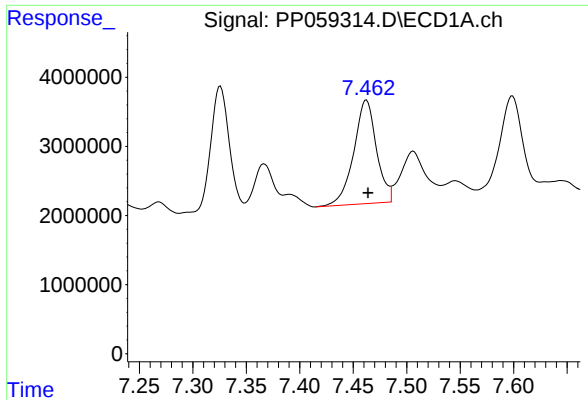


#32 AR-1260-2

R.T.: 7.462 min
Delta R.T.: -0.002 min
Response: 22204089
Conc: 372.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRADE-69-PAINT-CHIPS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/11/2023
Supervised By :Ankita Jodhani 08/11/2023

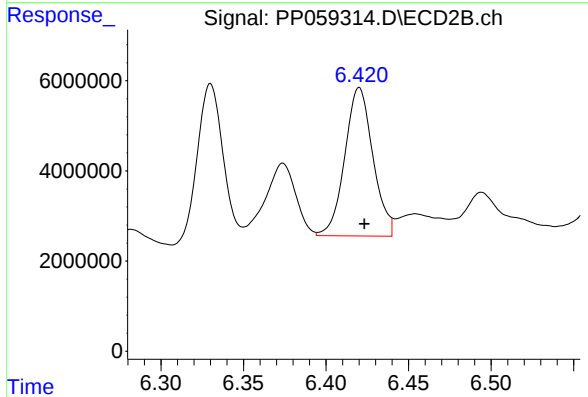


#32 AR-1260-2

R.T.: 6.420 min
Delta R.T.: -0.003 min
Response: 39280062
Conc: 339.47 ng/ml m

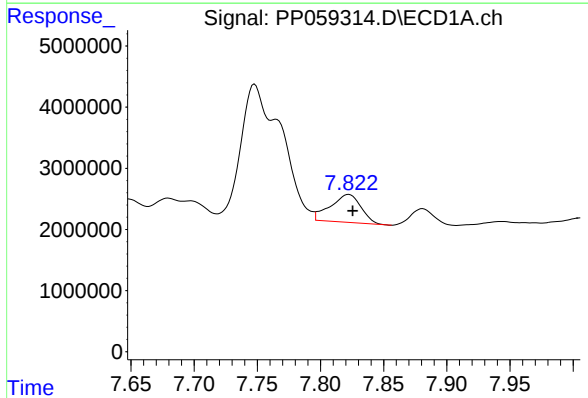


#33 AR-1260-3

R.T.: 7.822 min
Delta R.T.: -0.003 min
Response: 7694587
Conc: 195.52 ng/ml

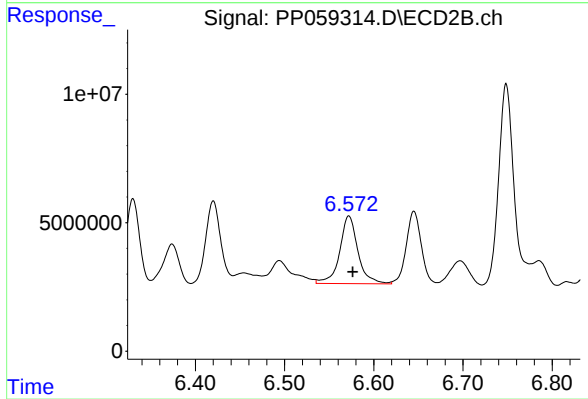

#33 AR-1260-3

R.T.: 6.572 min
Delta R.T.: -0.005 min
Response: 37547135
Conc: 337.55 ng/ml m

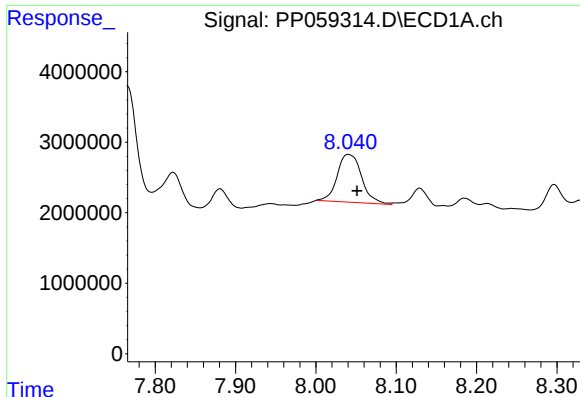


#34 AR-1260-4

R.T.: 8.040 min
Delta R.T.: -0.011 min
Response: 14288063
Conc: 321.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRADE-69-PAINT-CHIPS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/11/2023
Supervised By :Ankita Jodhani 08/11/2023

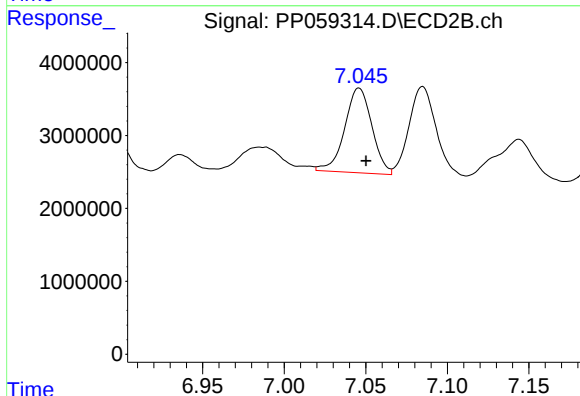


#34 AR-1260-4

R.T.: 7.046 min
Delta R.T.: -0.004 min
Response: 13507416
Conc: 155.80 ng/ml

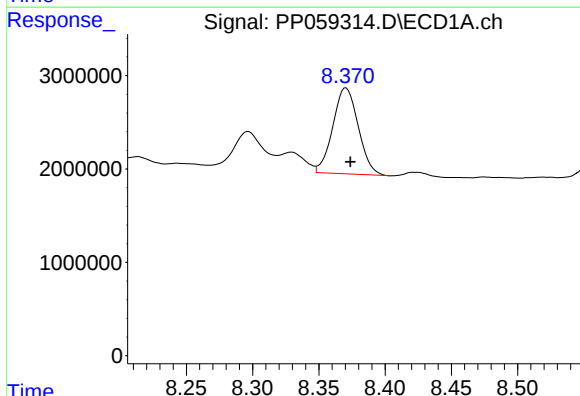

#35 AR-1260-5

R.T.: 8.371 min
Delta R.T.: -0.003 min
Response: 12294389
Conc: 153.74 ng/ml

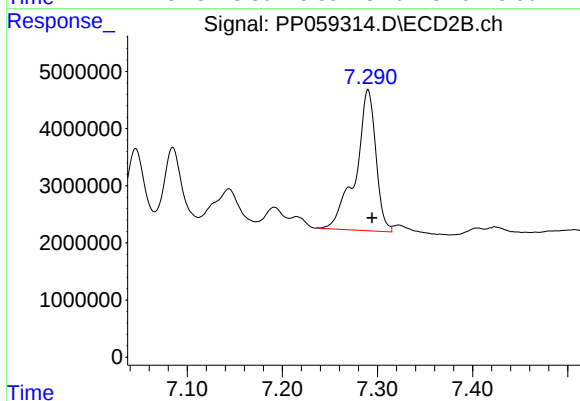

#35 AR-1260-5

R.T.: 7.290 min
Delta R.T.: -0.004 min
Response: 36256606
Conc: 196.70 ng/ml