

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081121\
 Data File : PP038234.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Aug 2021 9:46
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 13:13:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 06 03:08:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.892	3.878	993985	606442	22.366	23.546
2)	SA Decachlor...	10.882	9.143	510034	569602	22.421	22.015
Target Compounds							
9)	L2 AR-1221-2	0.000	4.225	0	7308	N.D.	31.051 #
20)	L4 AR-1242-5	0.000	6.014f	0	24475	N.D.	37.877 #
24)	L5 AR-1248-4	7.126f	0.000	55022	0	40.753	N.D. #
25)	L5 AR-1248-5	0.000	6.014f	0	24475	N.D.	25.997 #
26)	L6 AR-1254-1	7.126	6.014f	55022	24475	42.227	18.294 #
28)	L6 AR-1254-3	7.751f	0.000	15700	0	7.914	N.D. #
32)	L7 AR-1260-2	8.136f	6.921	13694	863	7.954	0.555 #
33)	L7 AR-1260-3	0.000	7.065	0	17512	N.D.	11.504 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081121\
Data File : PP038234.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Aug 2021 9:46
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 13:13:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 06 03:08:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

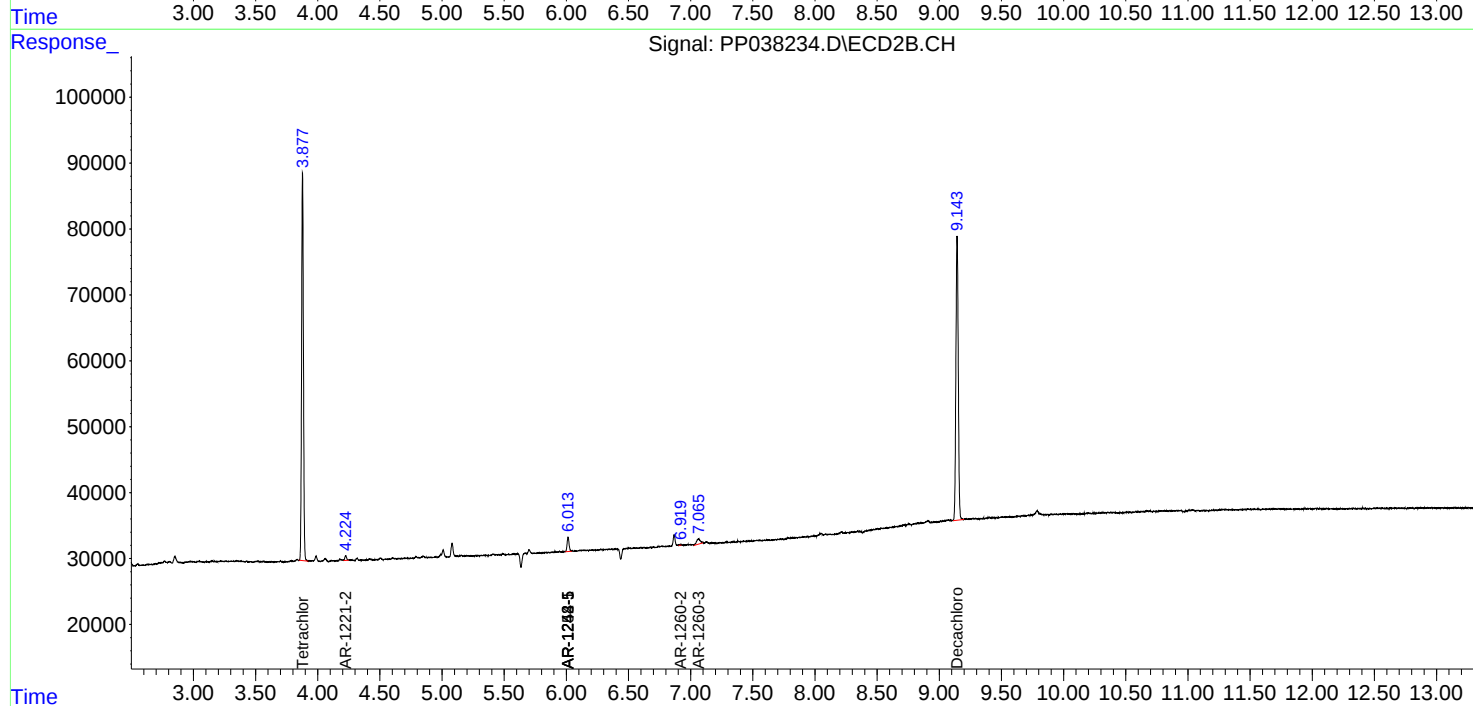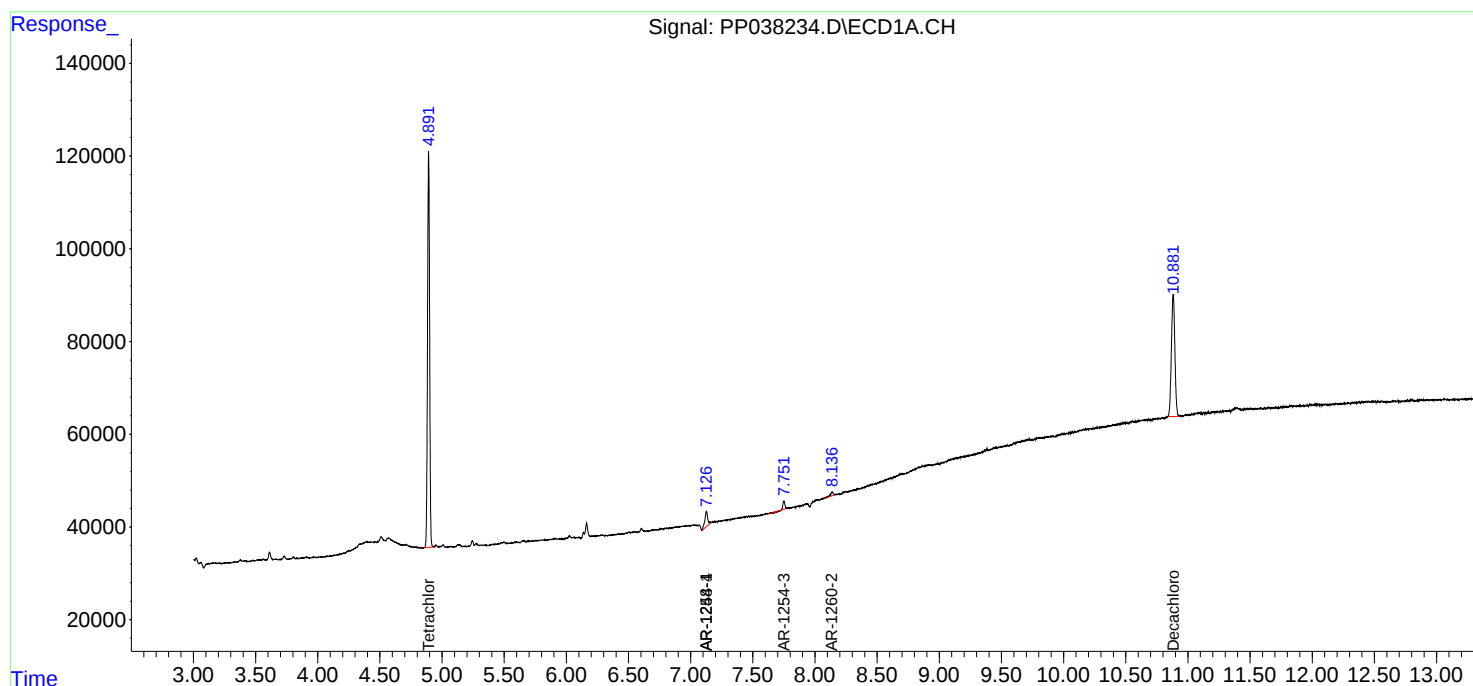


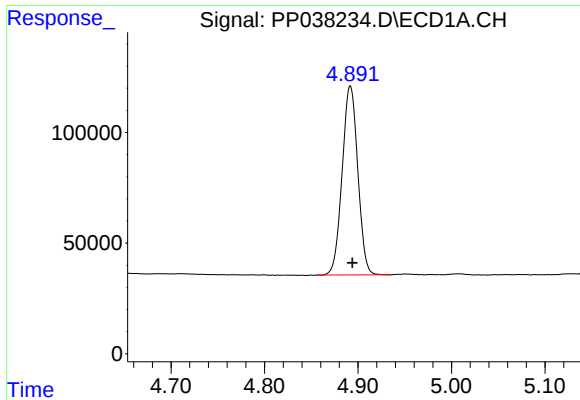

#1 Tetrachloro-m-xylene


R.T.: 4.892 min
Delta R.T.: -0.002 min
Response: 993985
Conc: 22.37 ng/ml

Instrument :
ECD_P
ClientSampleId :

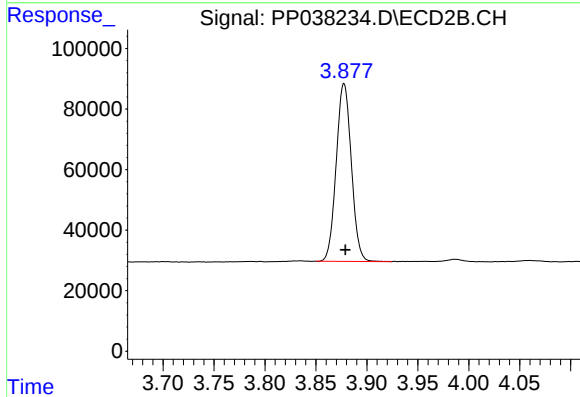


#1 Tetrachloro-m-xylene

R.T.: 3.878 min
Delta R.T.: -0.001 min
Response: 606442
Conc: 23.55 ng/ml

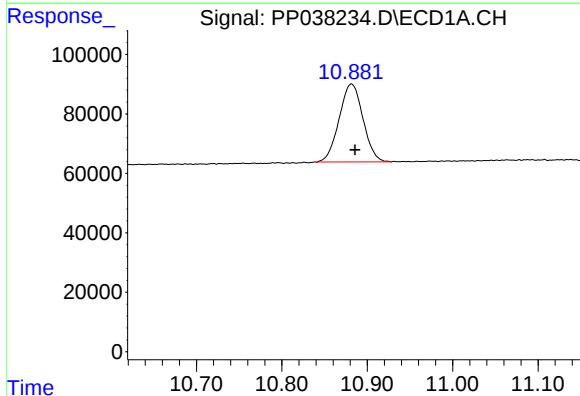


#2 Decachlorobiphenyl

R.T.: 10.882 min
Delta R.T.: -0.004 min
Response: 510034
Conc: 22.42 ng/ml

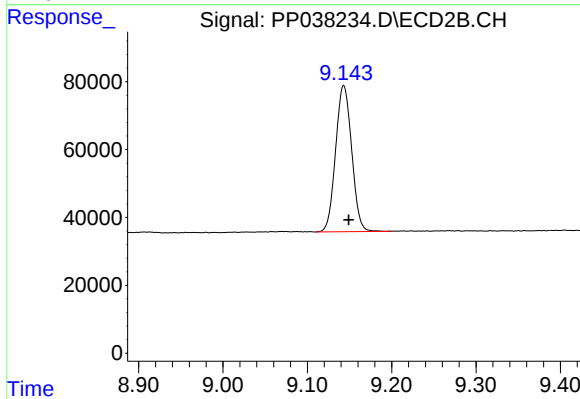

#2 Decachlorobiphenyl


R.T.: 9.143 min
Delta R.T.: -0.006 min
Response: 569602
Conc: 22.02 ng/ml

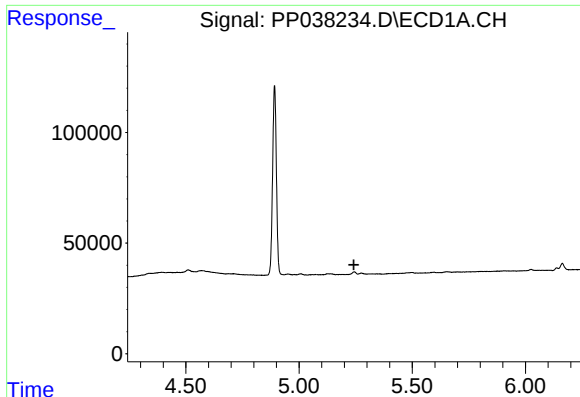

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 5.242 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

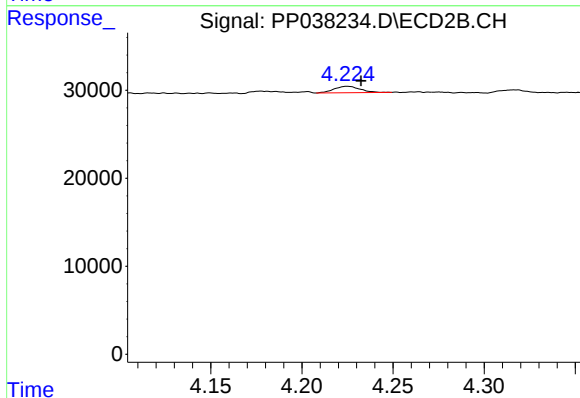


#9 AR-1221-2

R.T.: 4.225 min
Delta R.T.: -0.008 min
Response: 7308
Conc: 31.05 ng/ml

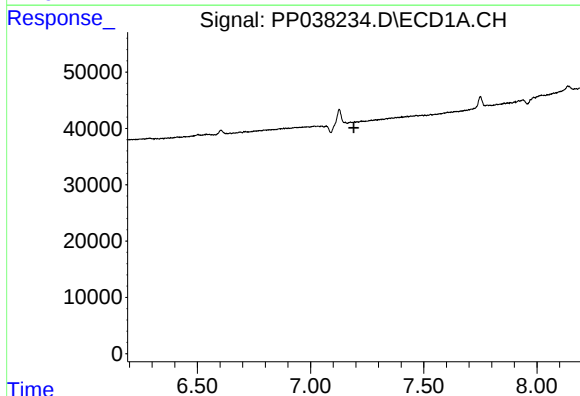


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 7.192 min
Response: 0
Conc: N.D.

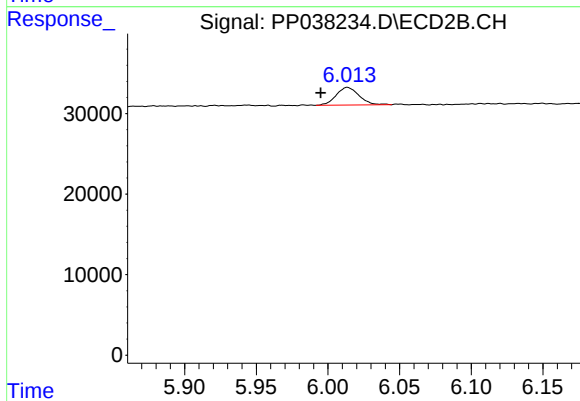

#20 AR-1242-5


R.T.: 6.014 min
Delta R.T.: 0.019 min
Response: 24475
Conc: 37.88 ng/ml

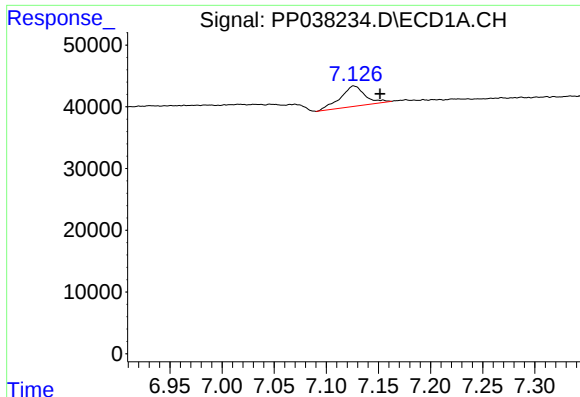

#24 AR-1248-4


R.T.: 7.126 min
Delta R.T.: -0.025 min
Response: 55022
Conc: 40.75 ng/ml

Instrument :
ECD_P
ClientSampleId :

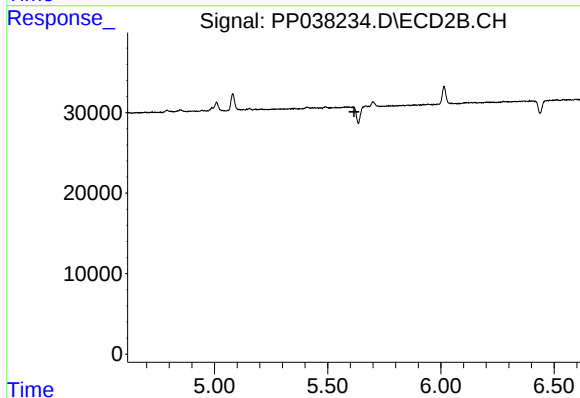


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.616 min
Response: 0
Conc: N.D.

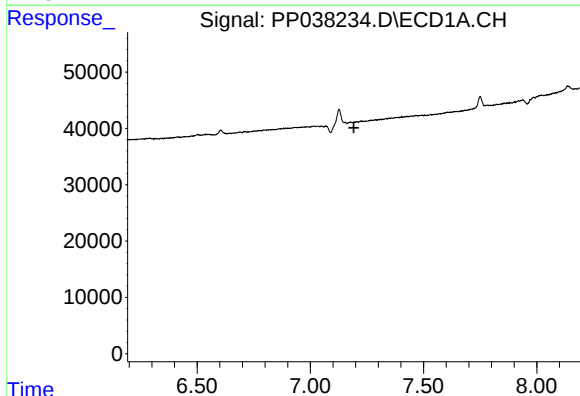


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 7.192 min
Response: 0
Conc: N.D.

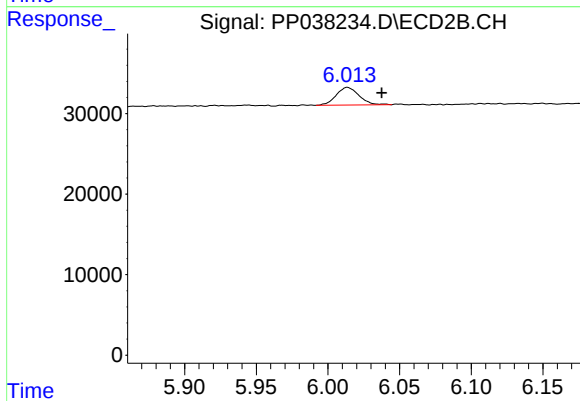

#25 AR-1248-5


R.T.: 6.014 min
Delta R.T.: -0.024 min
Response: 24475
Conc: 26.00 ng/ml

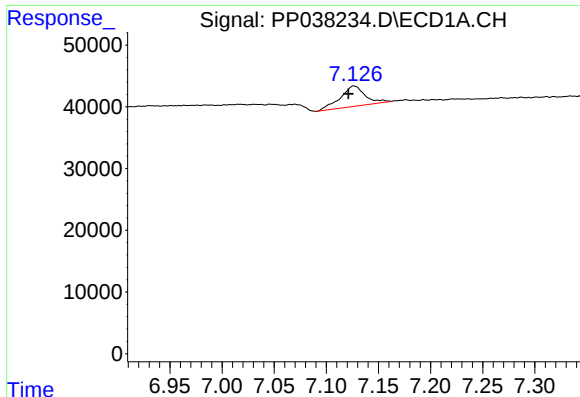

#26 AR-1254-1


R.T.: 7.126 min
Delta R.T.: 0.005 min
Response: 55022
Conc: 42.23 ng/ml

Instrument :
ECD_P
ClientSampleId :

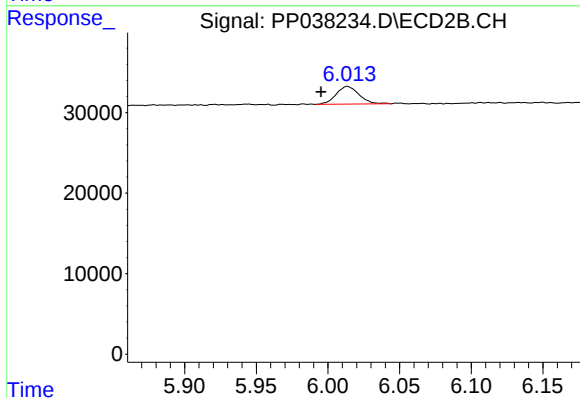


#26 AR-1254-1

R.T.: 6.014 min
Delta R.T.: 0.018 min
Response: 24475
Conc: 18.29 ng/ml

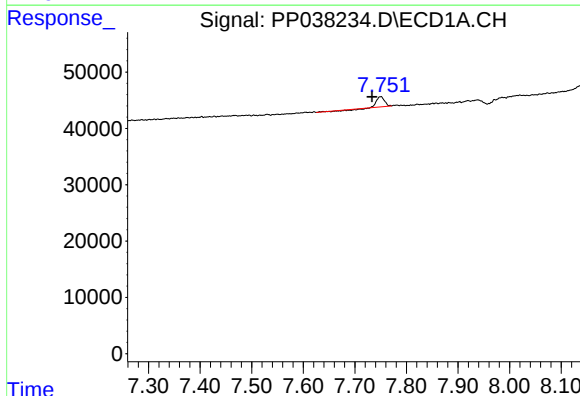


#28 AR-1254-3

R.T.: 7.751 min
Delta R.T.: 0.018 min
Response: 15700
Conc: 7.91 ng/ml

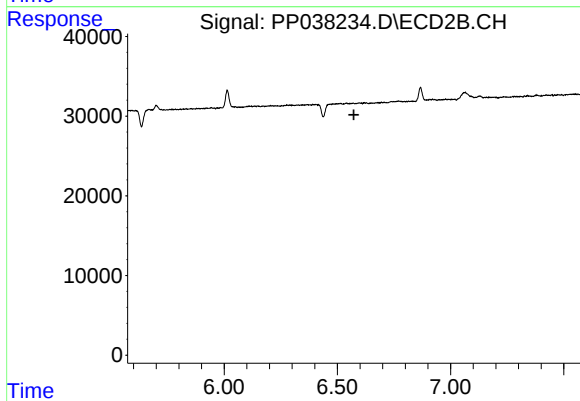

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 6.573 min
Response: 0
Conc: N.D.

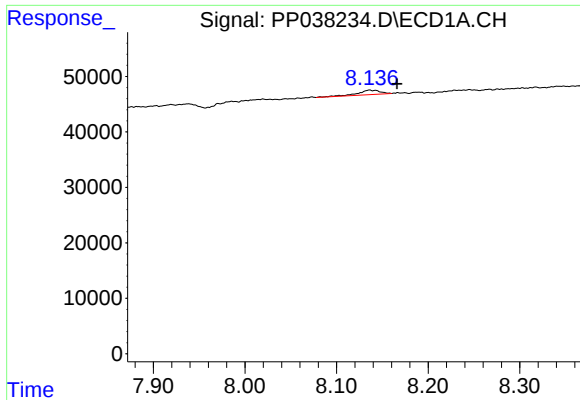

#32 AR-1260-2


R.T.: 8.136 min
Delta R.T.: -0.030 min
Response: 13694
Conc: 7.95 ng/ml

Instrument :
ECD_P
ClientSampleId :

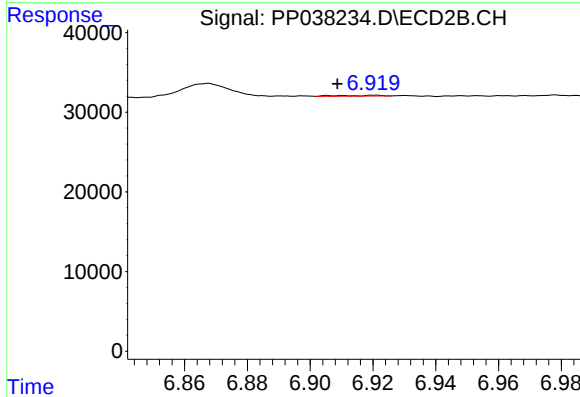


#32 AR-1260-2

R.T.: 6.921 min
Delta R.T.: 0.012 min
Response: 863
Conc: 0.55 ng/ml

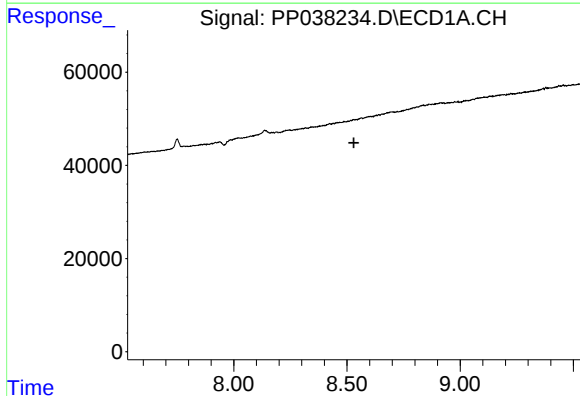

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.530 min
Response: 0
Conc: N.D.

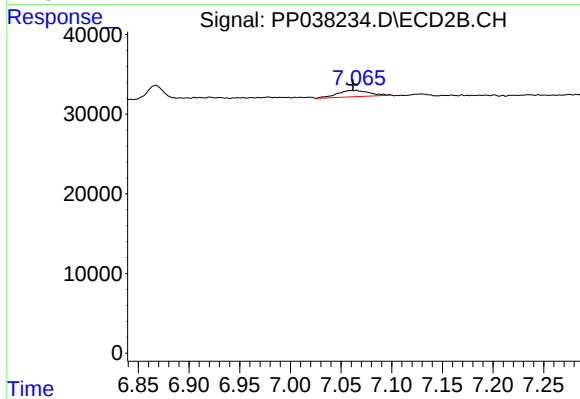

#33 AR-1260-3

R.T.: 7.065 min
Delta R.T.: 0.003 min
Response: 17512
Conc: 11.50 ng/ml