

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081121\
 Data File : PP038253.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Aug 2021 17:53
 Operator : AJ\MA
 Sample : M3343-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 20210542-COM-15

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 01:07:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 06 03:08:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.892	3.878	840134	503564	18.904	19.552
2) SA Decachlor...	10.881	9.143	393513	460222	17.298	17.788

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081121\
Data File : PP038253.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Aug 2021 17:53
Operator : AJ\MA
Sample : M3343-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
20210542-COM-15

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 01:07:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 06 03:08:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

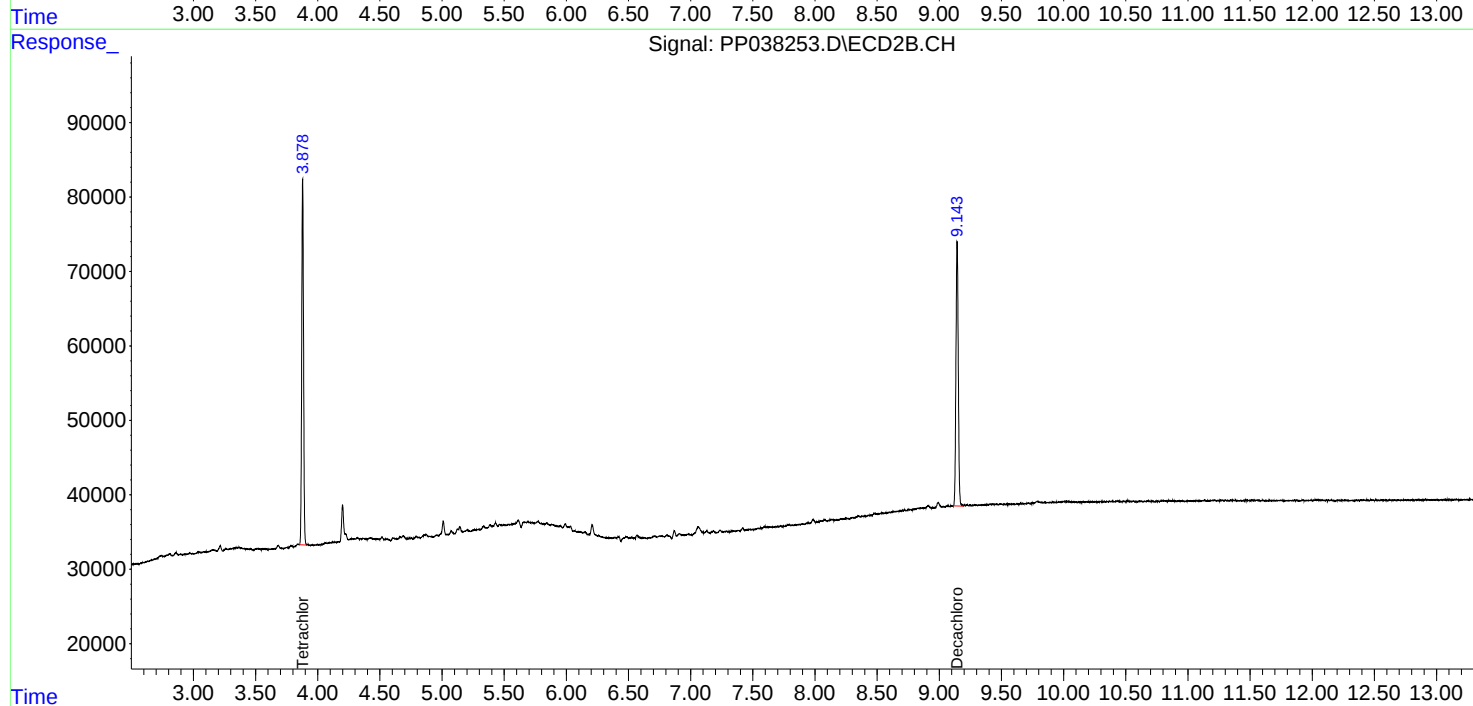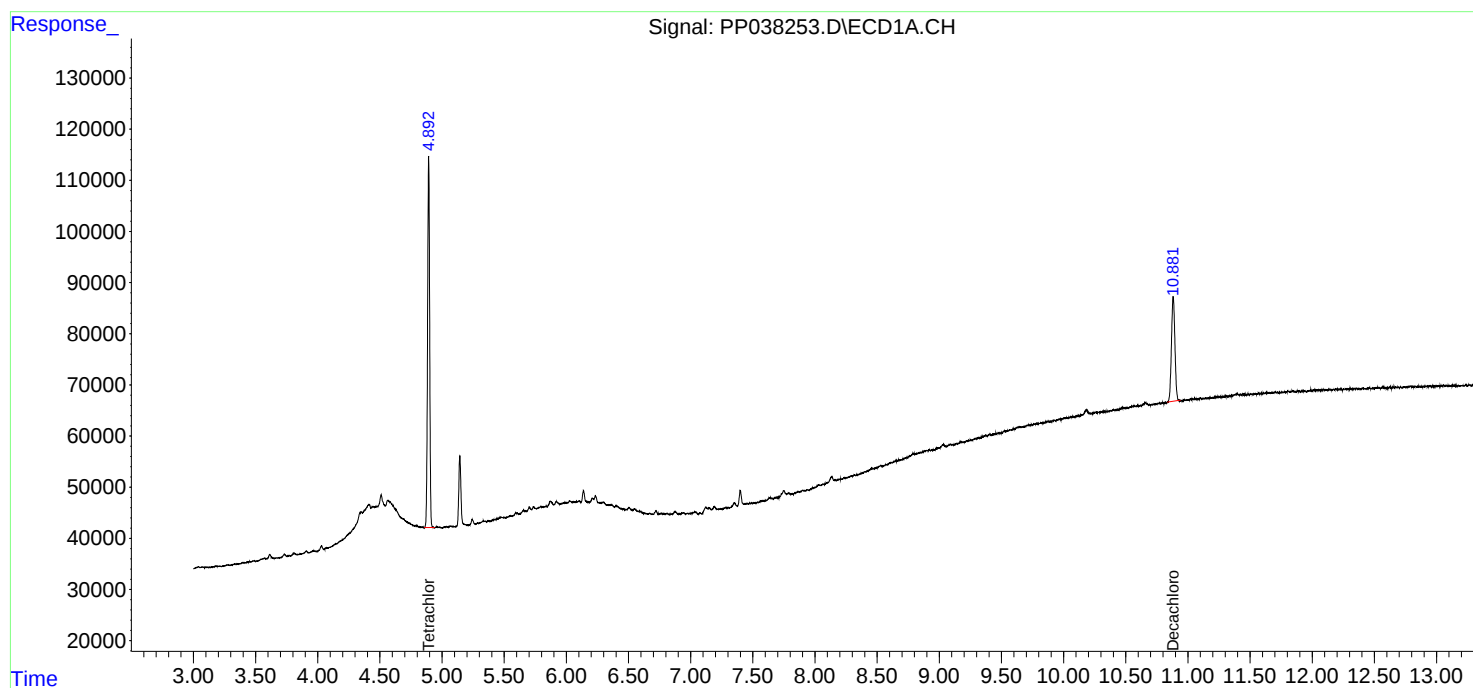


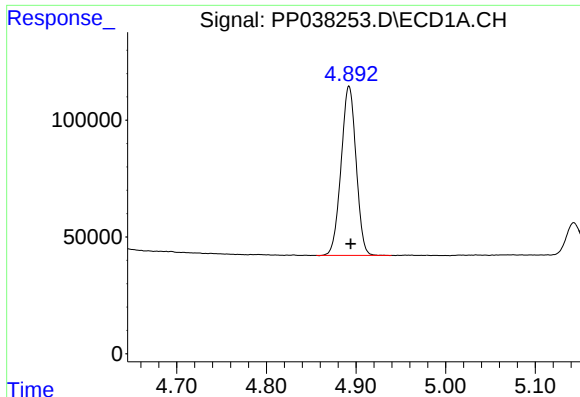

#1 Tetrachloro-m-xylene


R.T.: 4.892 min
Delta R.T.: -0.002 min
Response: 840134
Conc: 18.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
20210542-COM-15

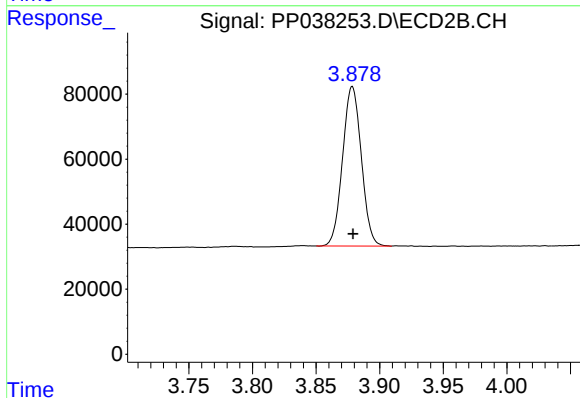


#1 Tetrachloro-m-xylene

R.T.: 3.878 min
Delta R.T.: 0.000 min
Response: 503564
Conc: 19.55 ng/ml

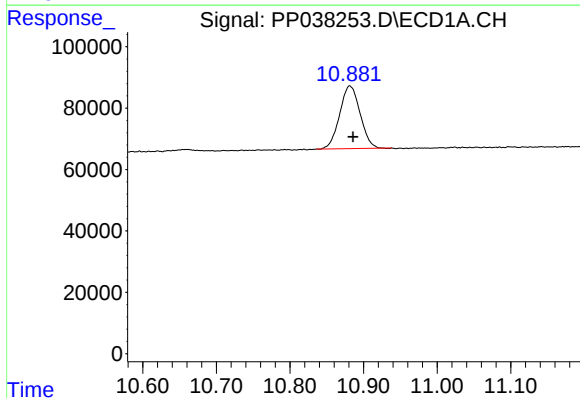

#2 Decachlorobiphenyl

R.T.: 10.881 min
Delta R.T.: -0.005 min
Response: 393513
Conc: 17.30 ng/ml

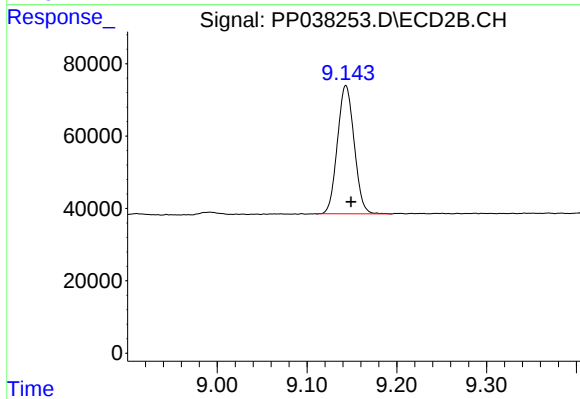

#2 Decachlorobiphenyl

R.T.: 9.143 min
Delta R.T.: -0.006 min
Response: 460222
Conc: 17.79 ng/ml