

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081121\
 Data File : PP038270.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Aug 2021 22:42
 Operator : AJ\MA
 Sample : M3348-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SPEEDIDRI-TRE-1237

Manual Integrations
 APPROVED

mohammad
 8/12/2021 11:58:32 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 01:17:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 06 03:08:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.893	3.878	674321	414540	15.173	16.095m
2) SA Decachlor...	10.884	9.145	199505	220148	8.770	8.509

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081121\
Data File : PP038270.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Aug 2021 22:42
Operator : AJ\MA
Sample : M3348-01
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SPEEDIDRI-TRE-1237


Manual Integrations
APPROVED

mohammad
8/12/2021 11:58:32 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 01:17:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 06 03:08:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

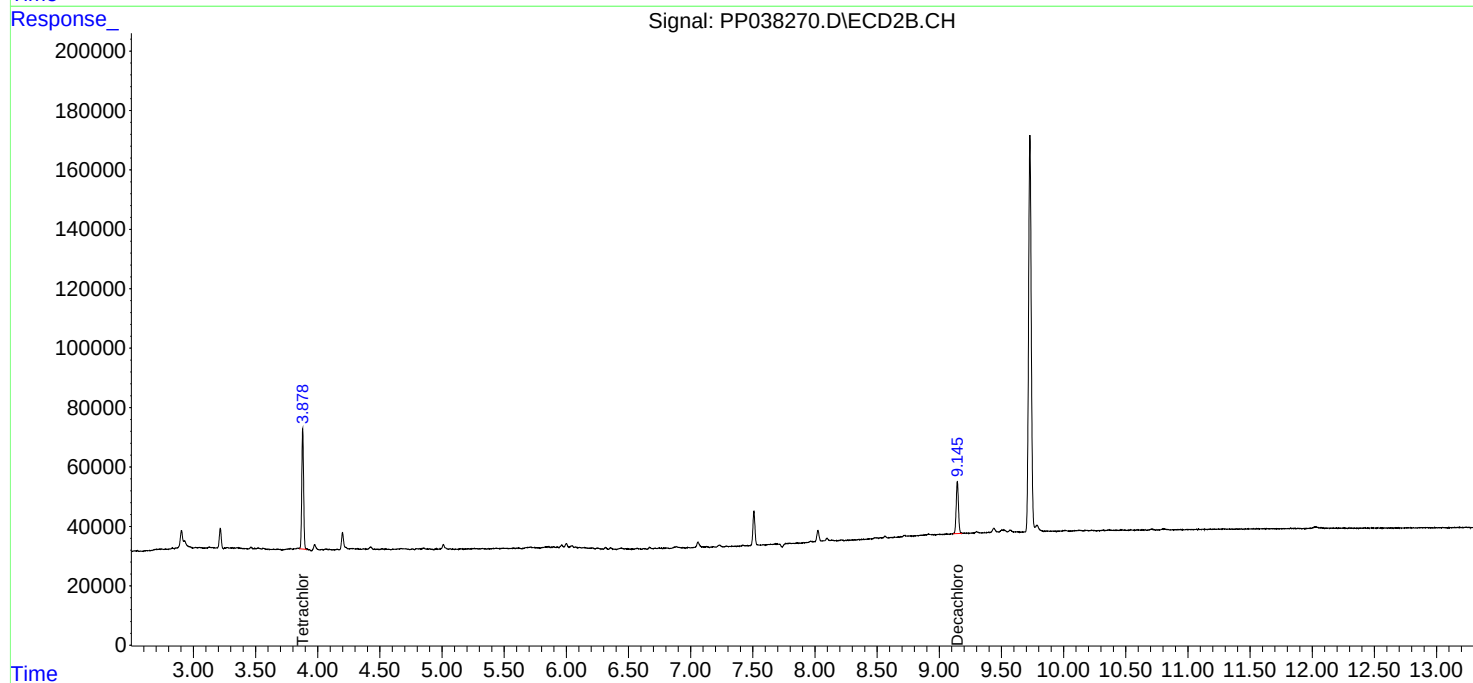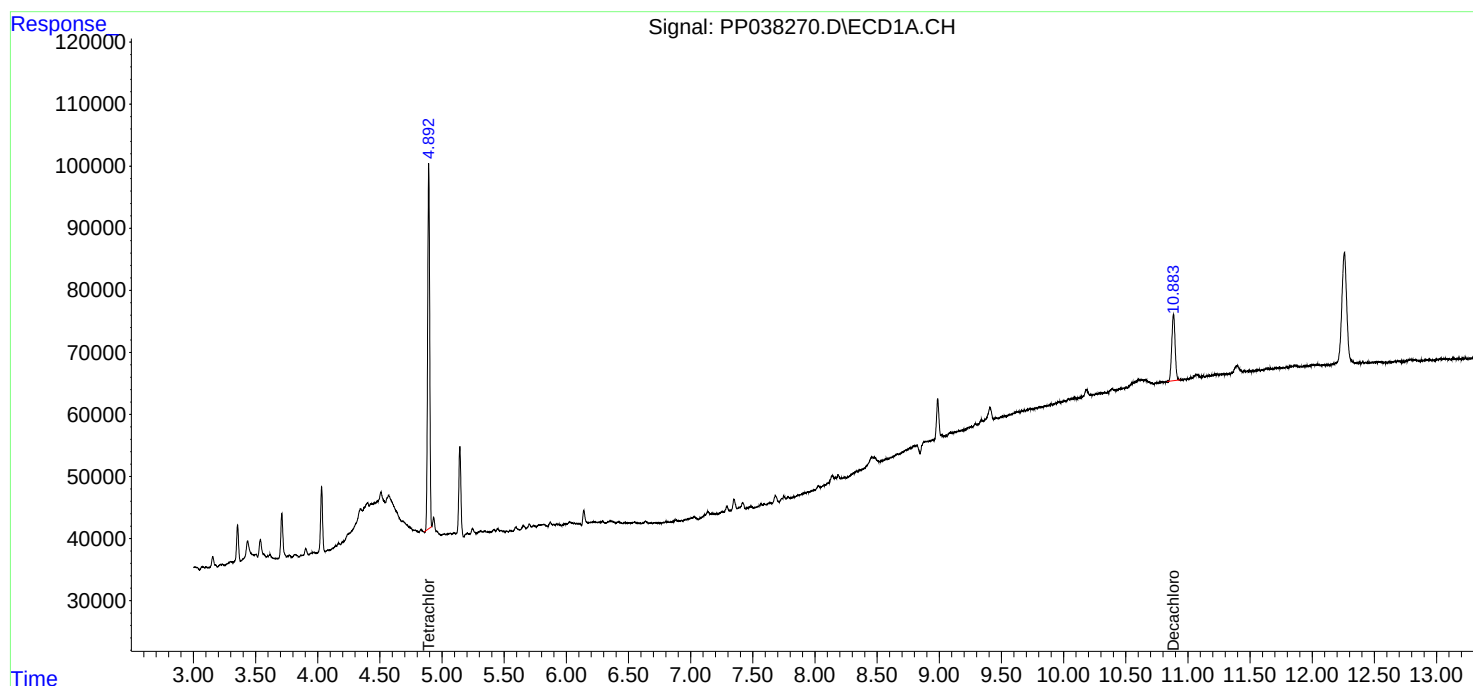

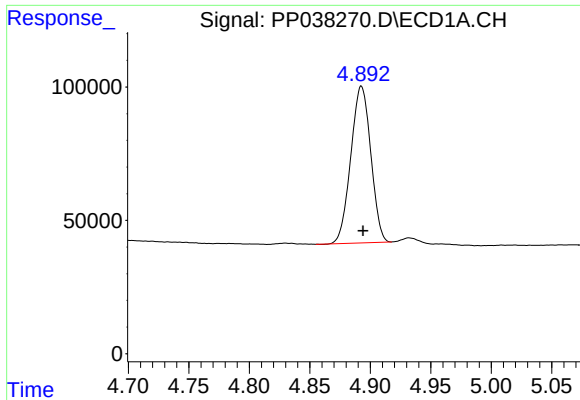


#1 Tetrachloro-m-xylene

R.T.: 4.893 min
Delta R.T.: -0.001 min
Response: 674321
Conc: 15.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
SPEEDIDRI-TRE-1237


Manual Integrations
APPROVED

mohammad
8/12/2021 11:58:32 AM

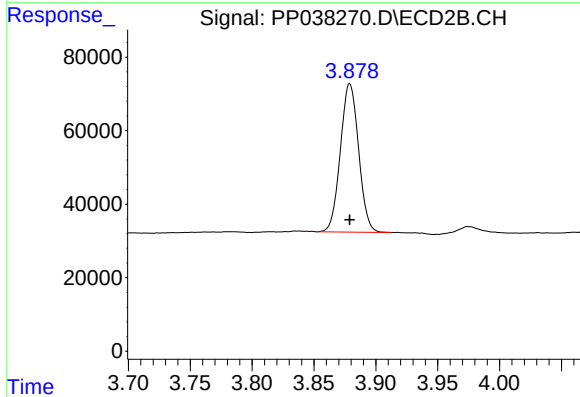


#1 Tetrachloro-m-xylene

R.T.: 3.878 min
Delta R.T.: 0.000 min
Response: 414540
Conc: 16.10 ng/ml m

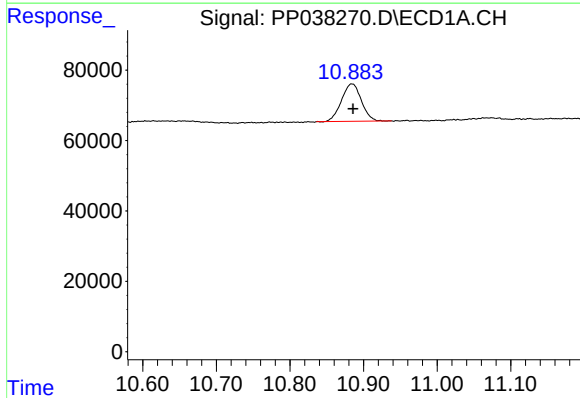

#2 Decachlorobiphenyl

R.T.: 10.884 min
Delta R.T.: -0.002 min
Response: 199505
Conc: 8.77 ng/ml

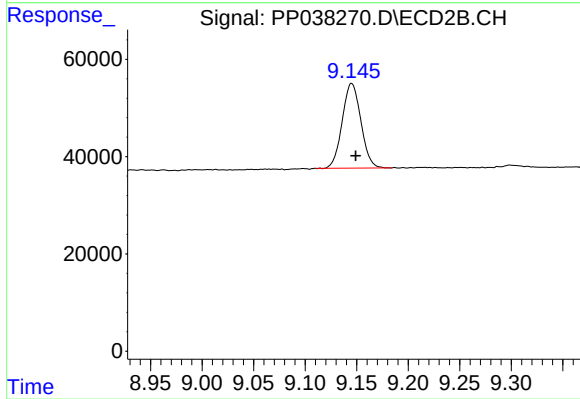

#2 Decachlorobiphenyl

R.T.: 9.145 min
Delta R.T.: -0.004 min
Response: 220148
Conc: 8.51 ng/ml