

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081122\
 Data File : PP050472.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2022 15:51
 Operator : YP\AJ
 Sample : N4082-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CRUSHED-MASONARY-PILE-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 23:10:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 09 11:38:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.346	3.592	34588314	68594433	21.488	21.900
2) SA Decachlor...	10.097	8.557	35094600	31167892	19.930	20.251

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081122\
Data File : PP050472.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2022 15:51
Operator : YP\AJ
Sample : N4082-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
CRUSHED-MASONARY-PILE-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 23:10:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 09 11:38:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

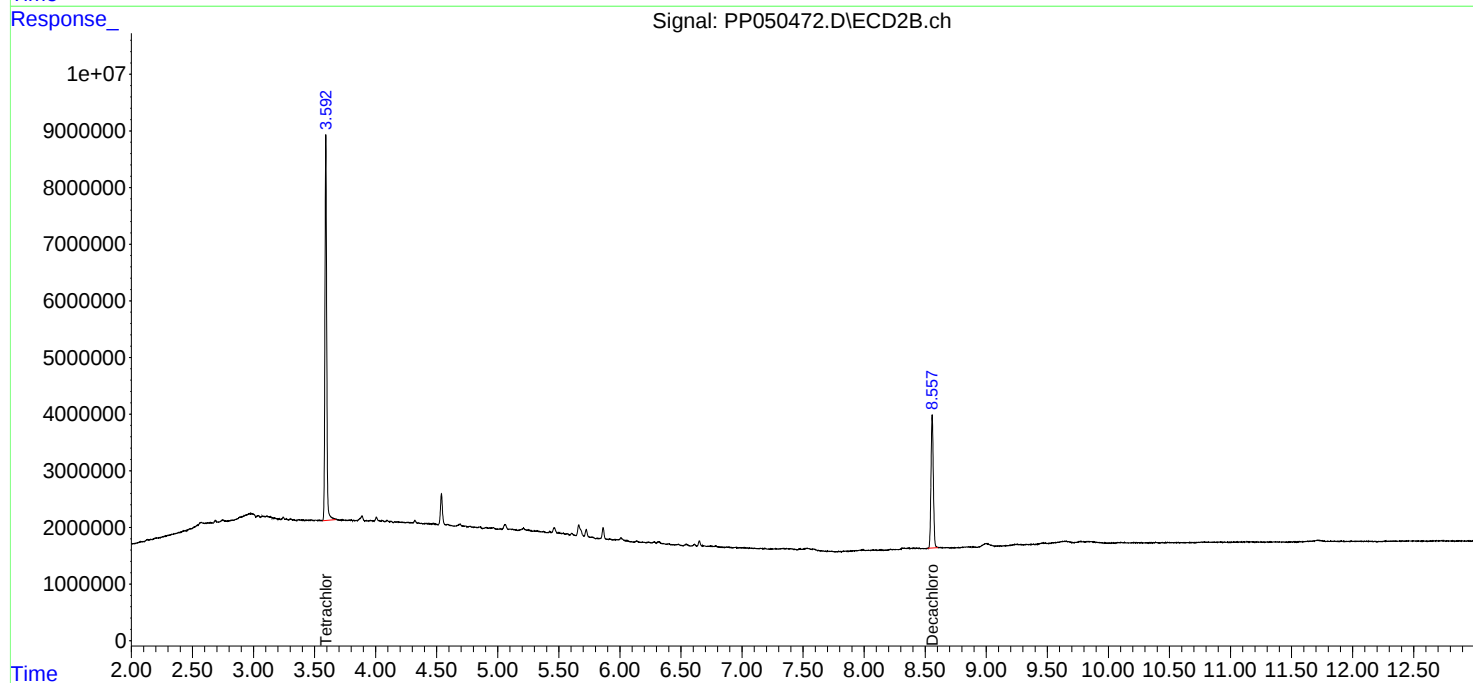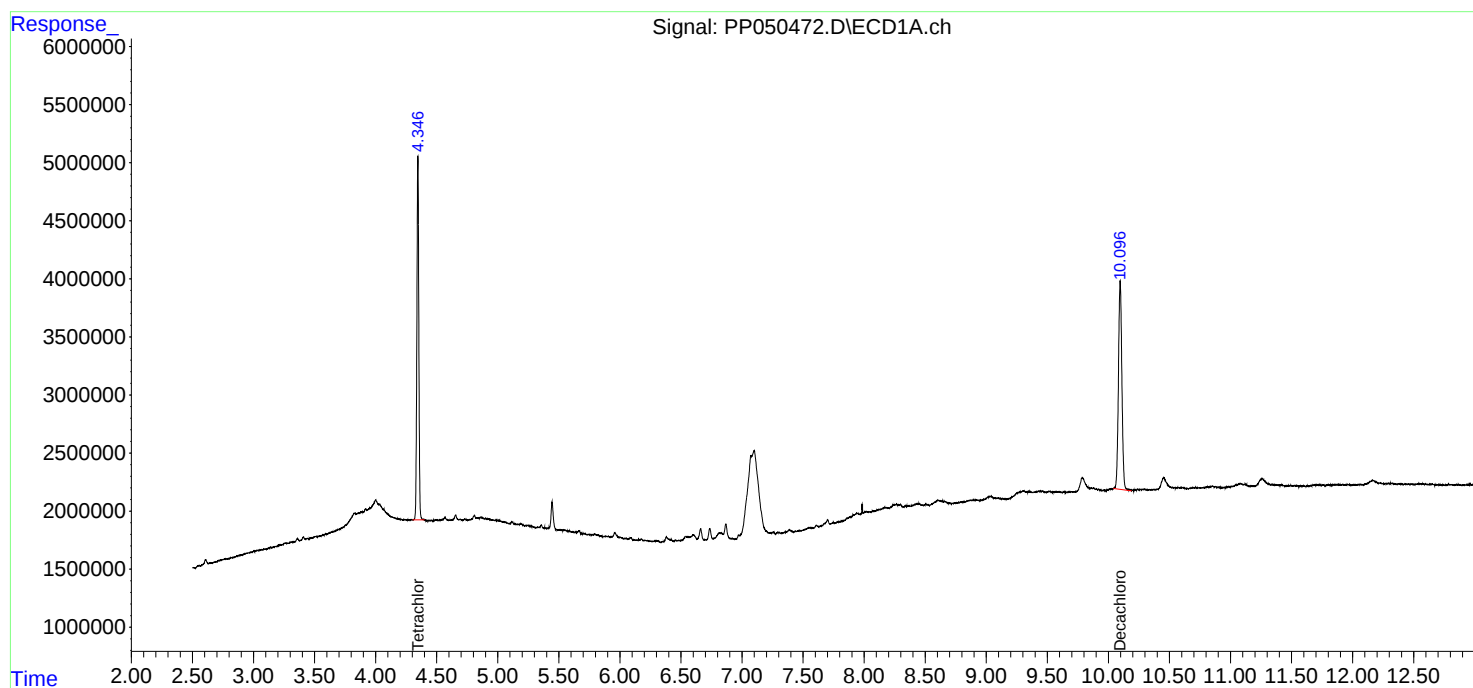


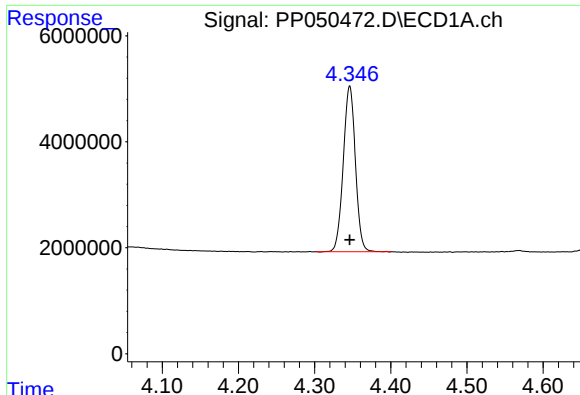

#1 Tetrachloro-m-xylene


R.T.: 4.346 min
Delta R.T.: 0.000 min
Response: 34588314
Conc: 21.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
CRUSHED-MASONARY-PILE-A

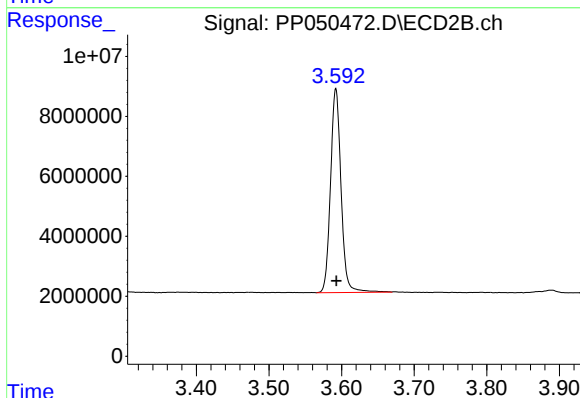


#1 Tetrachloro-m-xylene

R.T.: 3.592 min
Delta R.T.: 0.000 min
Response: 68594433
Conc: 21.90 ng/ml

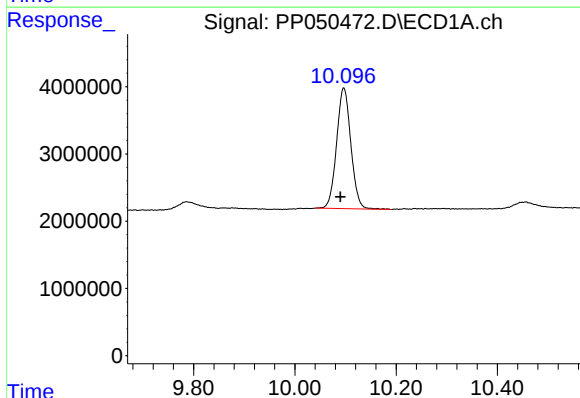

#2 Decachlorobiphenyl

R.T.: 10.097 min
Delta R.T.: 0.007 min
Response: 35094600
Conc: 19.93 ng/ml

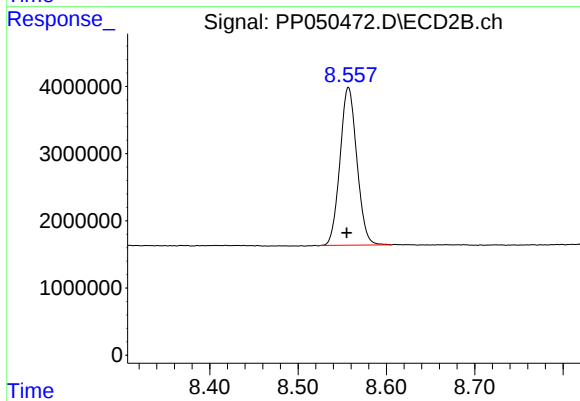

#2 Decachlorobiphenyl

R.T.: 8.557 min
Delta R.T.: 0.002 min
Response: 31167892
Conc: 20.25 ng/ml