

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081219\
 Data File : PP030309.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Aug 2019 12:39
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 07:01:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080919.M
 Quant Title : 8080.M
 QLast Update : Fri Aug 09 15:41:29 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

8) T	DICHLORPROP	12.624	0.000	31377187	0	26.029	N.D.	#
9) T	2,4-D	12.995	0.000	27522545	0	23.955	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081219\
Data File : PP030309.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Aug 2019 12:39
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 07:01:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080919.M
Quant Title : 8080.M
QLast Update : Fri Aug 09 15:41:29 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

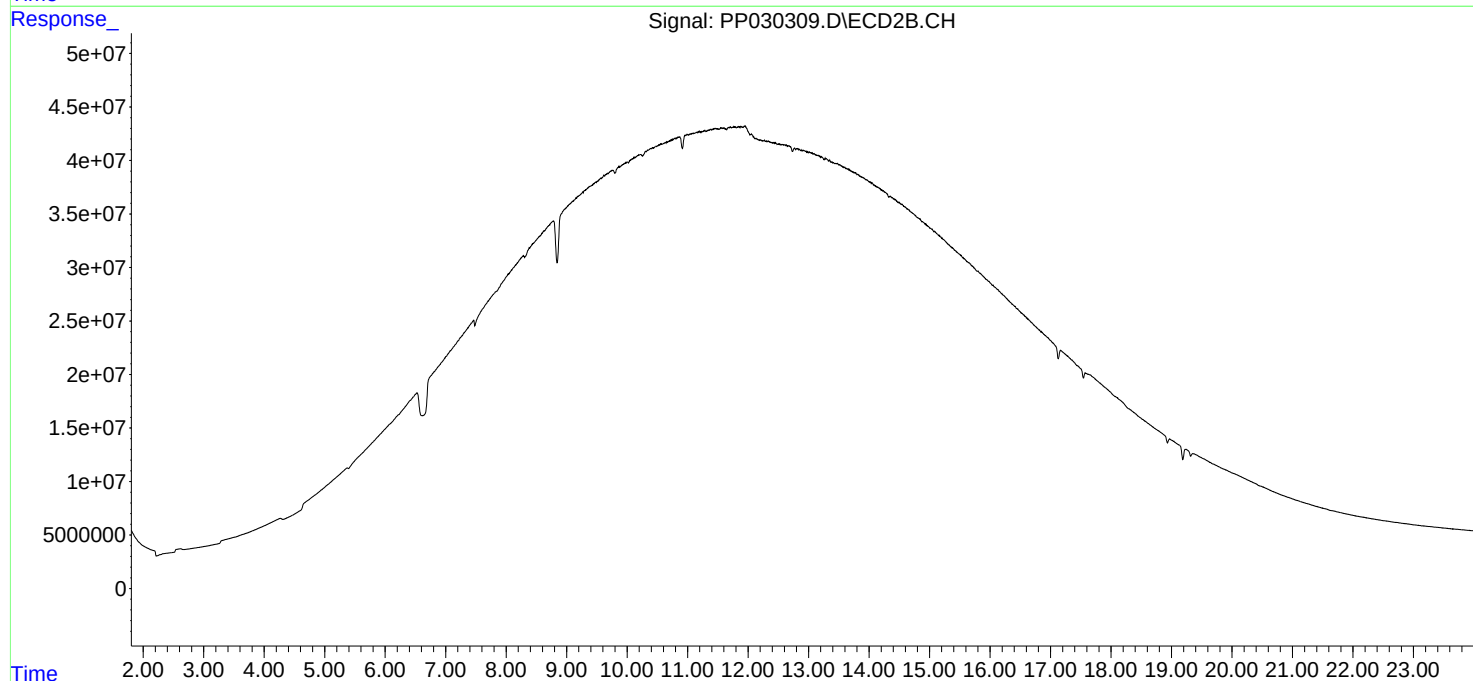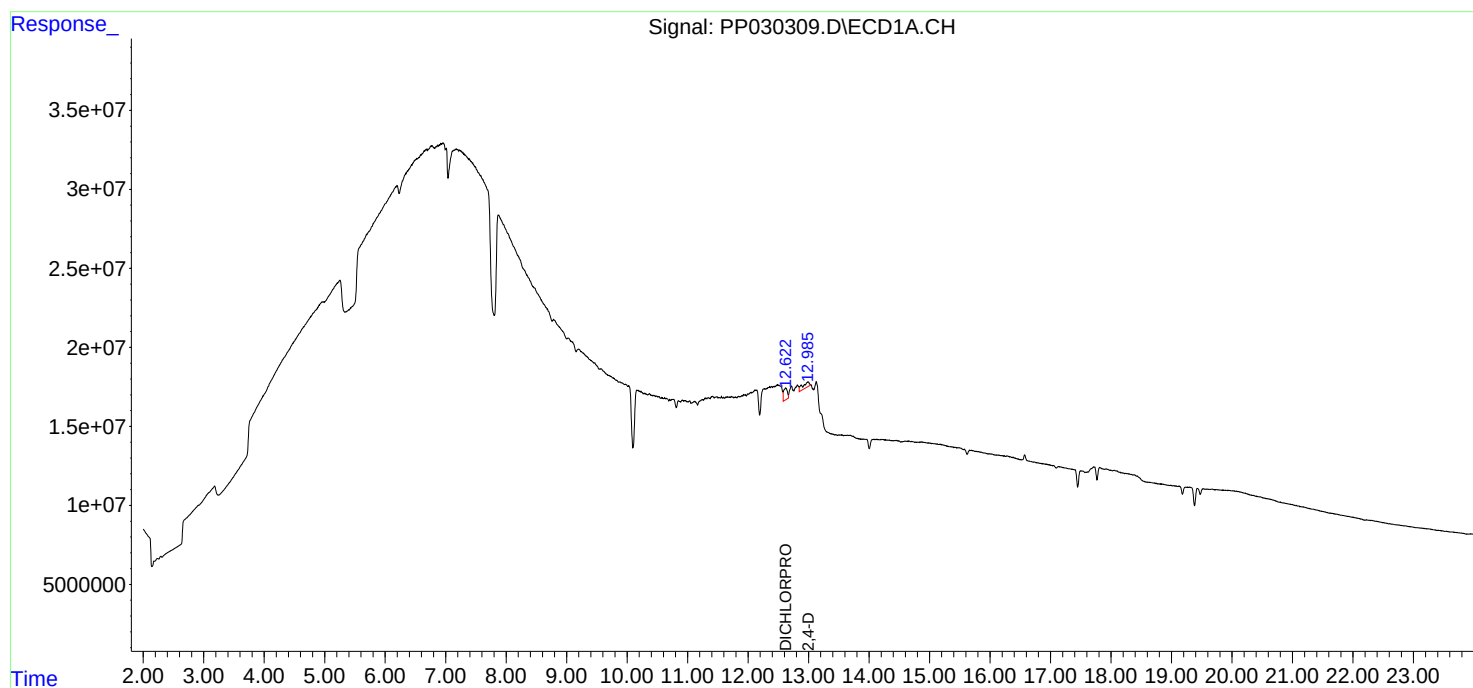


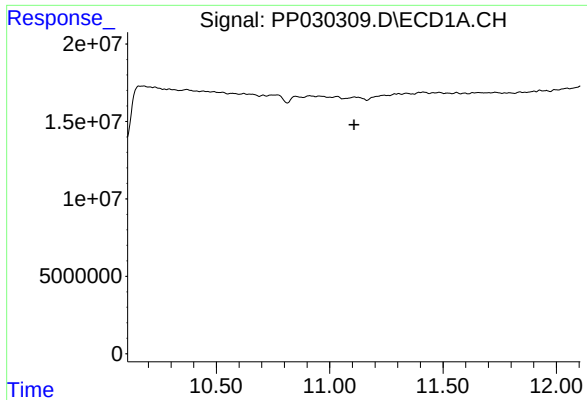

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 11.108 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

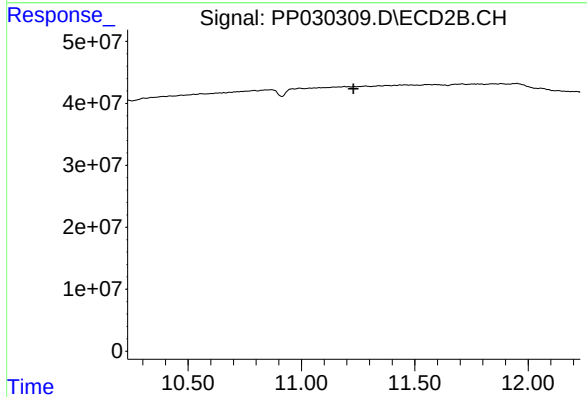


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 11.230 min
Response: 0
Conc: N.D.

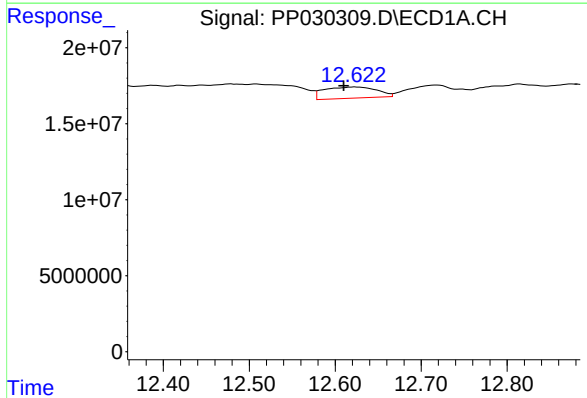


#8 DICHLORPROP

R.T.: 12.624 min
Delta R.T.: 0.014 min
Response: 31377187
Conc: 26.03 ng/ml

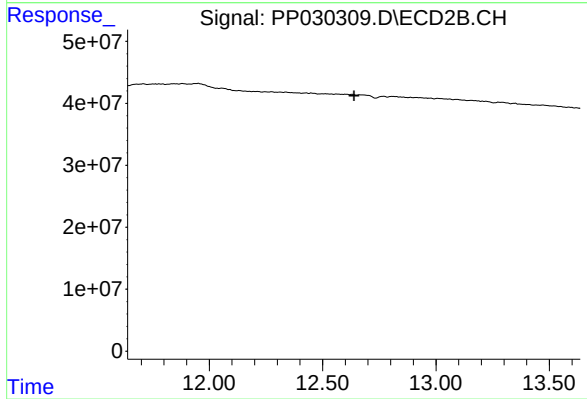

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 12.639 min
Response: 0
Conc: N.D.

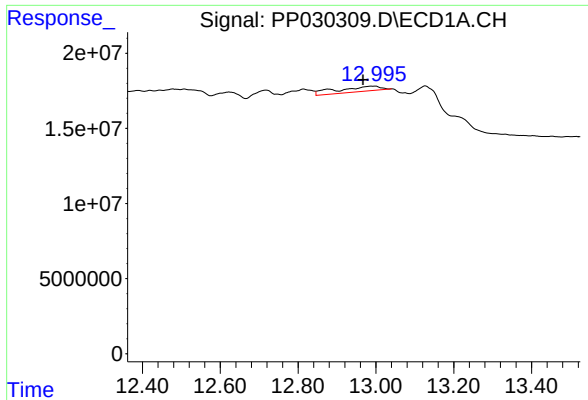

#9 2,4-D

R.T.: 12.995 min
Delta R.T.: 0.028 min
Response: 27522545
Conc: 23.96 ng/ml

Instrument :
ECD_P
ClientSampleId :

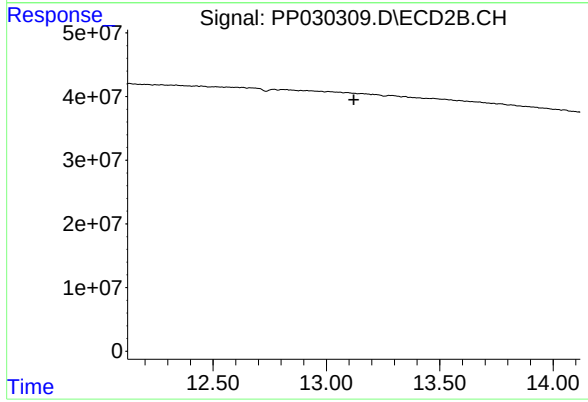

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.121 min
Response: 0
Conc: N.D.