

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081219\
 Data File : PP030323.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Aug 2019 19:19
 Operator : SM\AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 07:07:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080919.M
 Quant Title : 8080.M
 QLast Update : Fri Aug 09 15:41:29 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.108	11.229	946.4E6	761.5E6	772.850	820.608
Target Compounds							
1) T	Dalapon	2.607	2.409	457.1E6	327.4E6	611.320	641.871
2) T	3,5-DICHL...	9.525	9.356	1515.8E6	904.4E6	727.774	754.911
3) T	4-Nitroph...	10.677	10.384	856.7E6	363.4E6	707.591	748.492
5) T	DICAMBA	11.418	11.524	4021.4E6	2769.7E6	745.499	764.011
6) T	MCPD	11.774	11.743	232.3E6	160.8E6	76.043	78.286
7) T	MCPA	12.027	12.130	291.8E6	224.1E6	72.905	73.622
8) T	DICHLORPROP	12.610	12.639	875.9E6	636.8E6	726.638	746.268
9) T	2,4-D	12.966	13.121	817.1E6	623.1E6	711.195	737.004
10) T	Pentachlo...	13.328	13.680	13780.7E6	9141.3E6	719.279	727.686
11) T	2,4,5-TP ...	14.215	14.281	4896.5E6	3633.6E6	723.030	744.271
12) T	2,4,5-T	14.610	14.822	3725.7E6	2751.9E6	686.665	722.607
13) T	2,4-DB	15.356	15.503	618.8E6	464.1E6	669.935	701.299
14) T	DINOSEB	16.818	15.910	2354.5E6	1738.1E6	573.860	585.634
15) T	Picloram	16.595	17.223	5512.7E6	4045.4E6	1849.716	2279.915
16) T	DCPA	17.171	17.121	6281.7E6	4572.4E6	755.368	753.953



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081219\
Data File : PP030323.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Aug 2019 19:19
Operator : SM\AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 07:07:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080919.M
Quant Title : 8080.M
QLast Update : Fri Aug 09 15:41:29 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

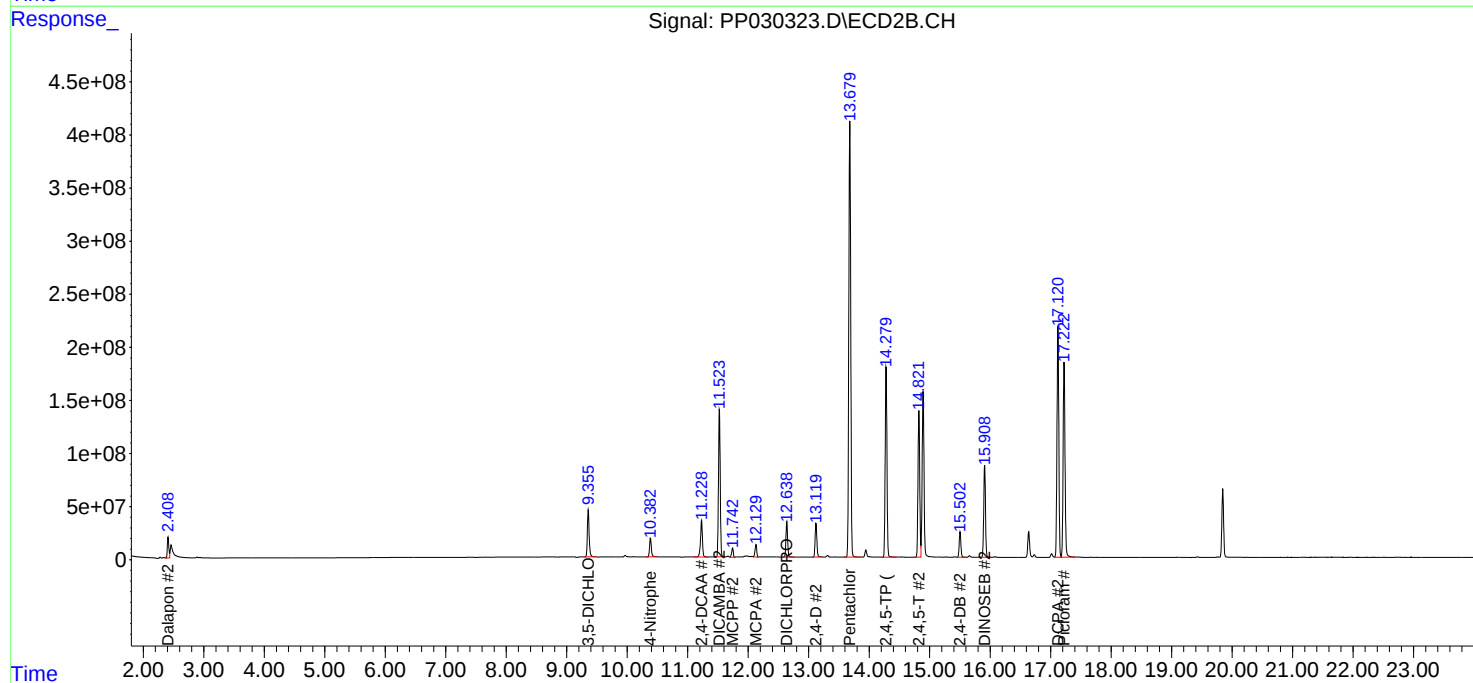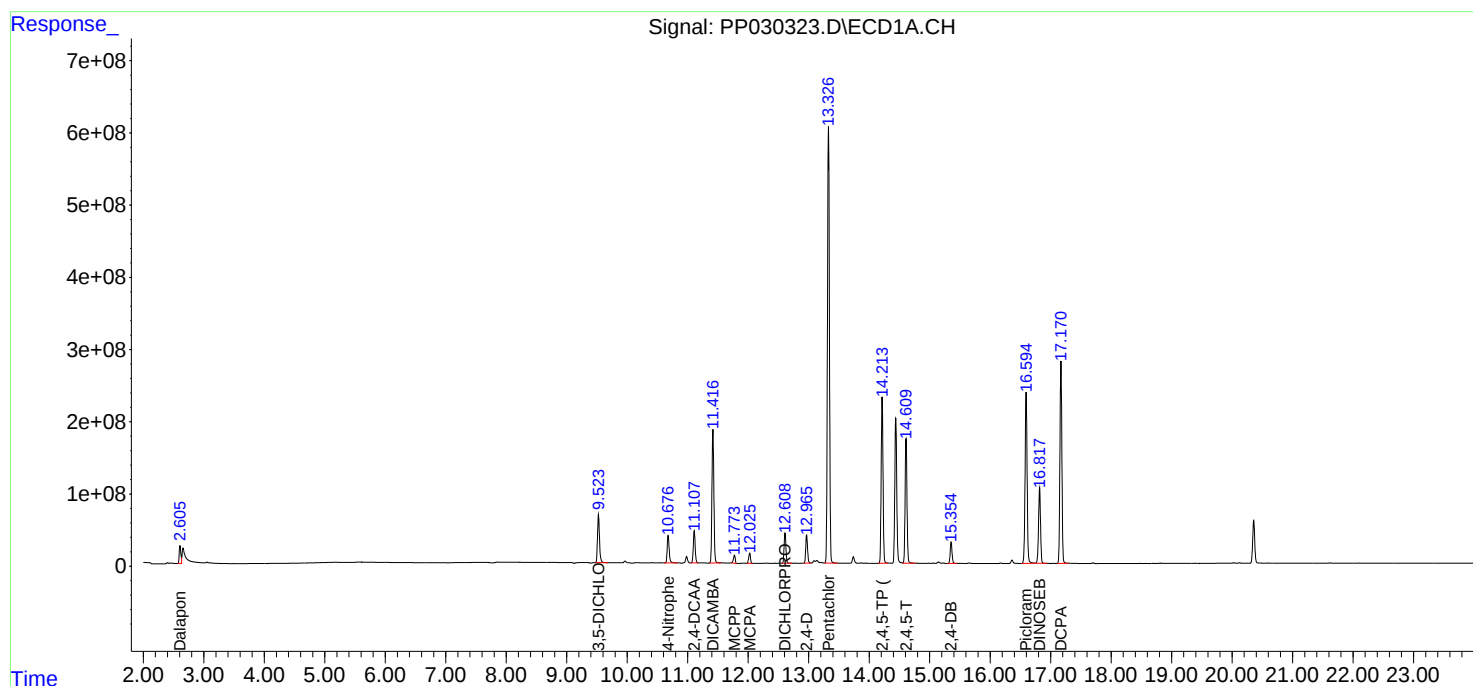


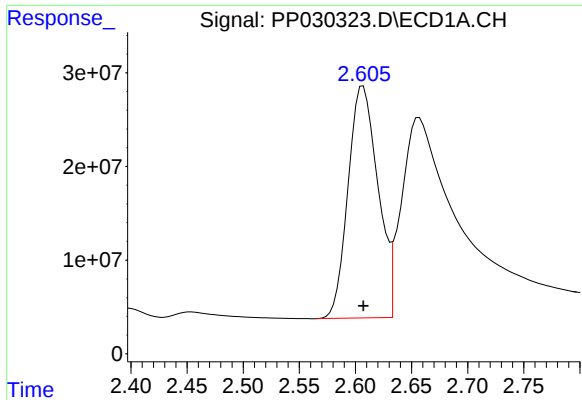

#1 Dalapon


R.T.: 2.607 min
Delta R.T.: 0.000 min
Response: 457125252
Conc: 611.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
HSTDCCC750

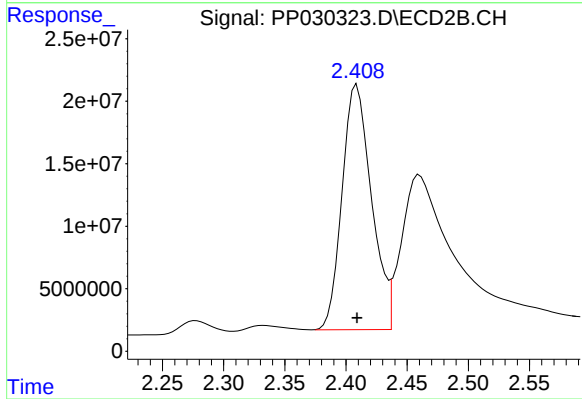


#1 Dalapon

R.T.: 2.409 min
Delta R.T.: 0.000 min
Response: 327442894
Conc: 641.87 ng/ml

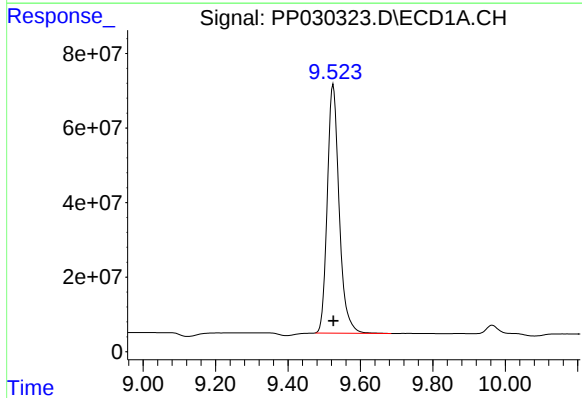


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.525 min
Delta R.T.: 0.000 min
Response: 1515843844
Conc: 727.77 ng/ml

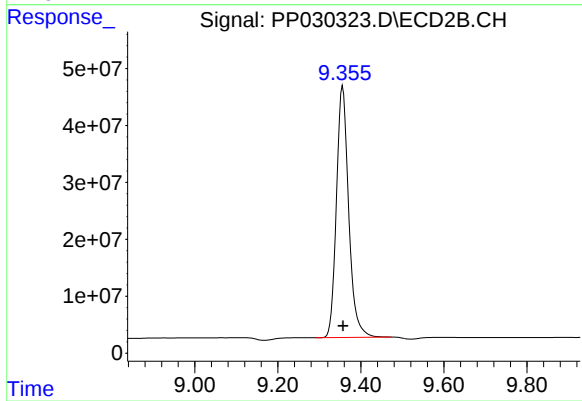

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.356 min
Delta R.T.: 0.000 min
Response: 904405182
Conc: 754.91 ng/ml

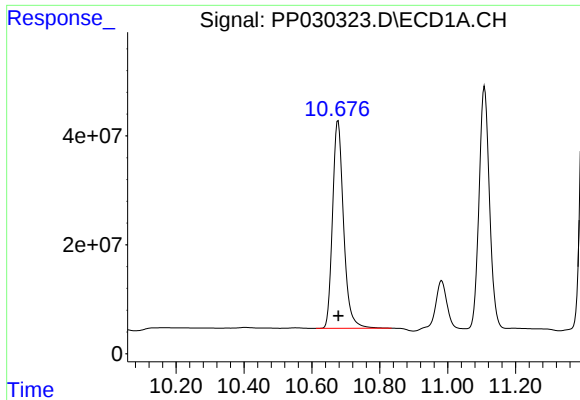

#3 4-Nitrophenol


R.T.: 10.677 min
Delta R.T.: 0.000 min
Response: 856719223
Conc: 707.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
HSTDCCC750

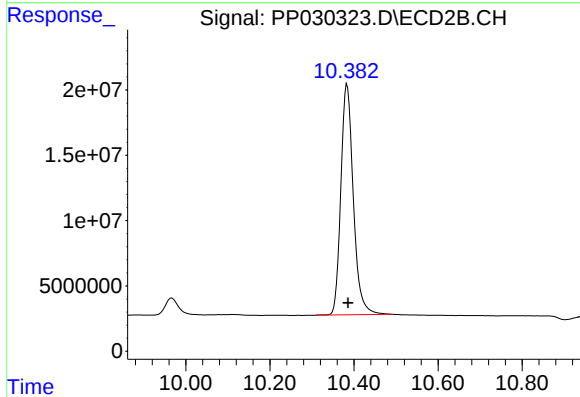


#3 4-Nitrophenol

R.T.: 10.384 min
Delta R.T.: -0.002 min
Response: 363398826
Conc: 748.49 ng/ml

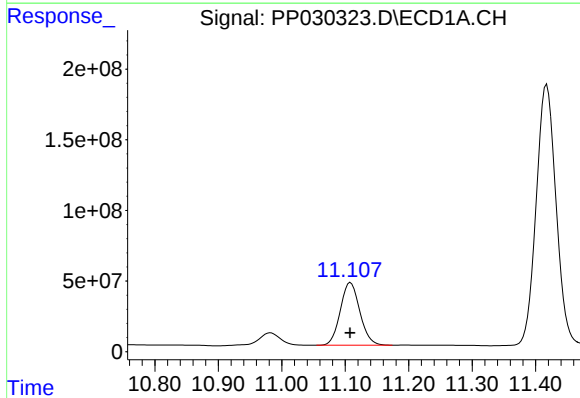


#4 2,4-DCAA

R.T.: 11.108 min
Delta R.T.: 0.000 min
Response: 946373453
Conc: 772.85 ng/ml

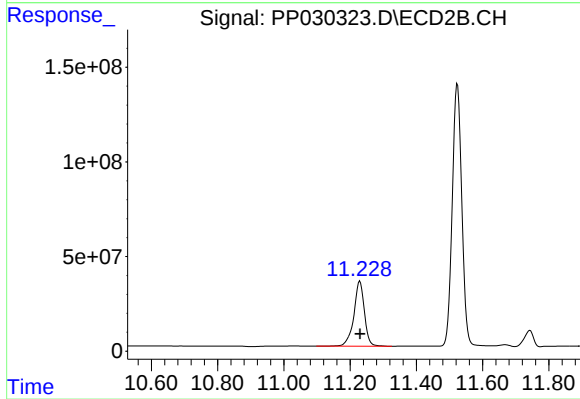

#4 2,4-DCAA


R.T.: 11.229 min
Delta R.T.: 0.000 min
Response: 761471373
Conc: 820.61 ng/ml

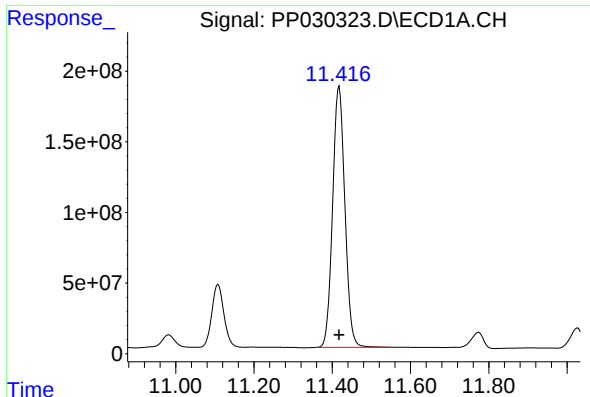

#5 DICAMBA


R.T.: 11.418 min
Delta R.T.: 0.000 min
Response: 4021384838
Conc: 745.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
HSTDCCC750

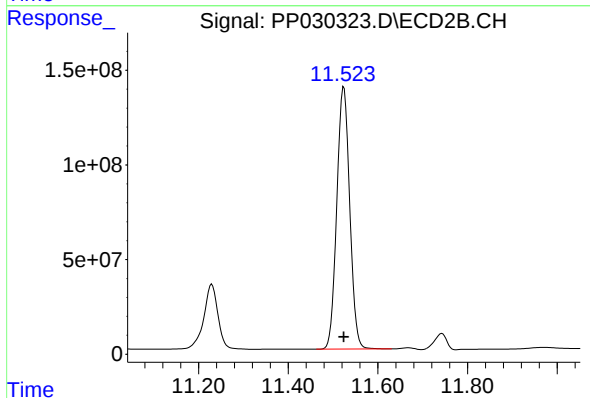


#5 DICAMBA

R.T.: 11.524 min
Delta R.T.: 0.000 min
Response: 2769672967
Conc: 764.01 ng/ml

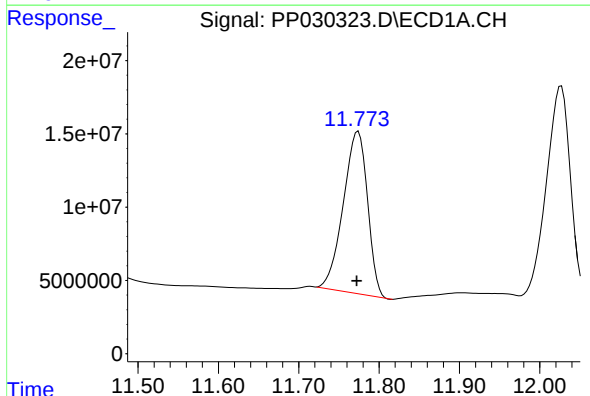


#6 MCP

R.T.: 11.774 min
Delta R.T.: 0.002 min
Response: 232275959
Conc: 76.04 ug/ml

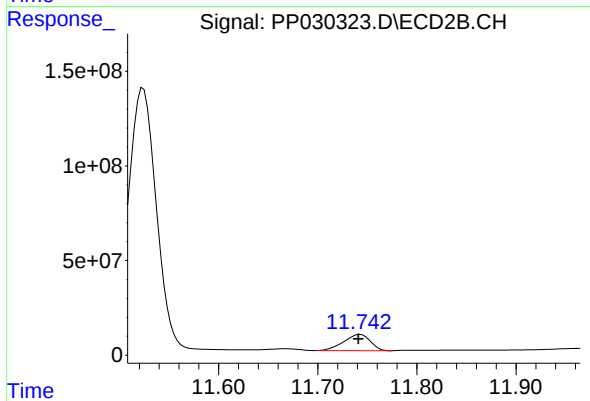

#6 MCP


R.T.: 11.743 min
Delta R.T.: 0.002 min
Response: 160840854
Conc: 78.29 ug/ml

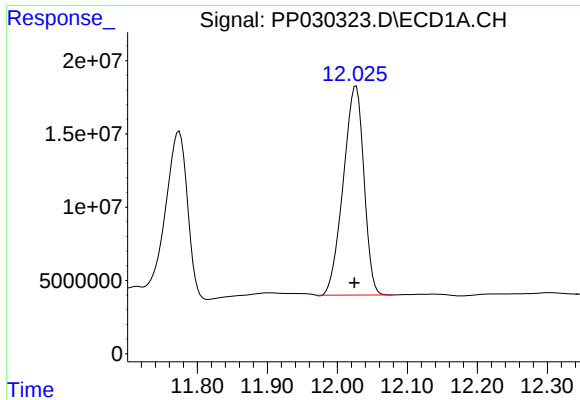

#7 MCPA


R.T.: 12.027 min
Delta R.T.: 0.002 min
Response: 291797551
Conc: 72.90 ug/ml

Instrument :
ECD_P
ClientSampleId :
HSTDCCC750

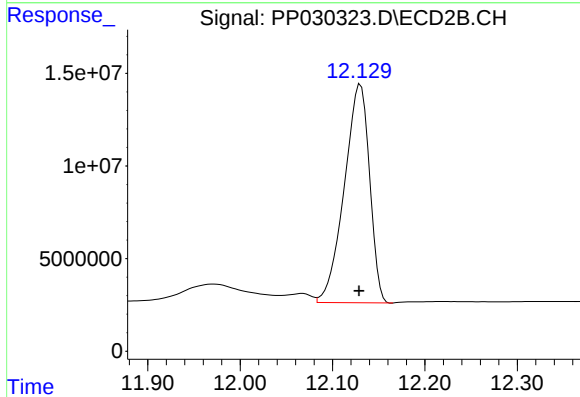


#7 MCPA

R.T.: 12.130 min
Delta R.T.: 0.002 min
Response: 224128020
Conc: 73.62 ug/ml

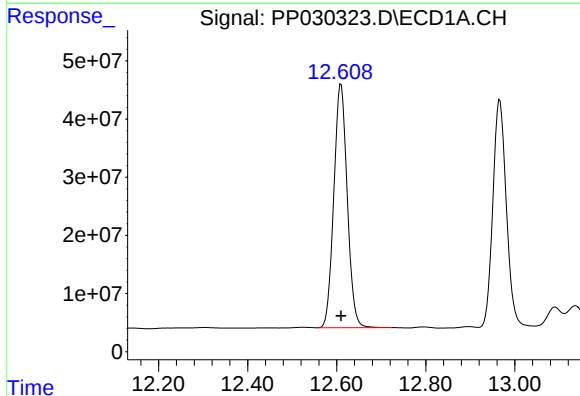


#8 DICHLORPROP

R.T.: 12.610 min
Delta R.T.: 0.000 min
Response: 875940465
Conc: 726.64 ng/ml

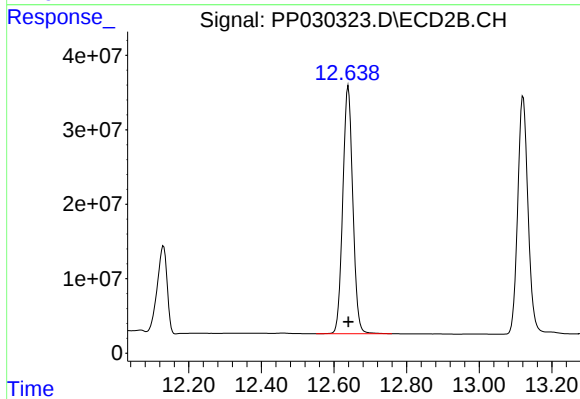

#8 DICHLORPROP


R.T.: 12.639 min
Delta R.T.: 0.000 min
Response: 636844881
Conc: 746.27 ng/ml

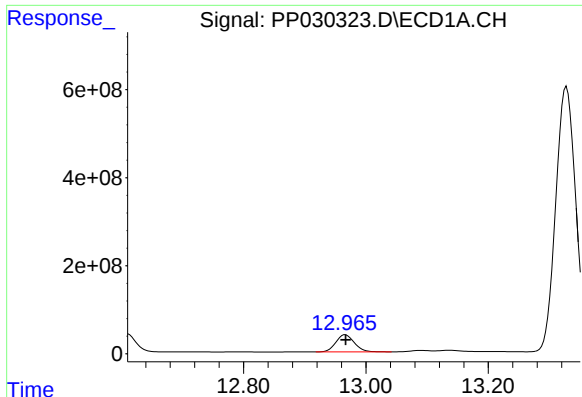

#9 2,4-D


R.T.: 12.966 min
Delta R.T.: 0.000 min
Response: 817096010
Conc: 711.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
HSTDCCC750

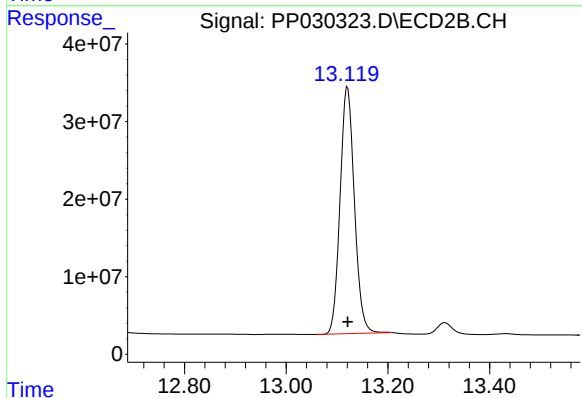


#9 2,4-D

R.T.: 13.121 min
Delta R.T.: 0.000 min
Response: 623147785
Conc: 737.00 ng/ml

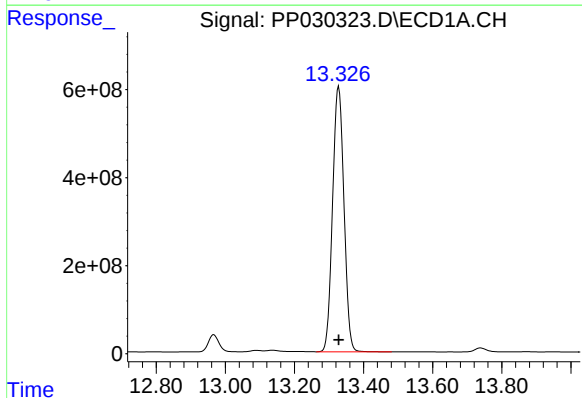


#10 Pentachlorophenol

R.T.: 13.328 min
Delta R.T.: 0.000 min
Response: 13780675836
Conc: 719.28 ng/ml

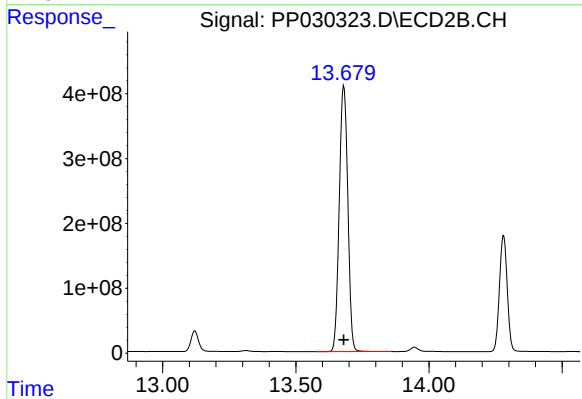

#10 Pentachlorophenol


R.T.: 13.680 min
Delta R.T.: 0.000 min
Response: 9141308862
Conc: 727.69 ng/ml

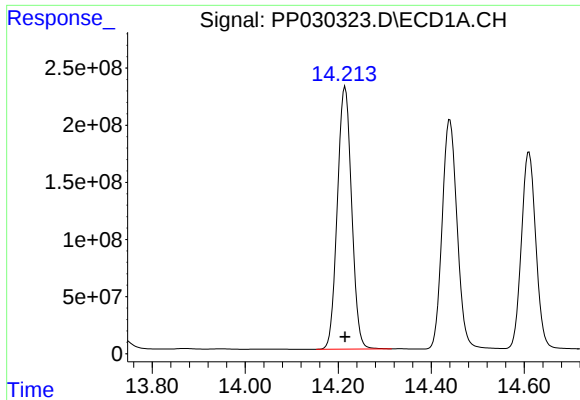

#11 2,4,5-TP (SILVEX)


R.T.: 14.215 min
Delta R.T.: 0.000 min
Response: 4896481856
Conc: 723.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
HSTDCCC750

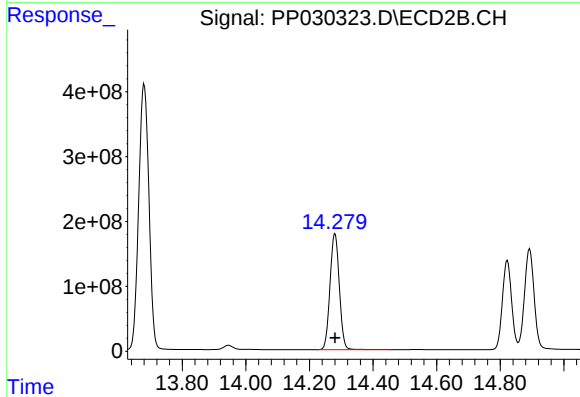


#11 2,4,5-TP (SILVEX)

R.T.: 14.281 min
Delta R.T.: 0.000 min
Response: 3633556692
Conc: 744.27 ng/ml

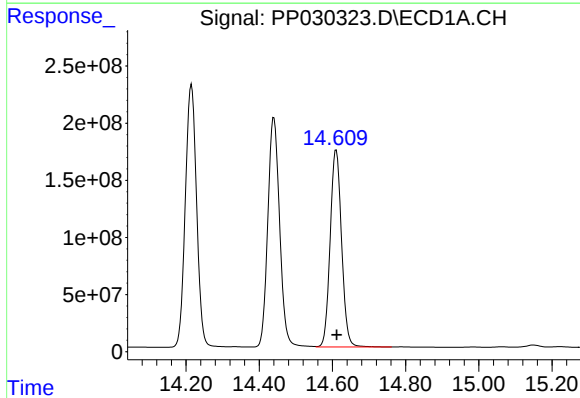


#12 2,4,5-T

R.T.: 14.610 min
Delta R.T.: -0.001 min
Response: 3725657749
Conc: 686.67 ng/ml

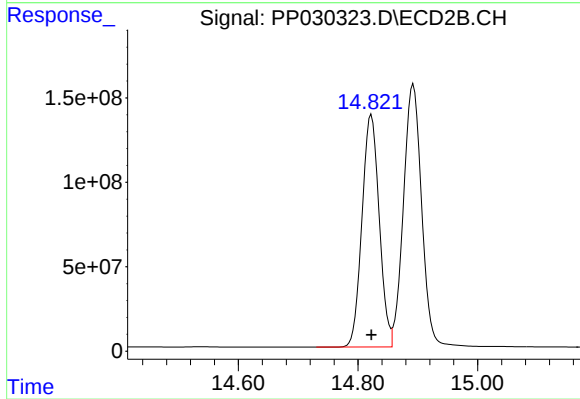

#12 2,4,5-T


R.T.: 14.822 min
Delta R.T.: 0.000 min
Response: 2751946550
Conc: 722.61 ng/ml

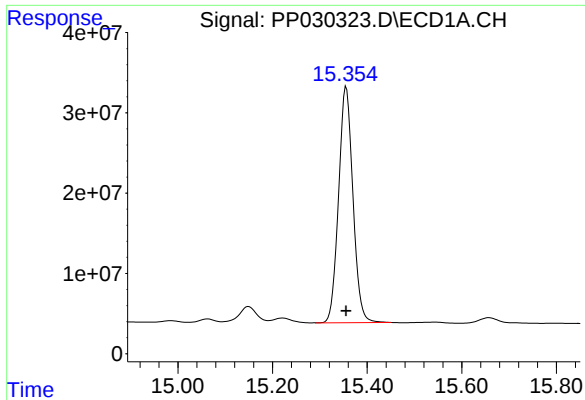

#13 2,4-DB


R.T.: 15.356 min
Delta R.T.: 0.000 min
Response: 618847067
Conc: 669.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
HSTDCCC750

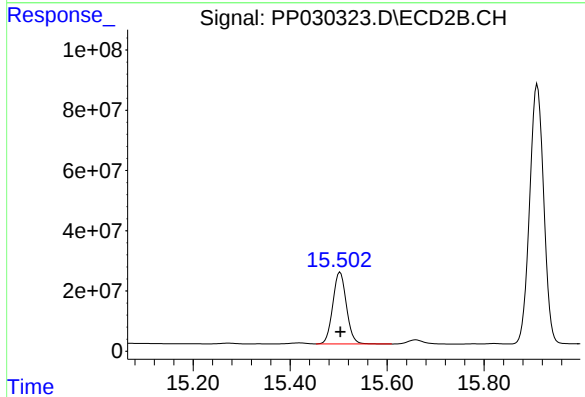


#13 2,4-DB

R.T.: 15.503 min
Delta R.T.: 0.000 min
Response: 464061723
Conc: 701.30 ng/ml

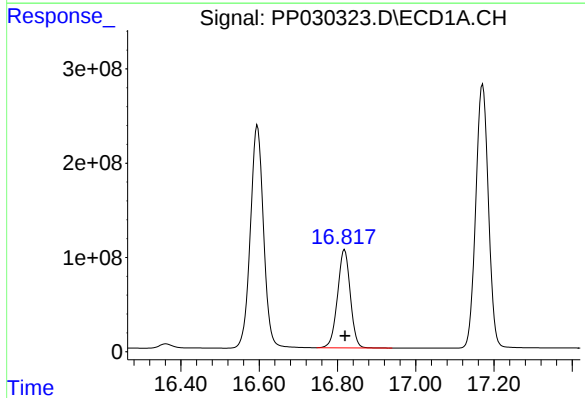


#14 DINOSEB

R.T.: 16.818 min
Delta R.T.: -0.001 min
Response: 2354522491
Conc: 573.86 ng/ml

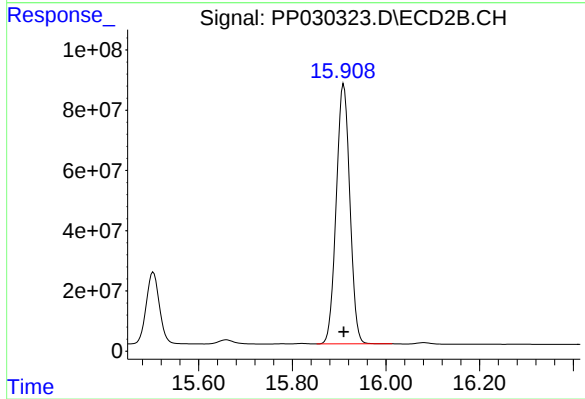

#14 DINOSEB


R.T.: 15.910 min
Delta R.T.: 0.000 min
Response: 1738075741
Conc: 585.63 ng/ml

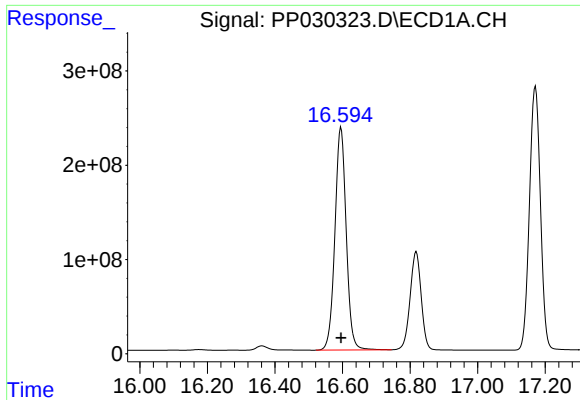

#15 Picloram


R.T.: 16.595 min
Delta R.T.: 0.000 min
Response: 5512745378
Conc: 1849.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
HSTDCCC750

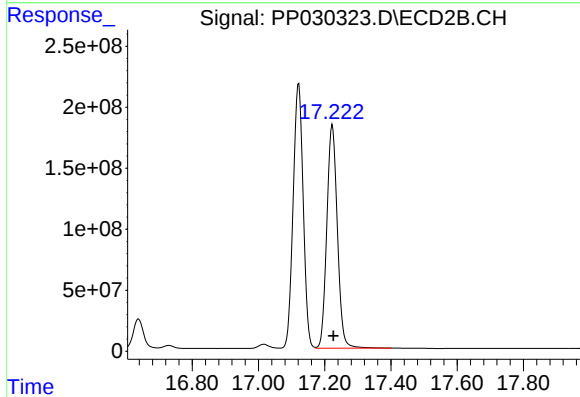


#15 Picloram

R.T.: 17.223 min
Delta R.T.: -0.003 min
Response: 4045427330
Conc: 2279.91 ng/ml

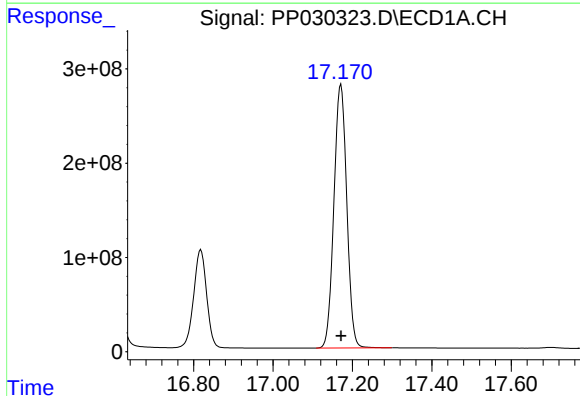

#16 DCPA

R.T.: 17.171 min
Delta R.T.: 0.000 min
Response: 6281741960
Conc: 755.37 ng/ml

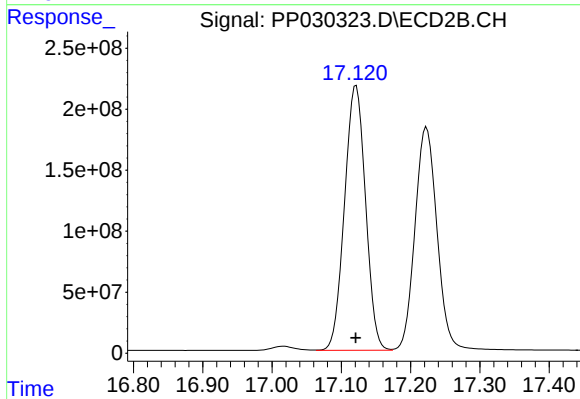

#16 DCPA

R.T.: 17.121 min
Delta R.T.: 0.000 min
Response: 4572436224
Conc: 753.95 ng/ml