

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081221\
Data File : PP038286.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Aug 2021 11:48
Operator : AJ\MA
Sample : M3343-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
20210591-AMENDED-COM-5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 02:46:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 06 03:08:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.890	3.877	796173	474306	17.915	18.416
2) SA Decachlor...	10.877	9.142	350354	427252	15.401	16.513

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081221\
Data File : PP038286.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Aug 2021 11:48
Operator : AJ\MA
Sample : M3343-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
20210591-AMENDED-COM-5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 02:46:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 06 03:08:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

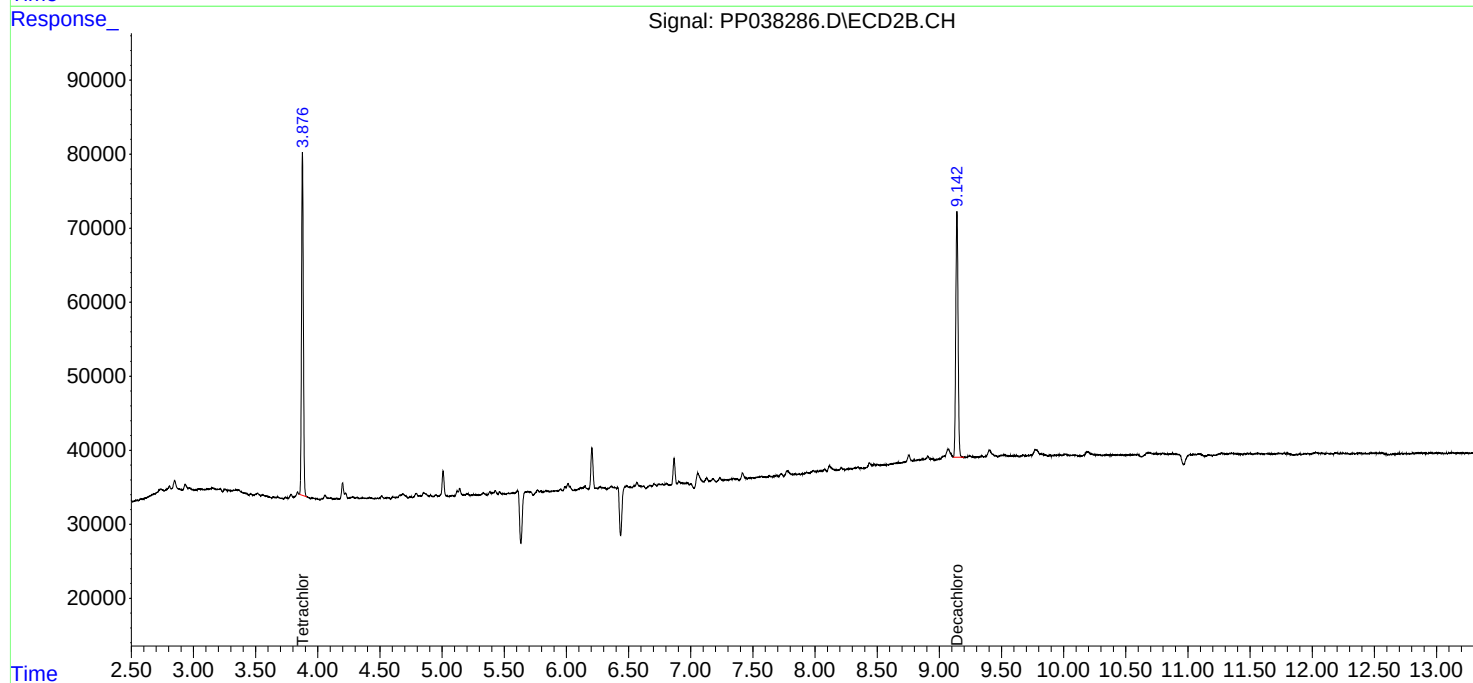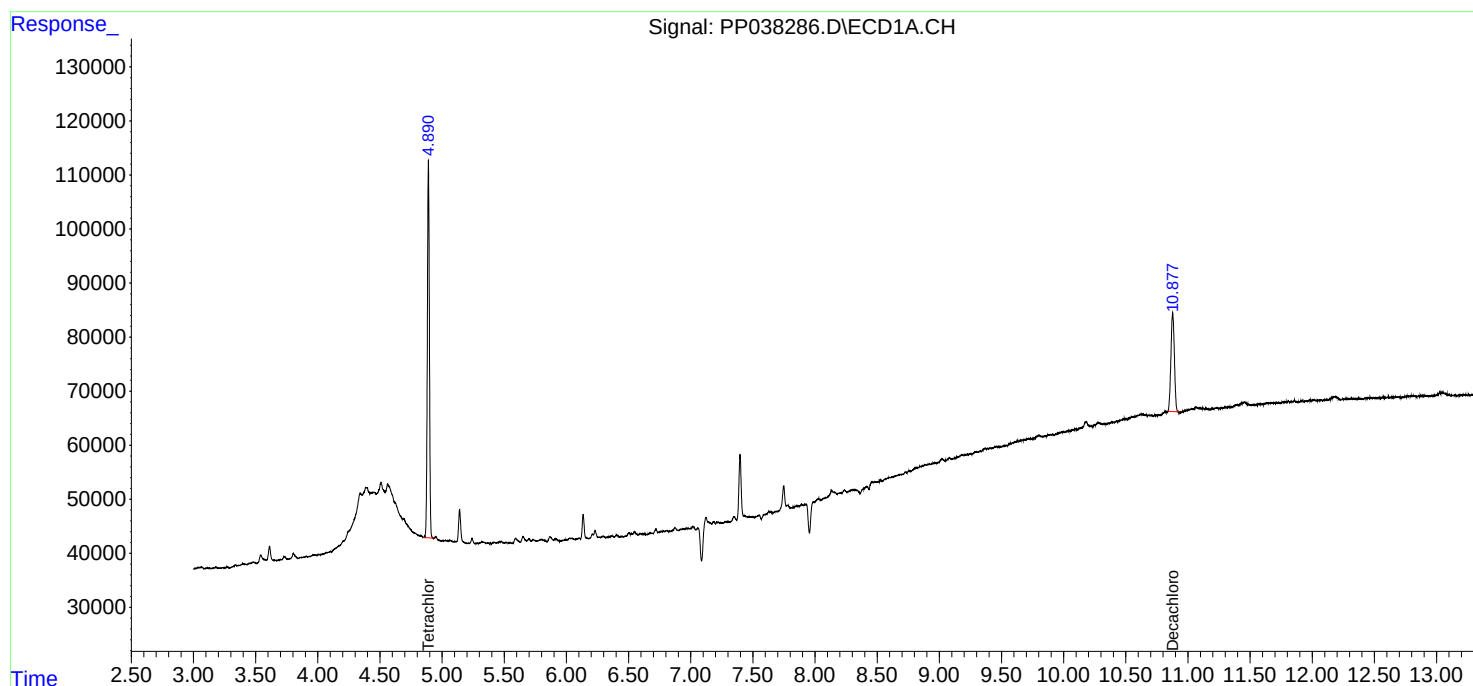


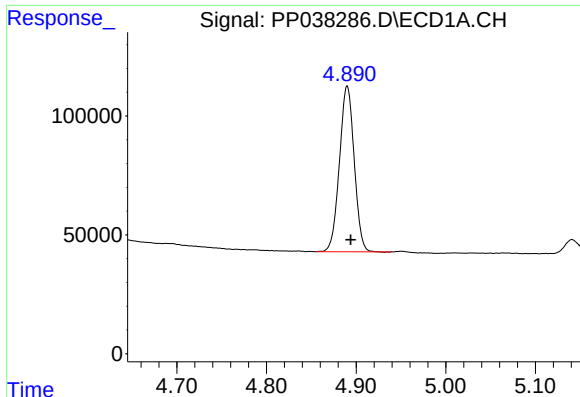

#1 Tetrachloro-m-xylene


R.T.: 4.890 min
Delta R.T.: -0.004 min
Response: 796173
Conc: 17.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
20210591-AMENDED-COM-5

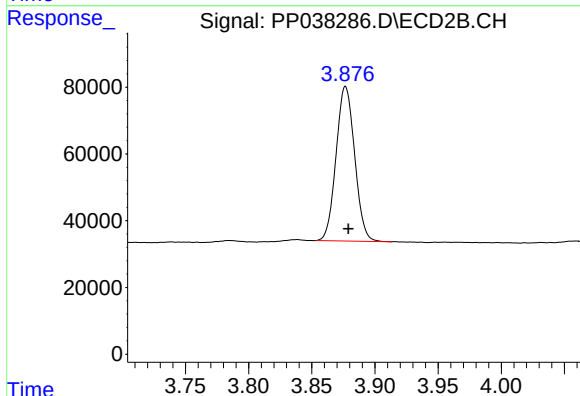


#1 Tetrachloro-m-xylene

R.T.: 3.877 min
Delta R.T.: -0.002 min
Response: 474306
Conc: 18.42 ng/ml

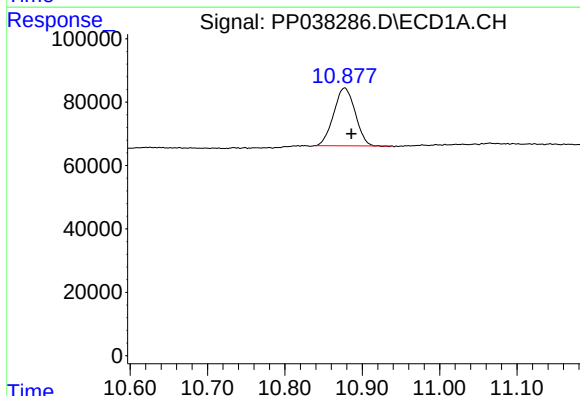

#2 Decachlorobiphenyl

R.T.: 10.877 min
Delta R.T.: -0.008 min
Response: 350354
Conc: 15.40 ng/ml

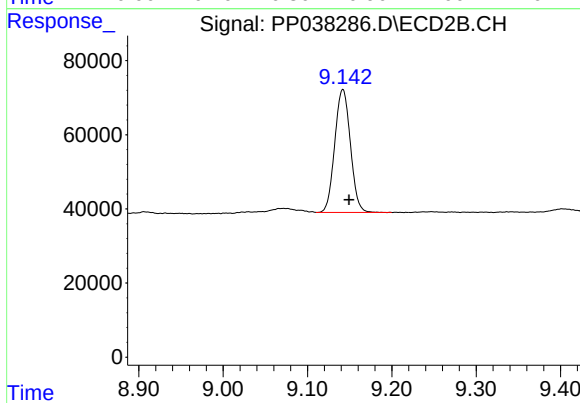

#2 Decachlorobiphenyl

R.T.: 9.142 min
Delta R.T.: -0.007 min
Response: 427252
Conc: 16.51 ng/ml