

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081221\
 Data File : PP038303.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Aug 2021 16:53
 Operator : AJ\MA
 Sample : M3361-15
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 07-08-11

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 02:57:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 06 03:08:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.892	3.878	809233	483190	18.209	18.761
2) SA Decachlor...	10.880	9.143	307379	370802	13.512	14.332

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081221\
Data File : PP038303.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Aug 2021 16:53
Operator : AJ\MA
Sample : M3361-15
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
07-08-11

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 02:57:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 06 03:08:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

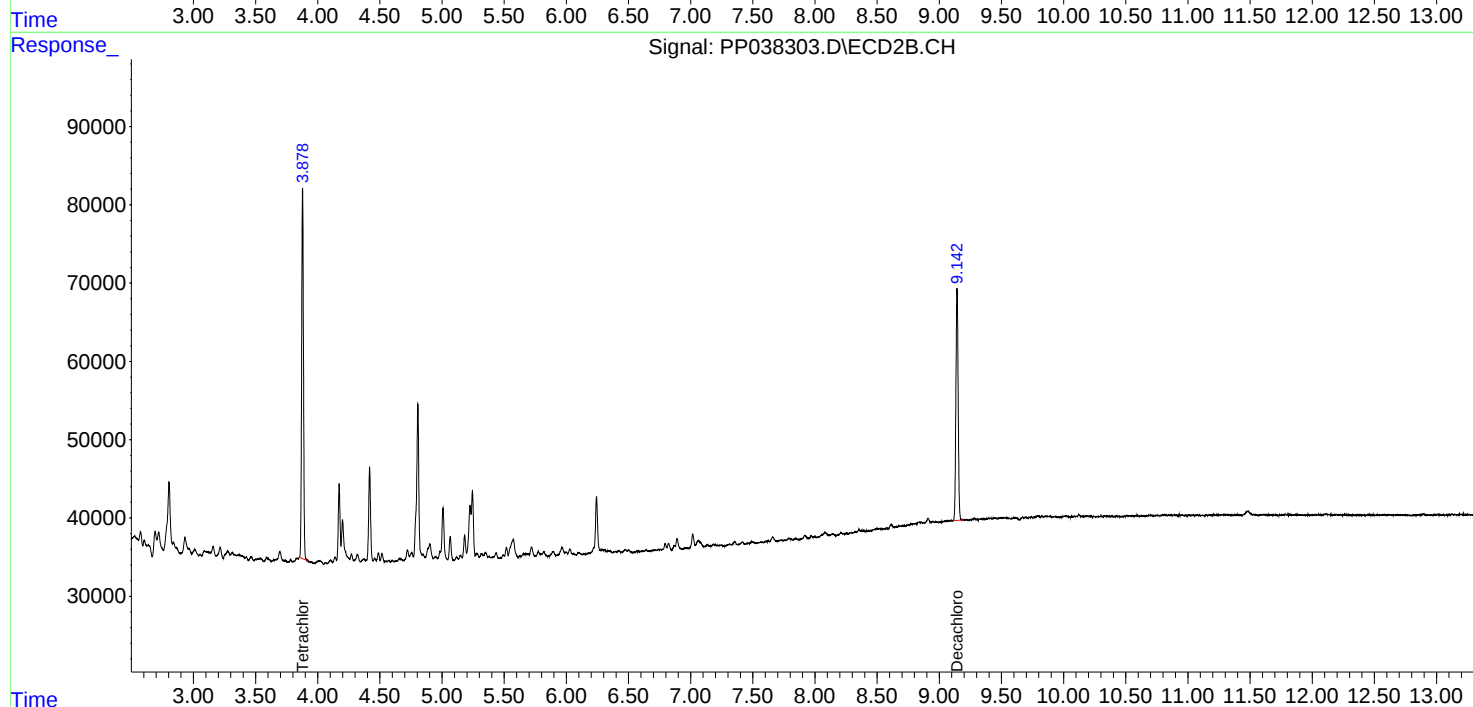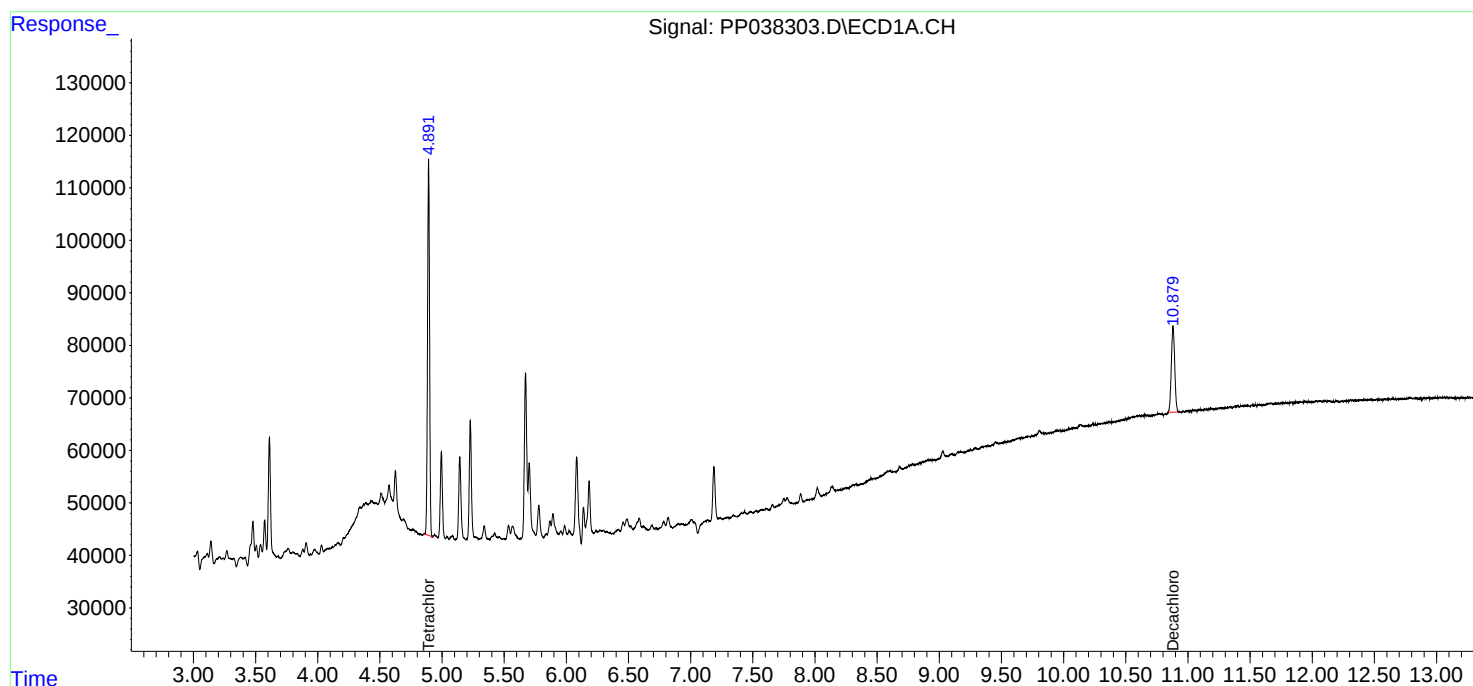


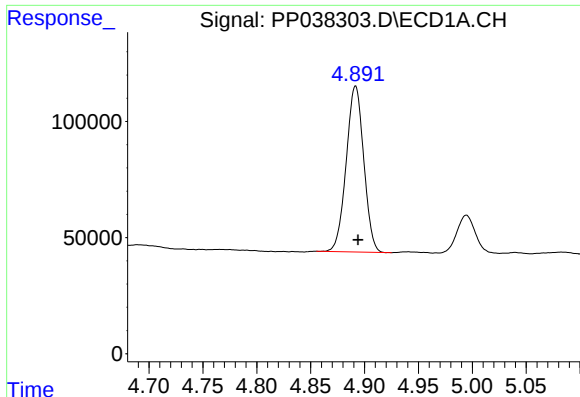

#1 Tetrachloro-m-xylene


R.T.: 4.892 min
Delta R.T.: -0.002 min
Response: 809233
Conc: 18.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
07-08-11

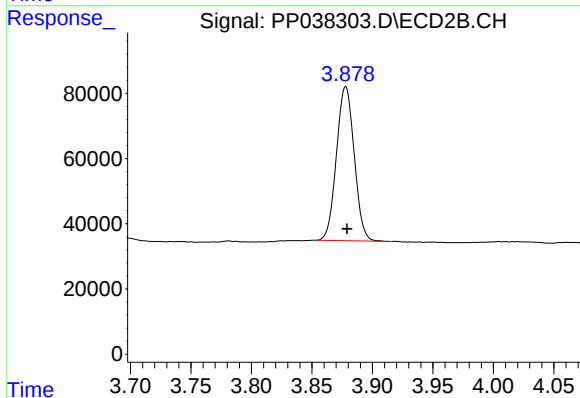


#1 Tetrachloro-m-xylene

R.T.: 3.878 min
Delta R.T.: 0.000 min
Response: 483190
Conc: 18.76 ng/ml

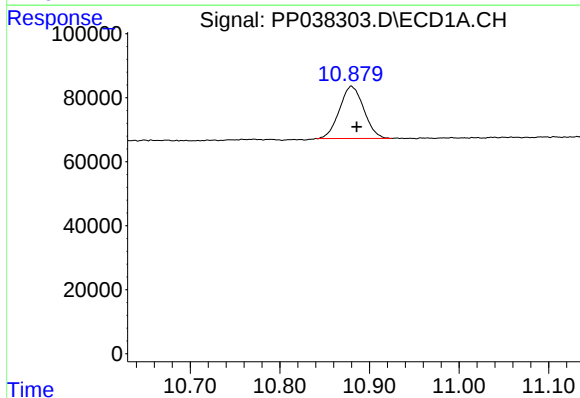

#2 Decachlorobiphenyl

R.T.: 10.880 min
Delta R.T.: -0.006 min
Response: 307379
Conc: 13.51 ng/ml

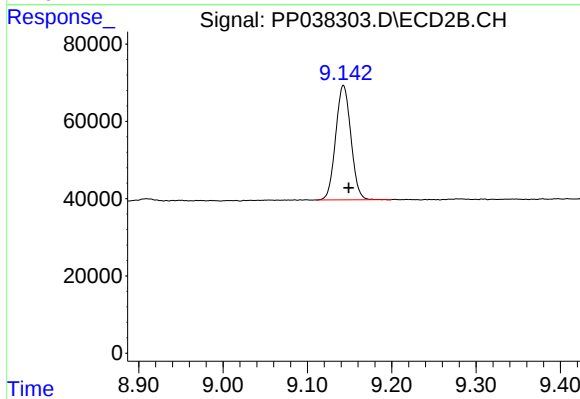

#2 Decachlorobiphenyl

R.T.: 9.143 min
Delta R.T.: -0.006 min
Response: 370802
Conc: 14.33 ng/ml