

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081221\
 Data File : PP038333.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Aug 2021 3:01
 Operator : AJ\MA
 Sample : M3385-01 10X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MAIN-BODY

Manual Integrations
 APPROVED

mohammad
 8/13/2021 10:07:12 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 07:05:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 06 03:08:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.890	3.878	77757	47236	1.750m	1.834
2) SA Decachlor...	10.880	9.140	64446	62898	2.833	2.431

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081221\
Data File : PP038333.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Aug 2021 3:01
Operator : AJ\MA
Sample : M3385-01 10X
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MAIN-BODY


Manual Integrations
APPROVED

mohammad
8/13/2021 10:07:12 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 07:05:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 06 03:08:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

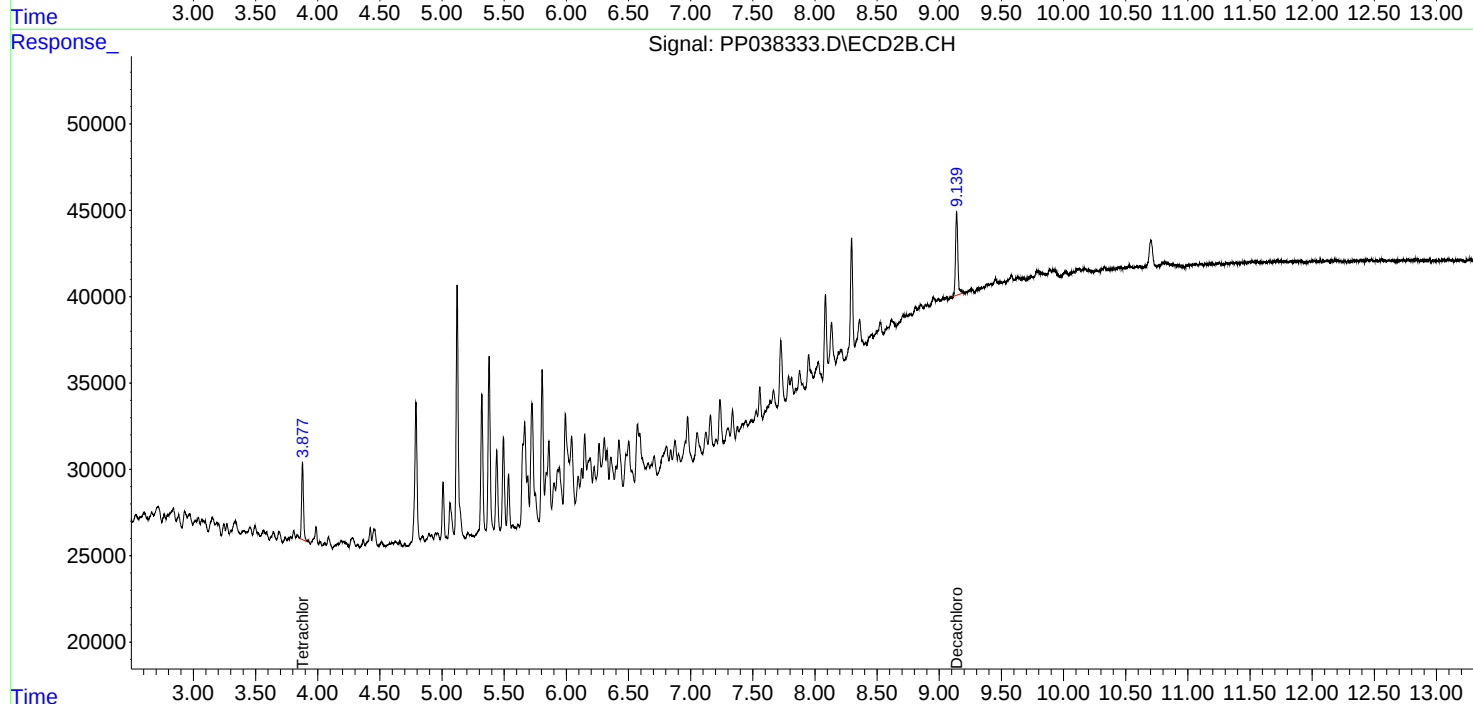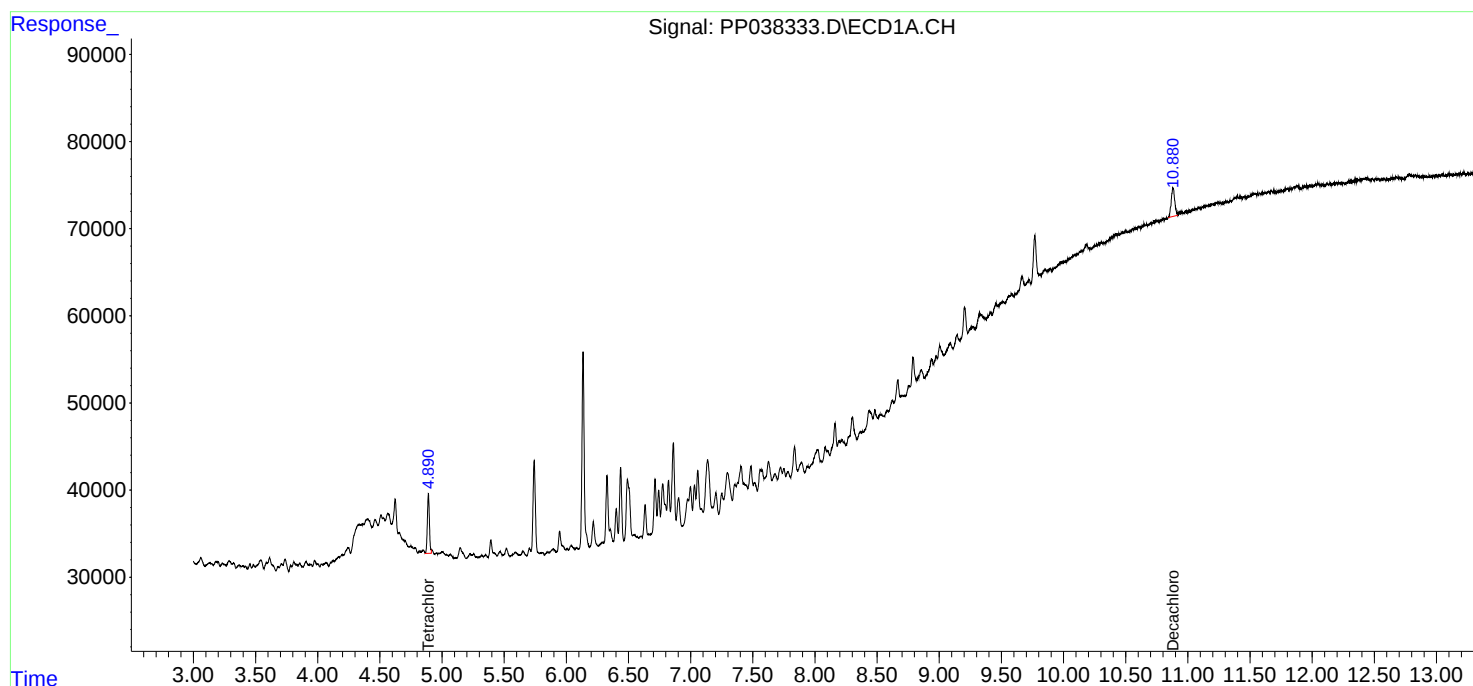

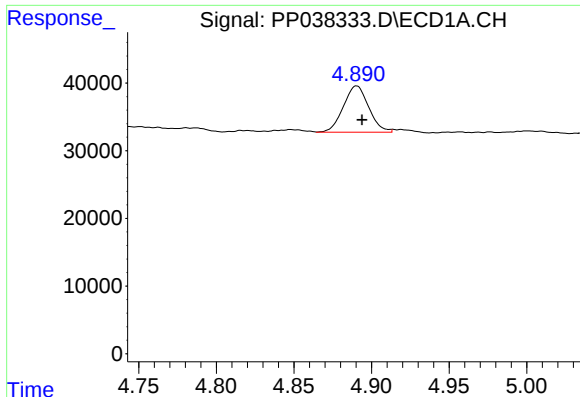


#1 Tetrachloro-m-xylene

R.T.: 4.890 min
Delta R.T.: -0.004 min
Response: 77757
Conc: 1.75 ng/ml m

Instrument :
ECD_P
ClientSampleId :
MAIN-BODY


Manual Integrations
APPROVED

mohammad
8/13/2021 10:07:12 AM

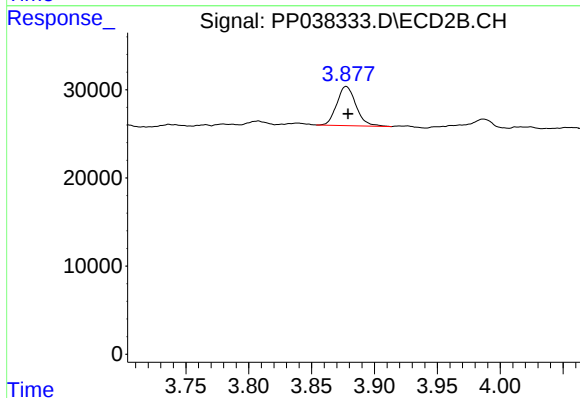


#1 Tetrachloro-m-xylene

R.T.: 3.878 min
Delta R.T.: -0.001 min
Response: 47236
Conc: 1.83 ng/ml

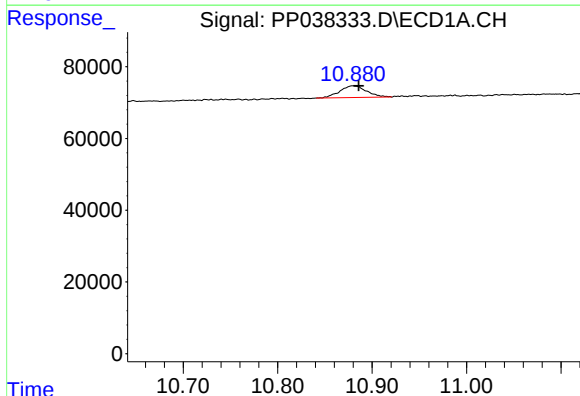

#2 Decachlorobiphenyl

R.T.: 10.880 min
Delta R.T.: -0.006 min
Response: 64446
Conc: 2.83 ng/ml

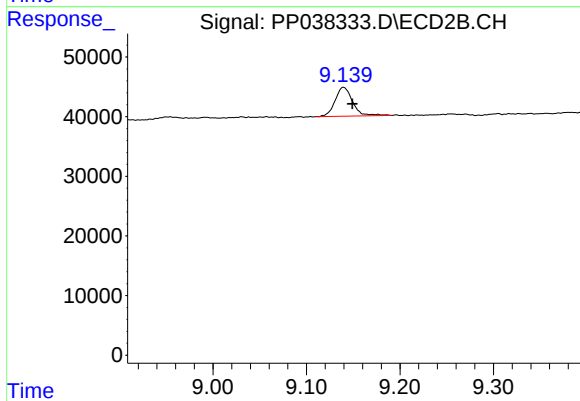

#2 Decachlorobiphenyl

R.T.: 9.140 min
Delta R.T.: -0.009 min
Response: 62898
Conc: 2.43 ng/ml