

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081222\
 Data File : PP050519.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2022 15:51
 Operator : YP\AJ
 Sample : N4153-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TR-04-081022

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/15/2022
 Supervised By :Ankita Jodhani 08/15/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 00:42:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 09 11:38:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.344	3.590	30858249	61646208	19.171m	19.681m
2) SA Decachlor...	10.095	8.556	30617968	27417259	17.388	17.814

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081222\
Data File : PP050519.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2022 15:51
Operator : YP\AJ
Sample : N4153-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TR-04-081022


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/15/2022
Supervised By :Ankita Jodhani 08/15/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 00:42:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 09 11:38:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

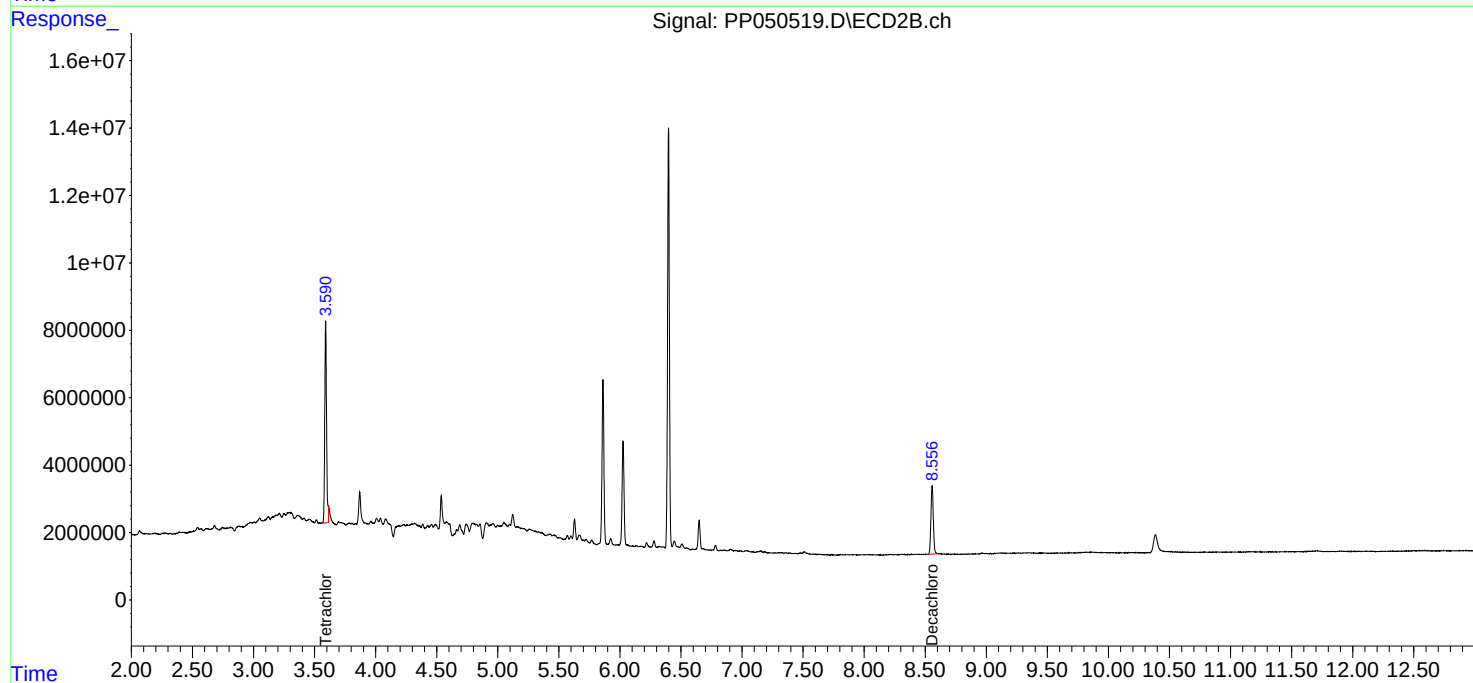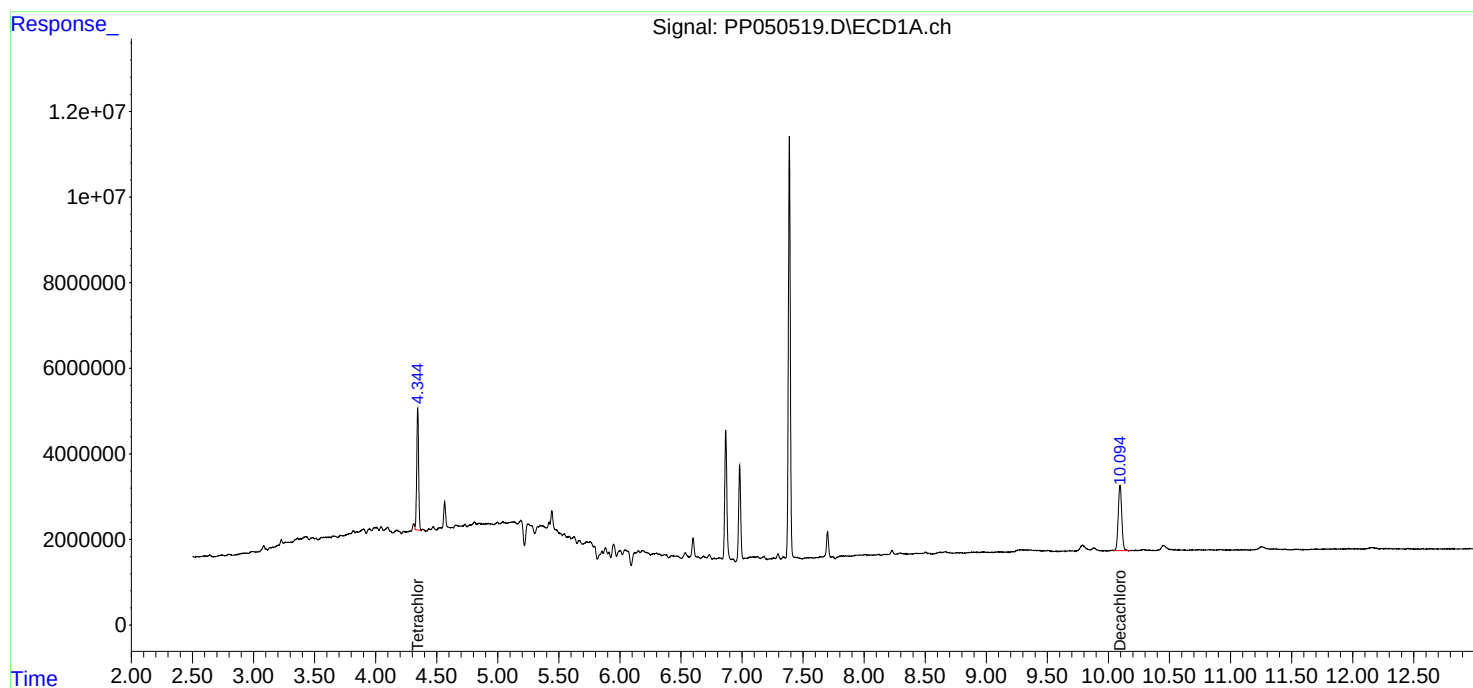

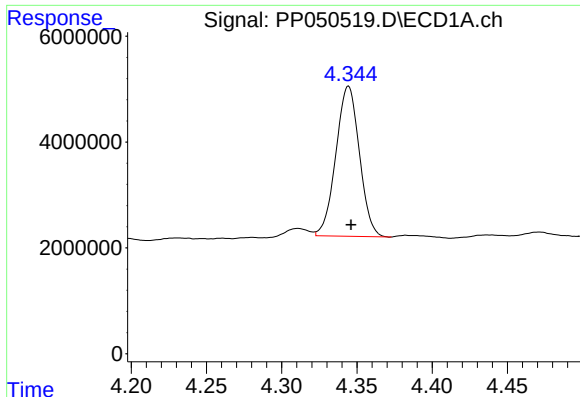


#1 Tetrachloro-m-xylene

R.T.: 4.344 min
Delta R.T.: -0.002 min
Response: 30858249
Conc: 19.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
TR-04-081022


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/15/2022
Supervised By :Ankita Jodhani 08/15/2022

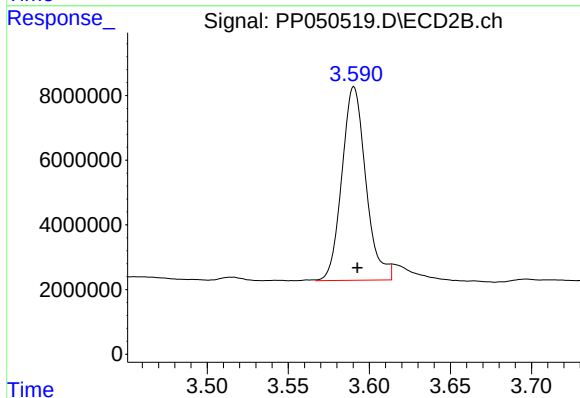


#1 Tetrachloro-m-xylene

R.T.: 3.590 min
Delta R.T.: -0.003 min
Response: 61646208
Conc: 19.68 ng/ml m

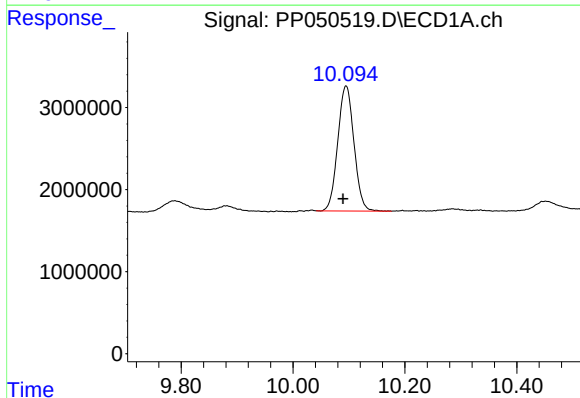

#2 Decachlorobiphenyl

R.T.: 10.095 min
Delta R.T.: 0.005 min
Response: 30617968
Conc: 17.39 ng/ml

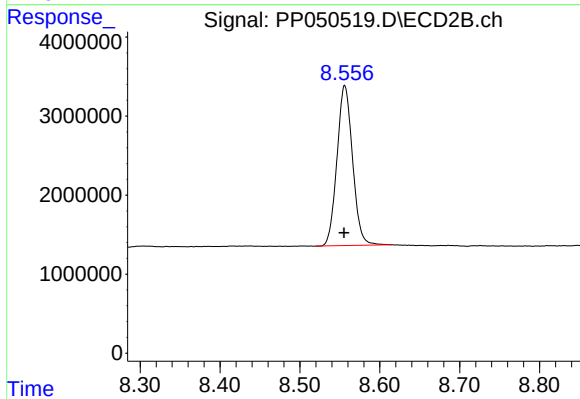

#2 Decachlorobiphenyl

R.T.: 8.556 min
Delta R.T.: 0.000 min
Response: 27417259
Conc: 17.81 ng/ml