

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081222\
 Data File : PP050545.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2022 02:00
 Operator : YP\AJ
 Sample : N4182-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-080222-HC-003

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 04:30:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 09 11:38:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.343	3.590	31094677	59505567	19.318	18.998
2) SA Decachlor...	10.087	8.551	30054840	28211806	17.068	18.330

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081222\
Data File : PP050545.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2022 02:00
Operator : YP\AJ
Sample : N4182-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PCB-080222-HC-003

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 04:30:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 09 11:38:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

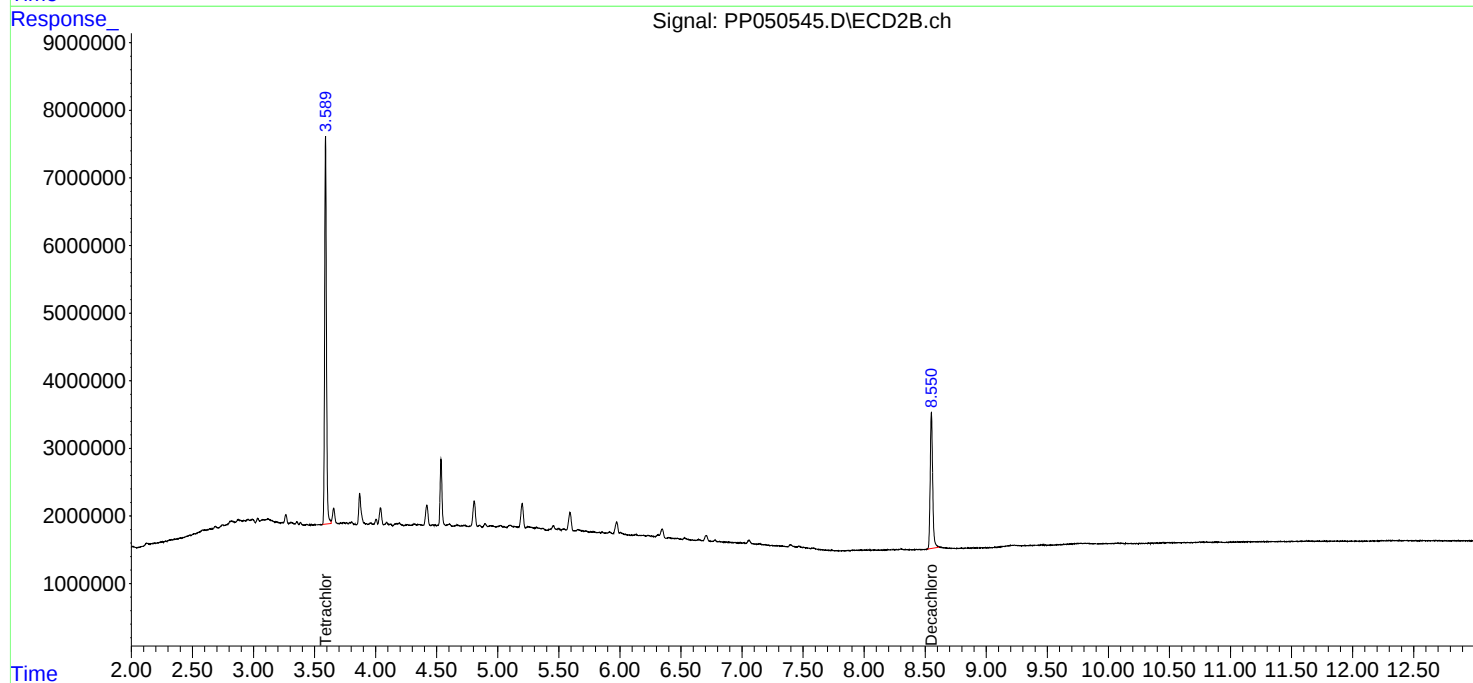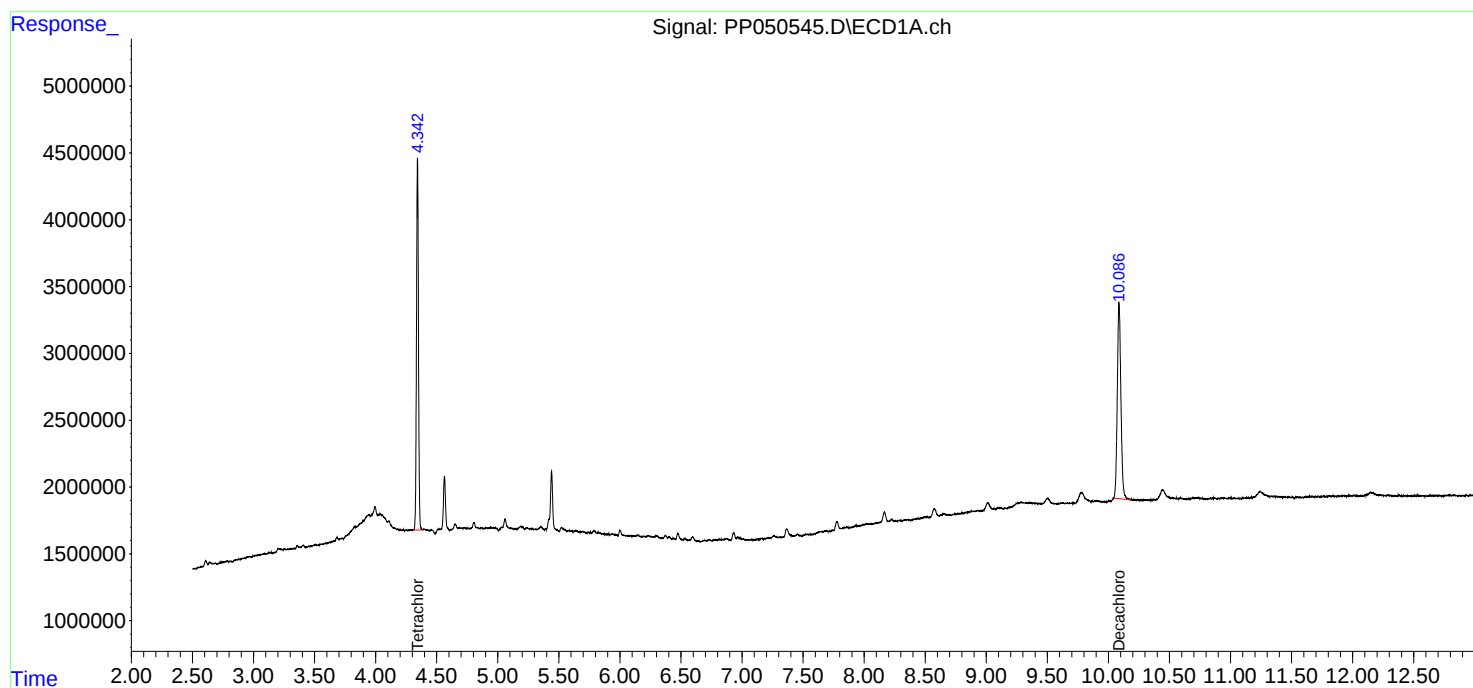


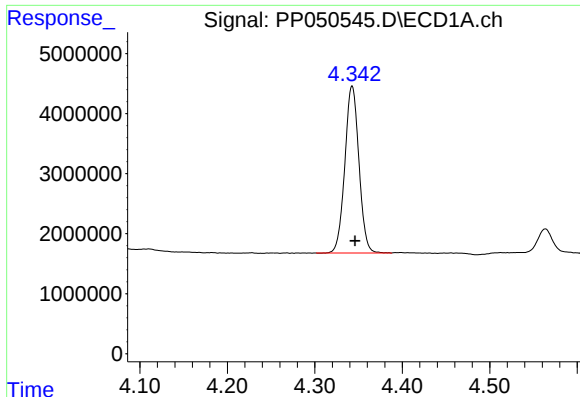

#1 Tetrachloro-m-xylene


R.T.: 4.343 min
Delta R.T.: -0.003 min
Response: 31094677
Conc: 19.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-080222-HC-003

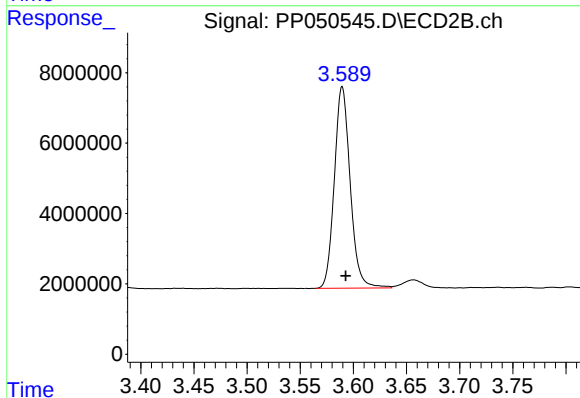


#1 Tetrachloro-m-xylene

R.T.: 3.590 min
Delta R.T.: -0.003 min
Response: 59505567
Conc: 19.00 ng/ml

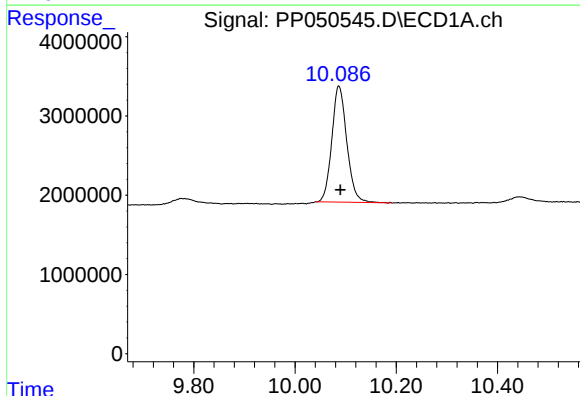

#2 Decachlorobiphenyl

R.T.: 10.087 min
Delta R.T.: -0.003 min
Response: 30054840
Conc: 17.07 ng/ml

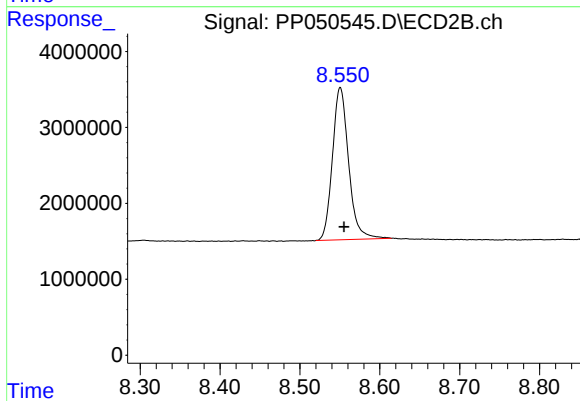

#2 Decachlorobiphenyl

R.T.: 8.551 min
Delta R.T.: -0.005 min
Response: 28211806
Conc: 18.33 ng/ml