

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081222\
 Data File : PP050550.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2022 03:23
 Operator : YP\AJ
 Sample : N4182-08
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-080222-HC-008

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/15/2022
 Supervised By :Ankita Jodhani 08/15/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 04:38:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 09 11:38:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.563f	3.868f	7334179	8617946	4.556m	2.751m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081222\
Data File : PP050550.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2022 03:23
Operator : YP\AJ
Sample : N4182-08
Misc :
ALS Vial : 33 Sample Multiplier: 1


Instrument :
ECD_P
ClientSampleId :
PCB-080222-HC-008


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/15/2022
Supervised By :Ankita Jodhani 08/15/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 04:38:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 09 11:38:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

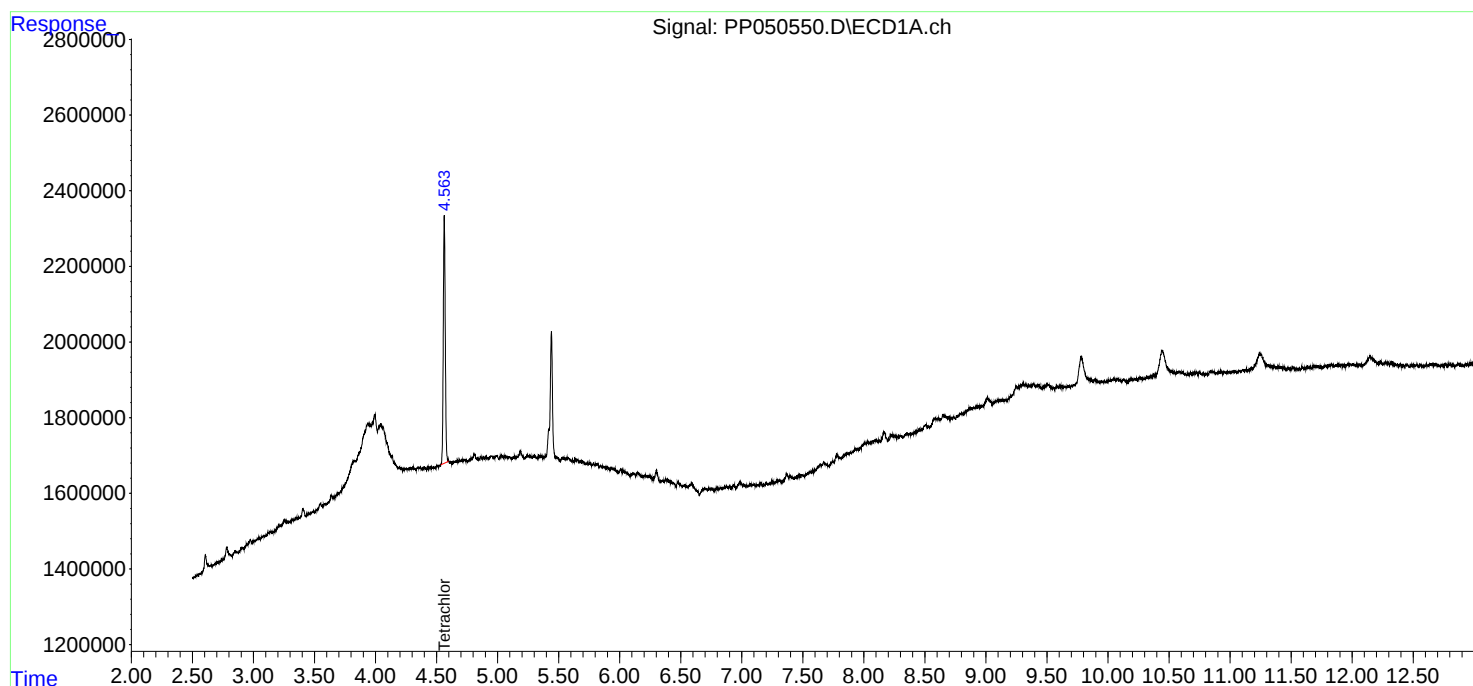

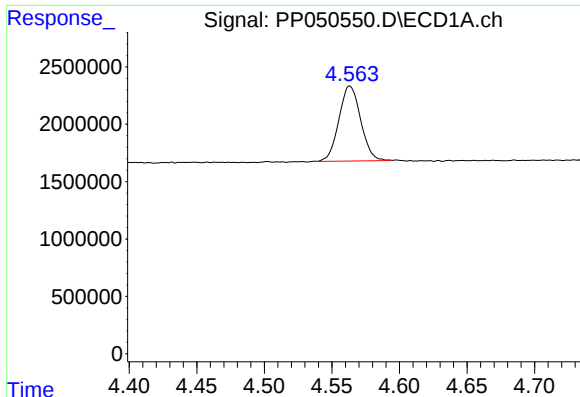


#1 Tetrachloro-m-xylene

R.T.: 4.563 min
Delta R.T.: 0.217 min
Response: 7334179
Conc: 4.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-080222-HC-008


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/15/2022
Supervised By :Ankita Jodhani 08/15/2022

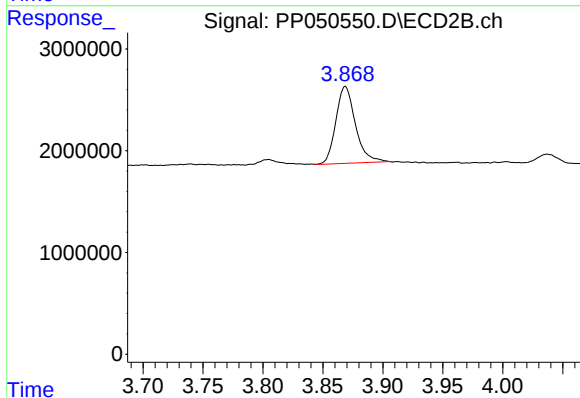


#1 Tetrachloro-m-xylene

R.T.: 3.868 min
Delta R.T.: 0.276 min
Response: 8617946
Conc: 2.75 ng/ml m

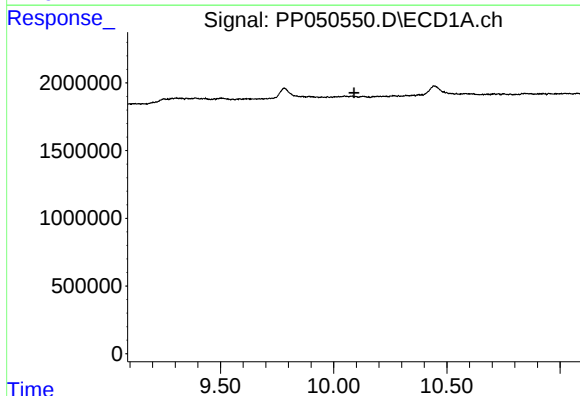

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.090 min
Response: 0
Conc: N.D.

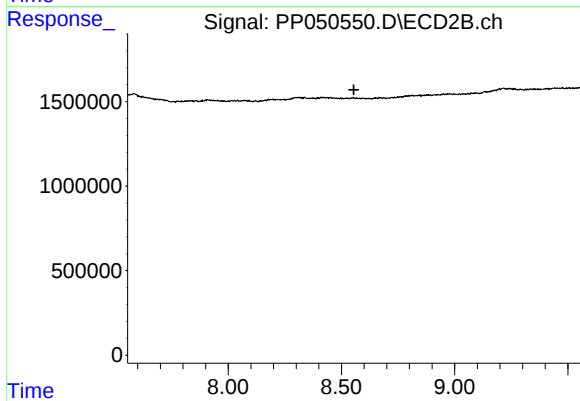

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.555 min
Response: 0
Conc: N.D.