

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP081225\  
 Data File : PP074306.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 12 Aug 2025 10:59  
 Operator : YP\AJ  
 Sample : DDT ANALOG  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 DDT ANALOG

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Aug 12 11:31:58 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP080125.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Mon Aug 04 11:01:49 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

#### System Monitoring Compounds

| Target Compounds |           |       |       |         |          |                     |
|------------------|-----------|-------|-------|---------|----------|---------------------|
| 30) L6           | AR-1254-5 | 7.951 | 6.878 | 438.2E6 | 2933.3E6 | 5400.260 7615.773 # |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP081225\  
Data File : PP074306.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 12 Aug 2025 10:59  
Operator : YP\AJ  
Sample : DDT ANALOG  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
DDT ANALOG

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Aug 12 11:31:58 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP080125.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Mon Aug 04 11:01:49 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

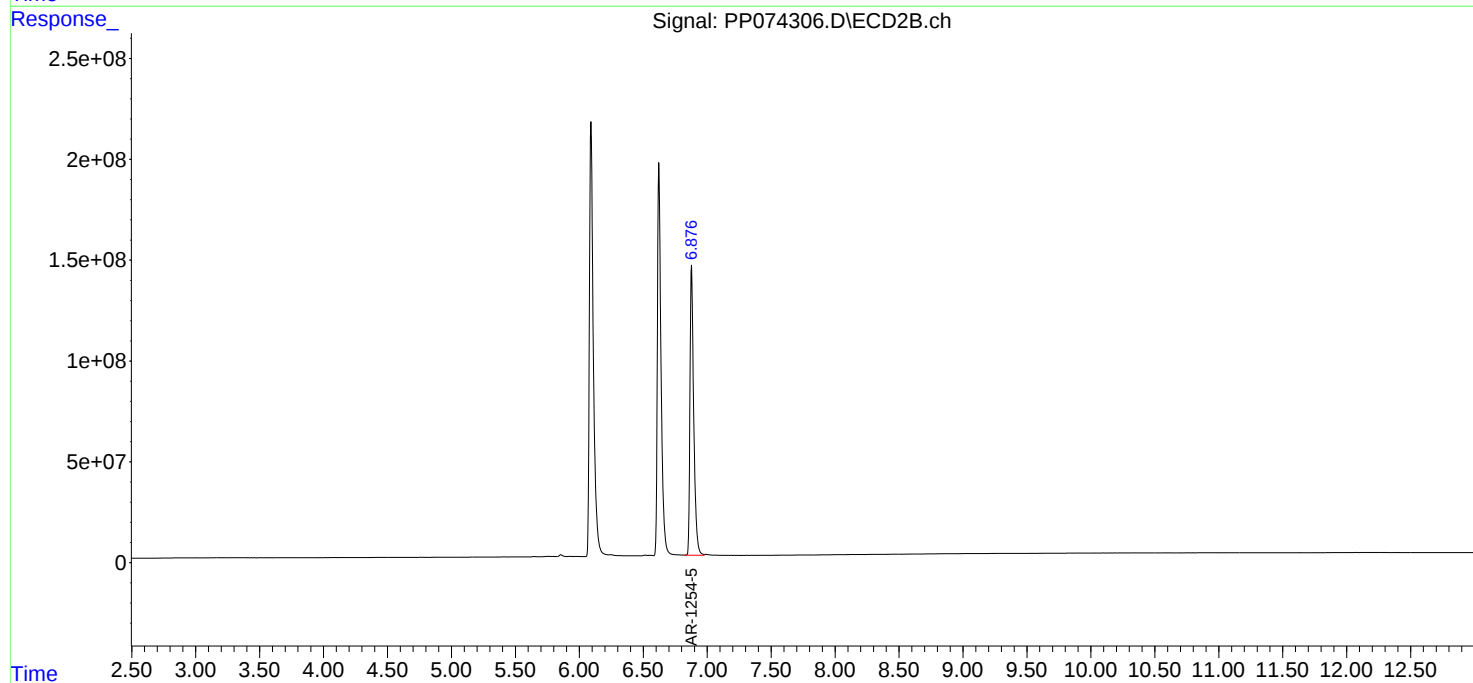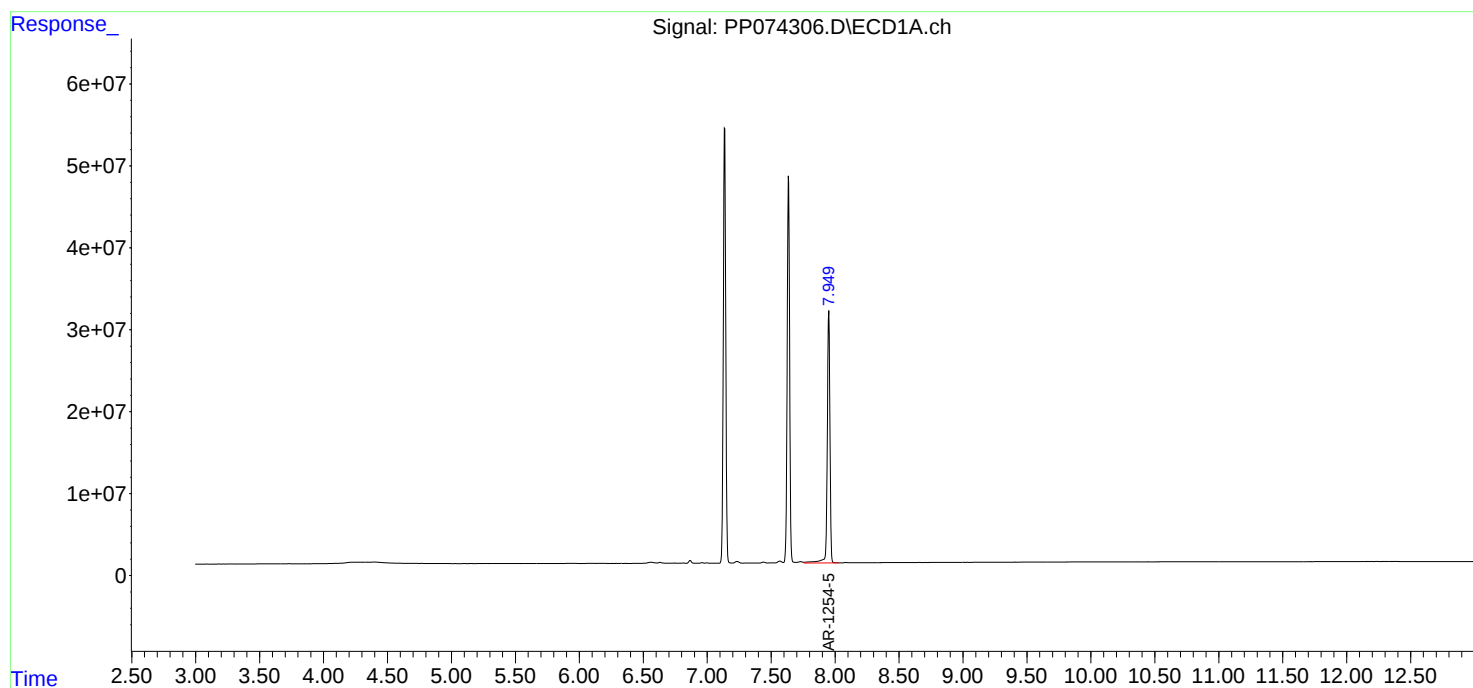


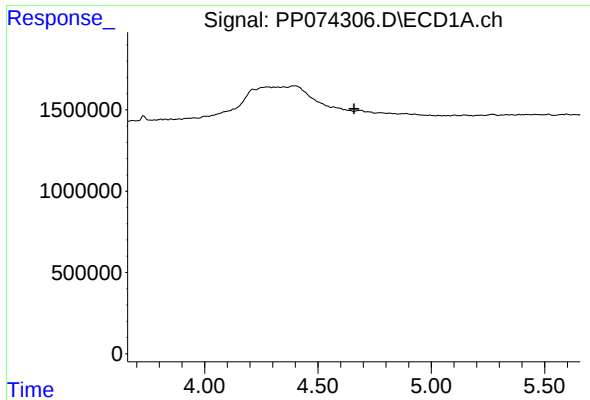

#1 Tetrachloro-m-xylene


R.T.: 0.000 min  
Exp R.T. : 4.660 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
DDT ANALOG

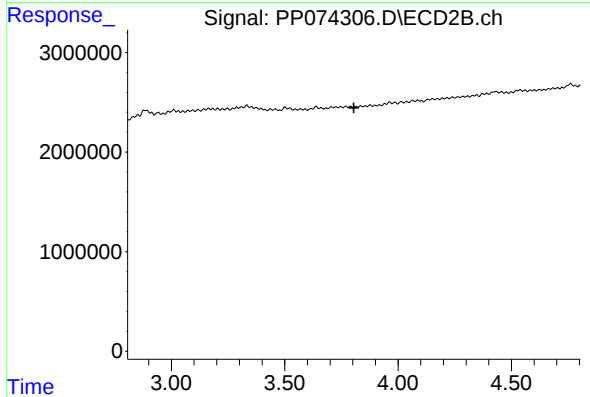


#1 Tetrachloro-m-xylene

R.T.: 0.000 min  
Exp R.T. : 3.805 min  
Response: 0  
Conc: N.D.

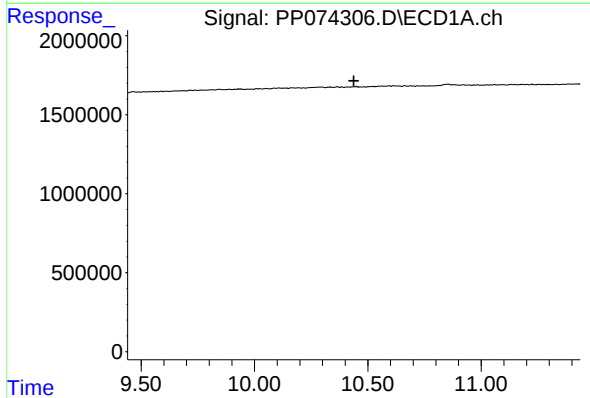


#2 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 10.438 min  
Response: 0  
Conc: N.D.

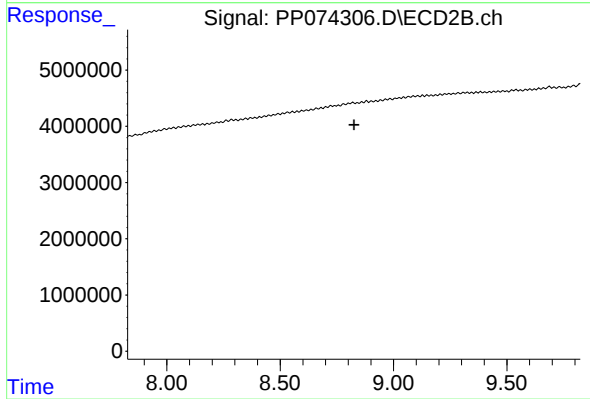

#2 Decachlorobiphenyl


R.T.: 0.000 min  
Exp R.T. : 8.826 min  
Response: 0  
Conc: N.D.

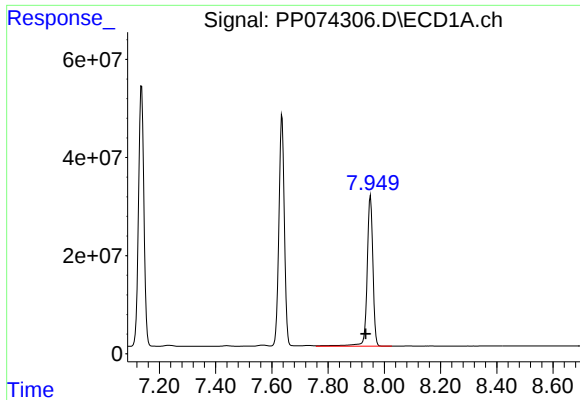

#30 AR-1254-5

R.T.: 7.951 min  
Delta R.T.: 0.016 min  
Response: 438202816  
Conc: 5400.26 ng/m

Instrument :  
ECD\_P  
ClientSampleId :  
DDT ANALOG

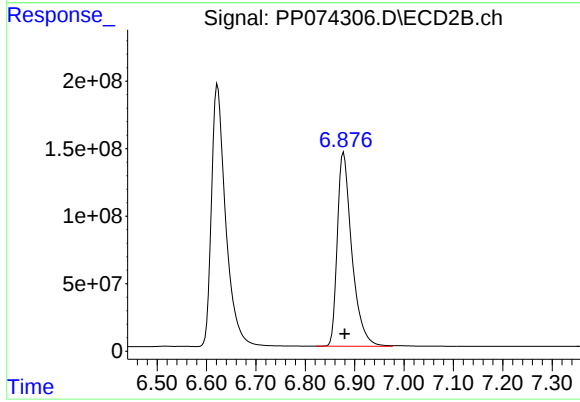

#30 AR-1254-5

R.T.: 6.878 min  
Delta R.T.: -0.002 min  
Response: 2933345331  
Conc: 7615.77 ng/ml