

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
 Data File : PP074326.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 19:03
 Operator : YP\AJ
 Sample : Q2839-14 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC226751-2-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/13/2025
 Supervised By :mohammad ahmed 08/14/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 01:56:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.655	3.799	1737288	3631395	1.554m	0.947m#
2) SA Decachlor...	10.433	8.820	1752821	6626511	1.805m	1.102 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
Data File : PP074326.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2025 19:03
Operator : YP\AJ
Sample : Q2839-14 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC226751-2-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 01:56:20 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Aug 04 11:01:49 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

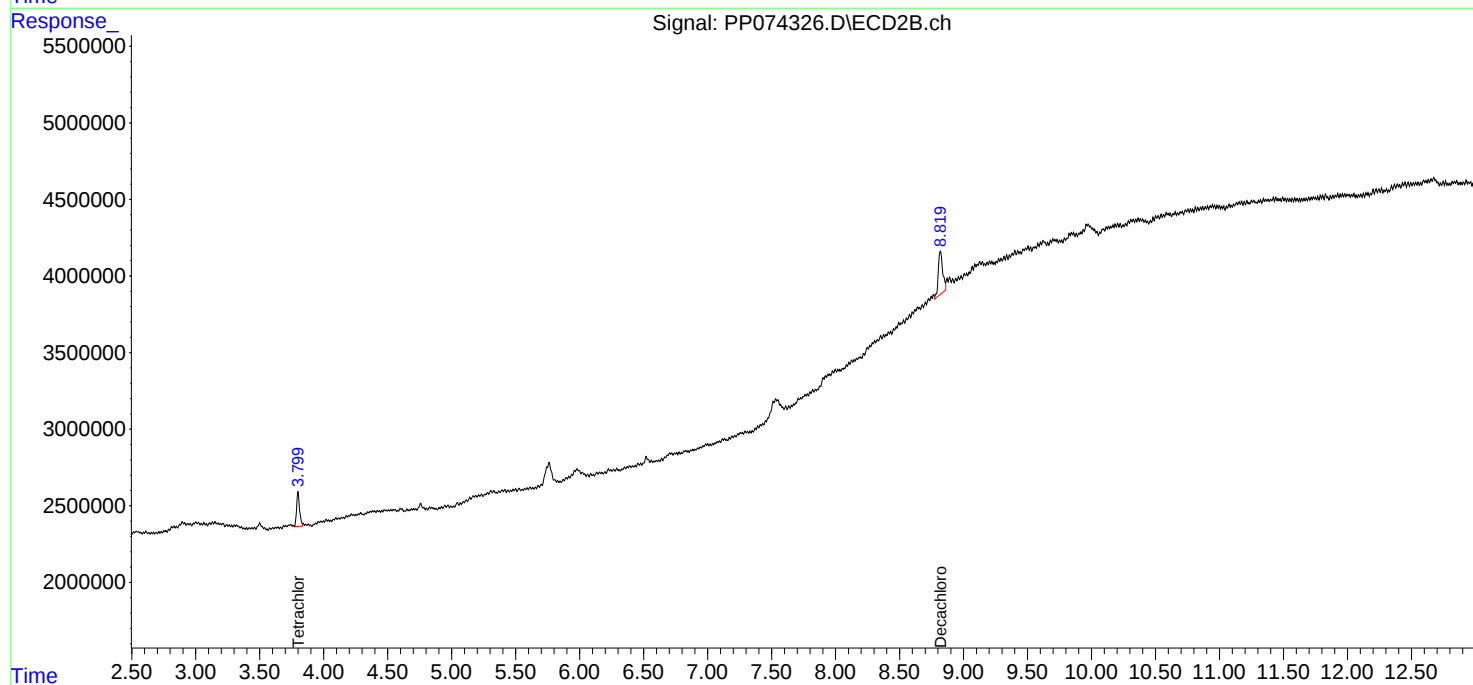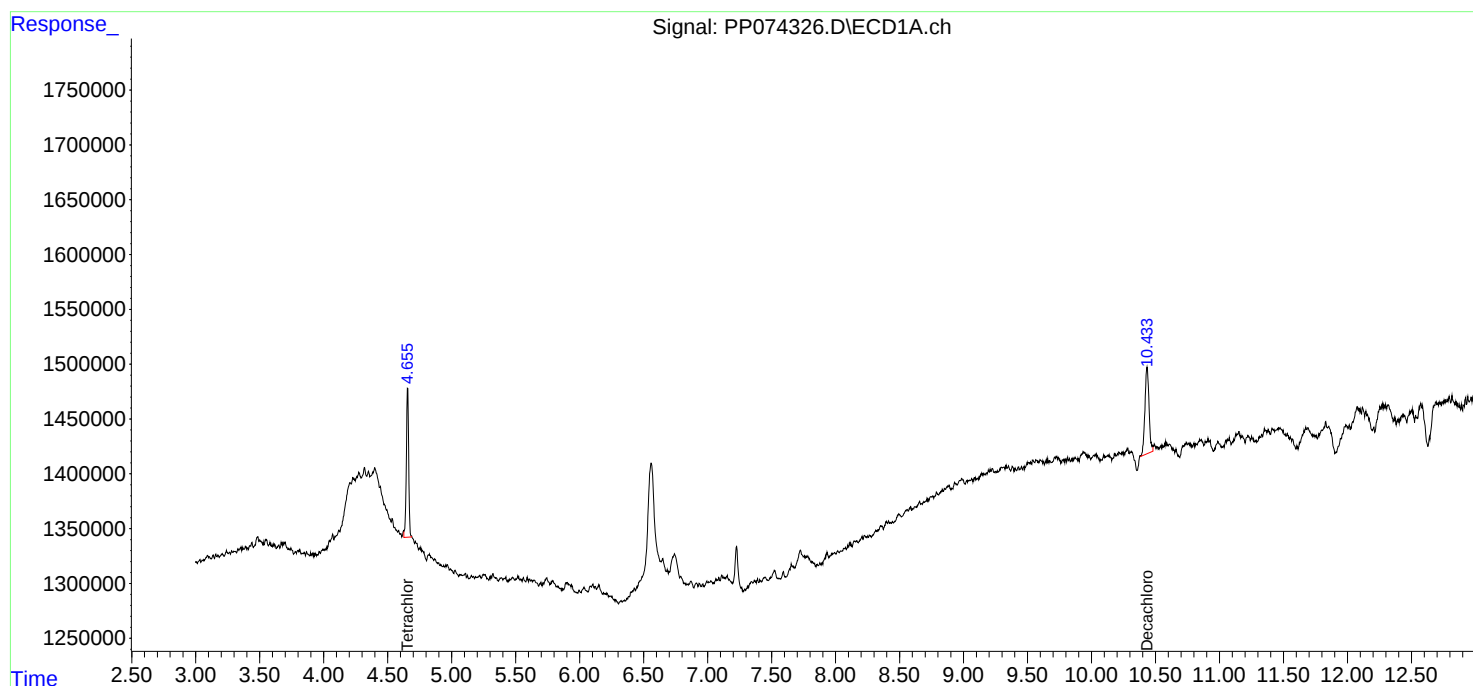

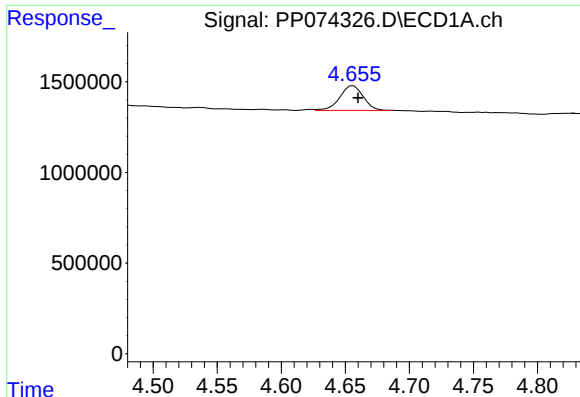


#1 Tetrachloro-m-xylene

R.T.: 4.655 min
Delta R.T.: -0.005 min
Response: 1737288
Conc: 1.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC226751-2-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

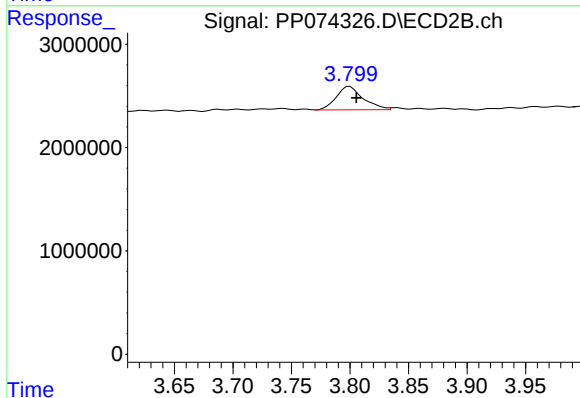


#1 Tetrachloro-m-xylene

R.T.: 3.799 min
Delta R.T.: -0.007 min
Response: 3631395
Conc: 0.95 ng/ml m

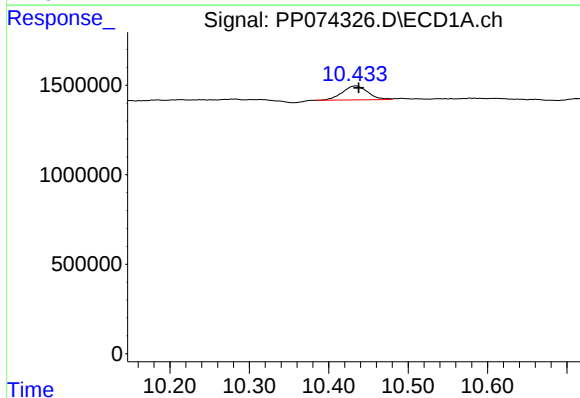

#2 Decachlorobiphenyl

R.T.: 10.433 min
Delta R.T.: -0.005 min
Response: 1752821
Conc: 1.80 ng/ml m

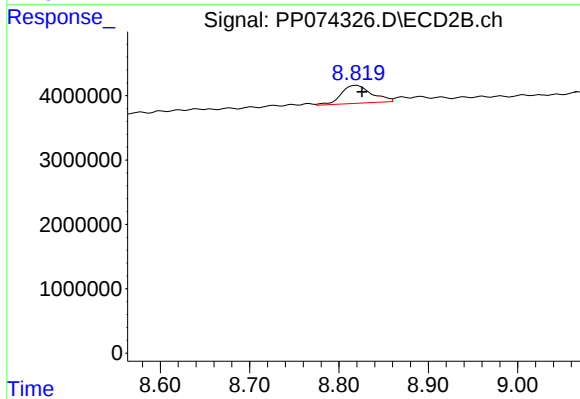

#2 Decachlorobiphenyl

R.T.: 8.820 min
Delta R.T.: -0.006 min
Response: 6626511
Conc: 1.10 ng/ml