

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
 Data File : PP074328.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 19:36
 Operator : YP\AJ
 Sample : Q2839-16 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 JEC773V-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/13/2025
 Supervised By :mohammad ahmed 08/14/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 01:56:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.660	3.804	2023362	4667979	1.809m	1.217 #
2) SA Decachlor...	10.439	8.823	1954328	9110112	2.012m	1.515

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
Data File : PP074328.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2025 19:36
Operator : YP\AJ
Sample : Q2839-16 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
JEC773V-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 01:56:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Aug 04 11:01:49 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

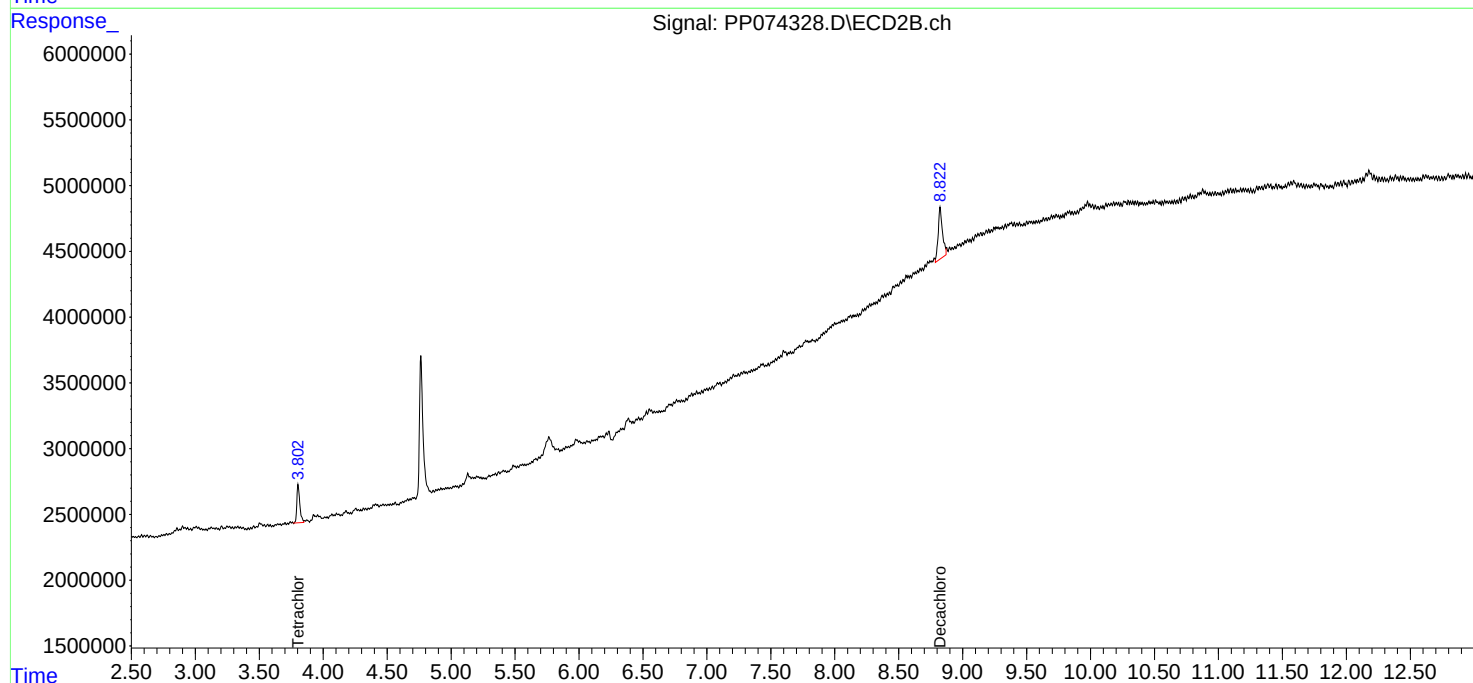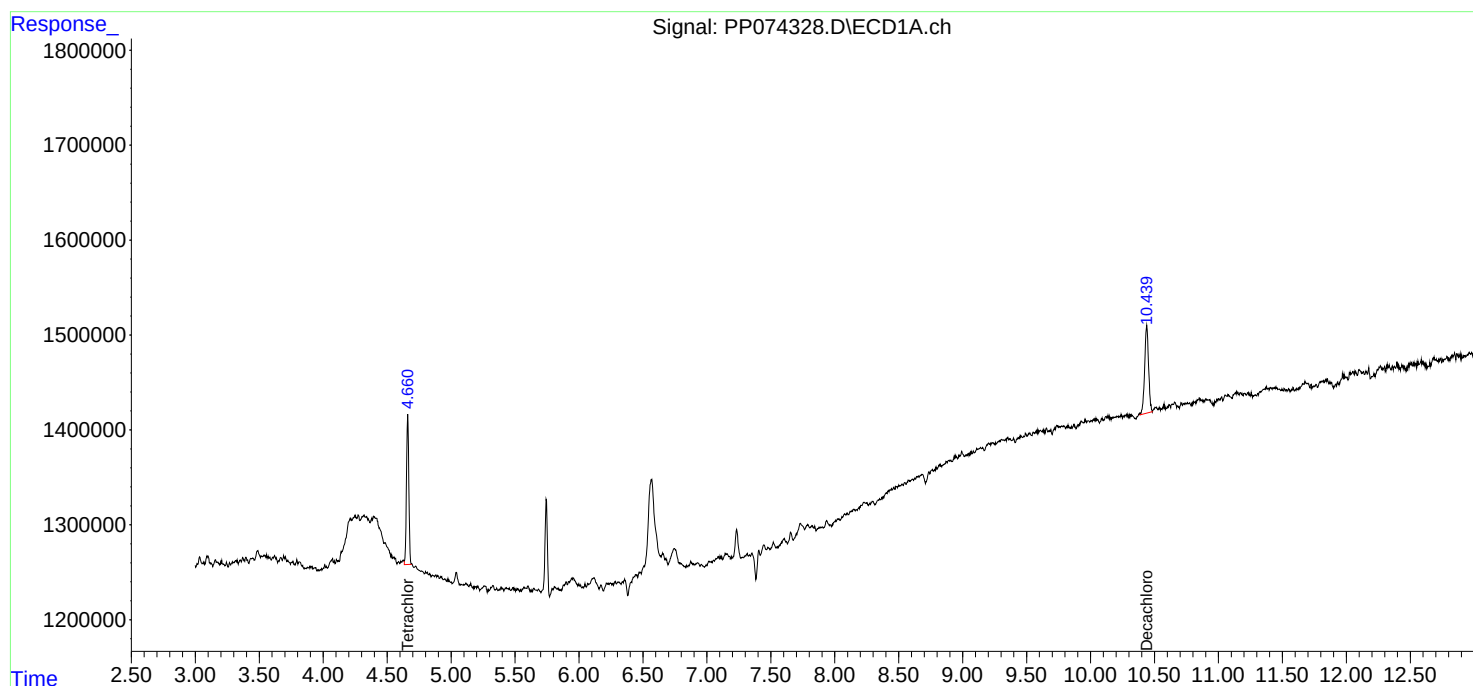

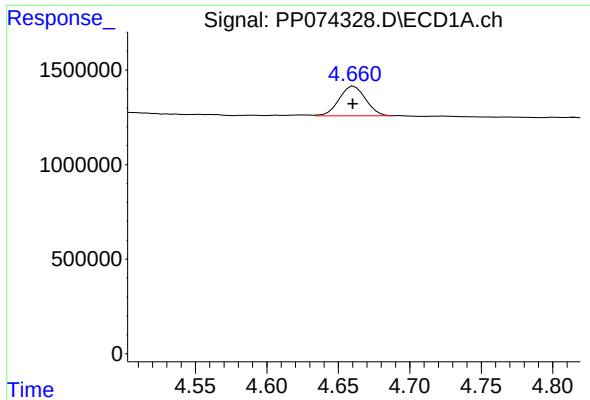


#1 Tetrachloro-m-xylene

R.T.: 4.660 min
Delta R.T.: 0.000 min
Response: 2023362
Conc: 1.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
JEC773V-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

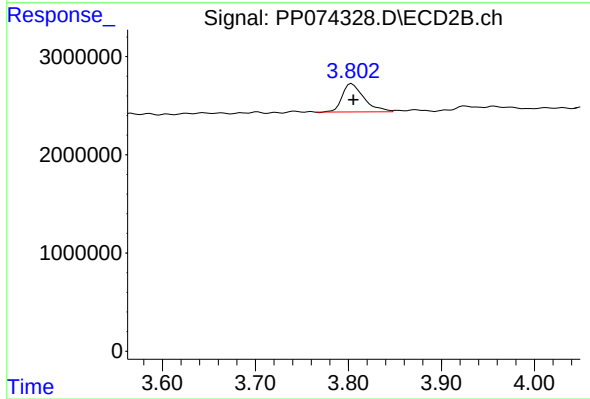


#1 Tetrachloro-m-xylene

R.T.: 3.804 min
Delta R.T.: -0.002 min
Response: 4667979
Conc: 1.22 ng/ml

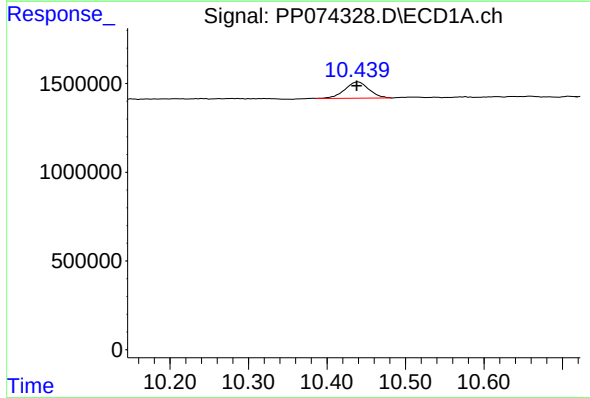

#2 Decachlorobiphenyl

R.T.: 10.439 min
Delta R.T.: 0.000 min
Response: 1954328
Conc: 2.01 ng/ml m

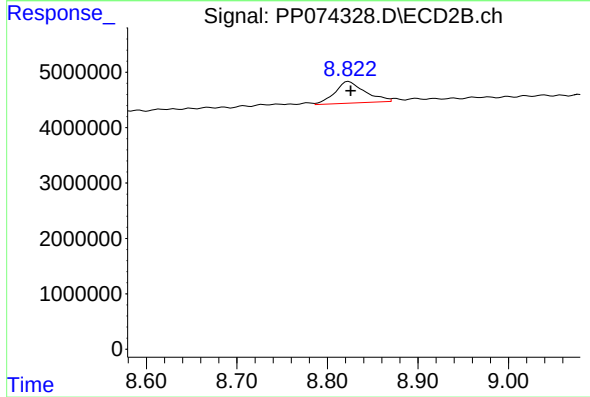

#2 Decachlorobiphenyl

R.T.: 8.823 min
Delta R.T.: -0.002 min
Response: 9110112
Conc: 1.51 ng/ml