

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081321\
 Data File : PP038373.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Aug 2021 17:58
 Operator : AJ\MA
 Sample : M3389-06
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CRT-18

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 01:22:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 06 03:08:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.890	3.876	903823	537149	20.338	20.856
2)	SA Decachlor...	10.880	9.140	543939	576341	23.911	22.276
Target Compounds							
8)	L2 AR-1221-1	5.142	0.000	147283	0	271.720	N.D. #
24)	L5 AR-1248-4	7.135f	0.000	154946	0	114.763	N.D. #
26)	L6 AR-1254-1	7.135	0.000	154946	0	118.914	N.D. #
28)	L6 AR-1254-3	7.747	0.000	13057	0	6.581	N.D. #
30)	L6 AR-1254-5	8.454	0.000	187631	0	129.111	N.D. #
32)	L7 AR-1260-2	8.159	0.000	15486	0	8.995	N.D. #
35)	L7 AR-1260-5	9.084	0.000	34775	0	13.098	N.D. #
37)	L8 AR-1262-2	9.084	0.000	34775	0	12.236	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081321\
Data File : PP038373.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Aug 2021 17:58
Operator : AJ\MA
Sample : M3389-06
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
CRT-18

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 01:22:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 06 03:08:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

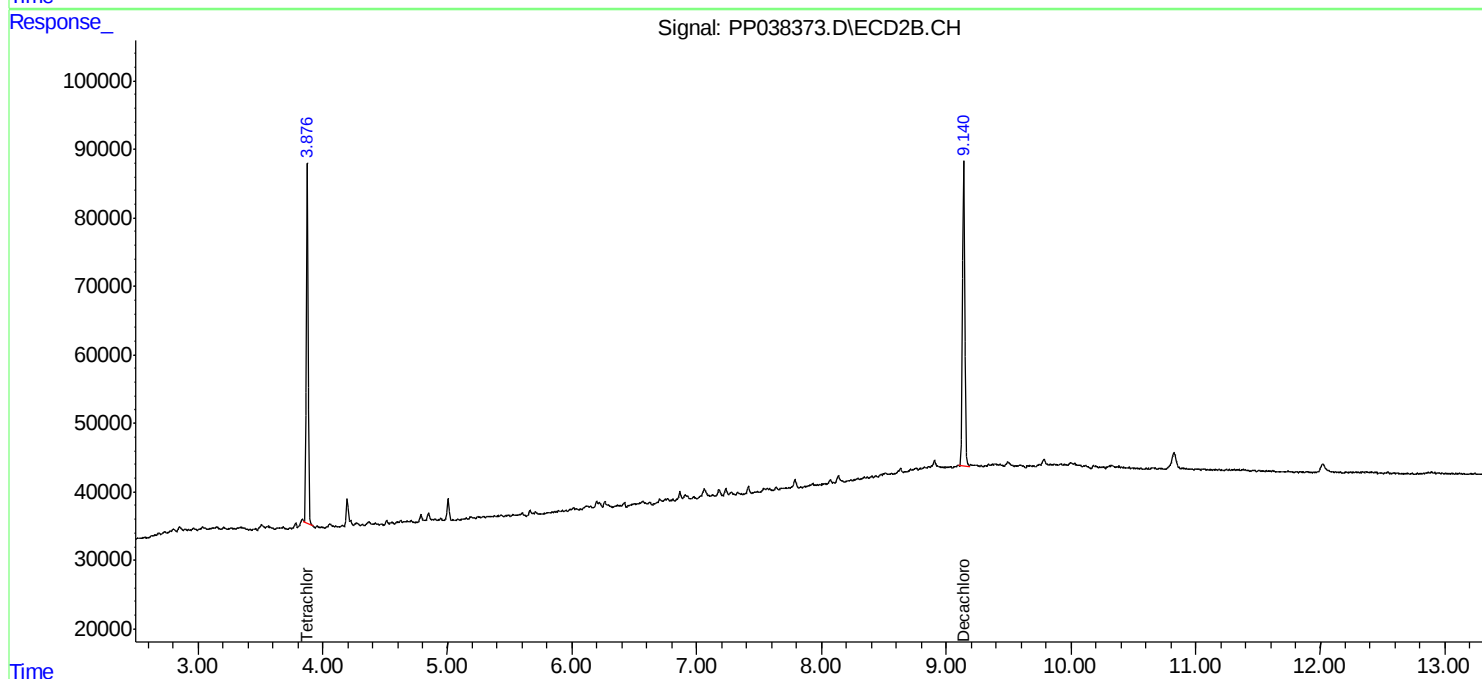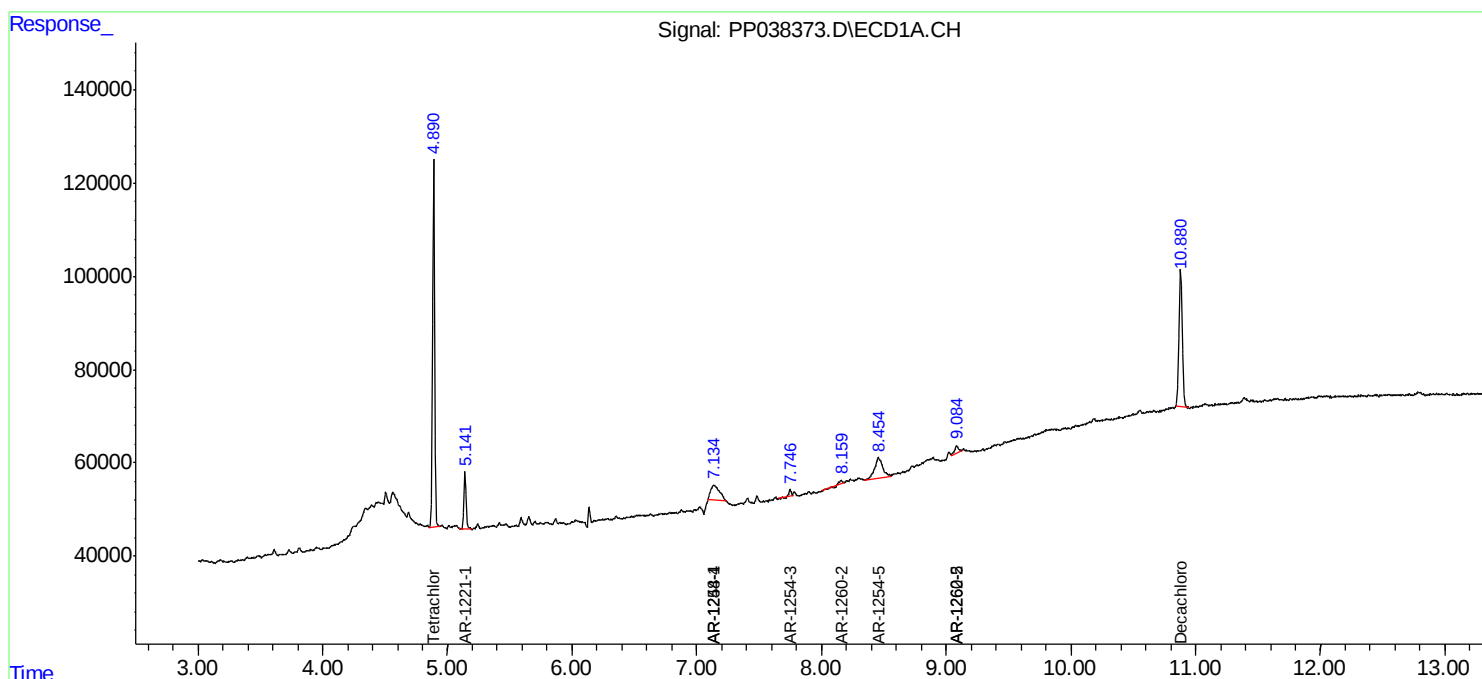


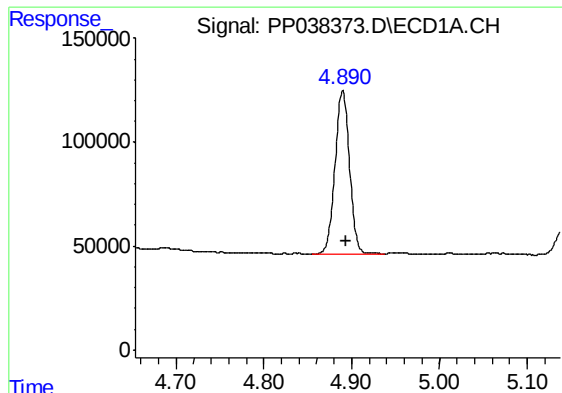

#1 Tetrachloro-m-xylene


R.T.: 4.890 min
Delta R.T.: -0.004 min
Response: 903823
Conc: 20.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
CRT-18

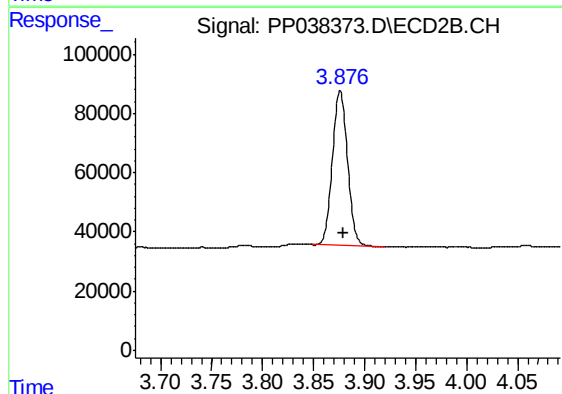


#1 Tetrachloro-m-xylene

R.T.: 3.876 min
Delta R.T.: -0.003 min
Response: 537149
Conc: 20.86 ng/ml

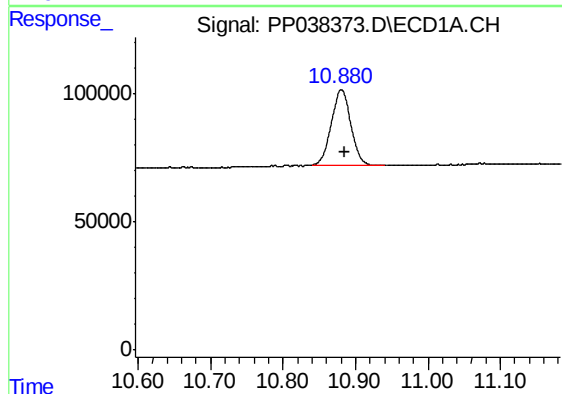


#2 Decachlorobiphenyl

R.T.: 10.880 min
Delta R.T.: -0.005 min
Response: 543939
Conc: 23.91 ng/ml

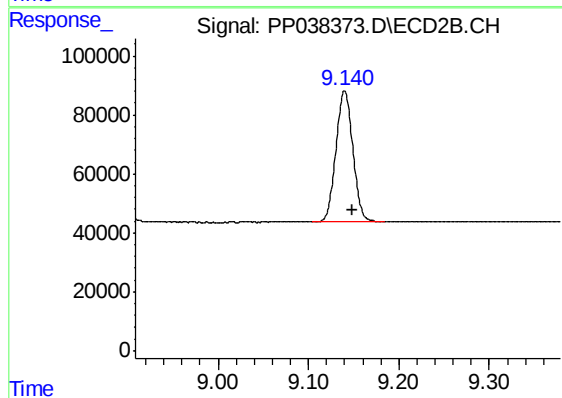

#2 Decachlorobiphenyl


R.T.: 9.140 min
Delta R.T.: -0.009 min
Response: 576341
Conc: 22.28 ng/ml

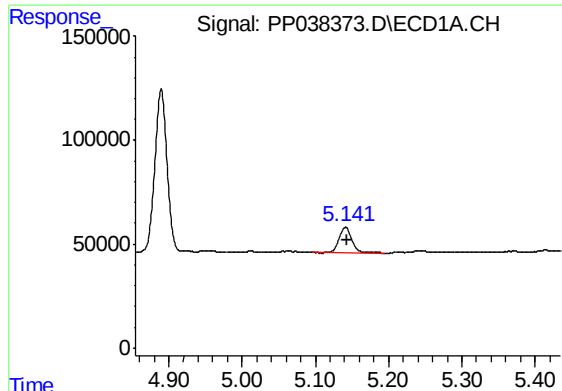

#8 AR-1221-1


R.T.: 5.142 min
Delta R.T.: -0.002 min
Response: 147283
Conc: 271.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
CRT-18

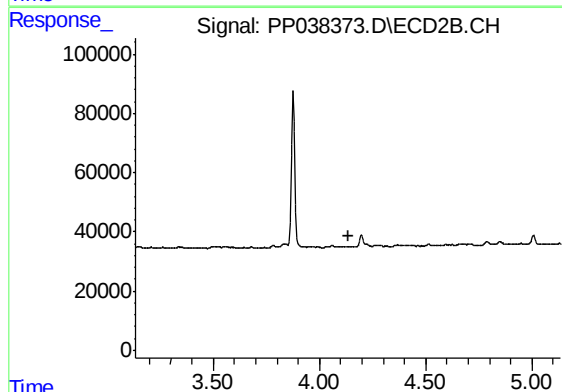


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.134 min
Response: 0
Conc: N.D.

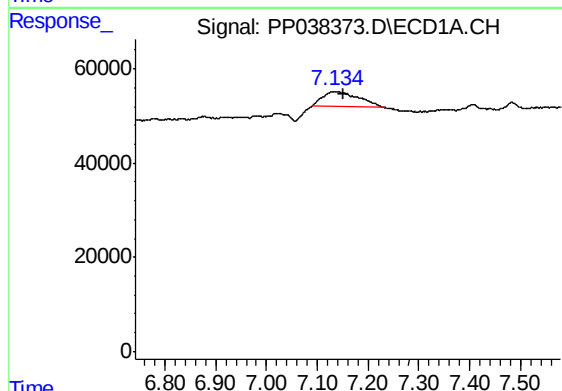


#24 AR-1248-4

R.T.: 7.135 min
Delta R.T.: -0.016 min
Response: 154946
Conc: 114.76 ng/ml

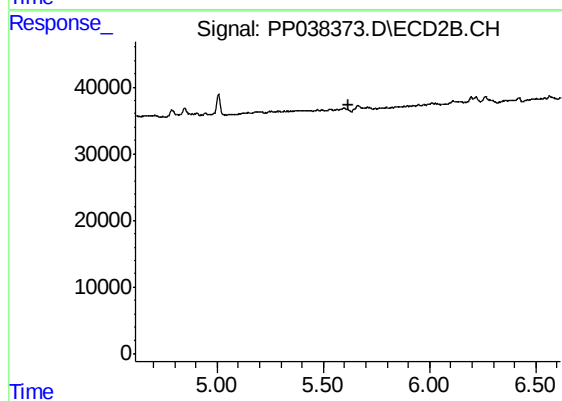

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.616 min
Response: 0
Conc: N.D.

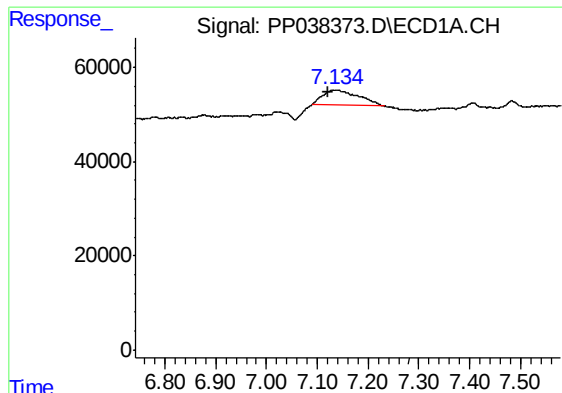

#26 AR-1254-1


R.T.: 7.135 min
Delta R.T.: 0.014 min
Response: 154946
Conc: 118.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
CRT-18

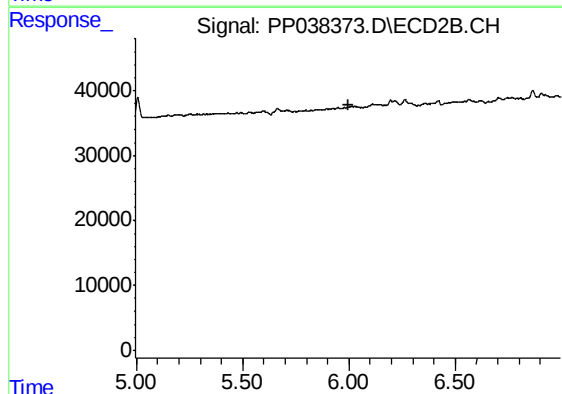


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 5.995 min
Response: 0
Conc: N.D.

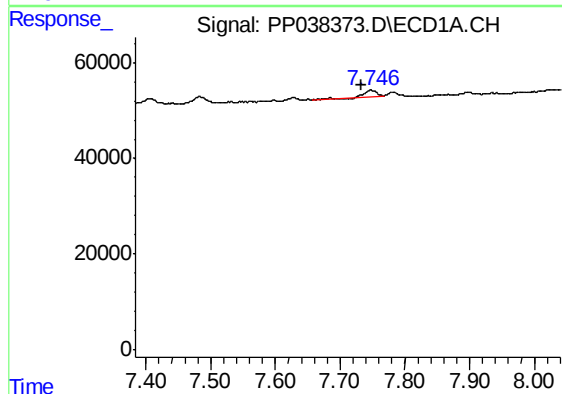


#28 AR-1254-3

R.T.: 7.747 min
Delta R.T.: 0.014 min
Response: 13057
Conc: 6.58 ng/ml

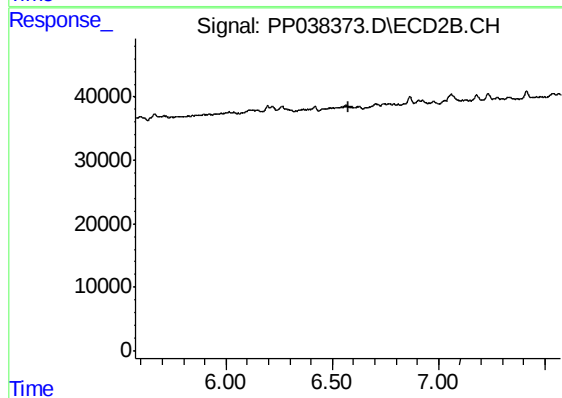

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.573 min
Response: 0
Conc: N.D.

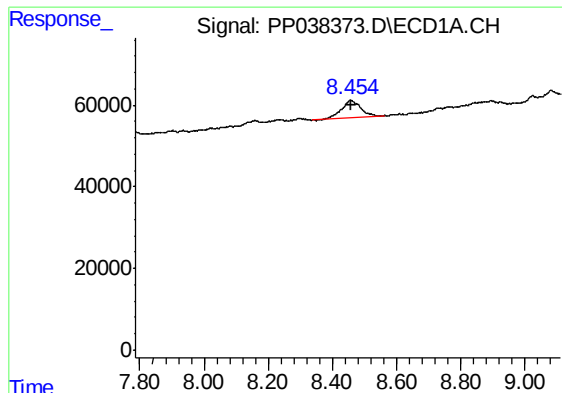

#30 AR-1254-5


R.T.: 8.454 min
Delta R.T.: -0.004 min
Response: 187631
Conc: 129.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
CRT-18

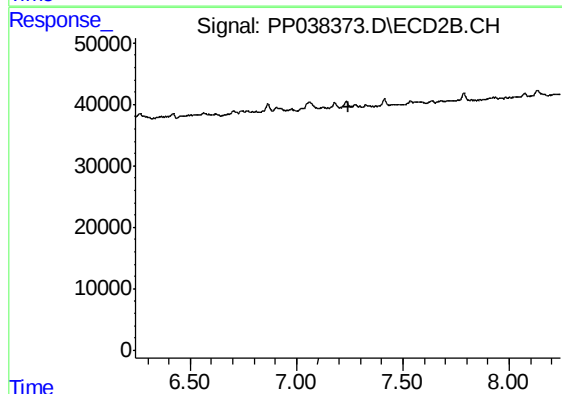


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.242 min
Response: 0
Conc: N.D.

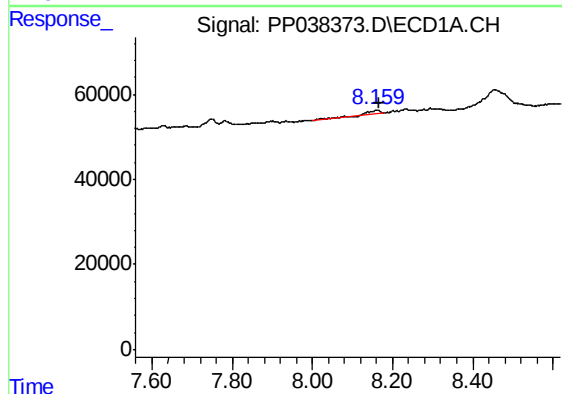


#32 AR-1260-2

R.T.: 8.159 min
Delta R.T.: -0.007 min
Response: 15486
Conc: 8.99 ng/ml

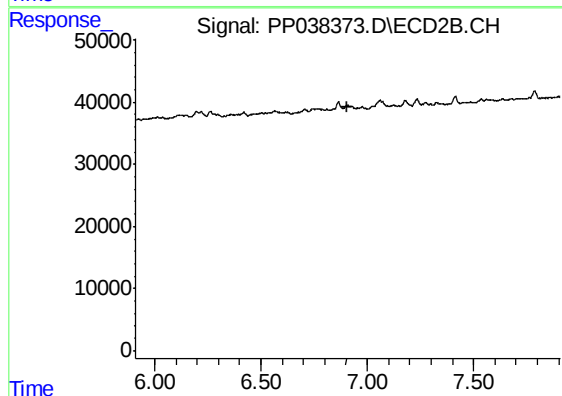

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.909 min
Response: 0
Conc: N.D.

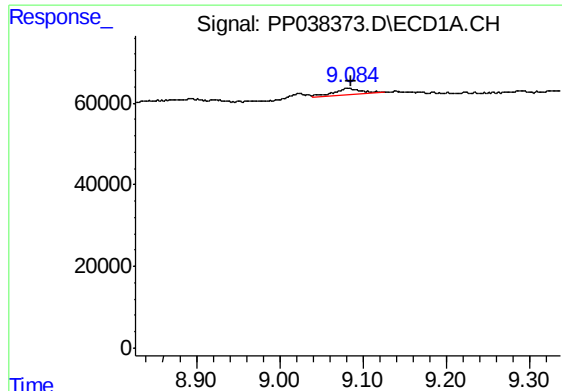

#35 AR-1260-5


R.T.: 9.084 min
Delta R.T.: -0.001 min
Response: 34775
Conc: 13.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
CRT-18

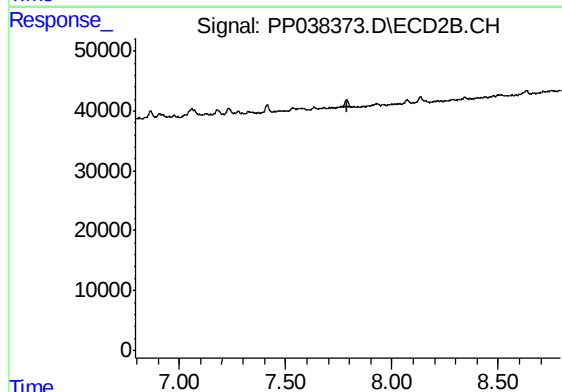


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.793 min
Response: 0
Conc: N.D.

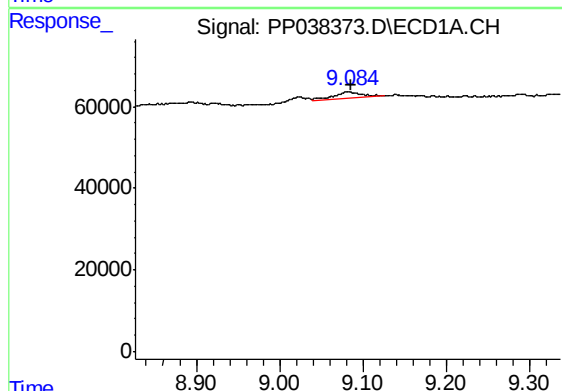

#37 AR-1262-2

R.T.: 9.084 min
Delta R.T.: -0.002 min
Response: 34775
Conc: 12.24 ng/ml

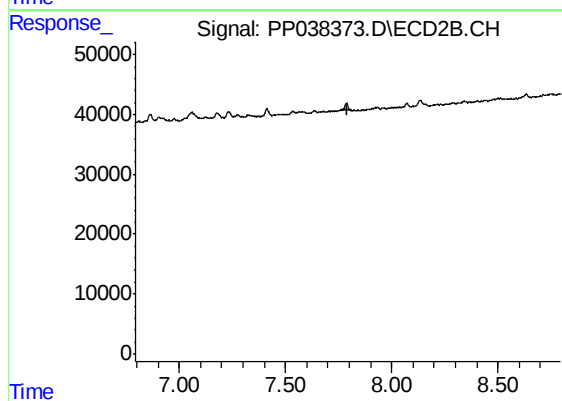

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.794 min
Response: 0
Conc: N.D.