

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081321\
Data File : PP038405.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Aug 2021 7:38
Operator : AJ\MA
Sample : M3397-21
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SWCS-06-1015

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 01:41:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 06 03:08:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.886	3.874	918040	544799	20.657	21.153
2)	SA Decachlor...	10.874	9.135	482743	509244	21.221	19.682

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081321\
Data File : PP038405.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Aug 2021 7:38
Operator : AJ\MA
Sample : M3397-21
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SWCS-06-1015

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 01:41:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 06 03:08:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

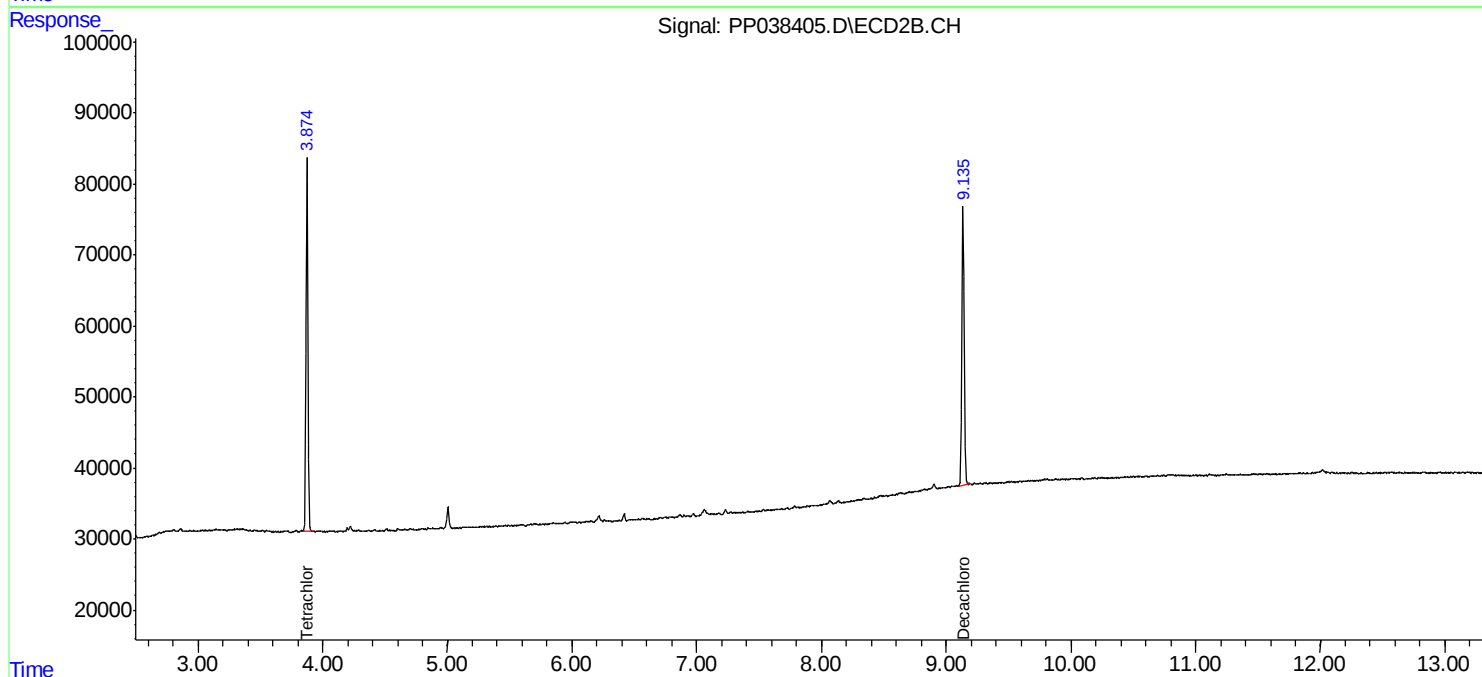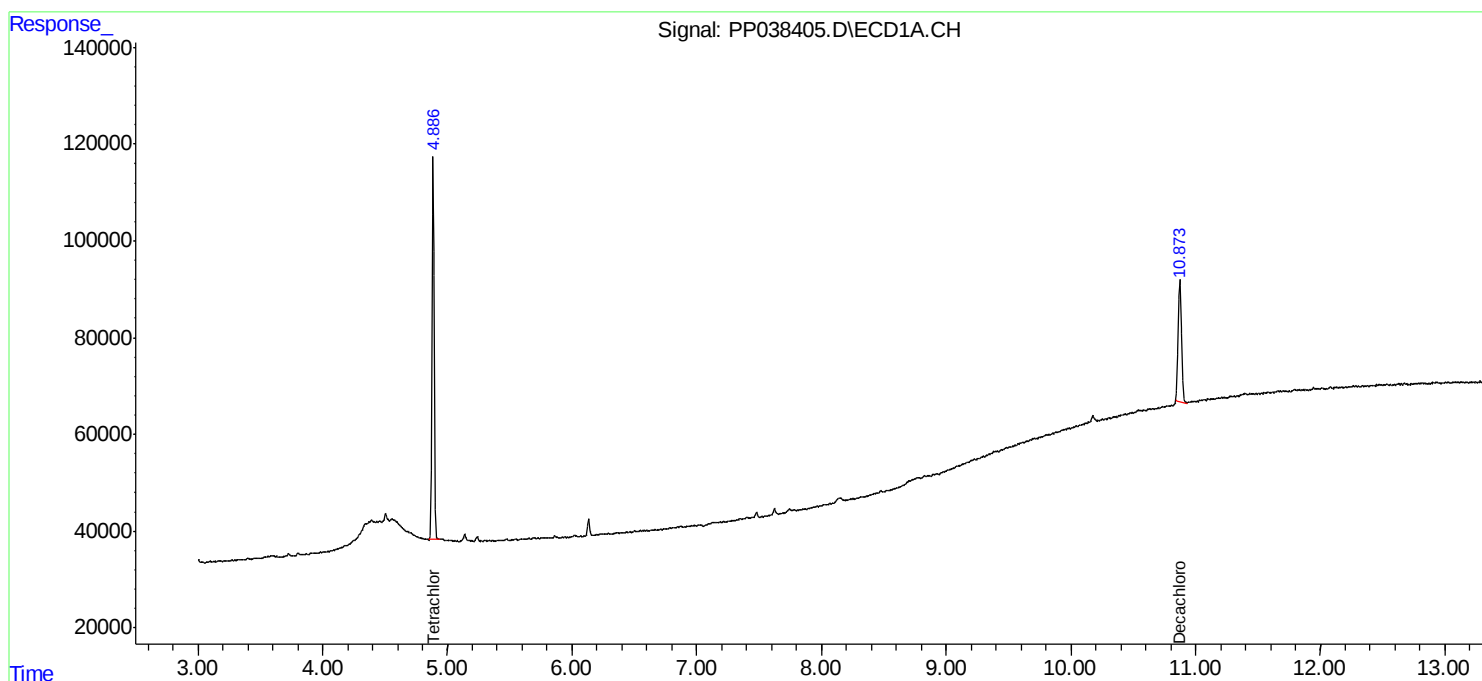


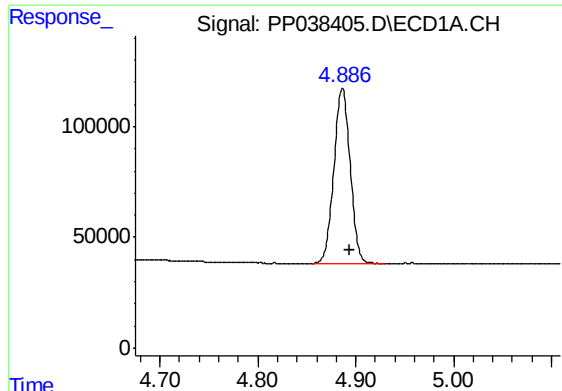

#1 Tetrachloro-m-xylene


R.T.: 4.886 min
Delta R.T.: -0.008 min
Response: 918040
Conc: 20.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
SWCS-06-1015

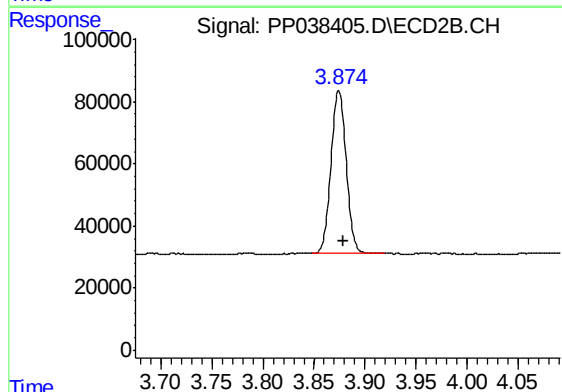


#1 Tetrachloro-m-xylene

R.T.: 3.874 min
Delta R.T.: -0.005 min
Response: 544799
Conc: 21.15 ng/ml

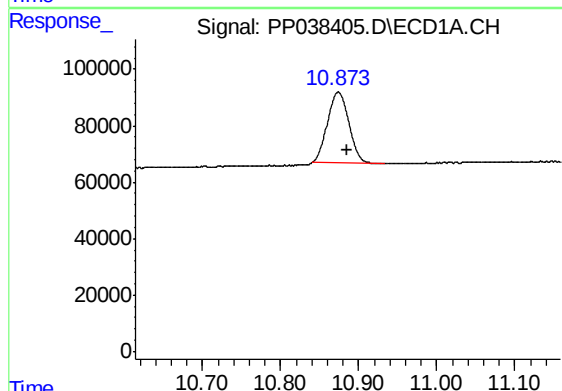

#2 Decachlorobiphenyl

R.T.: 10.874 min
Delta R.T.: -0.012 min
Response: 482743
Conc: 21.22 ng/ml

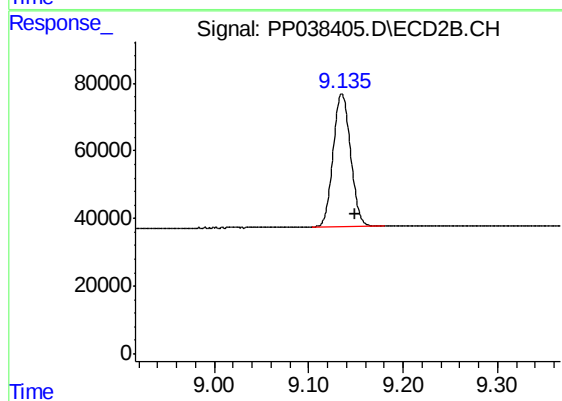

#2 Decachlorobiphenyl

R.T.: 9.135 min
Delta R.T.: -0.014 min
Response: 509244
Conc: 19.68 ng/ml