

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081321\
 Data File : PP038378.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Aug 2021 19:56
 Operator : AJ\MA
 Sample : M3394-10
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SWCS-01-1015

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 01:24:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 06 03:08:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.892	3.878	996444	581001	22.422	22.558
2)	SA Decachlor...	10.881	9.141	586016	612479	25.761	23.672

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081321\
Data File : PP038378.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Aug 2021 19:56
Operator : AJ\MA
Sample : M3394-10
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SWCS-01-1015

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 01:24:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 06 03:08:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

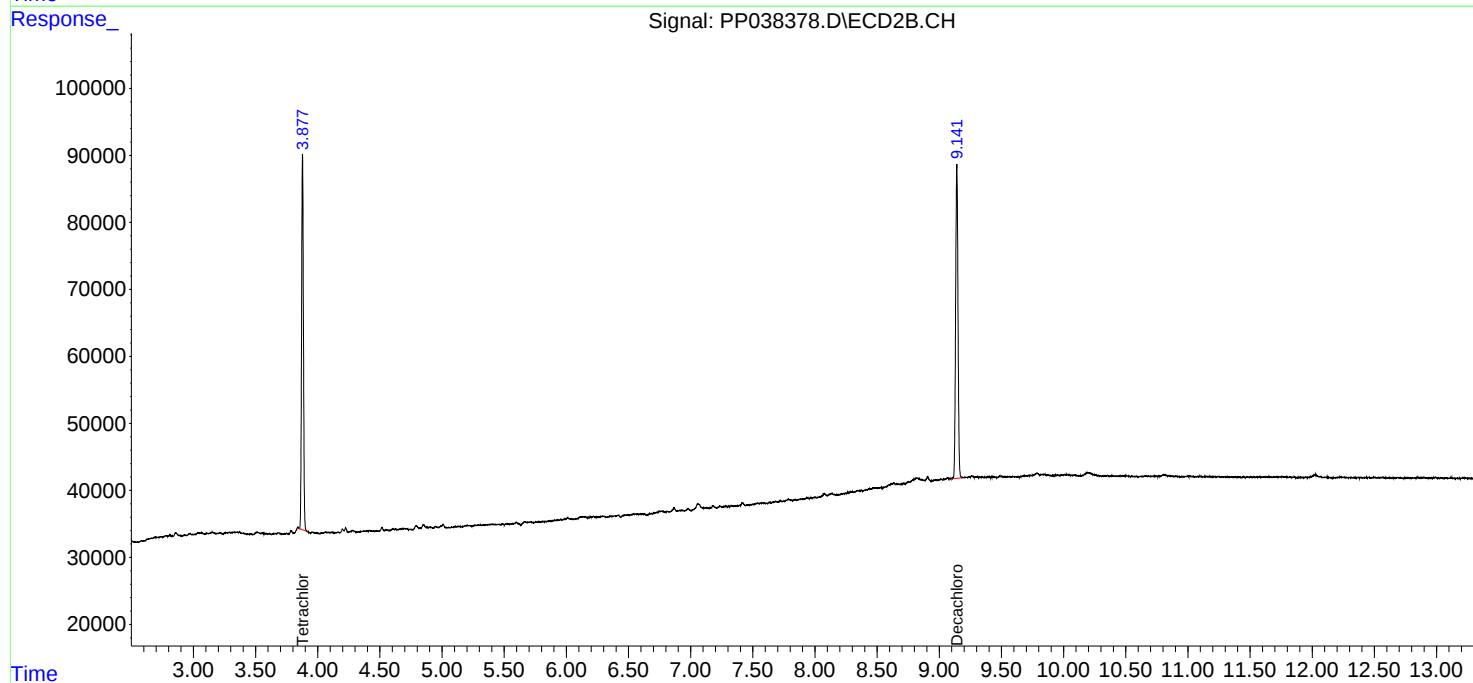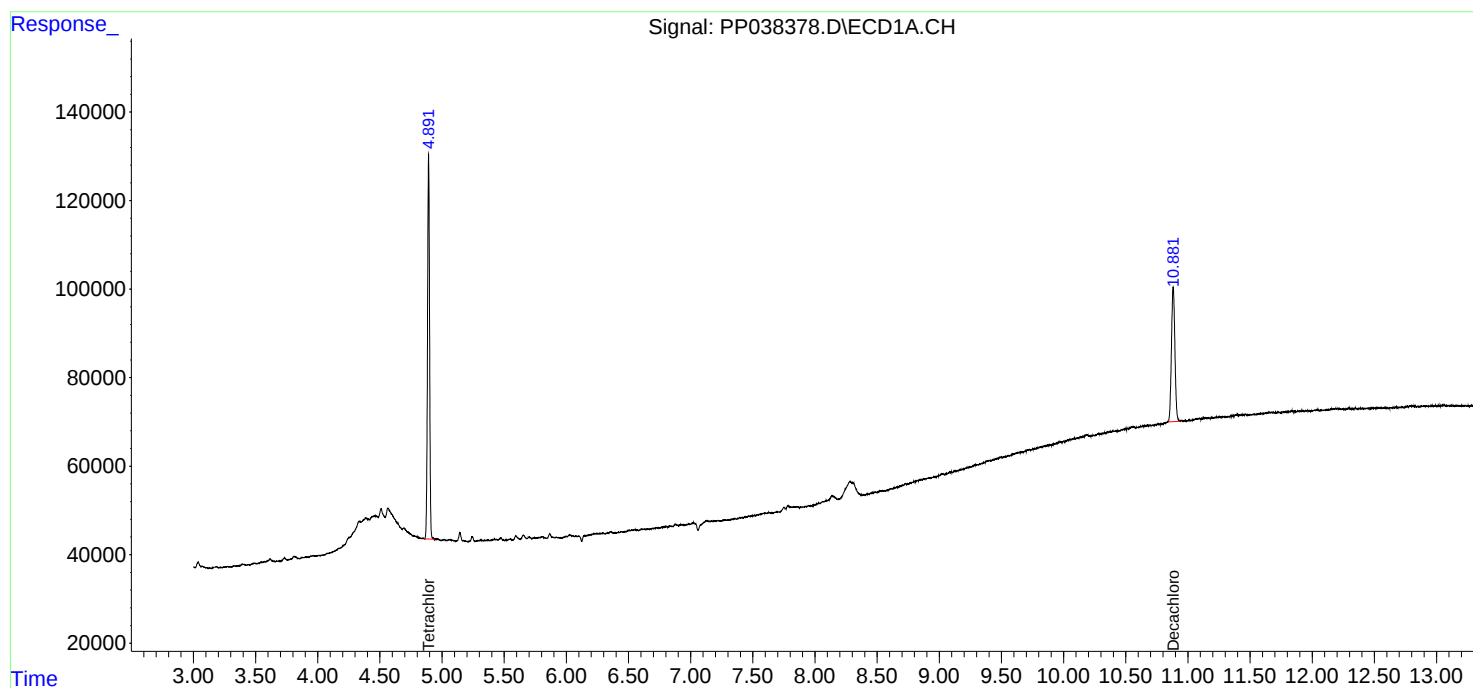


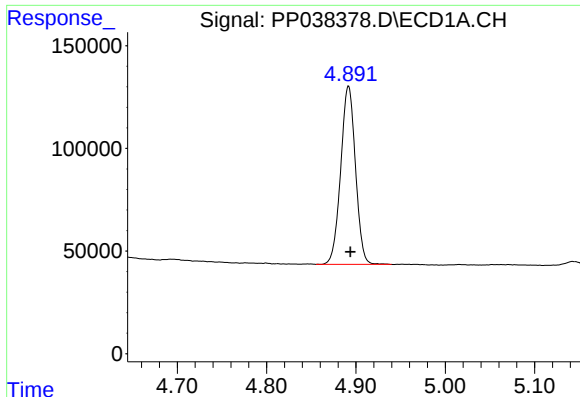

#1 Tetrachloro-m-xylene


R.T.: 4.892 min
Delta R.T.: -0.002 min
Response: 996444
Conc: 22.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
SWCS-01-1015

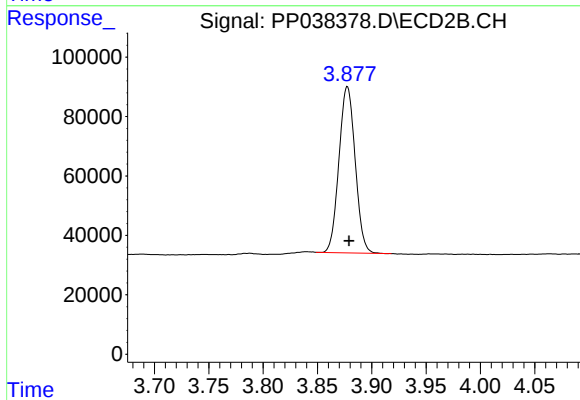


#1 Tetrachloro-m-xylene

R.T.: 3.878 min
Delta R.T.: -0.001 min
Response: 581001
Conc: 22.56 ng/ml

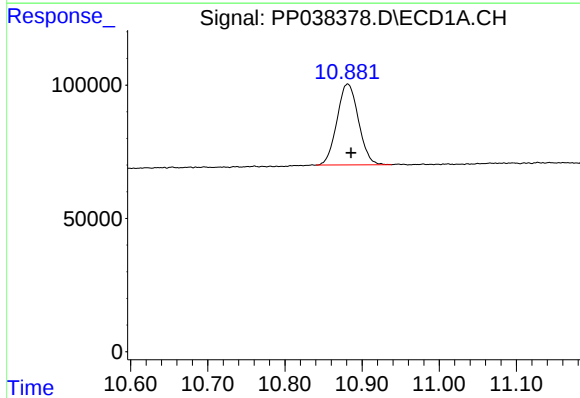

#2 Decachlorobiphenyl

R.T.: 10.881 min
Delta R.T.: -0.004 min
Response: 586016
Conc: 25.76 ng/ml

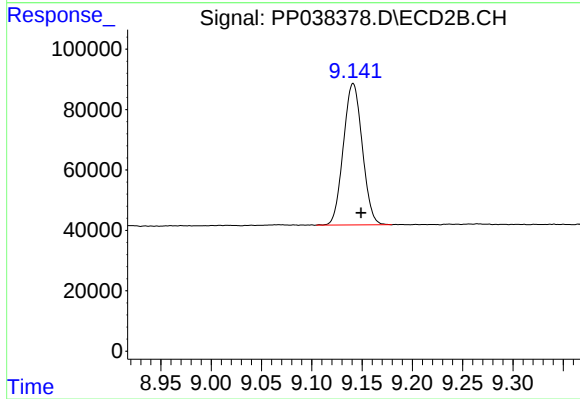

#2 Decachlorobiphenyl

R.T.: 9.141 min
Delta R.T.: -0.008 min
Response: 612479
Conc: 23.67 ng/ml