

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081325\
 Data File : PP074356.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2025 18:04
 Operator : YP\AJ
 Sample : Q2815-23
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TW-11M-N

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/14/2025
 Supervised By :mohammad ahmed 08/18/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 00:00:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.682	3.803	22287224	92833246	19.929m	24.210m
2) SA Decachlor...	10.462	8.821	11247710	59598185	11.582	9.911

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081325\
Data File : PP074356.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2025 18:04
Operator : YP\AJ
Sample : Q2815-23
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TW-11M-N


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/14/2025
Supervised By :mohammad ahmed 08/18/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 00:00:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Aug 04 11:01:49 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

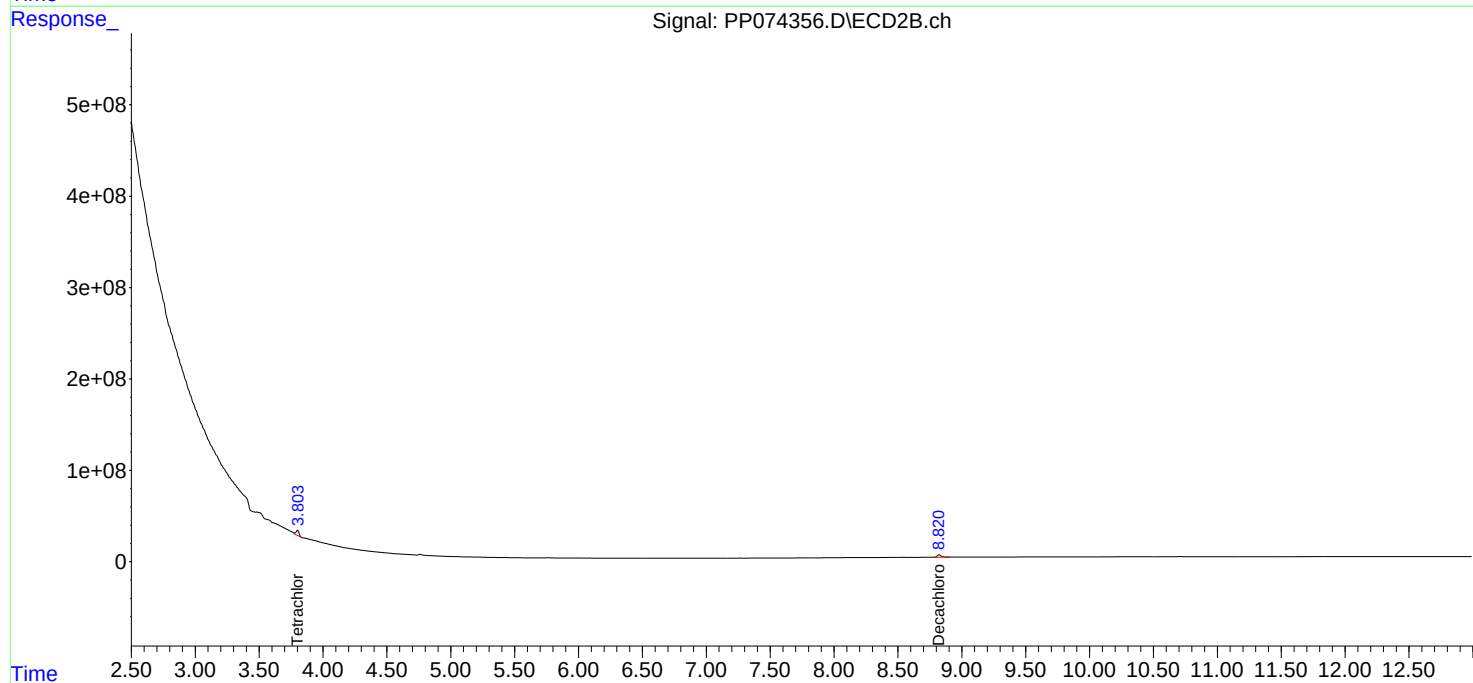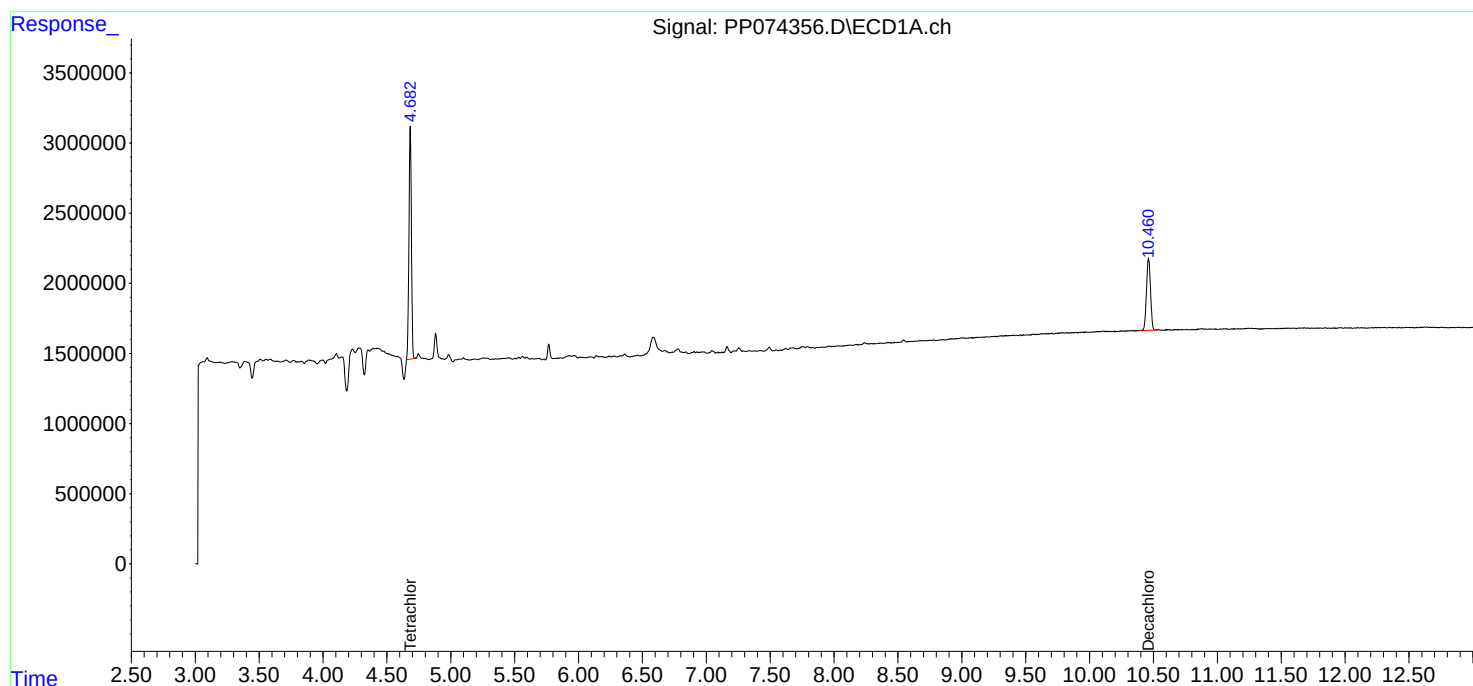

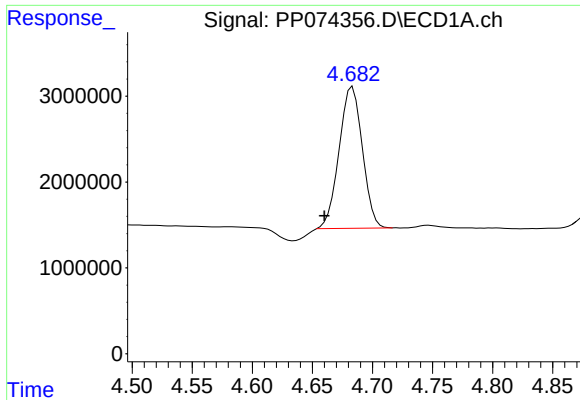


#1 Tetrachloro-m-xylene

R.T.: 4.682 min
Delta R.T.: 0.022 min
Response: 22287224
Conc: 19.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
TW-11M-N


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/14/2025
Supervised By :mohammad ahmed 08/18/2025

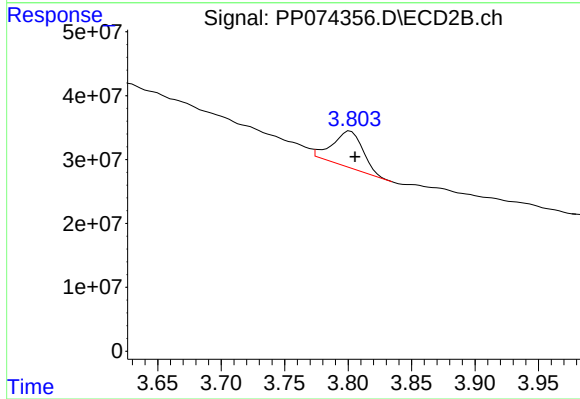


#1 Tetrachloro-m-xylene

R.T.: 3.803 min
Delta R.T.: -0.003 min
Response: 92833246
Conc: 24.21 ng/ml m

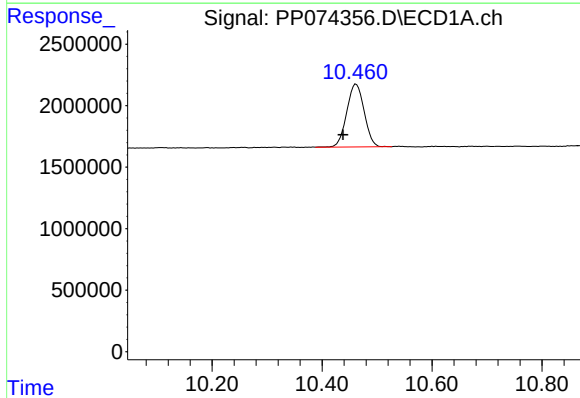

#2 Decachlorobiphenyl

R.T.: 10.462 min
Delta R.T.: 0.024 min
Response: 11247710
Conc: 11.58 ng/ml

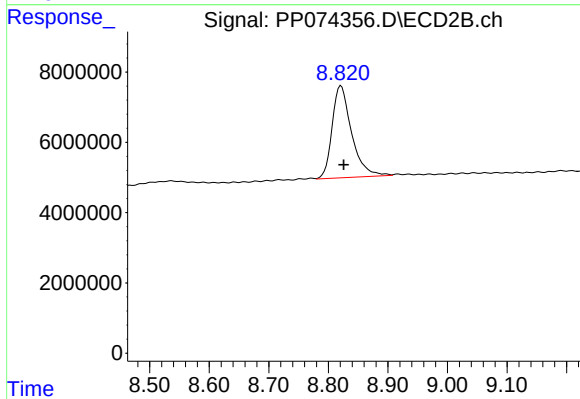

#2 Decachlorobiphenyl

R.T.: 8.821 min
Delta R.T.: -0.005 min
Response: 59598185
Conc: 9.91 ng/ml