

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081419\
 Data File : PP030368.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Aug 2019 13:15
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 17:37:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081419.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 15 11:48:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

5) T	DICAMBA	11.264	0.000	2592638	0	1.794	N.D.	#
7) T	MCPA	0.000	11.948	0	-3019108	N.D.	5.250	#
10) T	Pentachlo...	13.162	13.531	20708389	5619511	3.576	1.622	#
11) T	2,4,5-TP ...	14.055	0.000	3423363	0	1.622	N.D.	#
12) T	2,4,5-T	14.456	0.000	4698356	0	2.224	N.D.	#
15) T	Picloram	16.435	17.078	40177176	60353648	13.094	32.498	#
16) T	DCPA	17.000	0.000	4983973	0	1.810	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081419\
Data File : PP030368.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Aug 2019 13:15
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 17:37:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081419.M
Quant Title : 8080.M
QLast Update : Thu Aug 15 11:48:40 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

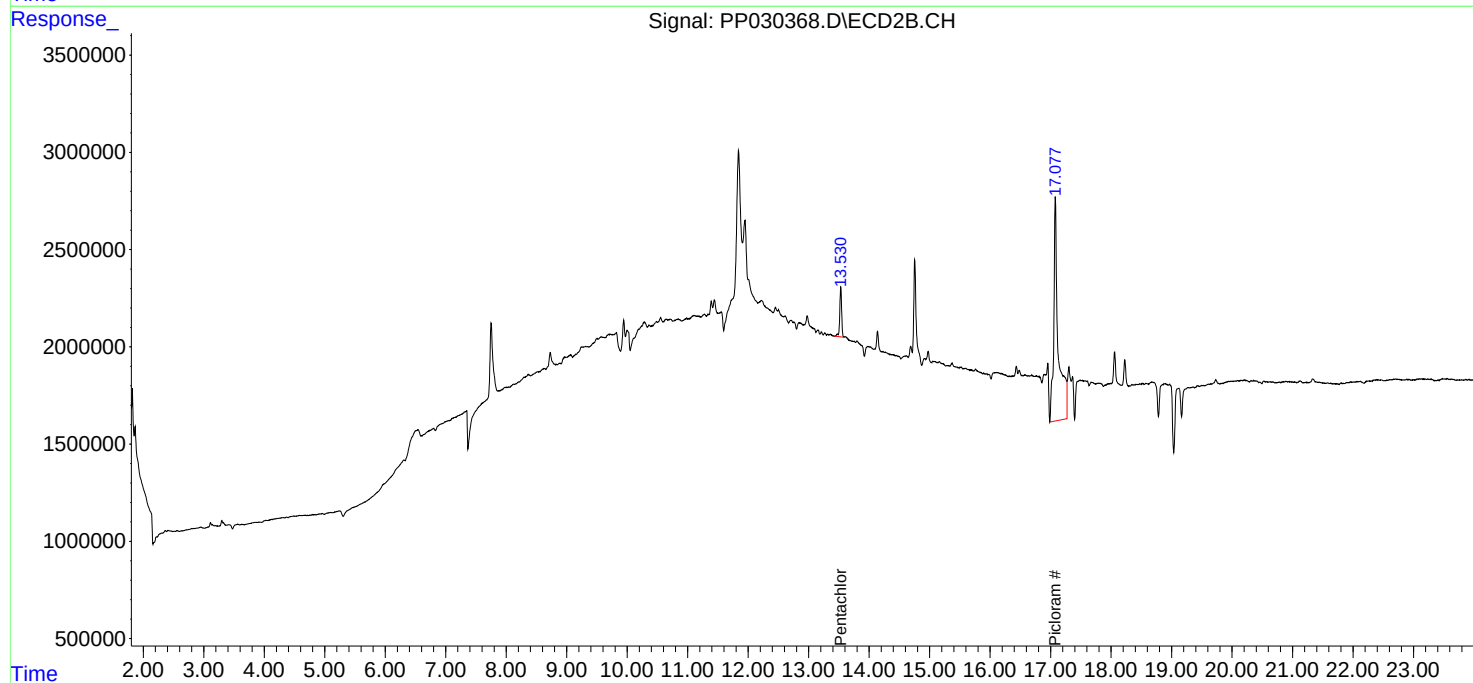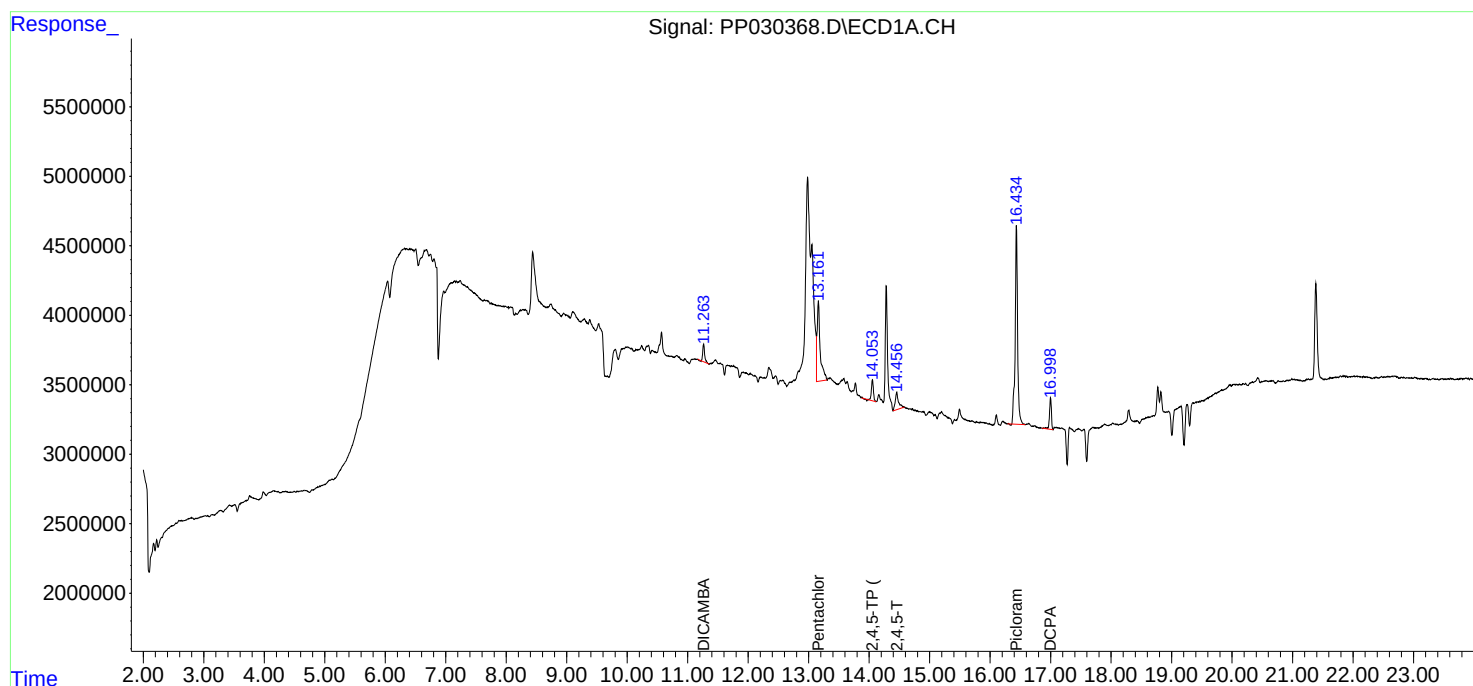


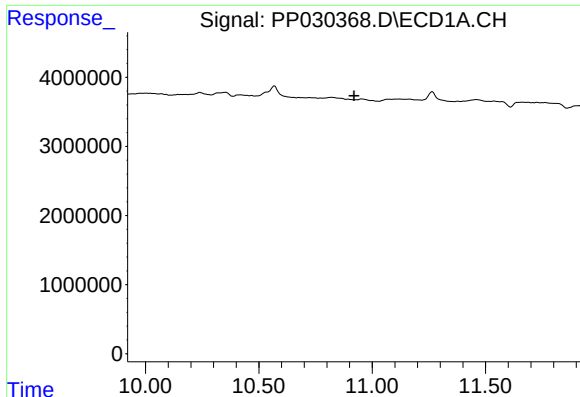

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 10.920 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

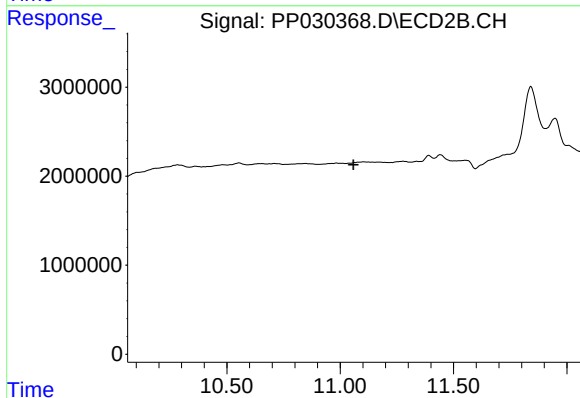


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 11.059 min
Response: 0
Conc: N.D.

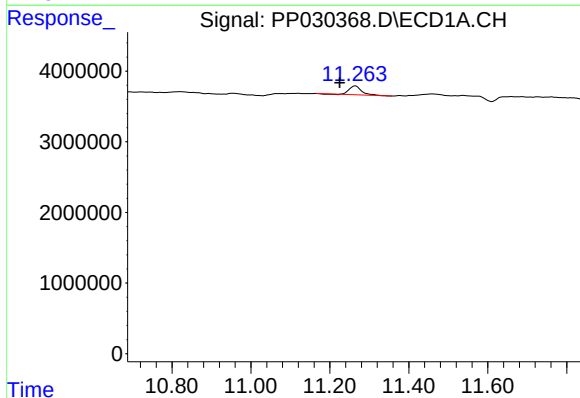


#5 DICAMBA

R.T.: 11.264 min
Delta R.T.: 0.039 min
Response: 2592638
Conc: 1.79 ng/ml

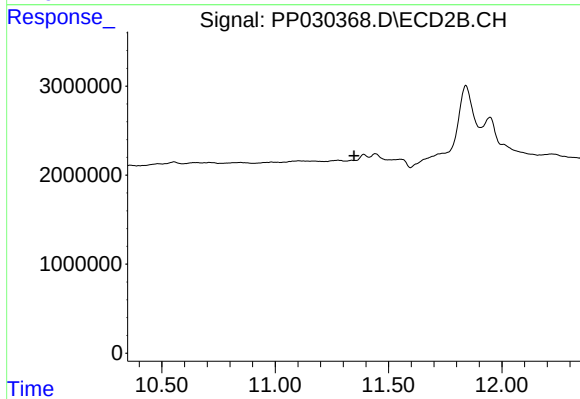

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.348 min
Response: 0
Conc: N.D.

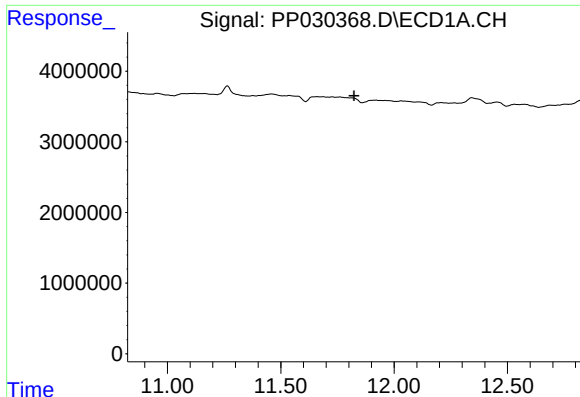

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 11.824 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

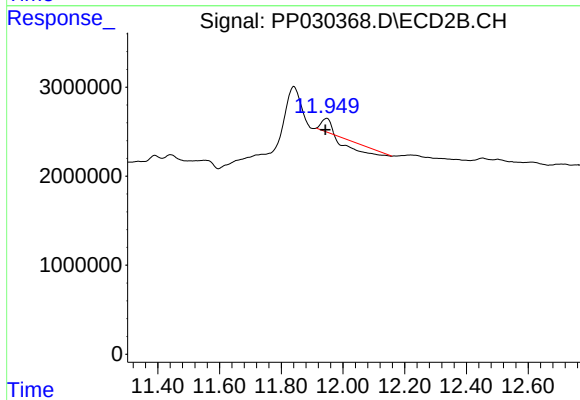


#7 MCPA

R.T.: 11.948 min
Delta R.T.: 0.005 min
Response: -3019108
Conc: 5.25 ug/ml

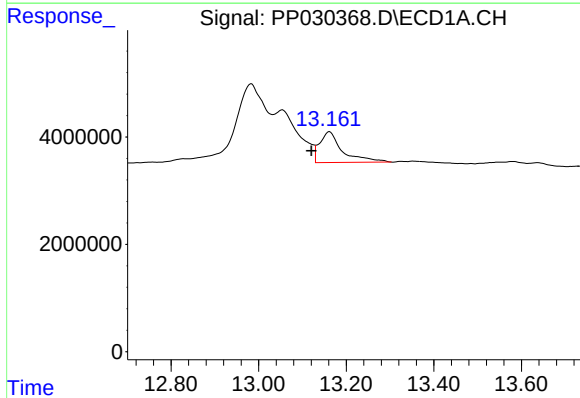


#10 Pentachlorophenol

R.T.: 13.162 min
Delta R.T.: 0.042 min
Response: 20708389
Conc: 3.58 ng/ml

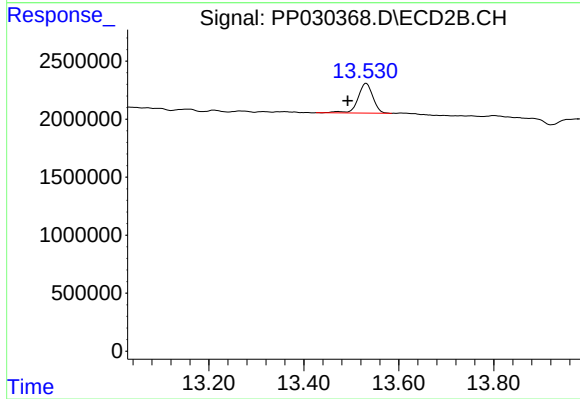

#10 Pentachlorophenol


R.T.: 13.531 min
Delta R.T.: 0.039 min
Response: 5619511
Conc: 1.62 ng/ml

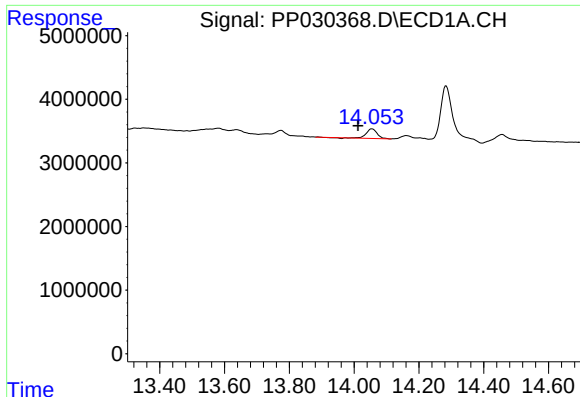

#11 2,4,5-TP (SILVEX)


R.T.: 14.055 min
Delta R.T.: 0.043 min
Response: 3423363
Conc: 1.62 ng/ml

Instrument :
ECD_P
ClientSampleId :

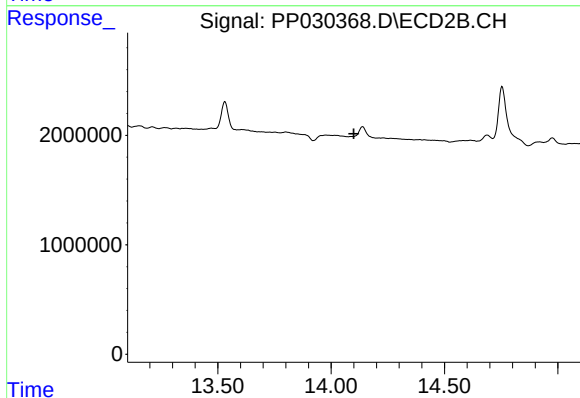


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.099 min
Response: 0
Conc: N.D.

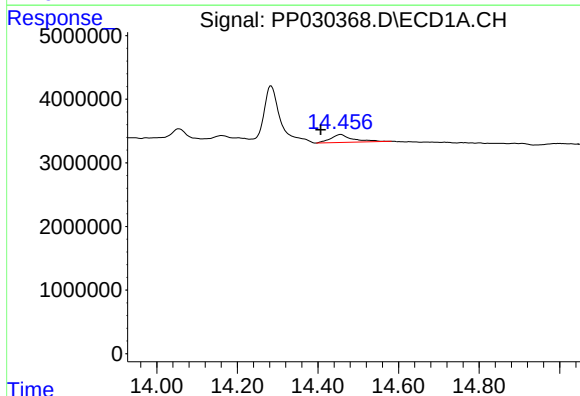


#12 2,4,5-T

R.T.: 14.456 min
Delta R.T.: 0.049 min
Response: 4698356
Conc: 2.22 ng/ml

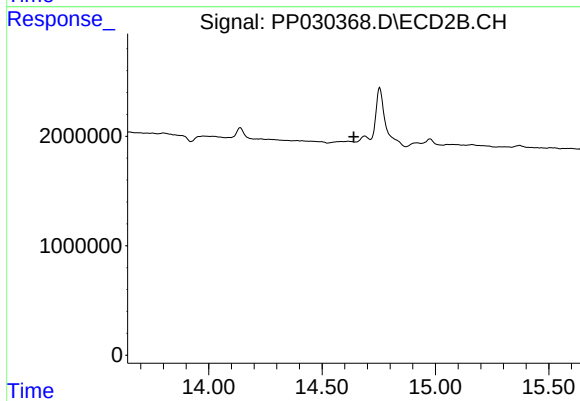

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.641 min
Response: 0
Conc: N.D.

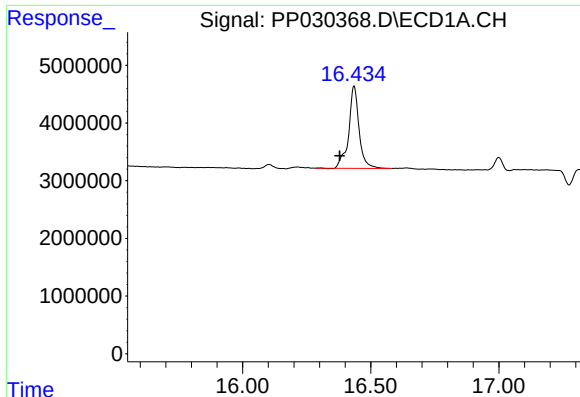

#15 Picloram


R.T.: 16.435 min
Delta R.T.: 0.057 min
Response: 40177176
Conc: 13.09 ng/ml

Instrument :
ECD_P
ClientSampleId :

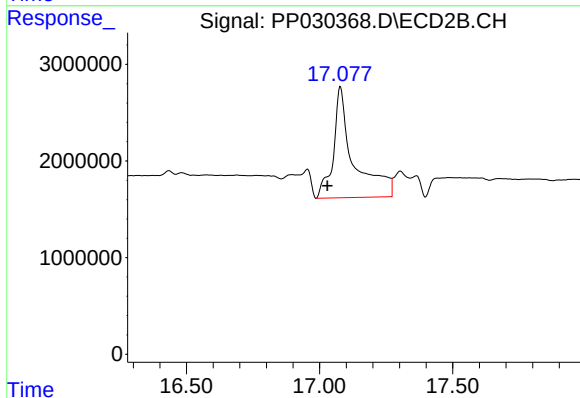


#15 Picloram

R.T.: 17.078 min
Delta R.T.: 0.049 min
Response: 60353648
Conc: 32.50 ng/ml

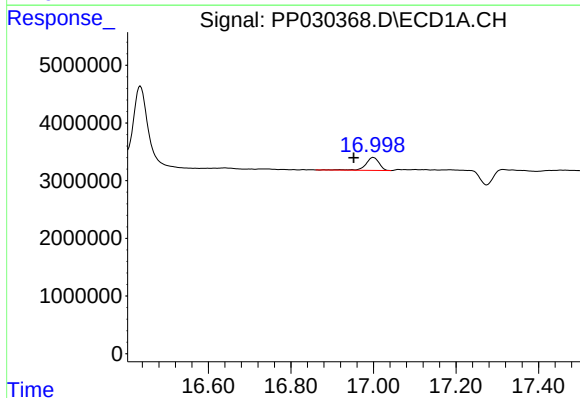

#16 DCPA

R.T.: 17.000 min
Delta R.T.: 0.047 min
Response: 4983973
Conc: 1.81 ng/ml

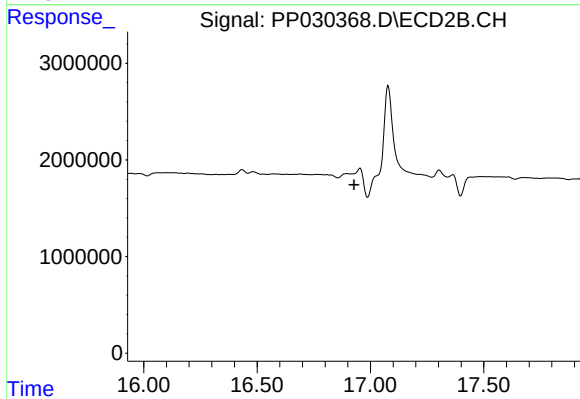

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 16.928 min
Response: 0
Conc: N.D.