

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081423\
 Data File : PP059337.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2023 16:06
 Operator : YP\AJ
 Sample : 03975-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 NEVINS-SB03-Z10-12-Q

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/15/2023
 Supervised By :Ankita Jodhani 08/15/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 00:02:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.413	3.647	16500664	22413203	13.448m	11.062
2) SA Decachlor...	10.203	8.679	12167508	21765699	15.942	15.472

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081423\
Data File : PP059337.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2023 16:06
Operator : YP\AJ
Sample : 03975-02
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
NEVINS-SB03-Z10-12-Q


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/15/2023
Supervised By :Ankita Jodhani 08/15/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 00:02:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 09 02:30:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

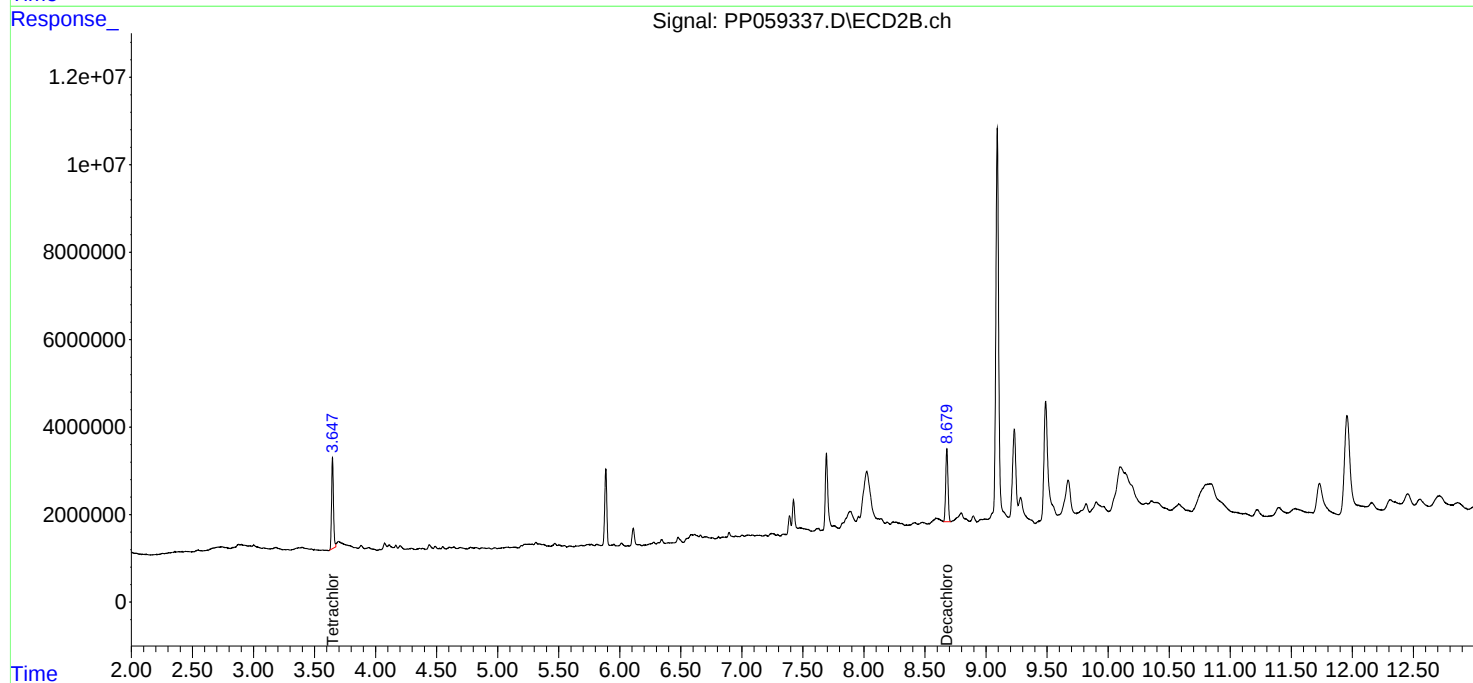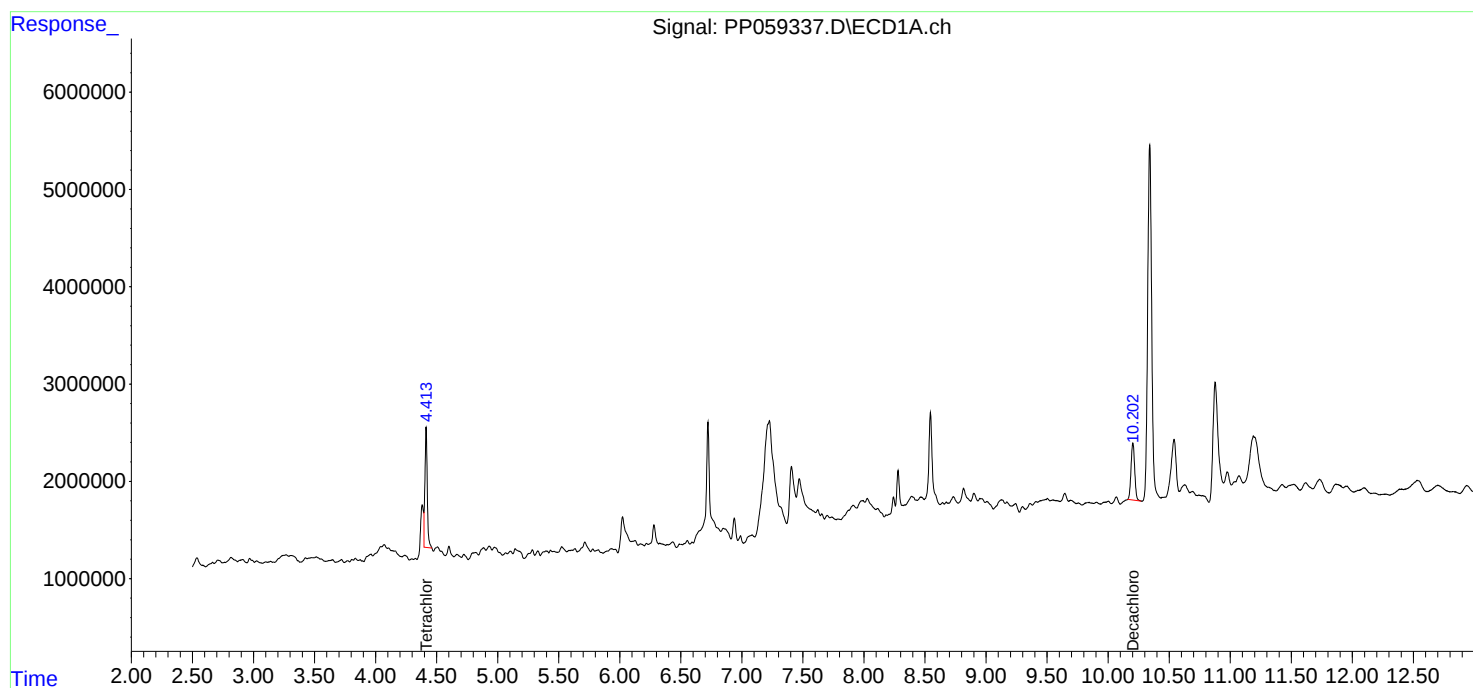

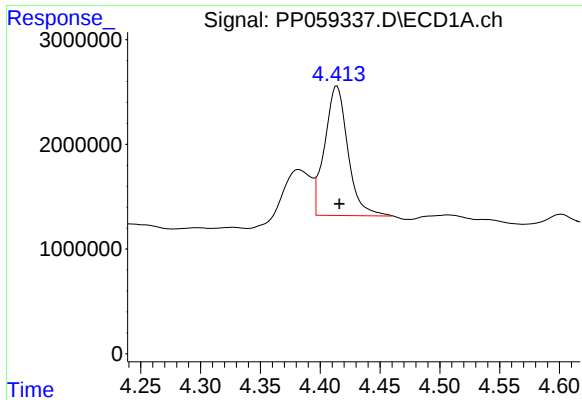


#1 Tetrachloro-m-xylene

R.T.: 4.413 min
Delta R.T.: -0.003 min
Response: 16500664
Conc: 13.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
NEVINS-SB03-Z10-12-Q


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/15/2023
Supervised By :Ankita Jodhani 08/15/2023

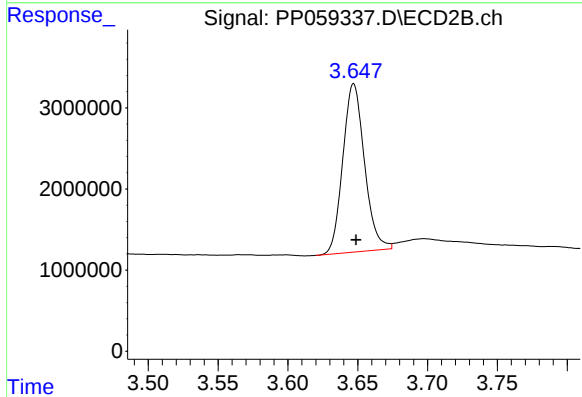


#1 Tetrachloro-m-xylene

R.T.: 3.647 min
Delta R.T.: -0.002 min
Response: 22413203
Conc: 11.06 ng/ml

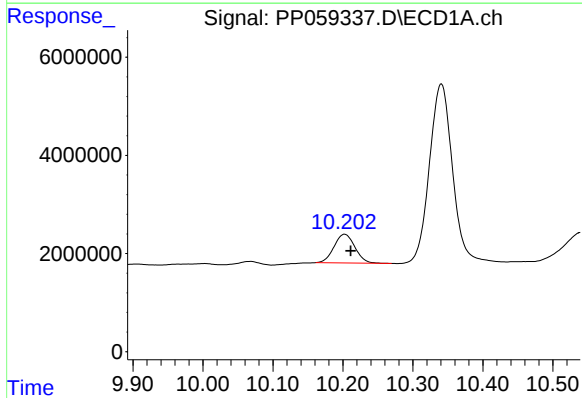

#2 Decachlorobiphenyl

R.T.: 10.203 min
Delta R.T.: -0.009 min
Response: 12167508
Conc: 15.94 ng/ml

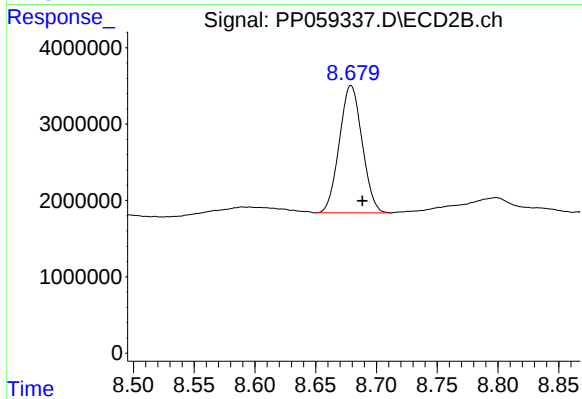

#2 Decachlorobiphenyl

R.T.: 8.679 min
Delta R.T.: -0.010 min
Response: 21765699
Conc: 15.47 ng/ml