

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081423\
 Data File : PP059338.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2023 16:22
 Operator : YP\AJ
 Sample : 03975-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 NEVINS-SB03-Z46-47

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 00:03:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.414	3.645	16486821	29941021	13.436	14.777
2) SA Decachlor...	10.204	8.679	13879904	24408128	18.186	17.350

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081423\
Data File : PP059338.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2023 16:22
Operator : YP\AJ
Sample : 03975-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
NEVINS-SB03-Z46-47

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 00:03:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 09 02:30:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

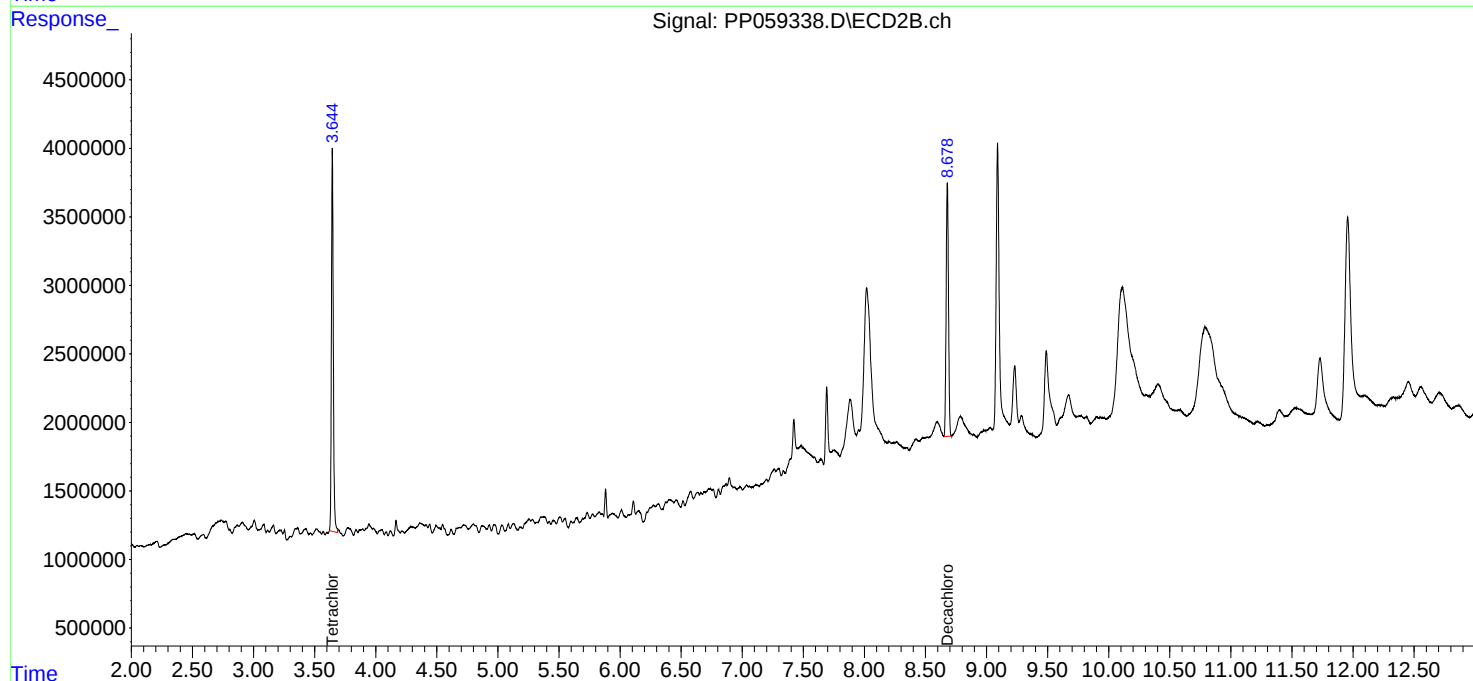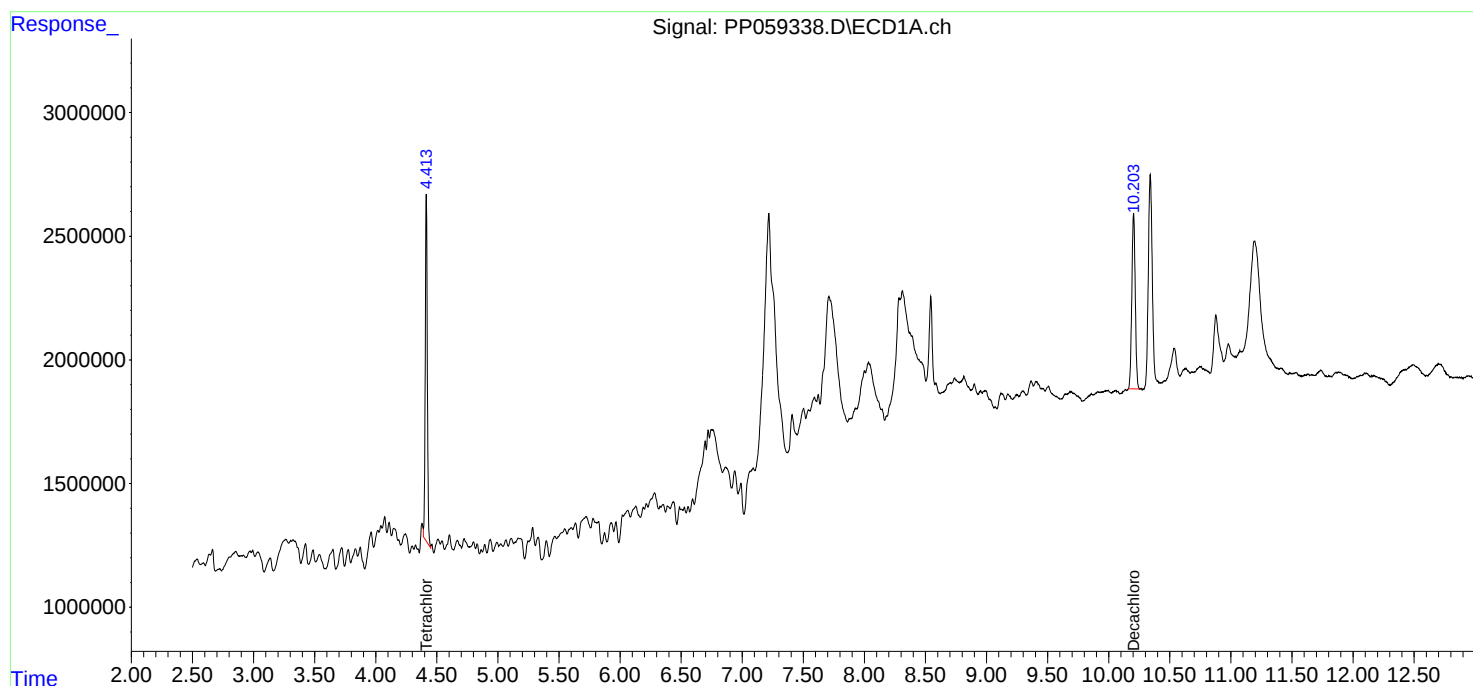


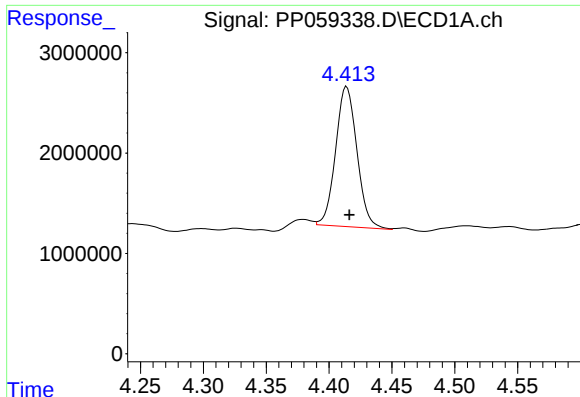

#1 Tetrachloro-m-xylene


R.T.: 4.414 min
Delta R.T.: -0.002 min
Response: 16486821
Conc: 13.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
NEVINS-SB03-Z46-47

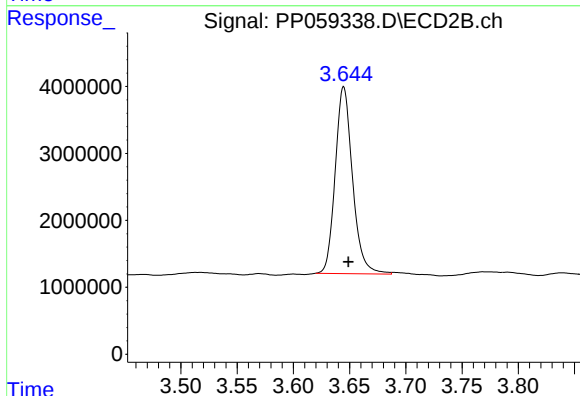


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: -0.004 min
Response: 29941021
Conc: 14.78 ng/ml

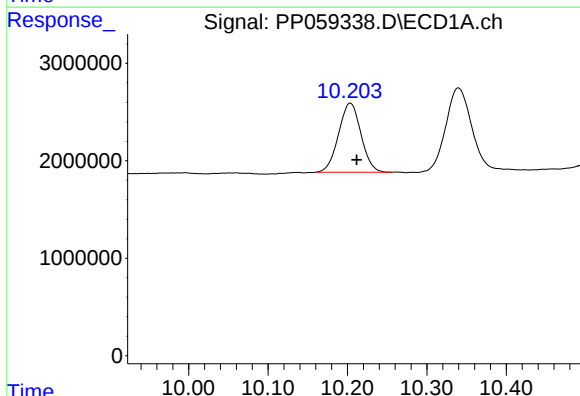

#2 Decachlorobiphenyl

R.T.: 10.204 min
Delta R.T.: -0.008 min
Response: 13879904
Conc: 18.19 ng/ml

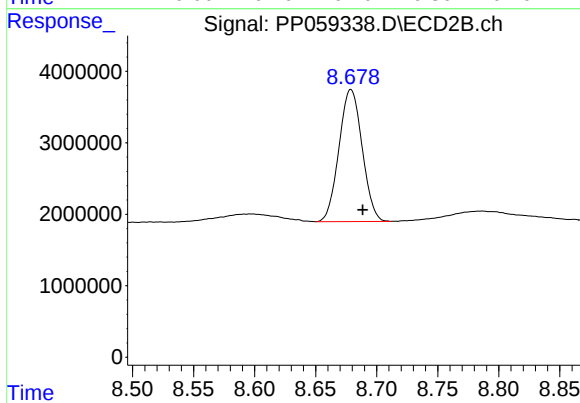

#2 Decachlorobiphenyl

R.T.: 8.679 min
Delta R.T.: -0.010 min
Response: 24408128
Conc: 17.35 ng/ml