

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081423\
 Data File : PP059346.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2023 18:32
 Operator : YP\AJ
 Sample : 03984-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BX6-2-23

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/15/2023
 Supervised By :Ankita Jodhani 08/15/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 00:11:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.414	3.645	27044727	43779764	22.041	21.607
2) SA Decachlor...	10.205	8.680	19470521	36871323	25.511	26.209
Target Compounds						
26) L6 AR-1254-1	6.452	5.544	14981276	27852512	320.697	274.909m
27) L6 AR-1254-2	6.673	5.693	18719139	15725280	272.049	178.133m#
28) L6 AR-1254-3	7.041	6.097	18106640	19996388	262.339	144.644m#
29) L6 AR-1254-4	7.324	6.328	6869395	14118231	152.600m	175.642
30) L6 AR-1254-5	7.751	6.746	8730743	159.9E6	185.812m	1337.502 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081423\
Data File : PP059346.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2023 18:32
Operator : YP\AJ
Sample : 03984-04
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BX6-2-23


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/15/2023
Supervised By :Ankita Jodhani 08/15/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 00:11:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 09 02:30:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

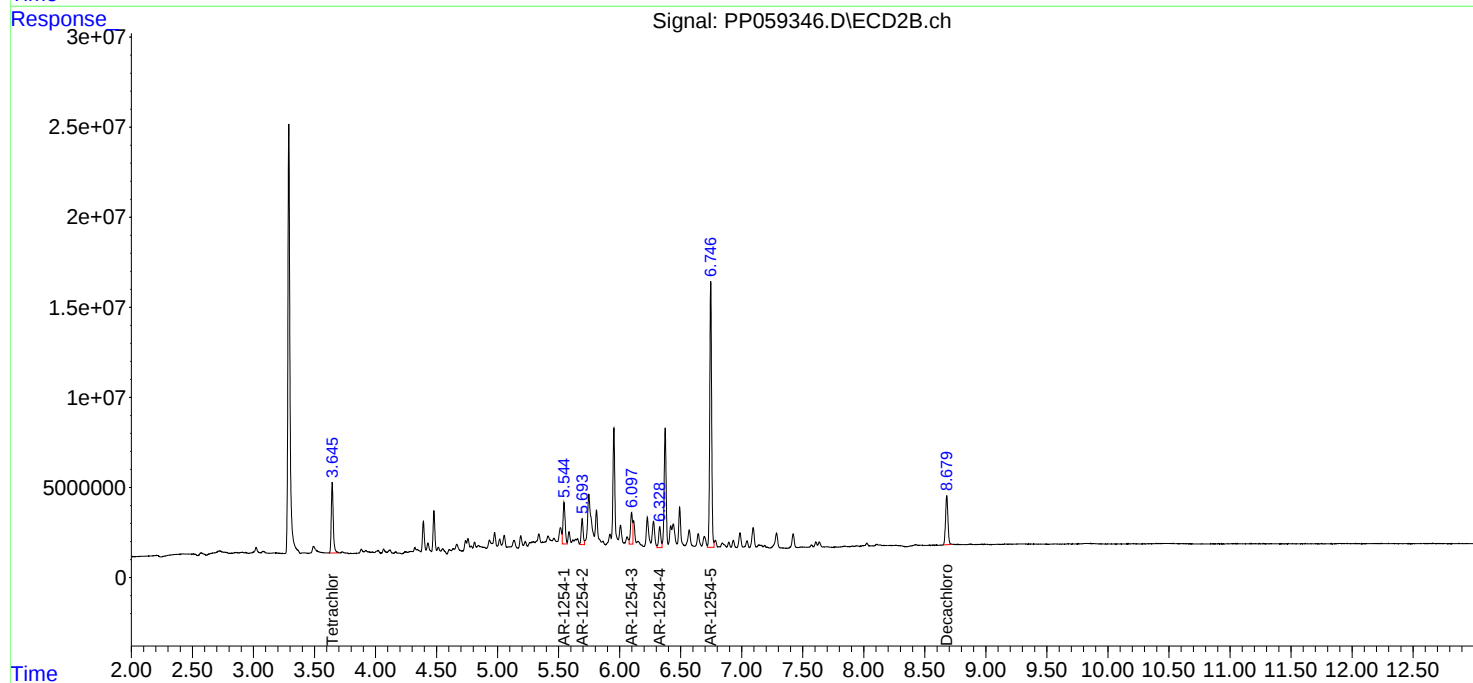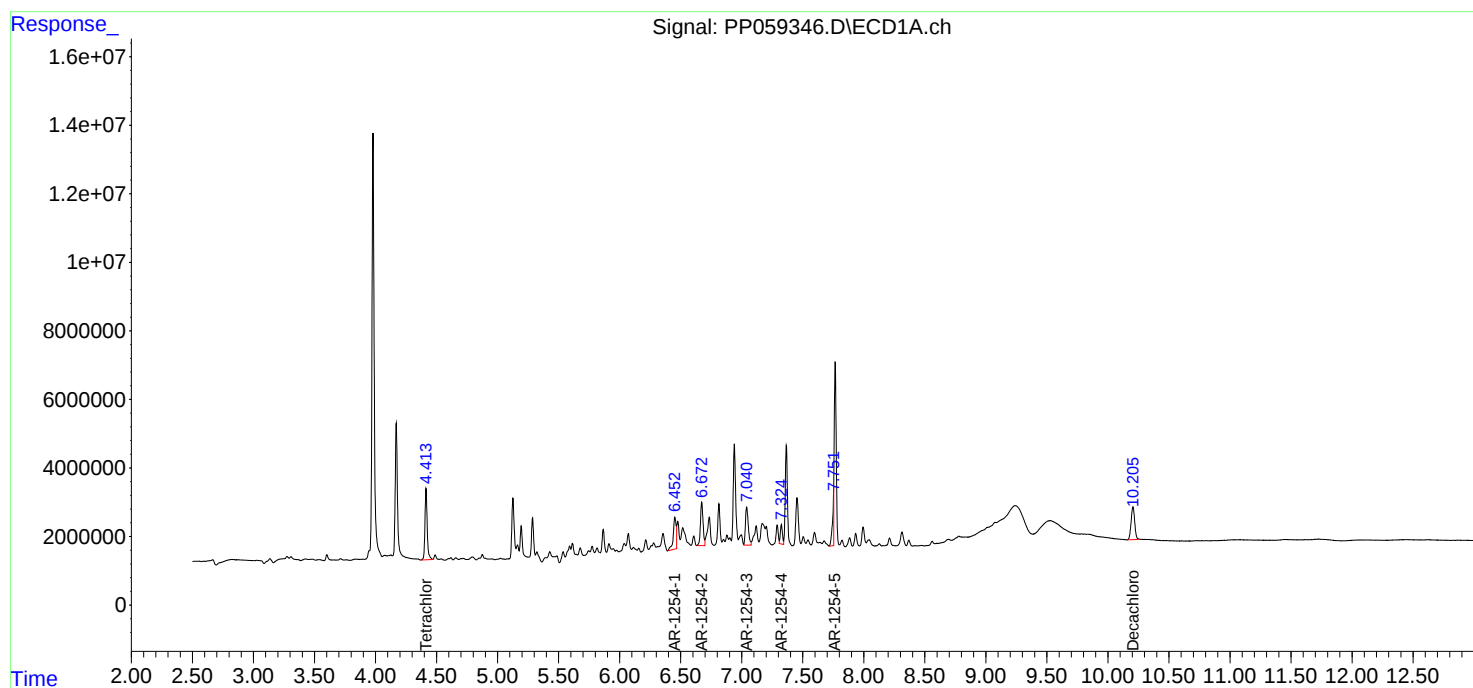

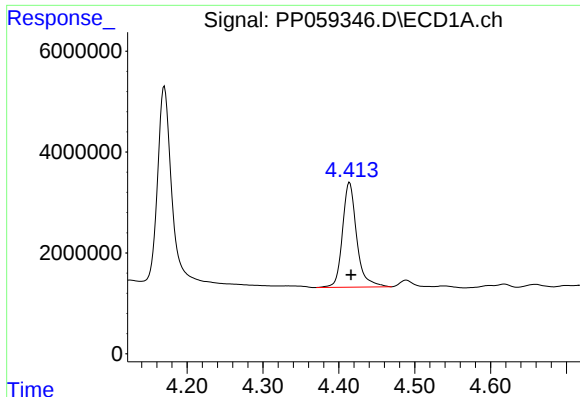


#1 Tetrachloro-m-xylene

R.T.: 4.414 min
Delta R.T.: -0.002 min
Response: 27044727
Conc: 22.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
BX6-2-23


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/15/2023
Supervised By :Ankita Jodhani 08/15/2023

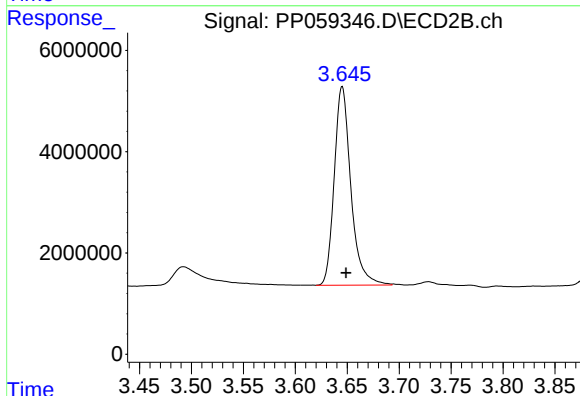


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: -0.004 min
Response: 43779764
Conc: 21.61 ng/ml

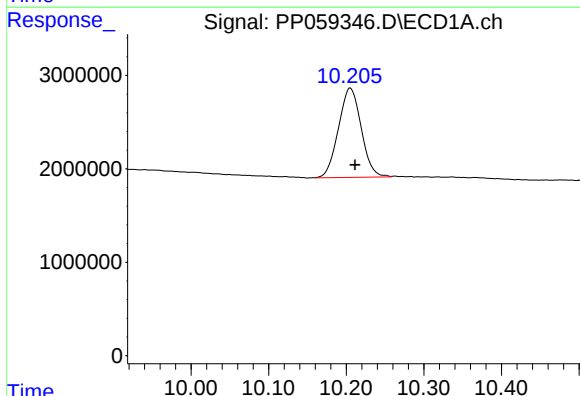


#2 Decachlorobiphenyl

R.T.: 10.205 min
Delta R.T.: -0.006 min
Response: 19470521
Conc: 25.51 ng/ml

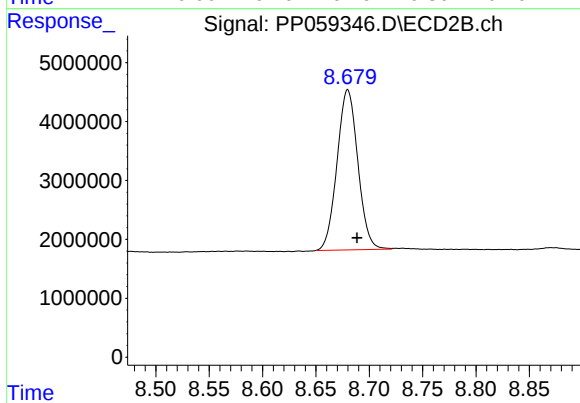

#2 Decachlorobiphenyl

R.T.: 8.680 min
Delta R.T.: -0.009 min
Response: 36871323
Conc: 26.21 ng/ml

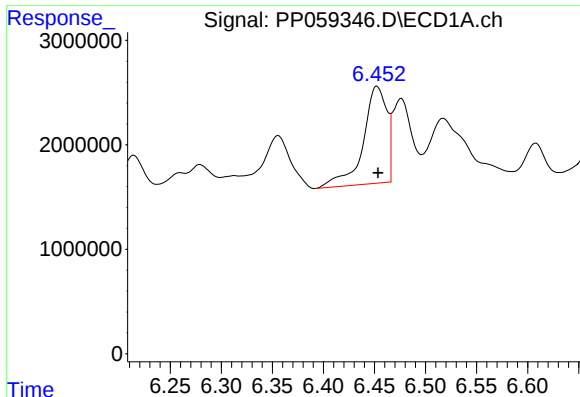


#26 AR-1254-1

R.T.: 6.452 min
Delta R.T.: 0.000 min
Response: 14981276
Conc: 320.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
BX6-2-23


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/15/2023
Supervised By :Ankita Jodhani 08/15/2023

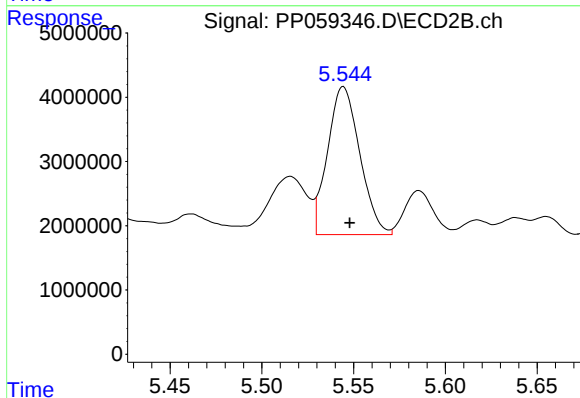


#26 AR-1254-1

R.T.: 5.544 min
Delta R.T.: -0.004 min
Response: 27852512
Conc: 274.91 ng/ml m

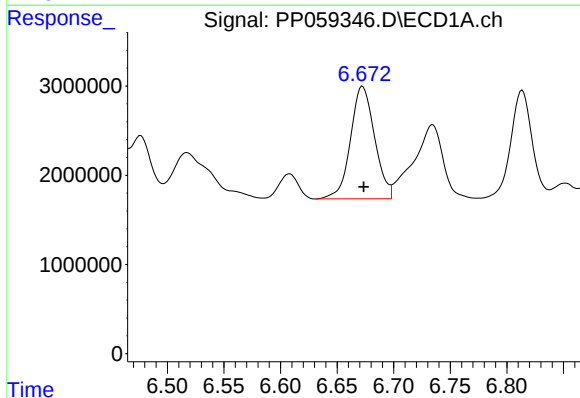


#27 AR-1254-2

R.T.: 6.673 min
Delta R.T.: 0.000 min
Response: 18719139
Conc: 272.05 ng/ml

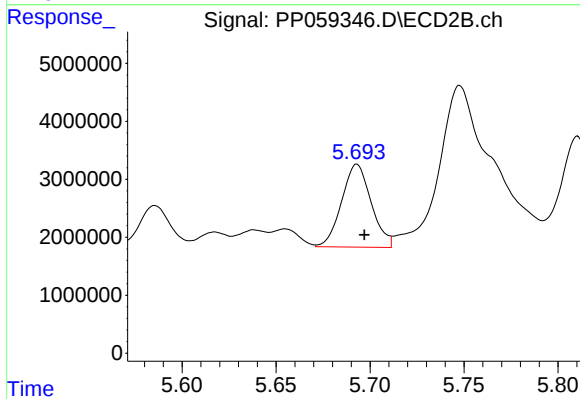

#27 AR-1254-2

R.T.: 5.693 min
Delta R.T.: -0.005 min
Response: 15725280
Conc: 178.13 ng/ml m

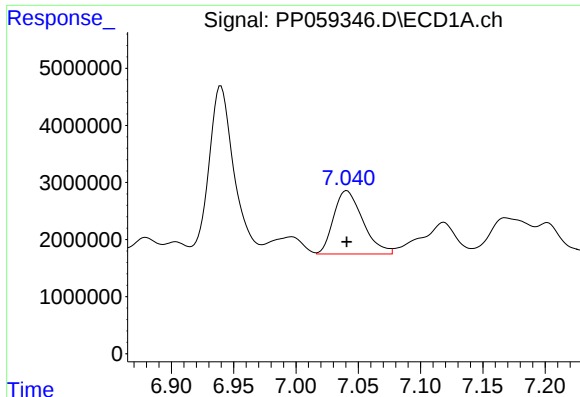


#28 AR-1254-3

R.T.: 7.041 min
Delta R.T.: 0.000 min
Response: 18106640
Conc: 262.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
BX6-2-23


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/15/2023
Supervised By :Ankita Jodhani 08/15/2023

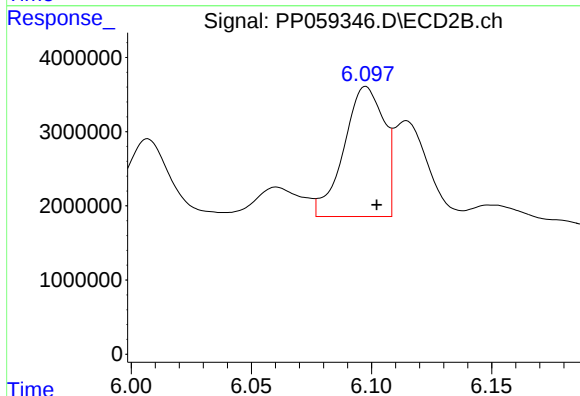


#28 AR-1254-3

R.T.: 6.097 min
Delta R.T.: -0.005 min
Response: 19996388
Conc: 144.64 ng/ml m

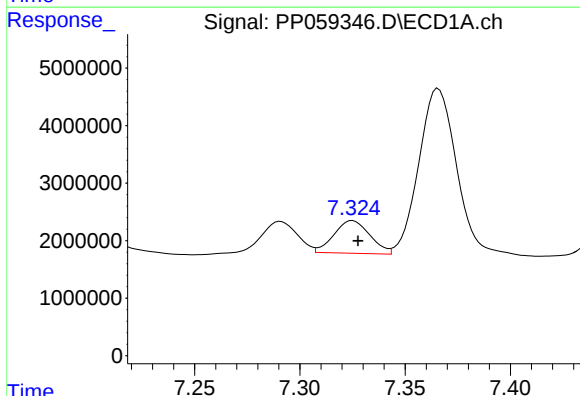


#29 AR-1254-4

R.T.: 7.324 min
Delta R.T.: -0.003 min
Response: 6869395
Conc: 152.60 ng/ml m

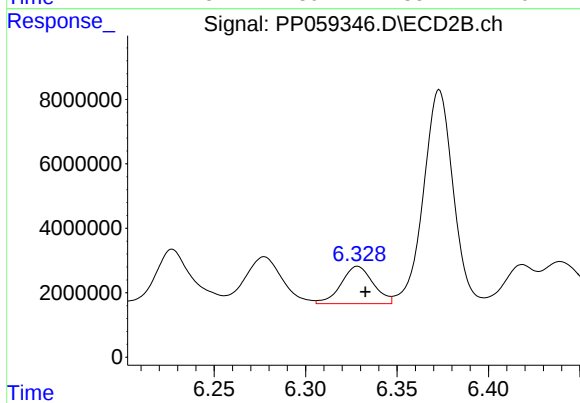

#29 AR-1254-4

R.T.: 6.328 min
Delta R.T.: -0.004 min
Response: 14118231
Conc: 175.64 ng/ml

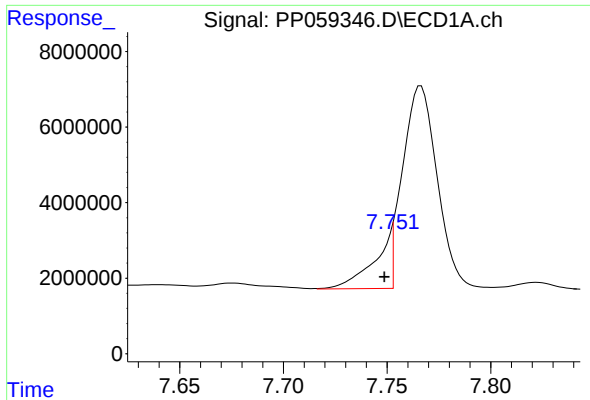


#30 AR-1254-5

R.T.: 7.751 min
Delta R.T.: 0.003 min
Response: 8730743
Conc: 185.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
BX6-2-23

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/15/2023
Supervised By :Ankita Jodhani 08/15/2023

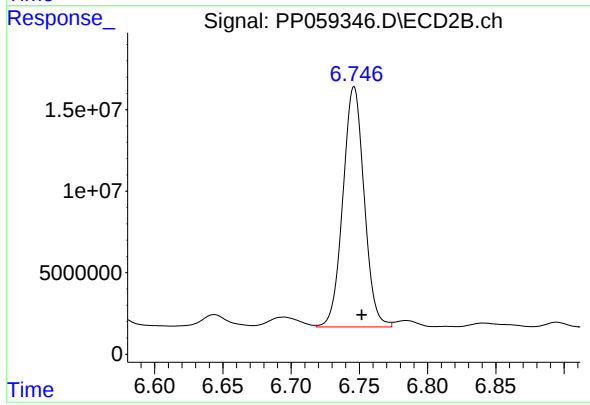

#30 AR-1254-5

R.T.: 6.746 min
Delta R.T.: -0.006 min
Response: 159947795
Conc: 1337.50 ng/ml