

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081425\
 Data File : PP074398.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2025 17:21
 Operator : YP\AJ
 Sample : Q2858-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 VNJ 216

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/15/2025
 Supervised By :mohammad ahmed 08/18/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 11:29:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.658	3.801	25974580	113.0E6	23.227	29.459m#
2) SA Decachlor...	10.437	8.818	19095078	114.1E6	19.662	18.975

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081425\
Data File : PP074398.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2025 17:21
Operator : YP\AJ
Sample : Q2858-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
VNJ 216


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/15/2025
Supervised By :mohammad ahmed 08/18/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 11:29:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Aug 04 11:01:49 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

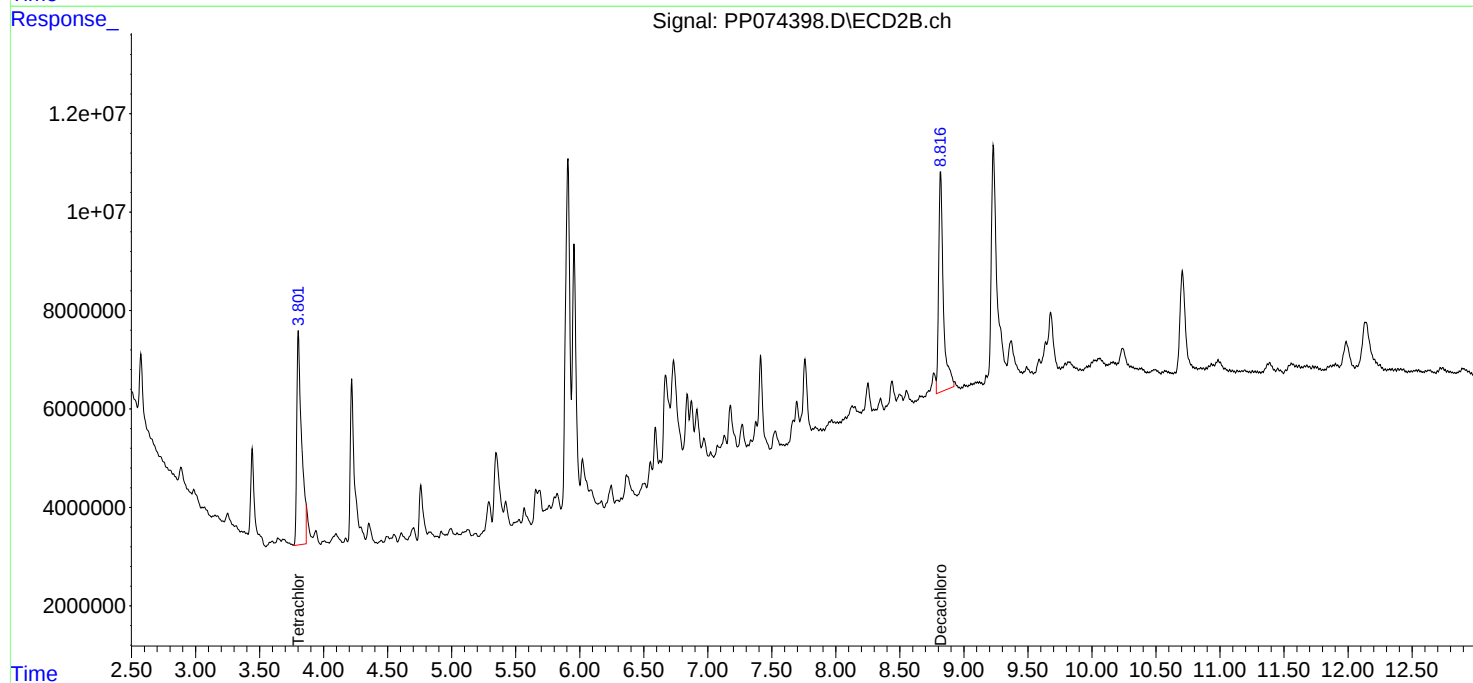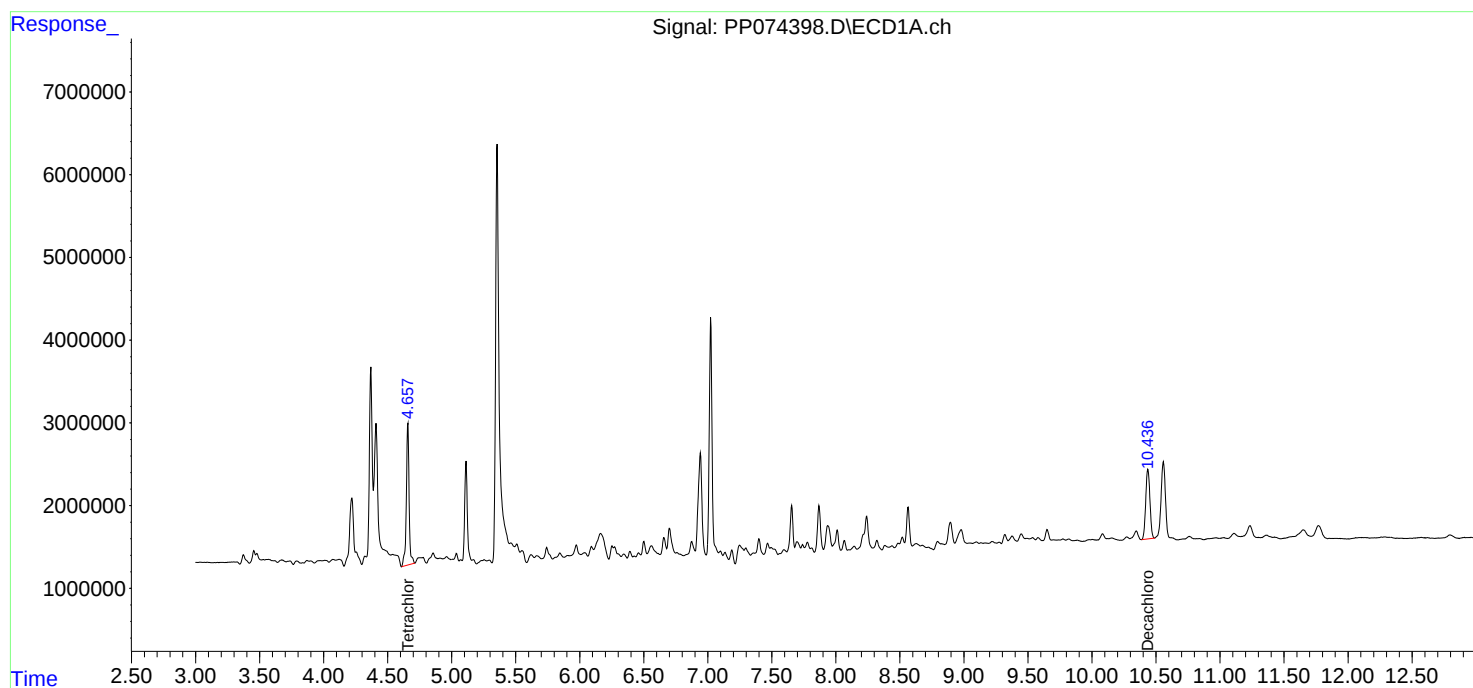

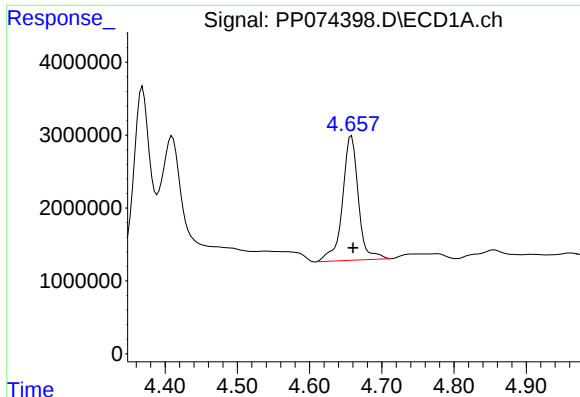


#1 Tetrachloro-m-xylene

R.T.: 4.658 min
Delta R.T.: -0.002 min
Response: 25974580
Conc: 23.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
VNJ 216


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/15/2025
Supervised By :mohammad ahmed 08/18/2025

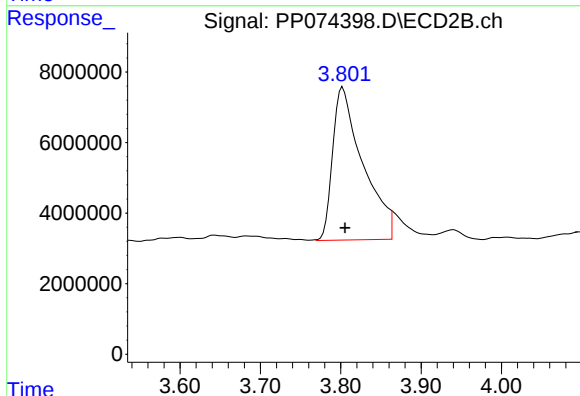


#1 Tetrachloro-m-xylene

R.T.: 3.801 min
Delta R.T.: -0.004 min
Response: 112958442
Conc: 29.46 ng/ml m

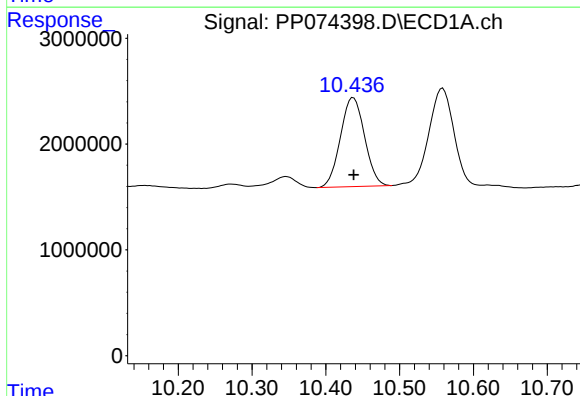

#2 Decachlorobiphenyl

R.T.: 10.437 min
Delta R.T.: 0.000 min
Response: 19095078
Conc: 19.66 ng/ml

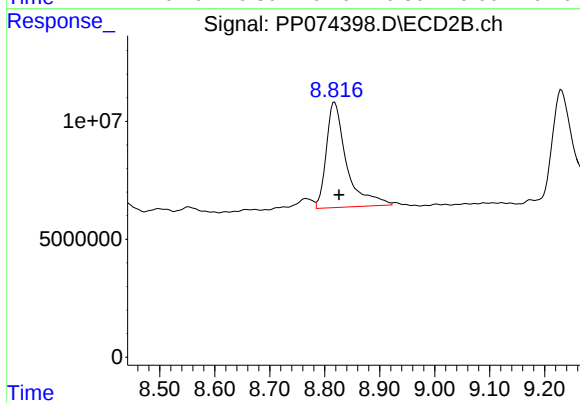

#2 Decachlorobiphenyl

R.T.: 8.818 min
Delta R.T.: -0.008 min
Response: 114106208
Conc: 18.97 ng/ml