

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081522\
 Data File : PP050604.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2022 02:31
 Operator : YP\AJ
 Sample : N4187-10 10X
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KMH368K-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/16/2022
 Supervised By :Ankita Jodhani 08/16/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 06:22:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 09 11:38:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.342	3.588	2556561	4078296	1.588	1.302
2) SA Decachlor...	10.089	8.550	2298764	1920236	1.305m	1.248

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081522\
Data File : PP050604.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2022 02:31
Operator : YP\AJ
Sample : N4187-10 10X
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KMH368K-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/16/2022
Supervised By :Ankita Jodhani 08/16/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 06:22:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 09 11:38:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

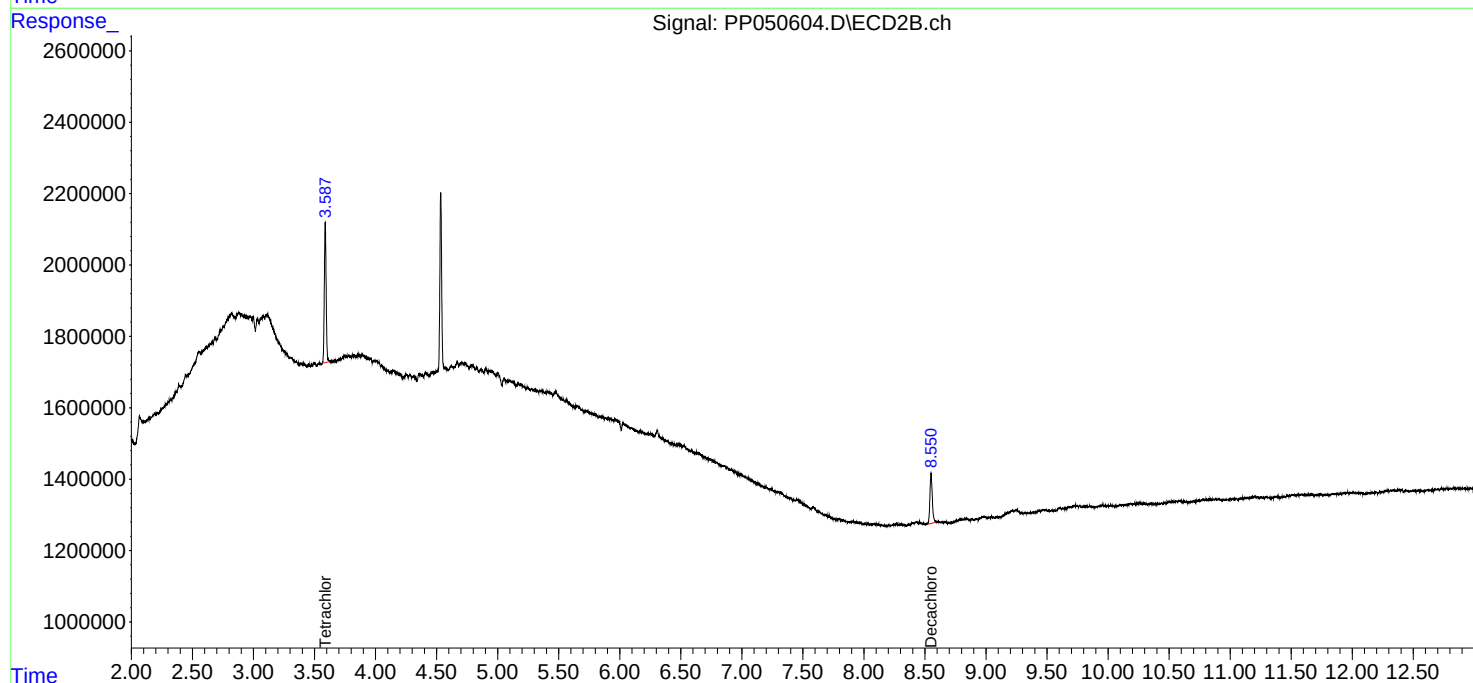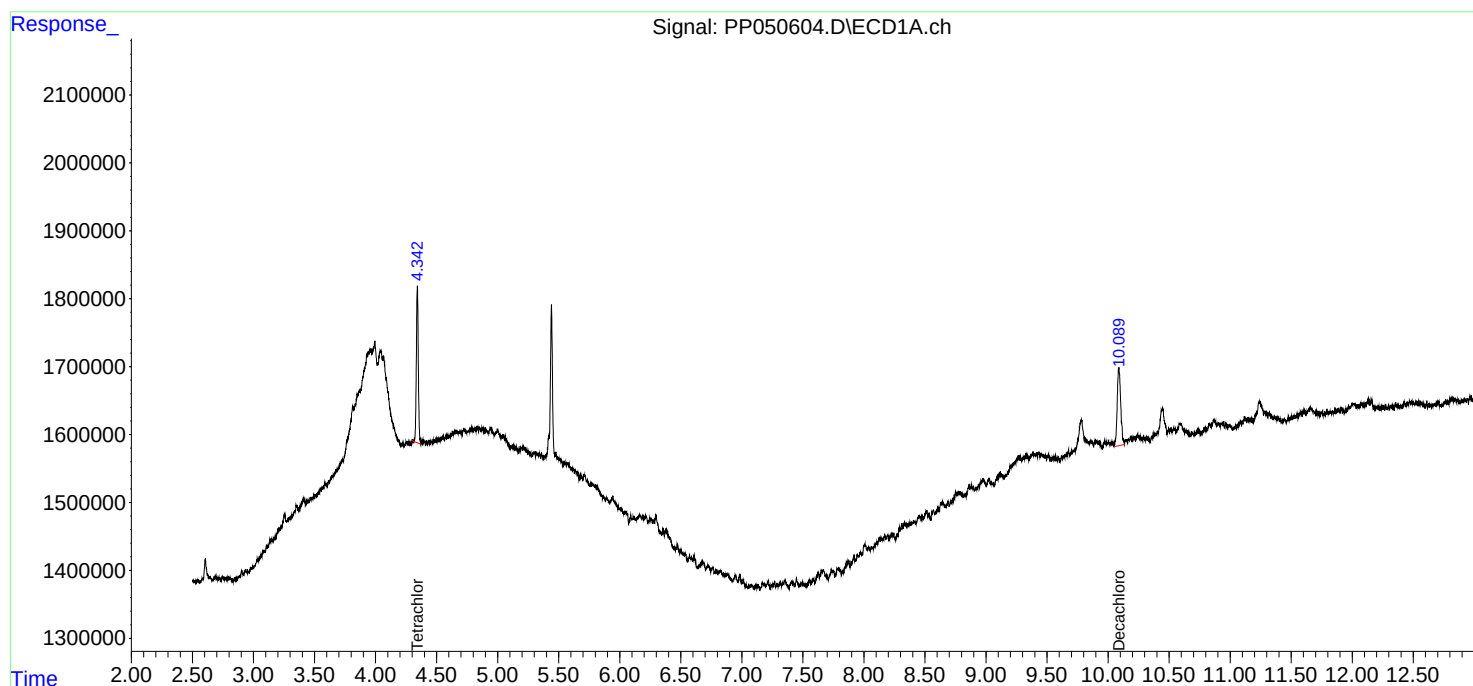

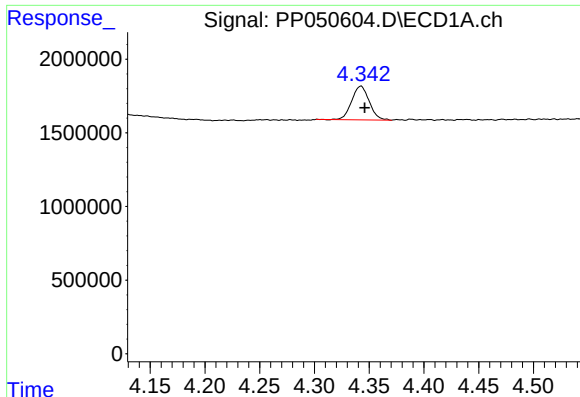


#1 Tetrachloro-m-xylene

R.T.: 4.342 min
Delta R.T.: -0.004 min
Response: 2556561
Conc: 1.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
KMH368K-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/16/2022
Supervised By :Ankita Jodhani 08/16/2022

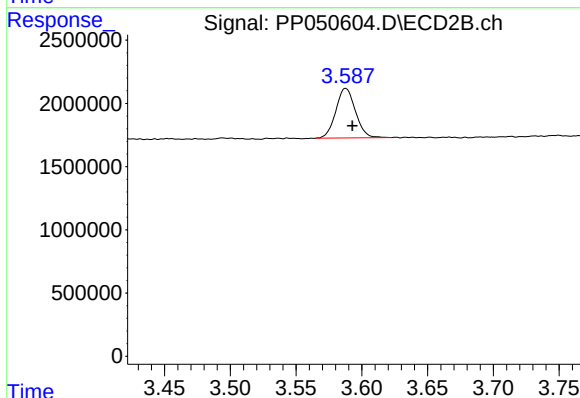


#1 Tetrachloro-m-xylene

R.T.: 3.588 min
Delta R.T.: -0.005 min
Response: 4078296
Conc: 1.30 ng/ml

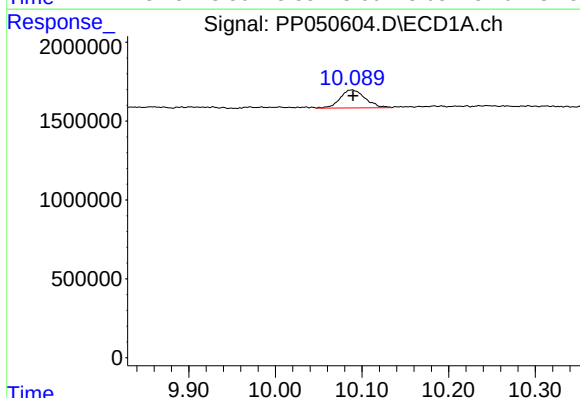

#2 Decachlorobiphenyl

R.T.: 10.089 min
Delta R.T.: 0.000 min
Response: 2298764
Conc: 1.31 ng/ml m

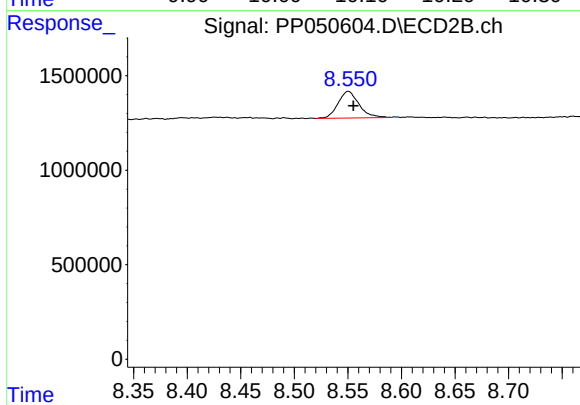

#2 Decachlorobiphenyl

R.T.: 8.550 min
Delta R.T.: -0.005 min
Response: 1920236
Conc: 1.25 ng/ml