

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081525\
Data File : PP074426.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2025 16:00
Operator : YP\AJ
Sample : Q2871-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DRILL CUTTING 1-3 COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 01:52:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Aug 04 11:01:49 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.658	3.801	25012447	77077825	22.366	20.102
2) SA Decachlor...	10.435	8.817	19791775	113.9E6	20.379	18.933

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081525\
Data File : PP074426.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2025 16:00
Operator : YP\AJ
Sample : Q2871-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DRILL CUTTING 1-3 COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 01:52:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Aug 04 11:01:49 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

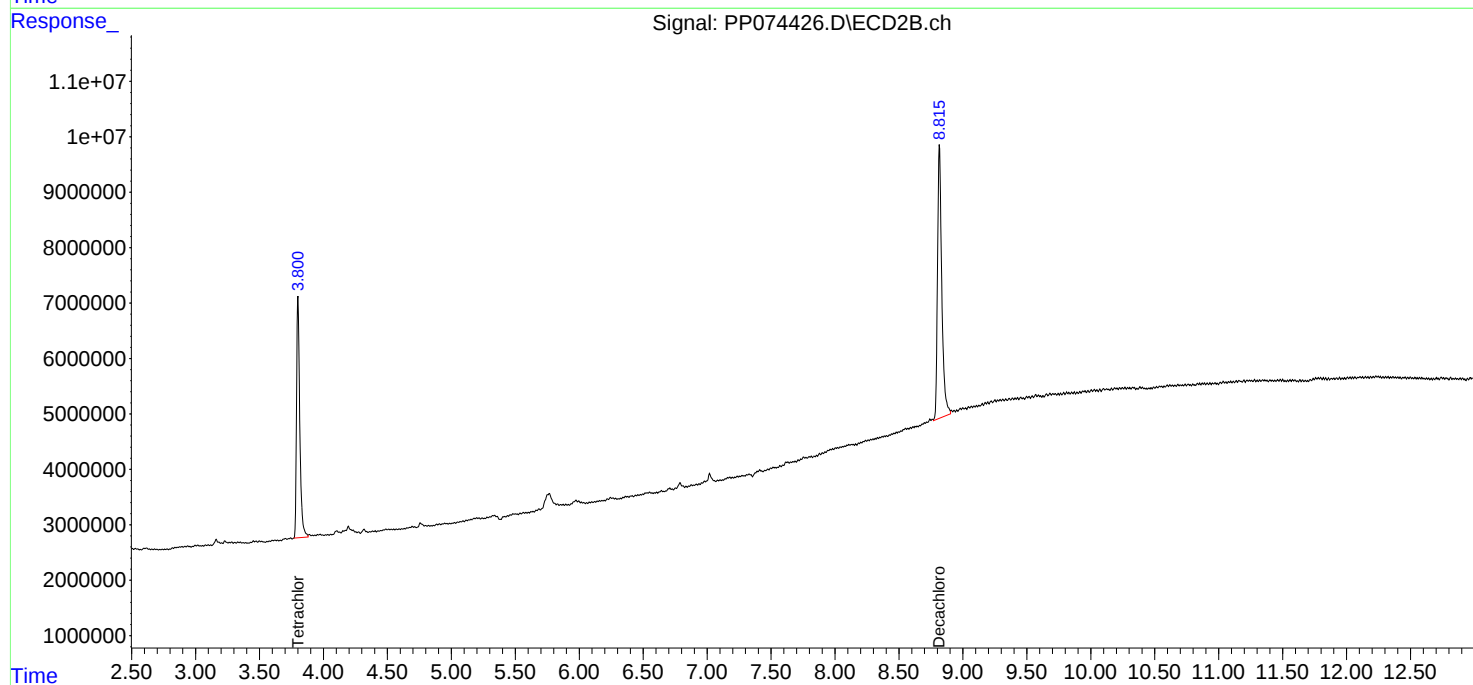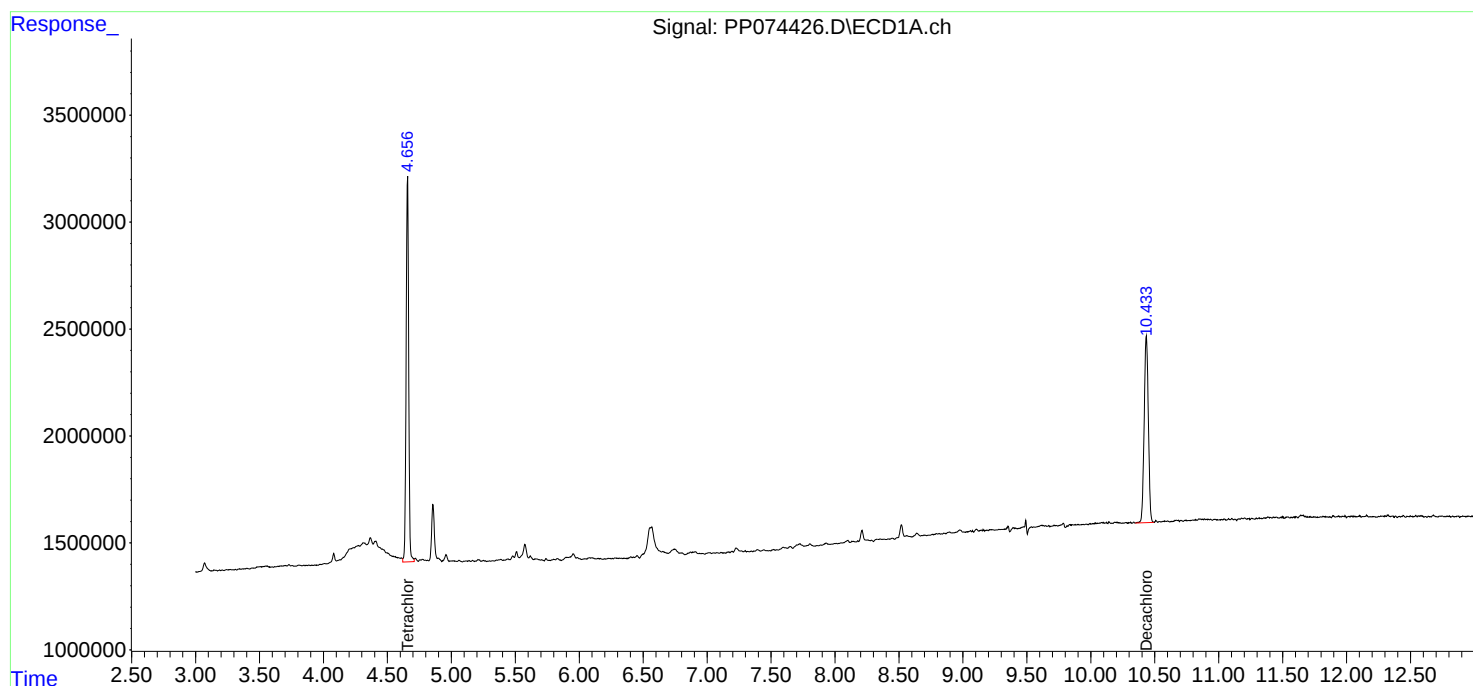


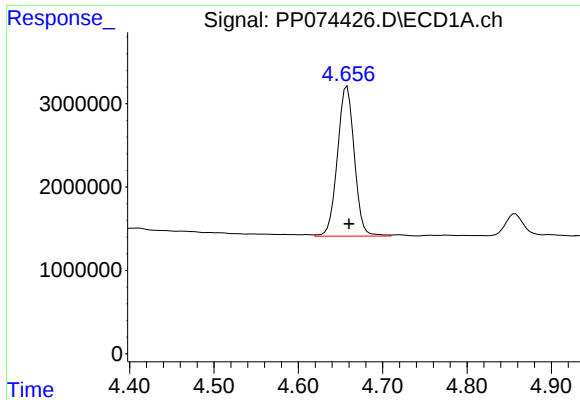

#1 Tetrachloro-m-xylene


R.T.: 4.658 min
Delta R.T.: -0.002 min
Response: 25012447
Conc: 22.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
DRILL CUTTING 1-3 COMP

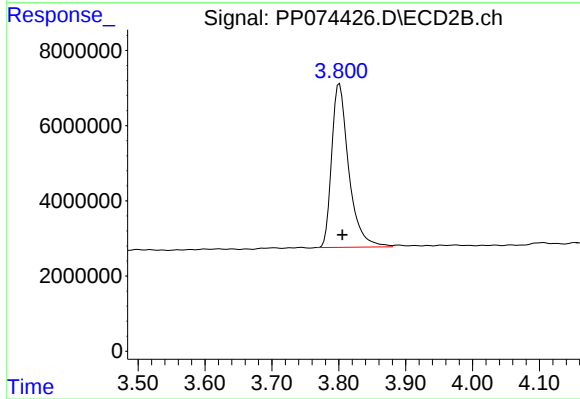


#1 Tetrachloro-m-xylene

R.T.: 3.801 min
Delta R.T.: -0.004 min
Response: 77077825
Conc: 20.10 ng/ml

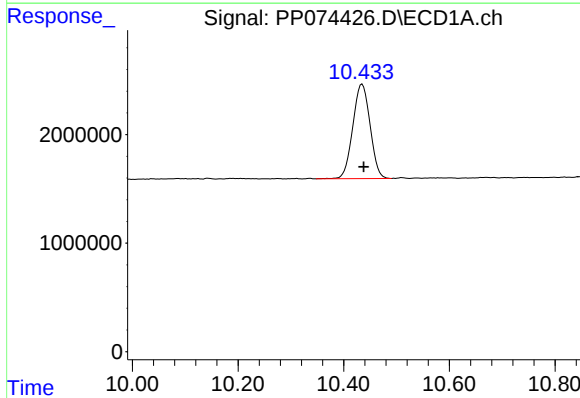

#2 Decachlorobiphenyl

R.T.: 10.435 min
Delta R.T.: -0.003 min
Response: 19791775
Conc: 20.38 ng/ml

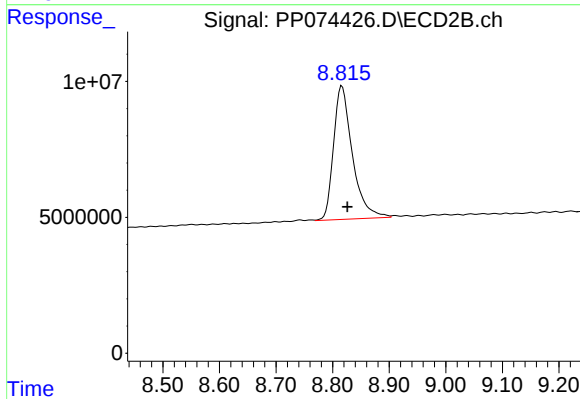

#2 Decachlorobiphenyl

R.T.: 8.817 min
Delta R.T.: -0.009 min
Response: 113856199
Conc: 18.93 ng/ml