

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081525\
Data File : PP074430.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2025 17:05
Operator : YP\AJ
Sample : Q2871-07
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DRILL CUTTING 1-5 COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 01:55:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Aug 04 11:01:49 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.659	3.802	27815556	90659618	24.873	23.644
2) SA Decachlor...	10.436	8.818	21223291	124.0E6	21.854	20.627

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081525\
Data File : PP074430.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2025 17:05
Operator : YP\AJ
Sample : Q2871-07
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DRILL CUTTING 1-5 COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 01:55:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Aug 04 11:01:49 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

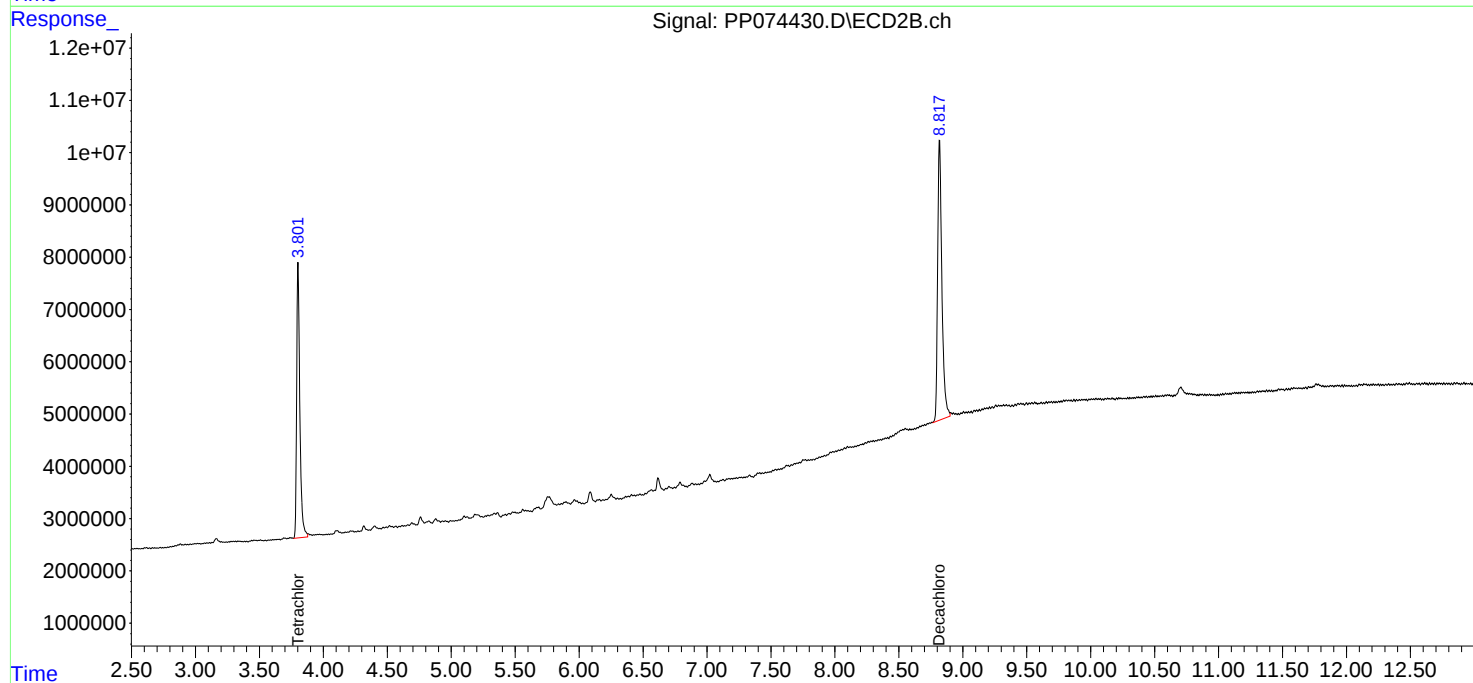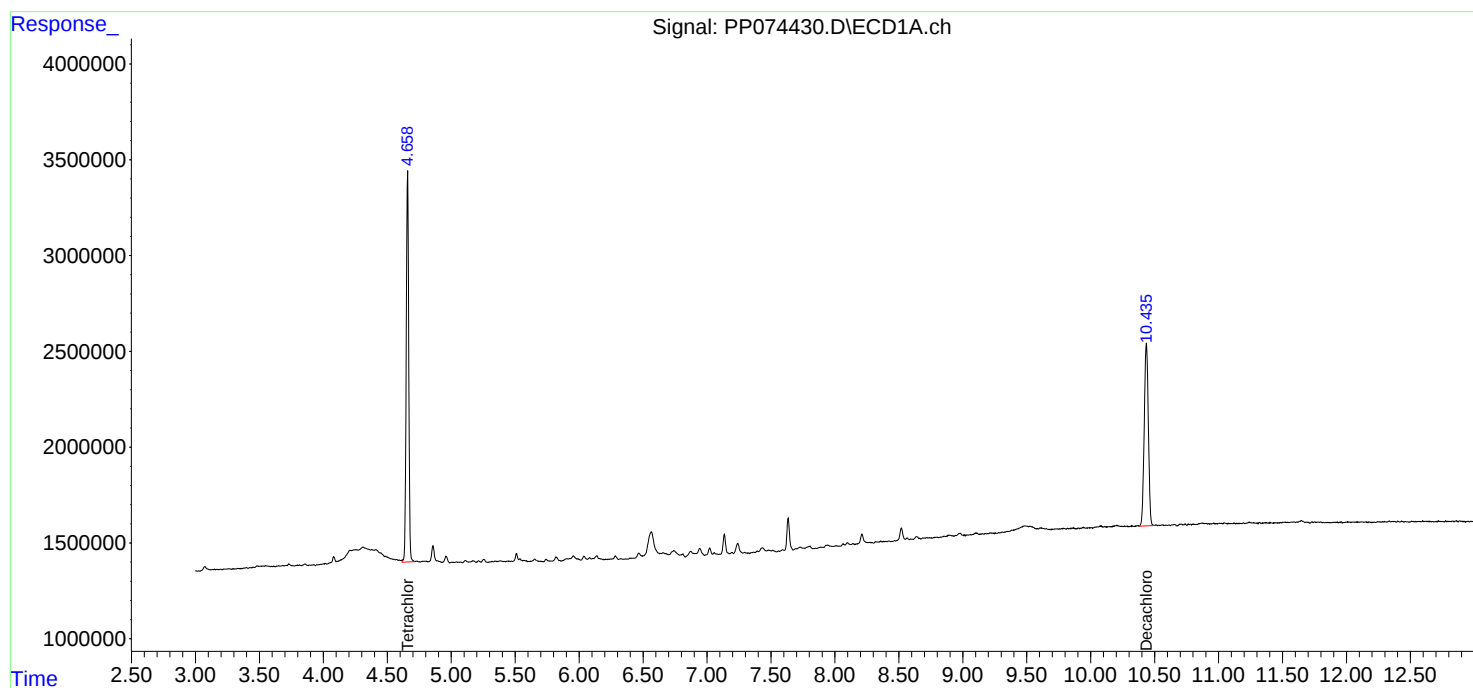


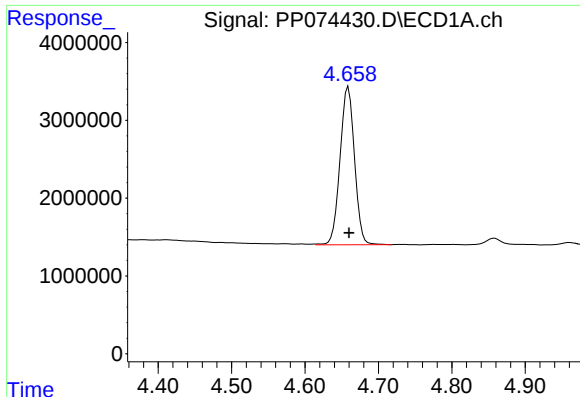

#1 Tetrachloro-m-xylene


R.T.: 4.659 min
Delta R.T.: 0.000 min
Response: 27815556
Conc: 24.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
DRILL CUTTING 1-5 COMP

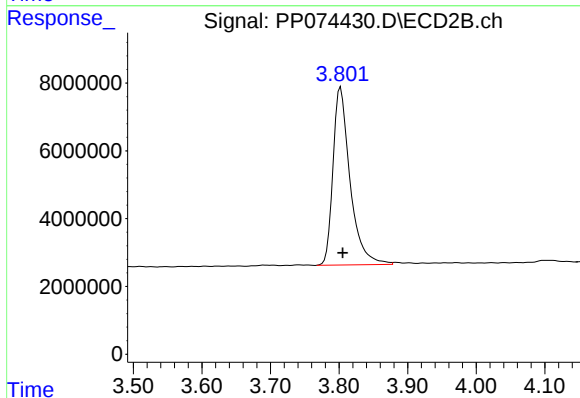


#1 Tetrachloro-m-xylene

R.T.: 3.802 min
Delta R.T.: -0.003 min
Response: 90659618
Conc: 23.64 ng/ml

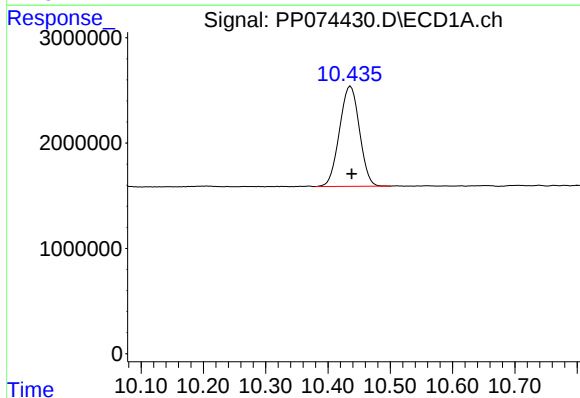

#2 Decachlorobiphenyl

R.T.: 10.436 min
Delta R.T.: -0.002 min
Response: 21223291
Conc: 21.85 ng/ml

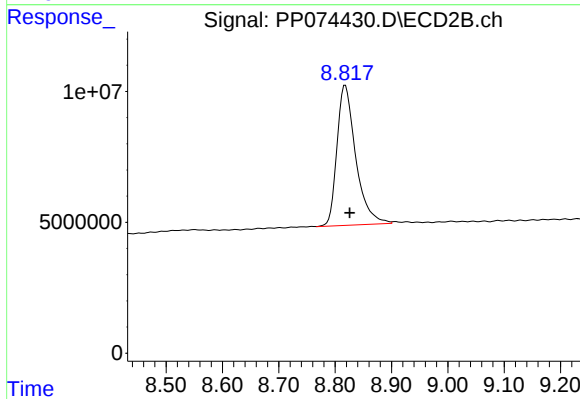

#2 Decachlorobiphenyl

R.T.: 8.818 min
Delta R.T.: -0.008 min
Response: 124043031
Conc: 20.63 ng/ml