

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081525\
 Data File : PP074433.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2025 17:53
 Operator : YP\AJ
 Sample : Q2873-04
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DRILL CUTTING 4-6 COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 01:58:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.659	3.803	25630259	81388133	22.919	21.226
2) SA Decachlor...	10.436	8.817	17504013	99141610	18.024	16.486

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081525\
Data File : PP074433.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2025 17:53
Operator : YP\AJ
Sample : Q2873-04
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DRILL CUTTING 4-6 COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 01:58:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Aug 04 11:01:49 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

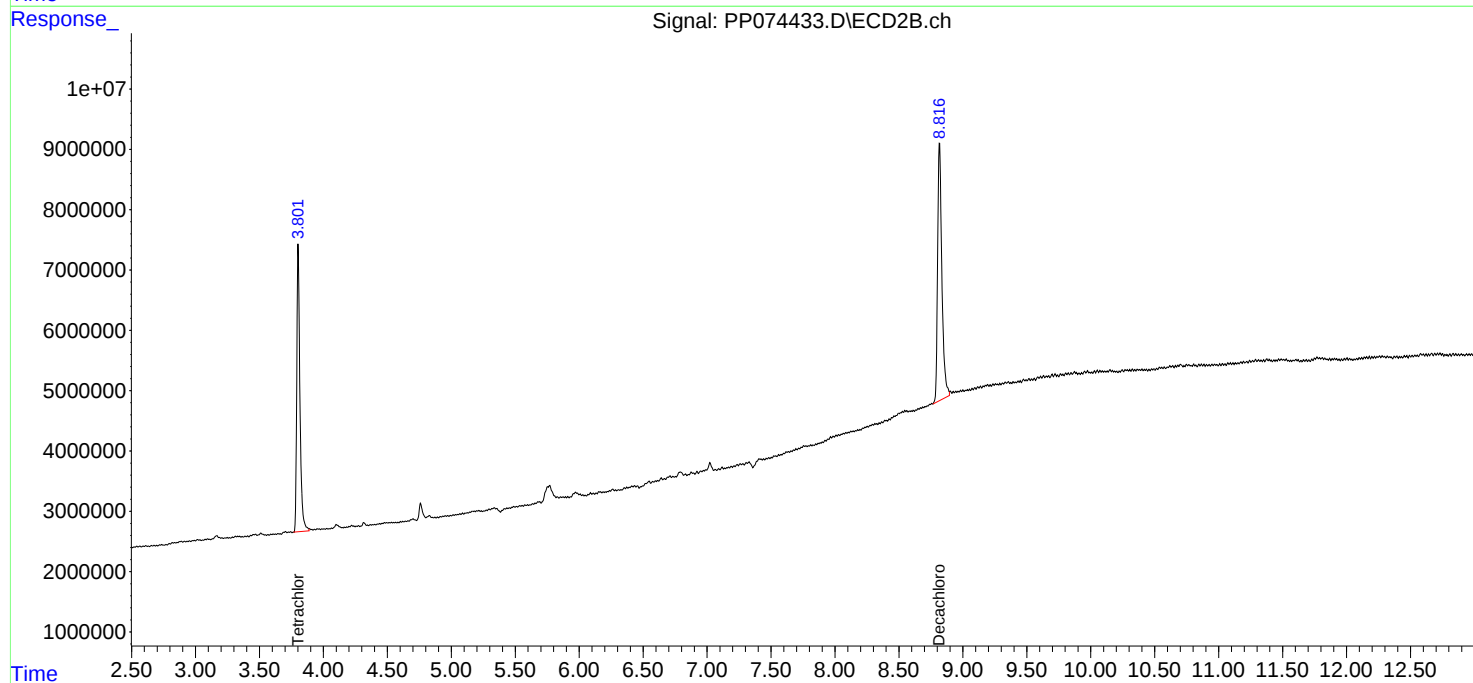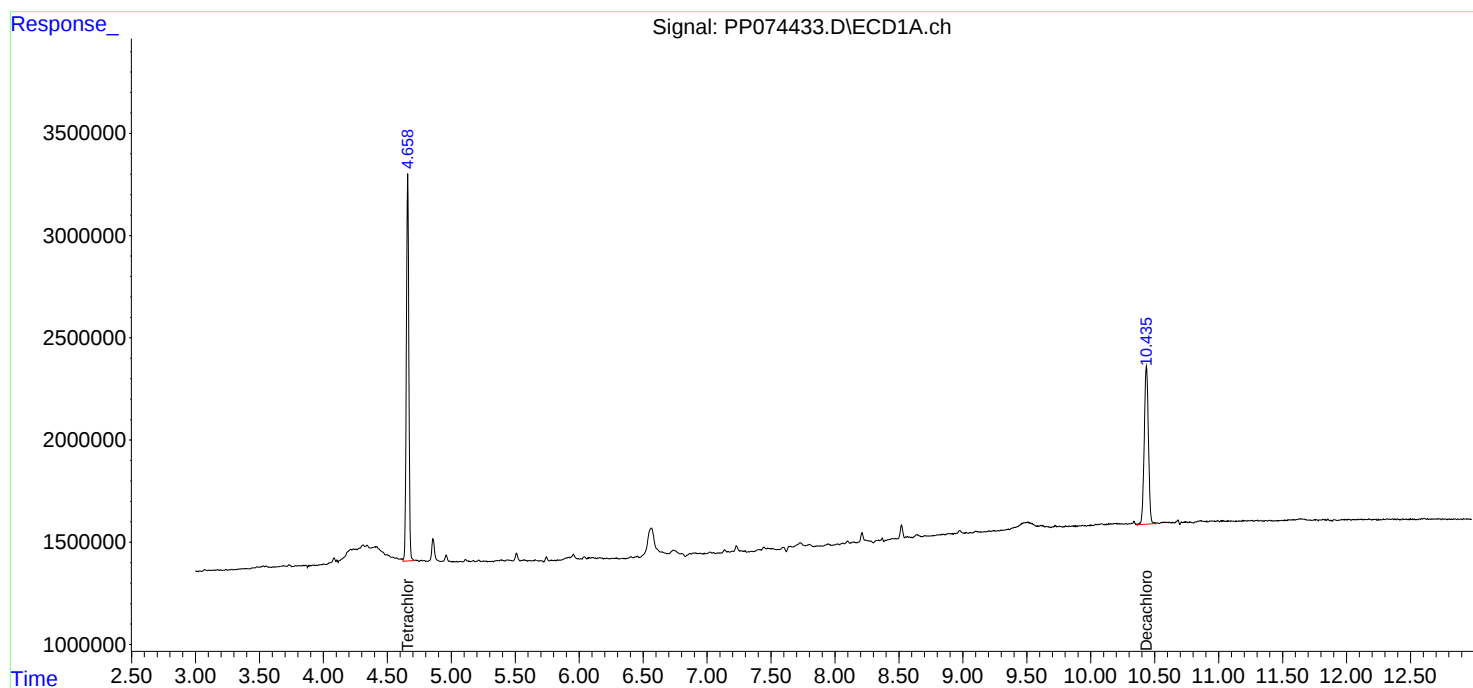


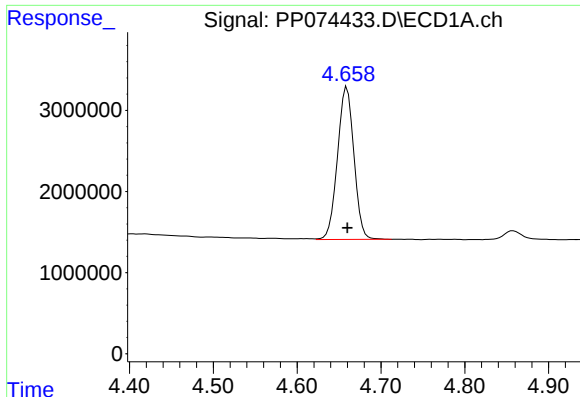

#1 Tetrachloro-m-xylene


R.T.: 4.659 min
Delta R.T.: 0.000 min
Response: 25630259
Conc: 22.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
DRILL CUTTING 4-6 COMP

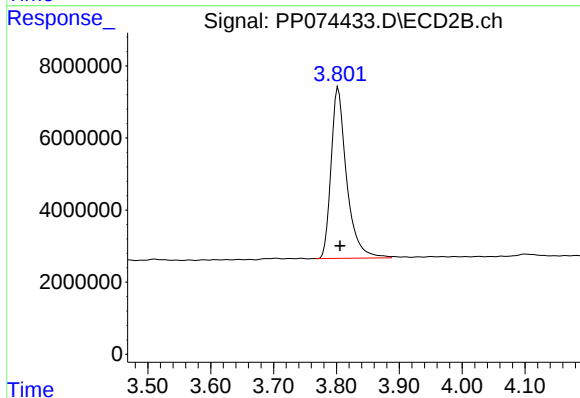


#1 Tetrachloro-m-xylene

R.T.: 3.803 min
Delta R.T.: -0.003 min
Response: 81388133
Conc: 21.23 ng/ml

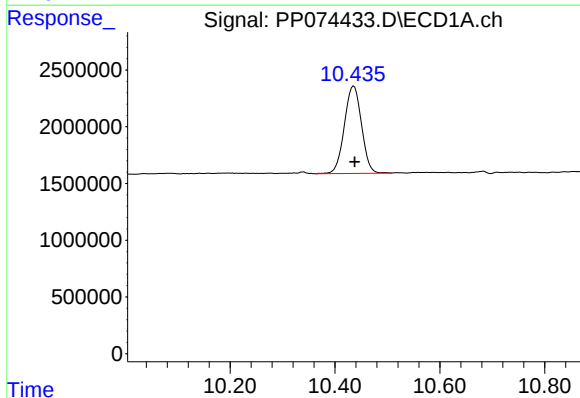

#2 Decachlorobiphenyl

R.T.: 10.436 min
Delta R.T.: -0.002 min
Response: 17504013
Conc: 18.02 ng/ml

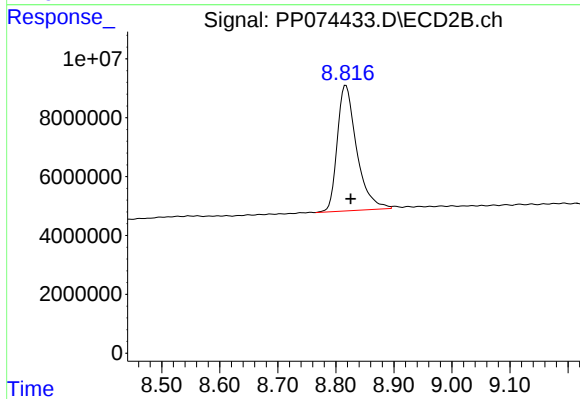

#2 Decachlorobiphenyl

R.T.: 8.817 min
Delta R.T.: -0.008 min
Response: 99141610
Conc: 16.49 ng/ml