

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081621\
 Data File : PP038441.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Aug 2021 19:24
 Operator : AJ\MA
 Sample : M3398-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 2021-08-10-FD-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 02:20:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 06 03:08:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.888	3.873	1031050	606069	23.200	23.532
2) SA Decachlor...	10.874	9.135	551973	560983	24.264	21.682
Target Compounds						
8) L2 AR-1221-1	5.139	0.000	78738	0	145.263	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081621\
Data File : PP038441.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Aug 2021 19:24
Operator : AJ\MA
Sample : M3398-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
2021-08-10-FD-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 02:20:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 06 03:08:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

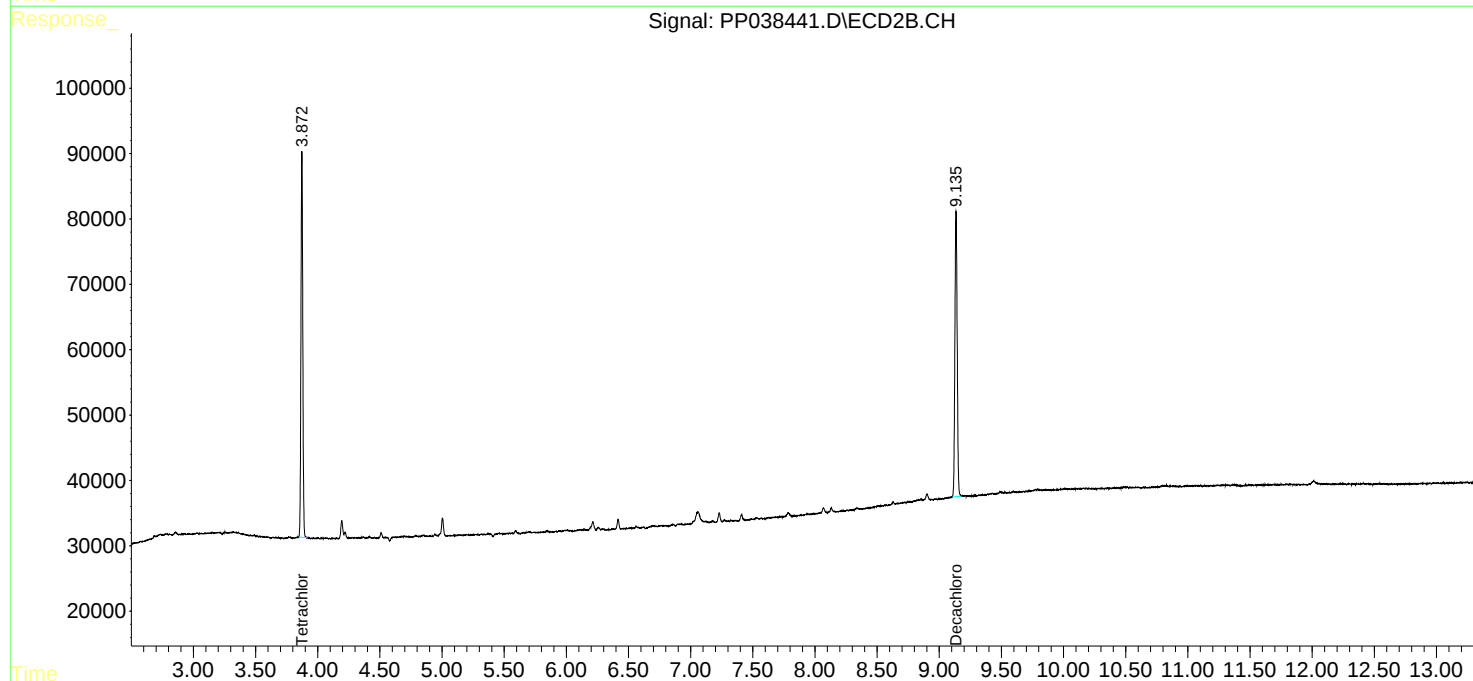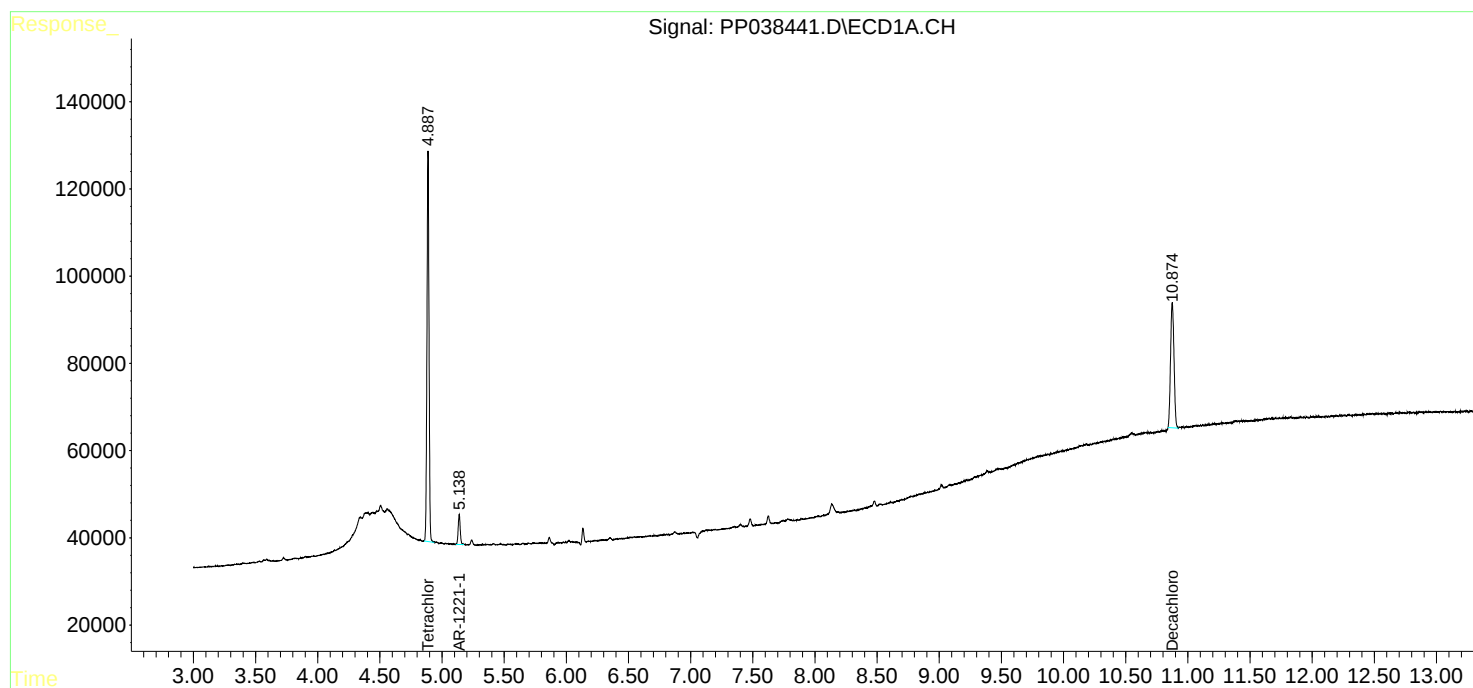


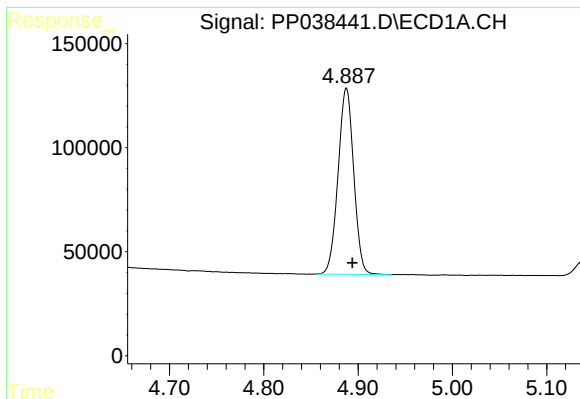

#1 Tetrachloro-m-xylene


R.T.: 4.888 min
Delta R.T.: -0.006 min
Response: 1031050
Conc: 23.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
2021-08-10-FD-01

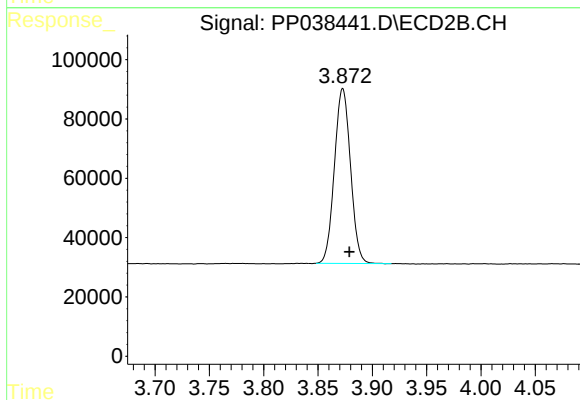


#1 Tetrachloro-m-xylene

R.T.: 3.873 min
Delta R.T.: -0.006 min
Response: 606069
Conc: 23.53 ng/ml

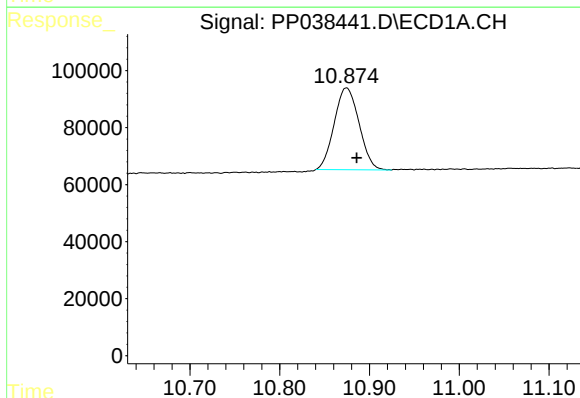


#2 Decachlorobiphenyl

R.T.: 10.874 min
Delta R.T.: -0.011 min
Response: 551973
Conc: 24.26 ng/ml

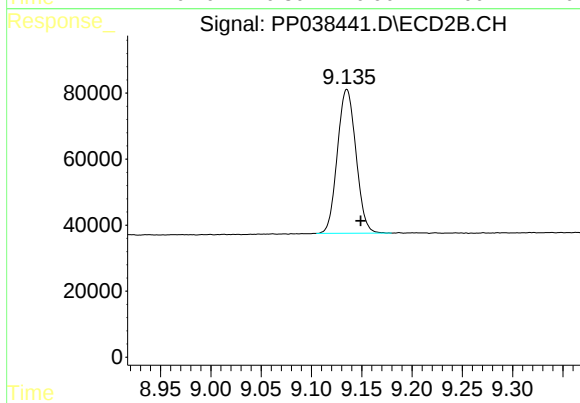

#2 Decachlorobiphenyl


R.T.: 9.135 min
Delta R.T.: -0.014 min
Response: 560983
Conc: 21.68 ng/ml

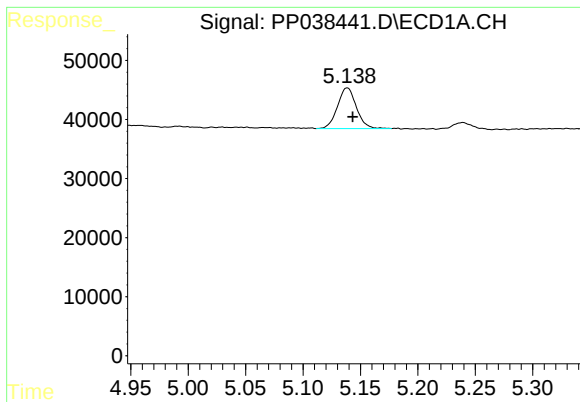

#8 AR-1221-1

R.T.: 5.139 min
Delta R.T.: -0.005 min
Response: 78738
Conc: 145.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
2021-08-10-FD-01

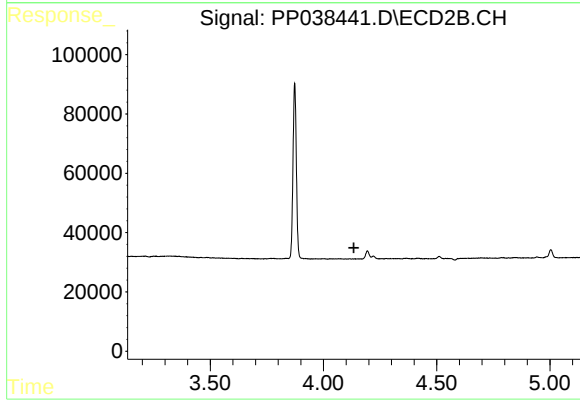

#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.134 min
Response: 0
Conc: N.D.