

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081621\
 Data File : PP038472.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Aug 2021 4:59
 Operator : AJ\MA
 Sample : M3398-17
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SWCS-04-0205

Manual Integrations
 APPROVED

mohammad
 8/17/2021 12:42:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 06:20:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 06 03:08:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.887	3.872	928154	560069	20.885	21.746
2) SA Decachlor...	10.870f	9.133f	454824	410007	19.994m	15.847

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081621\
Data File : PP038472.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Aug 2021 4:59
Operator : AJ\MA
Sample : M3398-17
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SWCS-04-0205


Manual Integrations
APPROVED

mohammad
8/17/2021 12:42:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 06:20:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080521.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 06 03:08:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

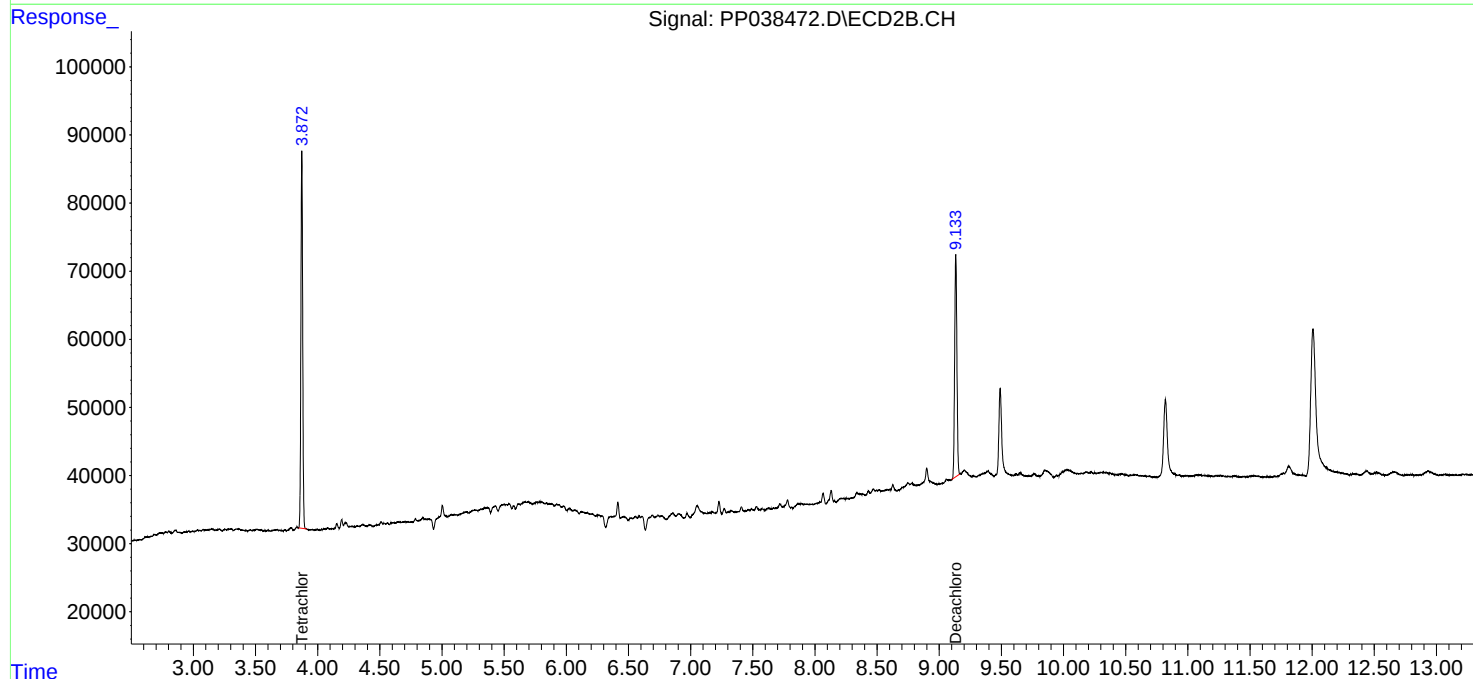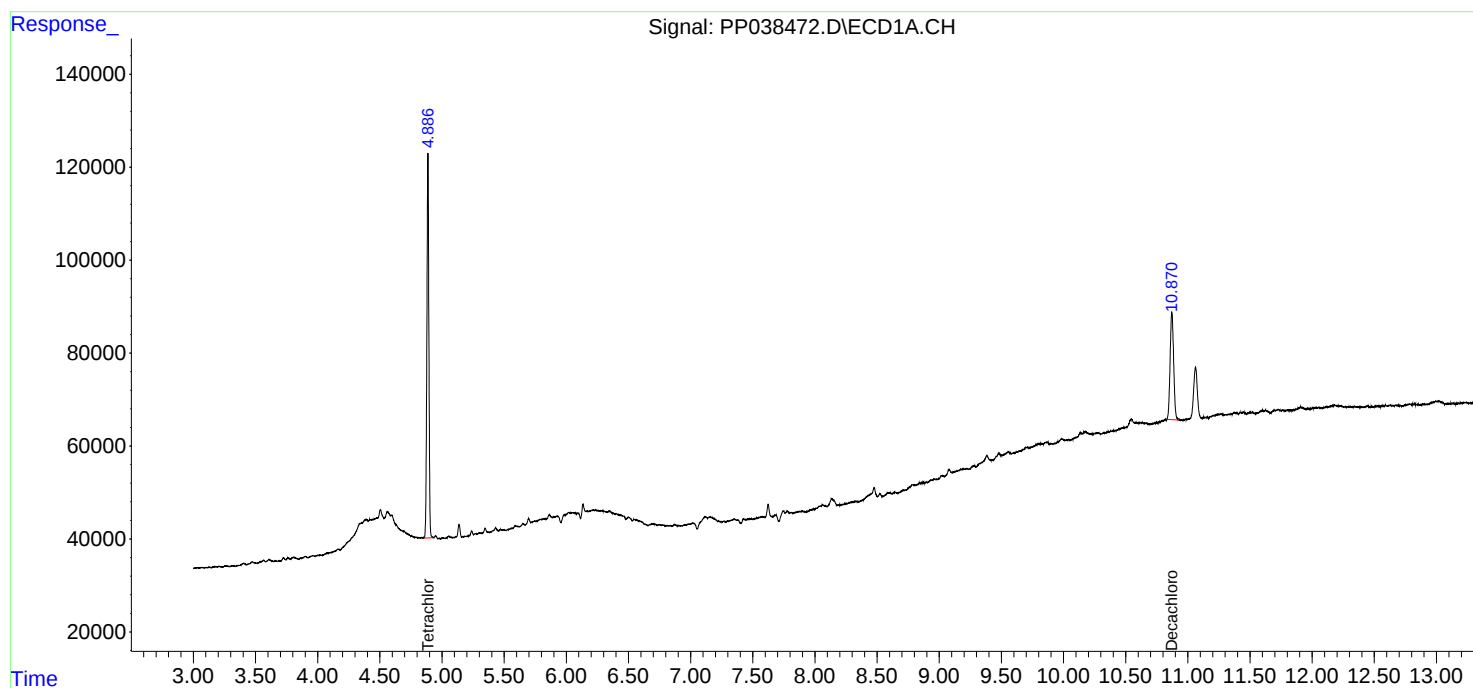

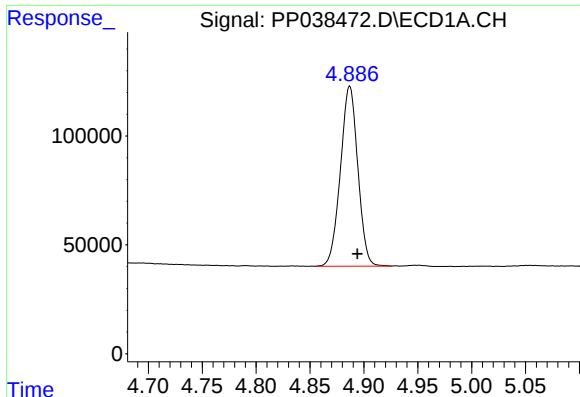


#1 Tetrachloro-m-xylene

R.T.: 4.887 min
Delta R.T.: -0.007 min
Response: 928154
Conc: 20.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
SWCS-04-0205


Manual Integrations
APPROVED

mohammad
8/17/2021 12:42:52 PM

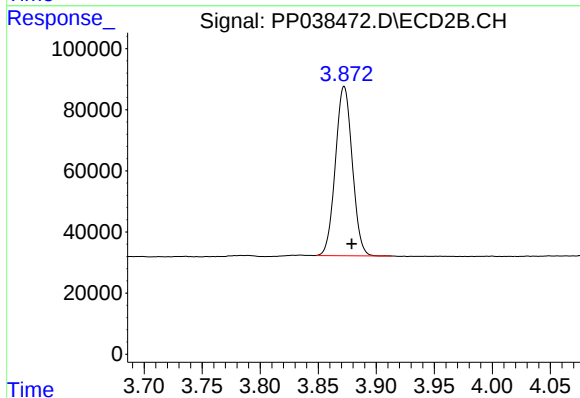


#1 Tetrachloro-m-xylene

R.T.: 3.872 min
Delta R.T.: -0.007 min
Response: 560069
Conc: 21.75 ng/ml

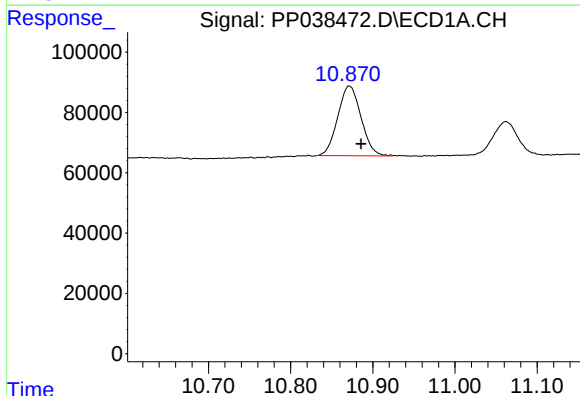

#2 Decachlorobiphenyl

R.T.: 10.870 min
Delta R.T.: -0.016 min
Response: 454824
Conc: 19.99 ng/ml m

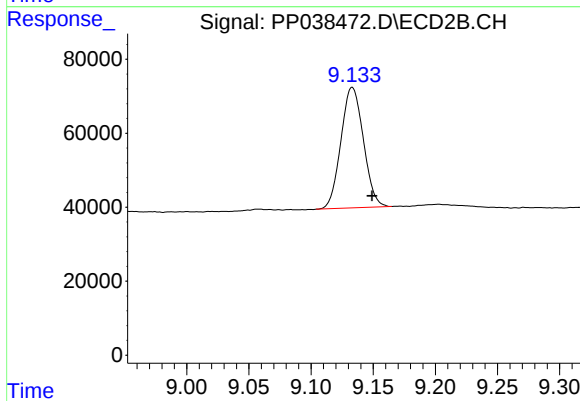

#2 Decachlorobiphenyl

R.T.: 9.133 min
Delta R.T.: -0.016 min
Response: 410007
Conc: 15.85 ng/ml