

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081722\
 Data File : PP050645.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2022 14:27
 Operator : YP\AJ
 Sample : N4214-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 ETGI-354

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/18/2022
 Supervised By :Ankita Jodhani 08/18/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 03:38:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 09 11:38:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.344	3.589	33447332	66194434	20.779	21.133
2) SA Decachlor...	10.089	8.551	33020164	28681883	18.752m	18.636m
Target Compounds						
31) L7 AR-1260-1	7.127	6.132	4161587	6416523	45.566	56.624m
32) L7 AR-1260-2	7.384	6.322	10105679	7250384	88.453	53.970m#
33) L7 AR-1260-3	7.741	6.472	3454180	5485349	40.563	45.535
34) L7 AR-1260-4	7.970	6.942	4957254	4515447	52.079m	50.937
35) L7 AR-1260-5	8.293	7.183	7899933	8794061	42.262	45.112

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081722\
Data File : PP050645.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2022 14:27
Operator : YP\AJ
Sample : N4214-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
ETGI-354


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/18/2022
Supervised By :Ankita Jodhani 08/18/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 03:38:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 09 11:38:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

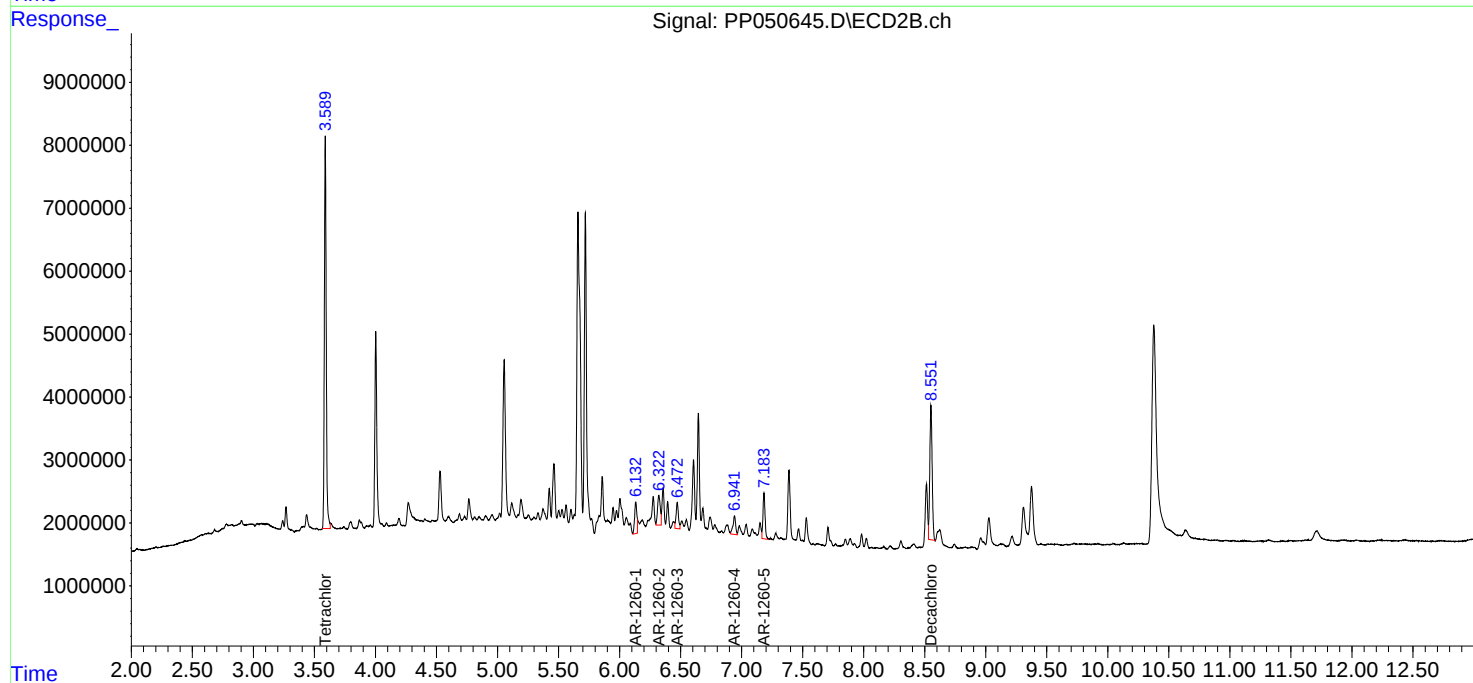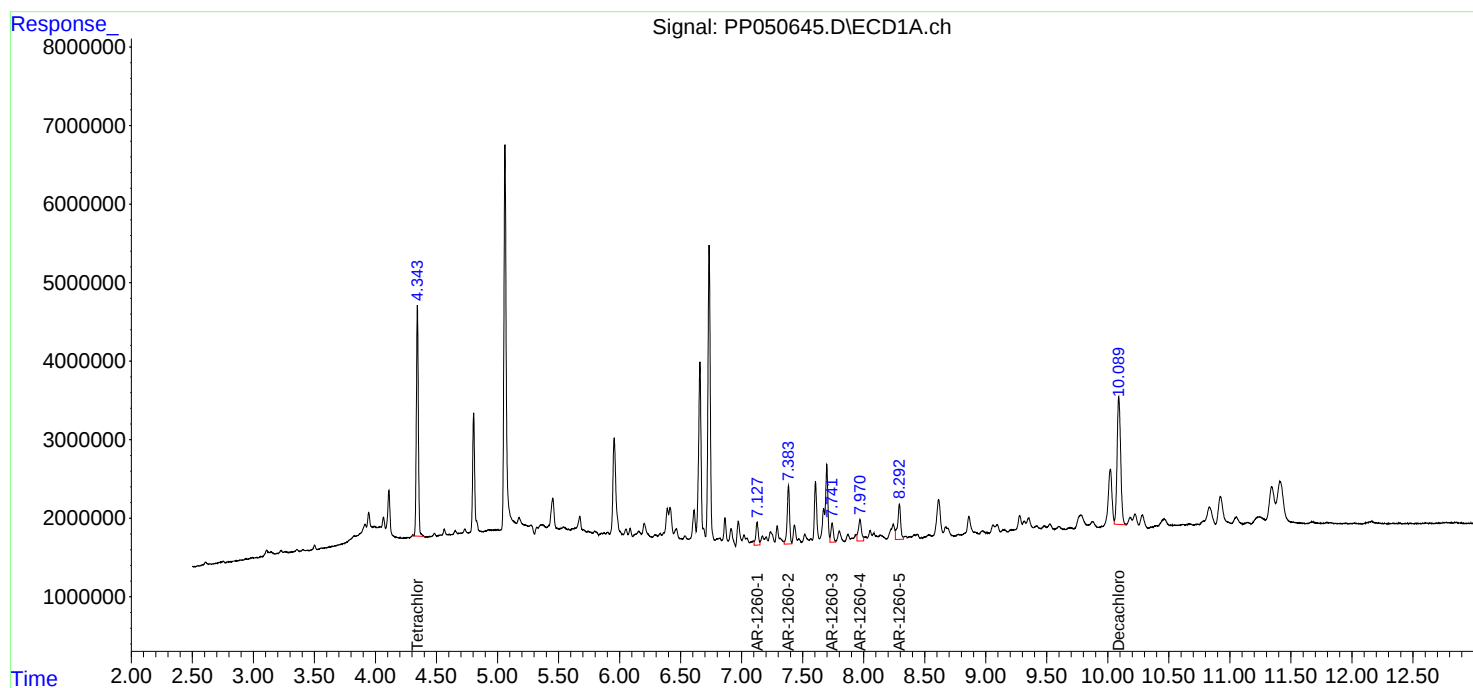

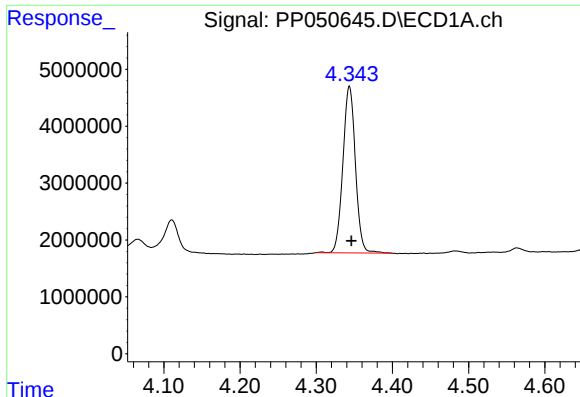


#1 Tetrachloro-m-xylene

R.T.: 4.344 min
Delta R.T.: -0.002 min
Response: 33447332
Conc: 20.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
ETGI-354


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/18/2022
Supervised By :Ankita Jodhani 08/18/2022

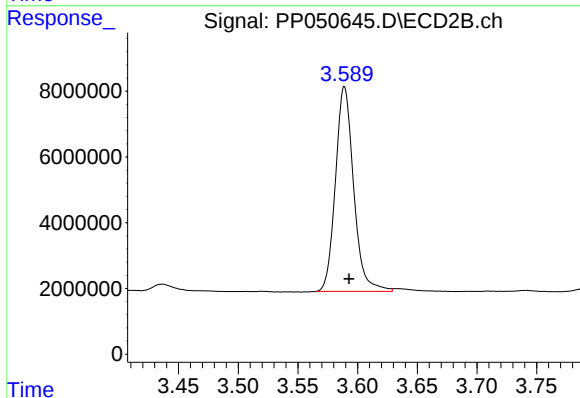


#1 Tetrachloro-m-xylene

R.T.: 3.589 min
Delta R.T.: -0.004 min
Response: 66194434
Conc: 21.13 ng/ml

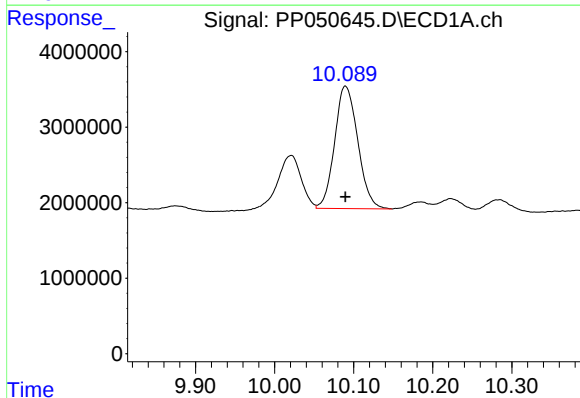


#2 Decachlorobiphenyl

R.T.: 10.089 min
Delta R.T.: 0.000 min
Response: 33020164
Conc: 18.75 ng/ml m

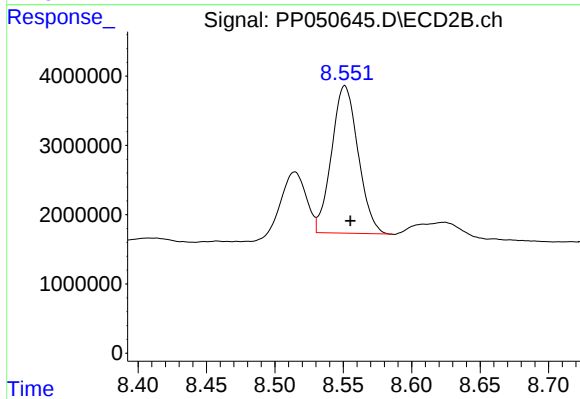

#2 Decachlorobiphenyl

R.T.: 8.551 min
Delta R.T.: -0.004 min
Response: 28681883
Conc: 18.64 ng/ml m

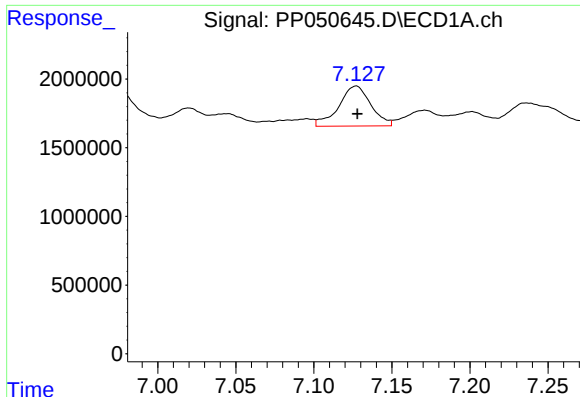


#31 AR-1260-1

R.T.: 7.127 min
Delta R.T.: 0.000 min
Response: 4161587
Conc: 45.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
ETGI-354


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/18/2022
Supervised By :Ankita Jodhani 08/18/2022

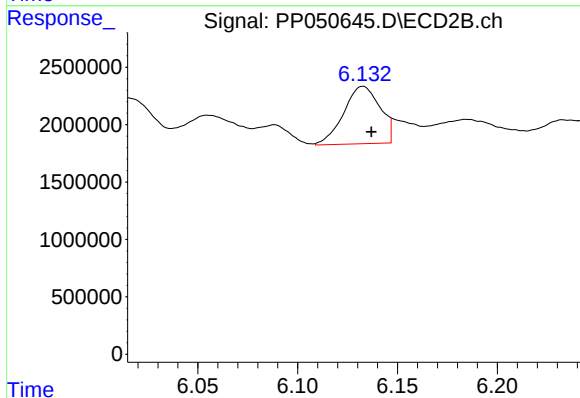


#31 AR-1260-1

R.T.: 6.132 min
Delta R.T.: -0.005 min
Response: 6416523
Conc: 56.62 ng/ml m

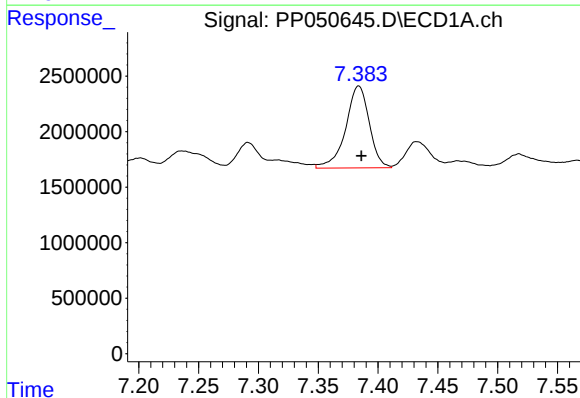


#32 AR-1260-2

R.T.: 7.384 min
Delta R.T.: -0.002 min
Response: 10105679
Conc: 88.45 ng/ml

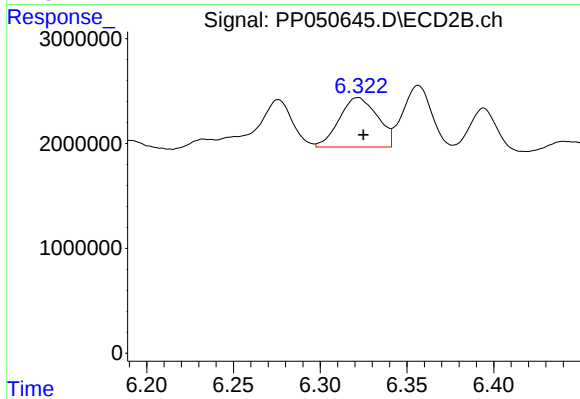

#32 AR-1260-2

R.T.: 6.322 min
Delta R.T.: -0.003 min
Response: 7250384
Conc: 53.97 ng/ml m

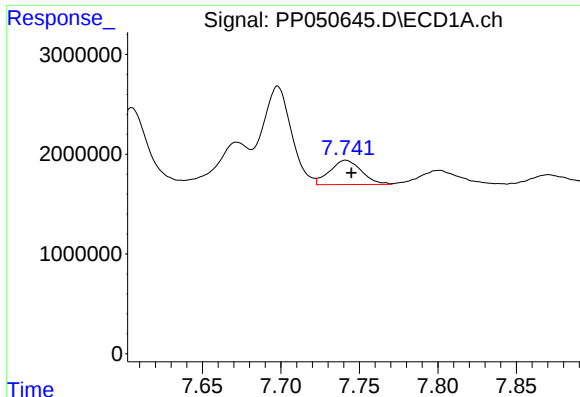


#33 AR-1260-3

R.T.: 7.741 min
Delta R.T.: -0.004 min
Response: 3454180
Conc: 40.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
ETGI-354


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/18/2022
Supervised By :Ankita Jodhani 08/18/2022

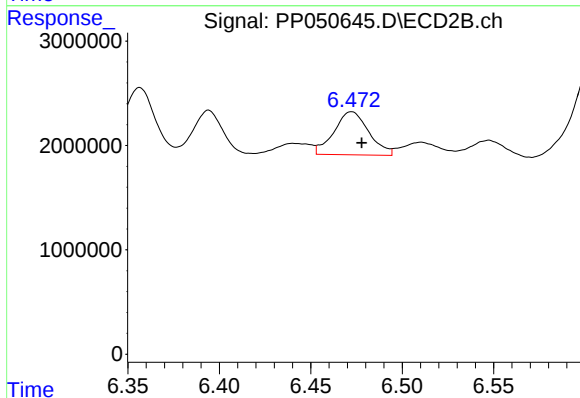


#33 AR-1260-3

R.T.: 6.472 min
Delta R.T.: -0.006 min
Response: 5485349
Conc: 45.54 ng/ml

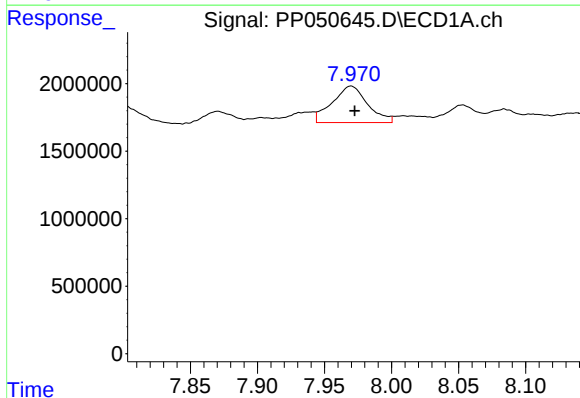


#34 AR-1260-4

R.T.: 7.970 min
Delta R.T.: -0.003 min
Response: 4957254
Conc: 52.08 ng/ml m

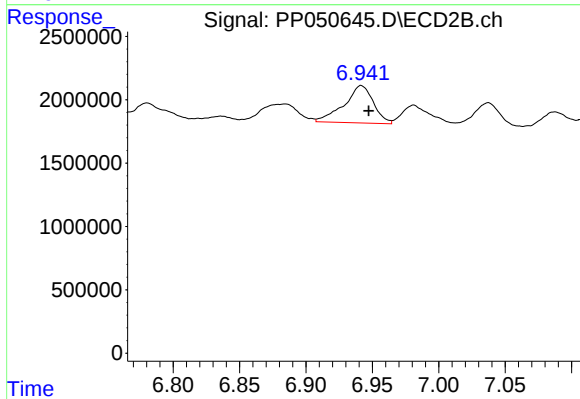

#34 AR-1260-4

R.T.: 6.942 min
Delta R.T.: -0.006 min
Response: 4515447
Conc: 50.94 ng/ml

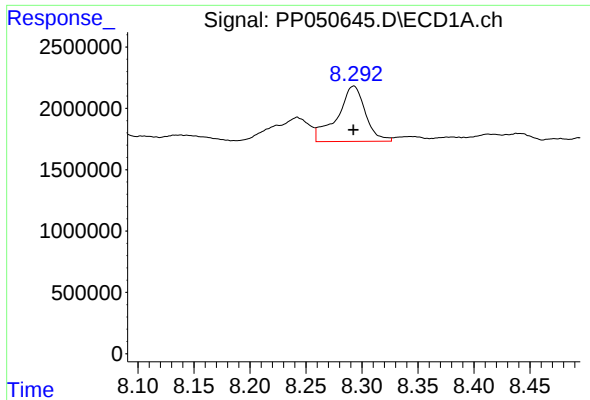


#35 AR-1260-5

R.T.: 8.293 min
Delta R.T.: 0.000 min
Response: 7899933
Conc: 42.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
ETGI-354

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/18/2022
Supervised By :Ankita Jodhani 08/18/2022

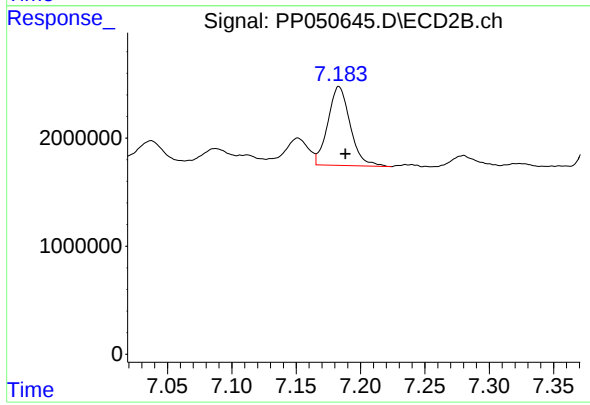

#35 AR-1260-5

R.T.: 7.183 min
Delta R.T.: -0.005 min
Response: 8794061
Conc: 45.11 ng/ml