

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081723\
 Data File : PP059393.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2023 19:05
 Operator : YP\AJ
 Sample : 04056-19
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 P001-SS023-0002-01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/18/2023
 Supervised By :Ankita Jodhani 08/18/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 01:23:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.414	3.644	24050198	42081757	19.600	20.769
2) SA Decachlor...	10.202	8.676	13141434	24679993	17.218	17.543

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081723\
Data File : PP059393.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2023 19:05
Operator : YP\AJ
Sample : 04056-19
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
P001-SS023-0002-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/18/2023
Supervised By :Ankita Jodhani 08/18/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 01:23:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 09 02:30:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

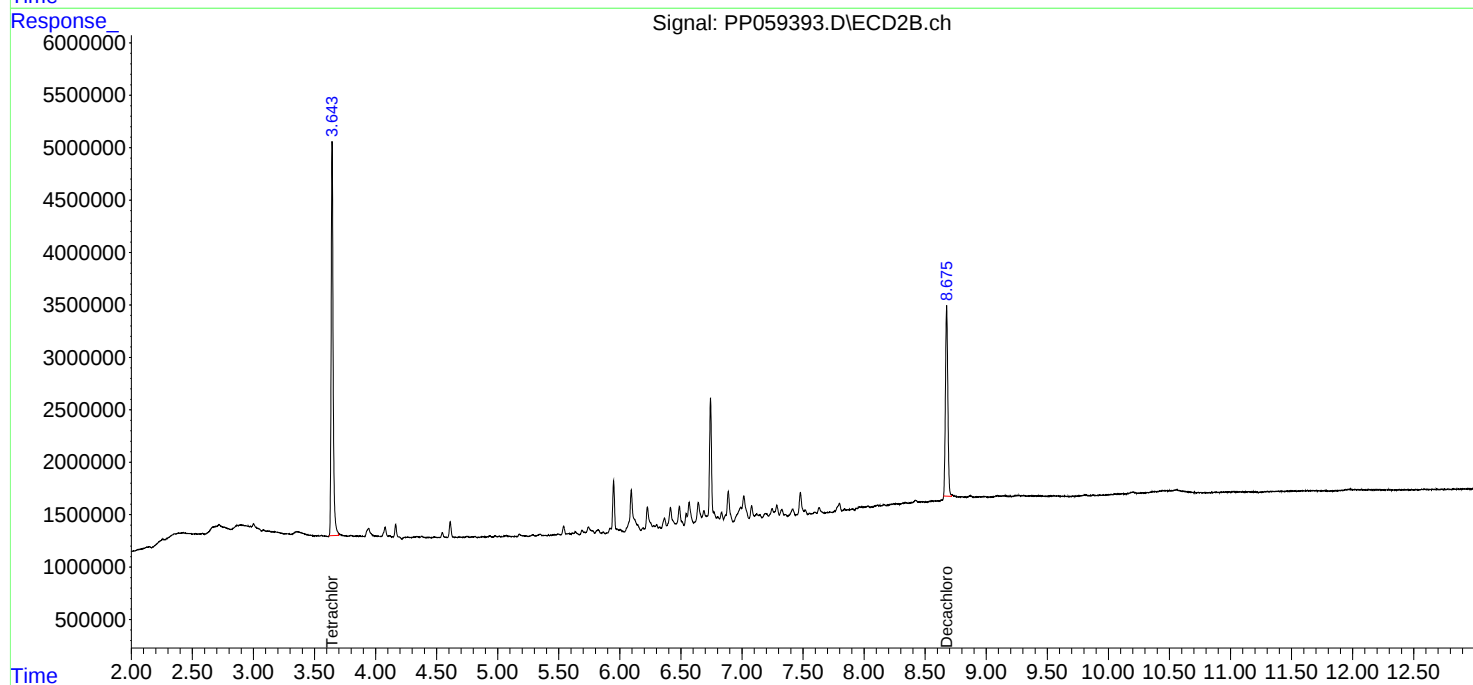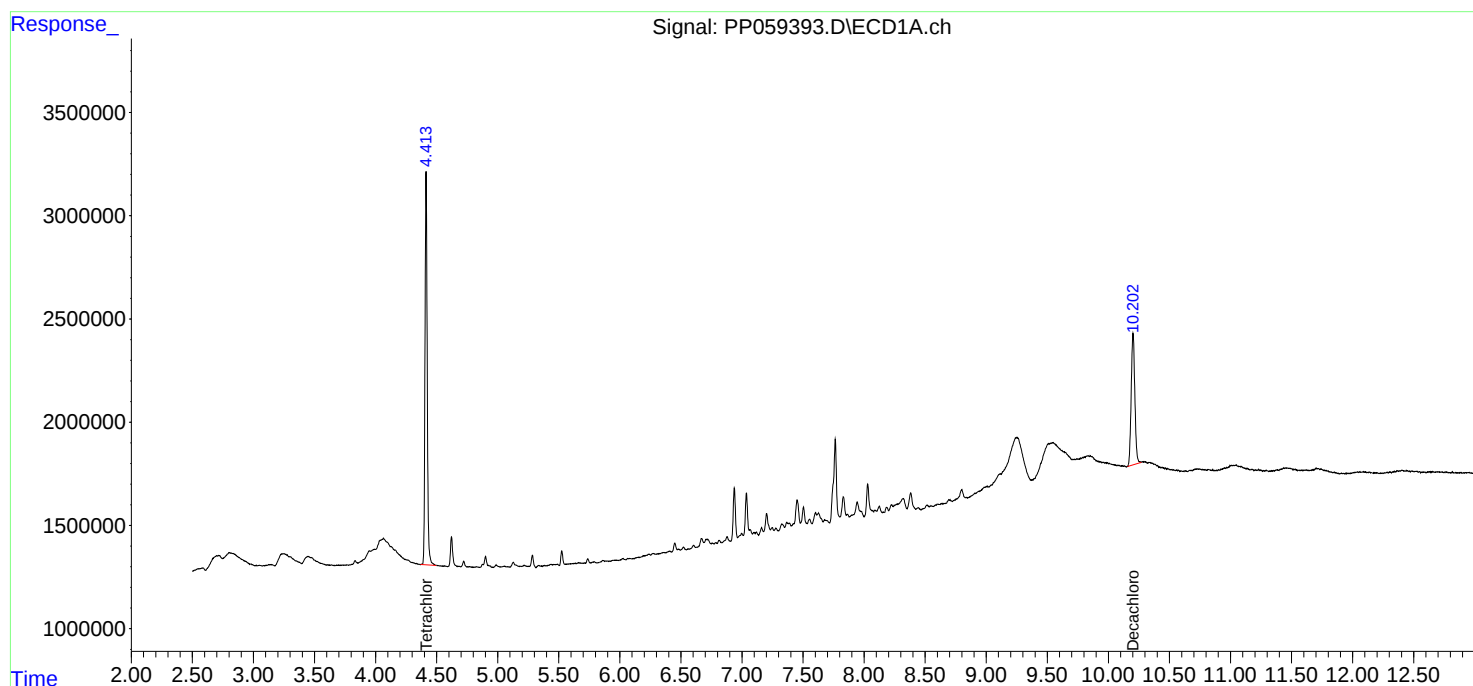

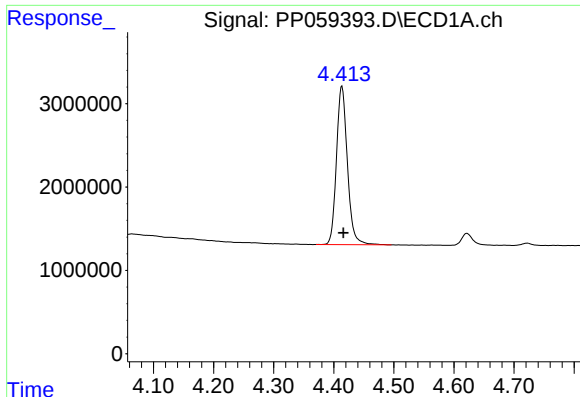


#1 Tetrachloro-m-xylene

R.T.: 4.414 min
Delta R.T.: -0.002 min
Response: 24050198
Conc: 19.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
P001-SS023-0002-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/18/2023
Supervised By :Ankita Jodhani 08/18/2023

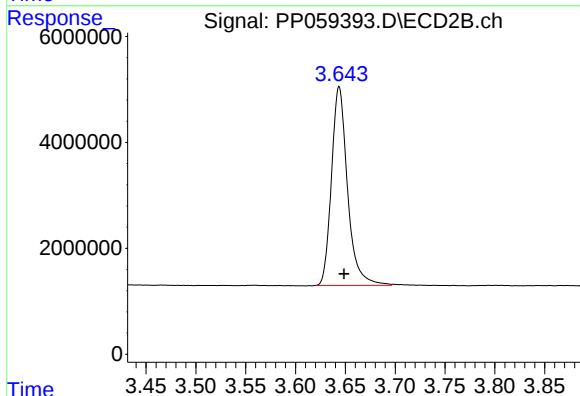


#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: -0.005 min
Response: 42081757
Conc: 20.77 ng/ml

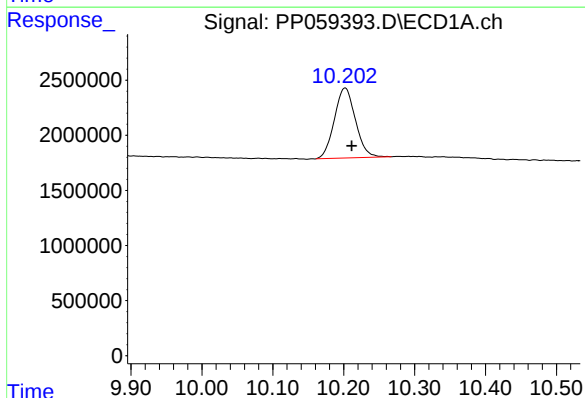

#2 Decachlorobiphenyl

R.T.: 10.202 min
Delta R.T.: -0.009 min
Response: 13141434
Conc: 17.22 ng/ml

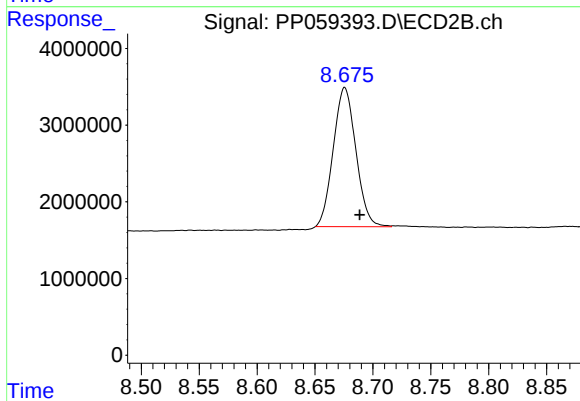

#2 Decachlorobiphenyl

R.T.: 8.676 min
Delta R.T.: -0.013 min
Response: 24679993
Conc: 17.54 ng/ml