

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081821\
 Data File : PP038560.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Aug 2021 21:03
 Operator : AJ\MA
 Sample : M3435-29
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 02:55:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 18 04:51:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.885	3.871	438554	260801	10.867	10.883
2)	SA Decachlor...	10.871	9.130	99887	98157	4.060	4.030
Target Compounds							
8)	L2 AR-1221-1	5.137	0.000	76151	0	162.835	N.D. #
28)	L6 AR-1254-3	7.743f	0.000	30915	0	17.221	N.D. #
32)	L7 AR-1260-2	8.154	0.000	46443	0	31.655	N.D. #
35)	L7 AR-1260-5	9.073	0.000	15172	0	6.761	N.D. #
37)	L8 AR-1262-2	9.073	0.000	15172	0	5.699	N.D. #
38)	L8 AR-1262-3	0.000	8.062	0	26967	N.D.	21.464 #
41)	L9 AR-1268-1	0.000	8.062	0	26967	N.D.	7.385 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081821\
Data File : PP038560.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Aug 2021 21:03
Operator : AJ\MA
Sample : M3435-29
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 02:55:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 18 04:51:26 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

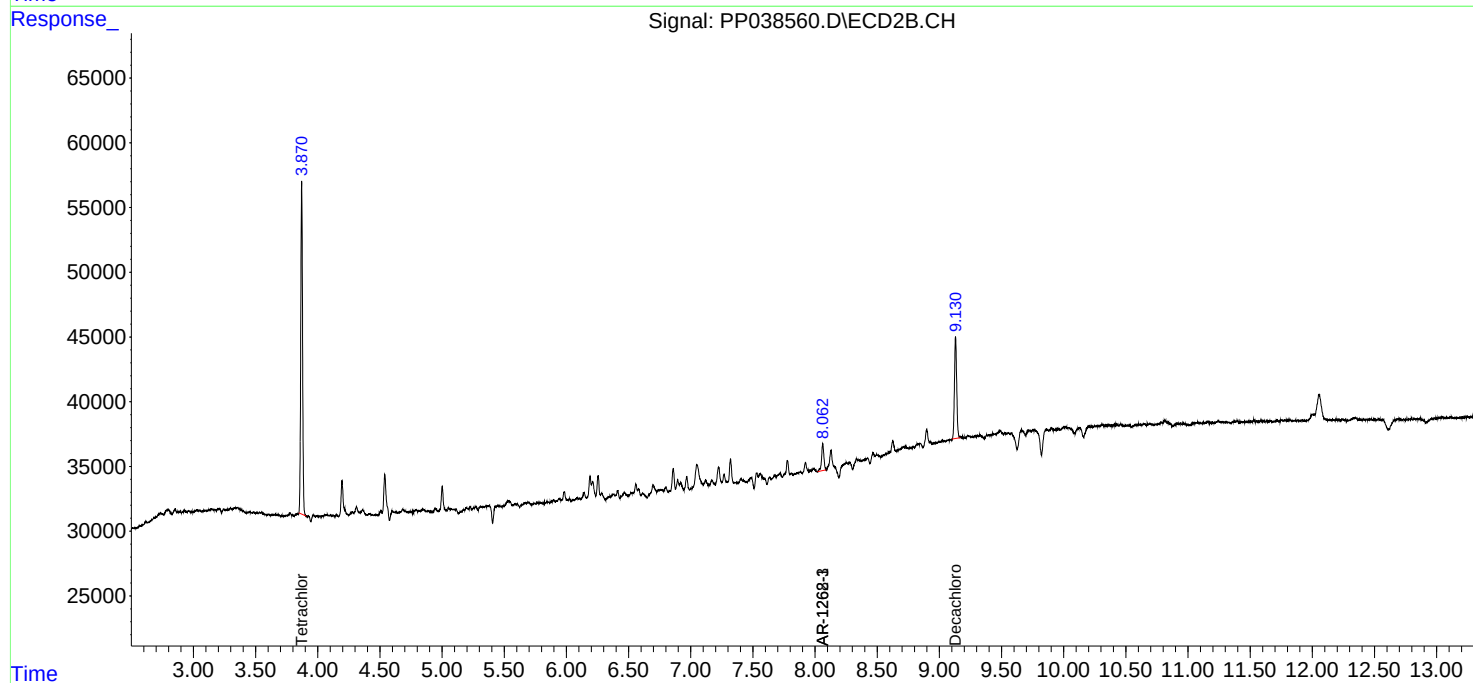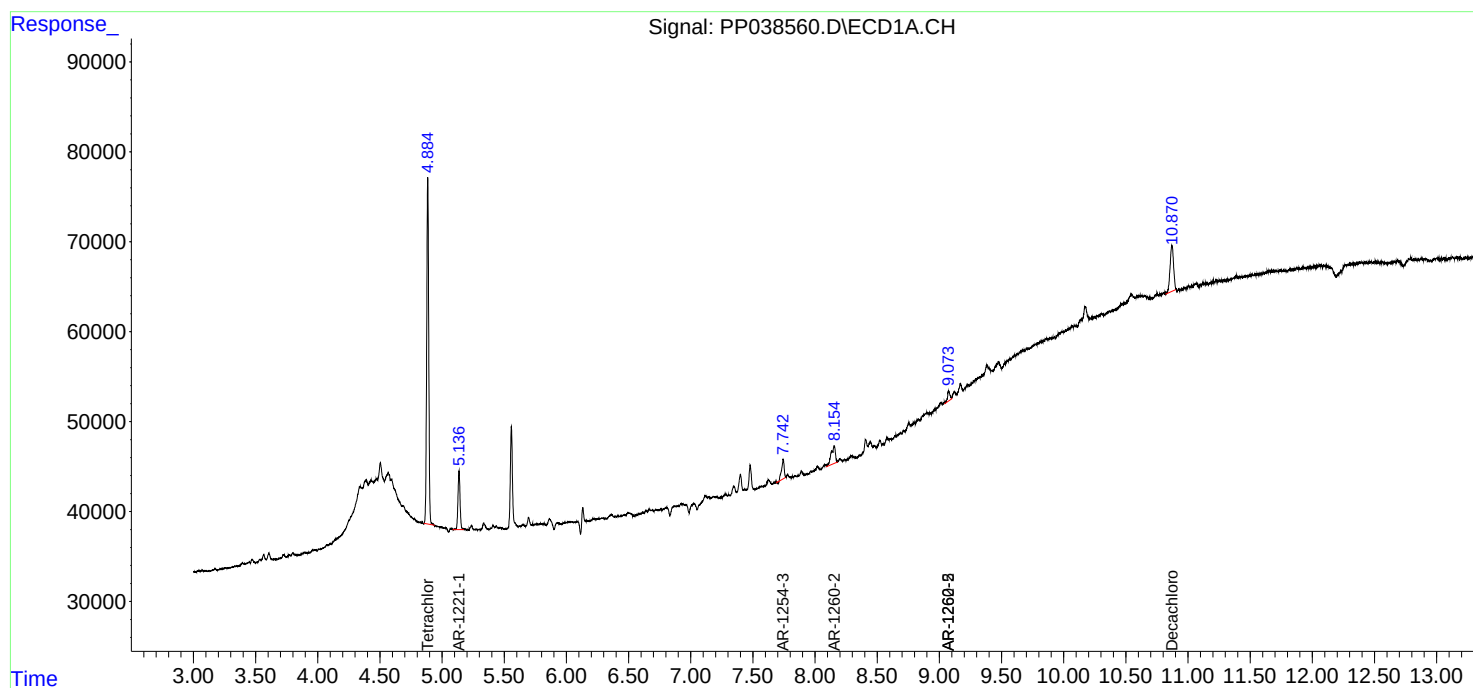


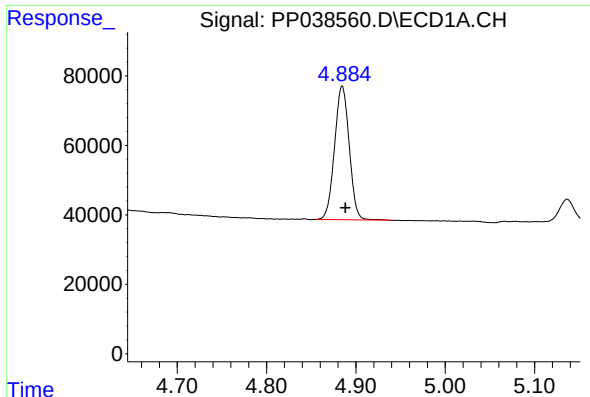

#1 Tetrachloro-m-xylene


R.T.: 4.885 min
Delta R.T.: -0.003 min
Response: 438554
Conc: 10.87 ng/ml

Instrument :
ECD_P
ClientSampleId :

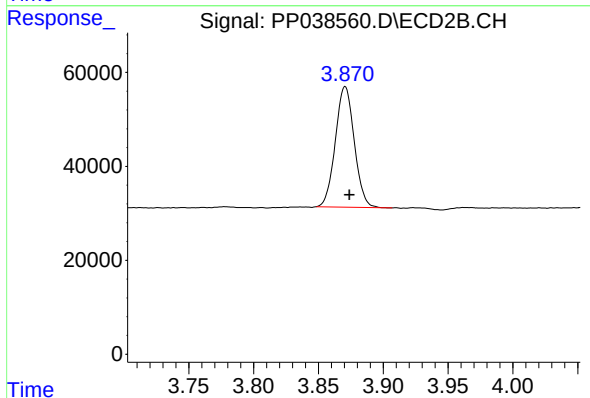


#1 Tetrachloro-m-xylene

R.T.: 3.871 min
Delta R.T.: -0.003 min
Response: 260801
Conc: 10.88 ng/ml

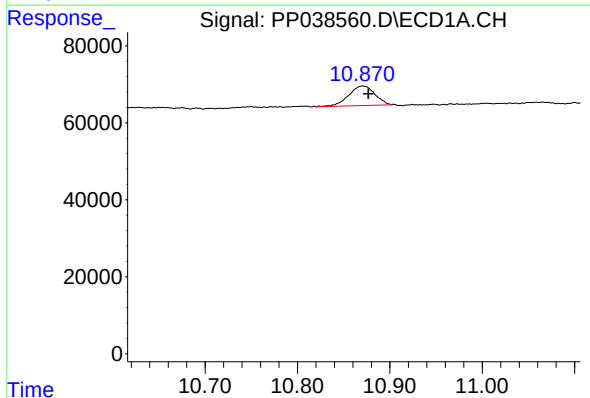


#2 Decachlorobiphenyl

R.T.: 10.871 min
Delta R.T.: -0.006 min
Response: 99887
Conc: 4.06 ng/ml

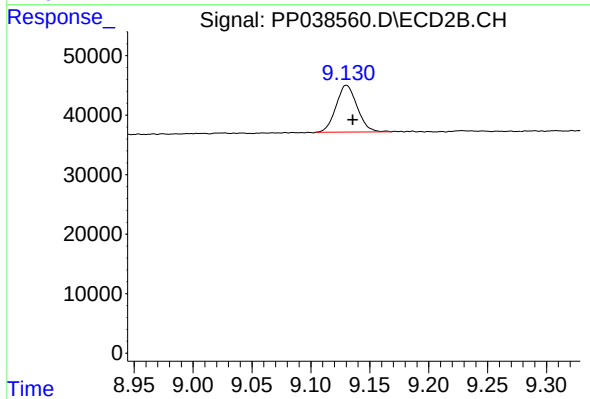

#2 Decachlorobiphenyl


R.T.: 9.130 min
Delta R.T.: -0.005 min
Response: 98157
Conc: 4.03 ng/ml

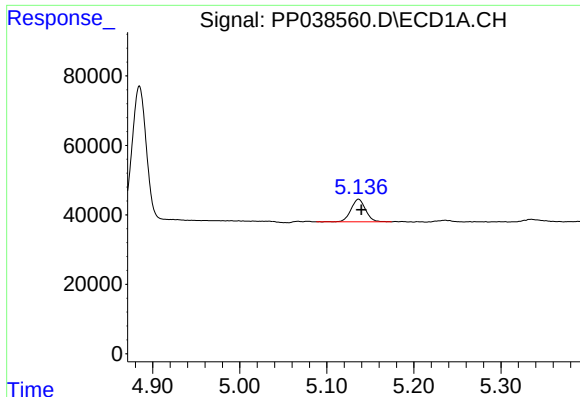

#8 AR-1221-1


R.T.: 5.137 min
Delta R.T.: -0.003 min
Response: 76151
Conc: 162.84 ng/ml

Instrument :
ECD_P
ClientSampleId :

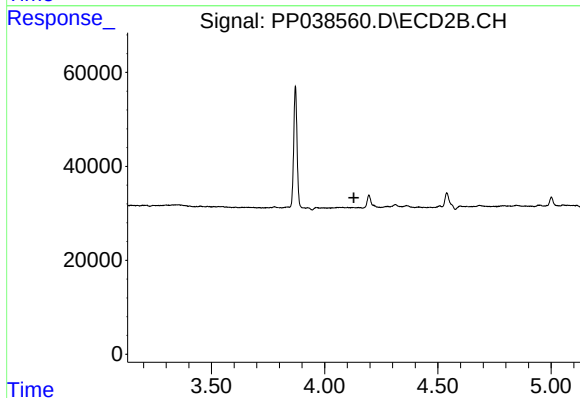


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.129 min
Response: 0
Conc: N.D.

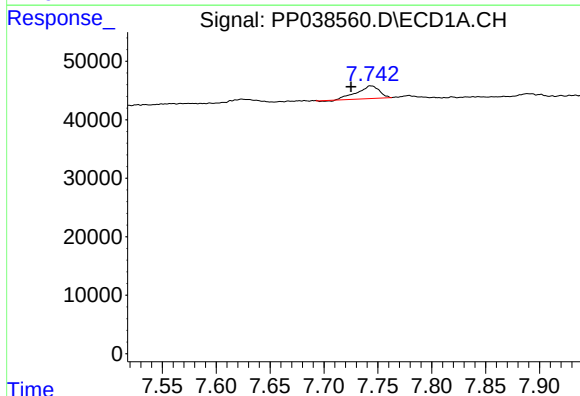


#28 AR-1254-3

R.T.: 7.743 min
Delta R.T.: 0.018 min
Response: 30915
Conc: 17.22 ng/ml

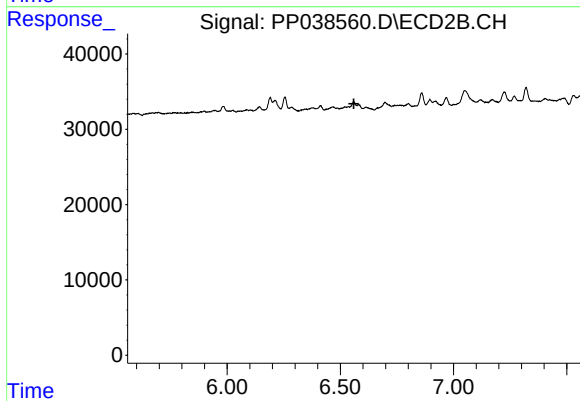

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.560 min
Response: 0
Conc: N.D.

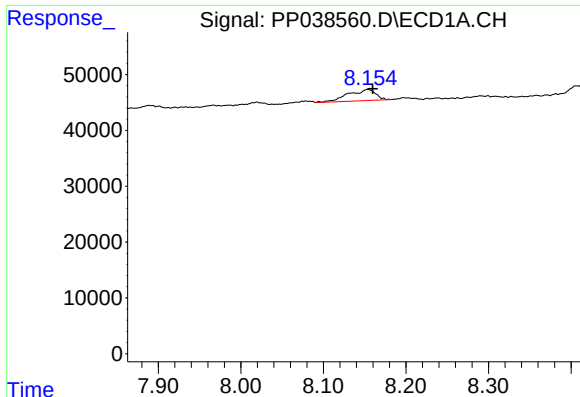

#32 AR-1260-2


R.T.: 8.154 min
Delta R.T.: -0.006 min
Response: 46443
Conc: 31.65 ng/ml

Instrument :
ECD_P
ClientSampleId :

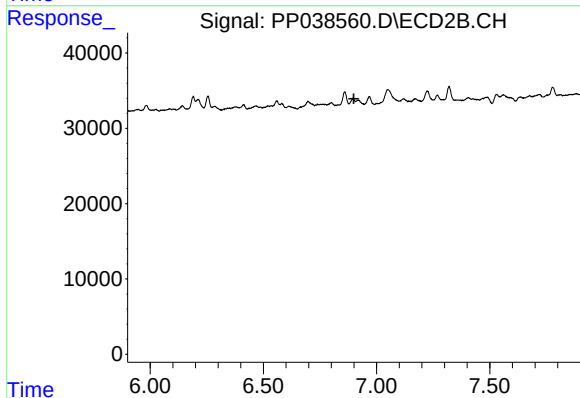


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.899 min
Response: 0
Conc: N.D.

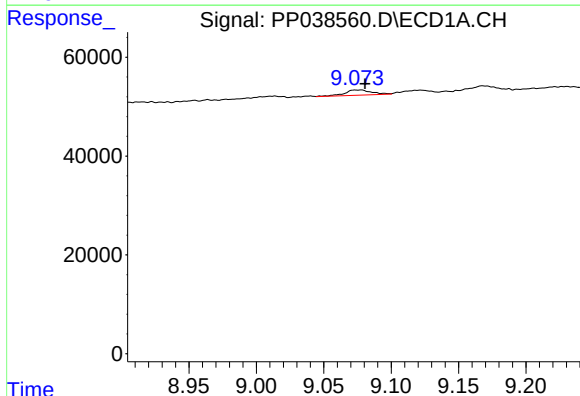


#35 AR-1260-5

R.T.: 9.073 min
Delta R.T.: -0.007 min
Response: 15172
Conc: 6.76 ng/ml

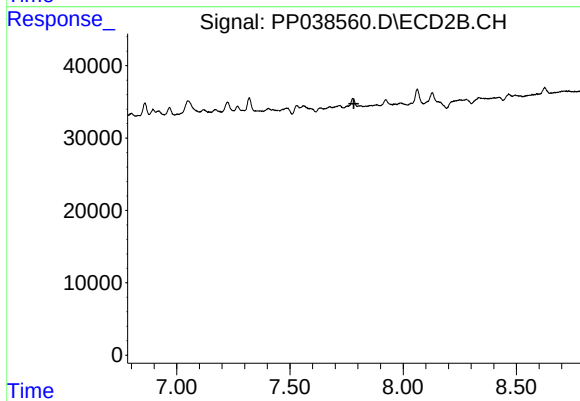

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.783 min
Response: 0
Conc: N.D.

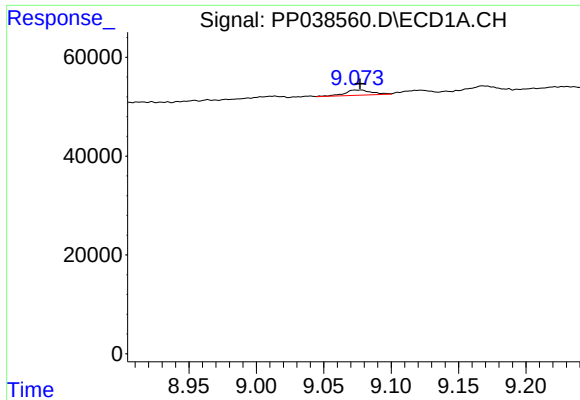

#37 AR-1262-2


R.T.: 9.073 min
Delta R.T.: -0.004 min
Response: 15172
Conc: 5.70 ng/ml

Instrument :
ECD_P
ClientSampleId :

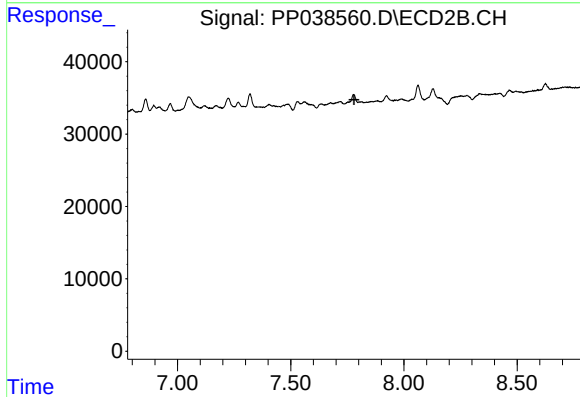


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.779 min
Response: 0
Conc: N.D.

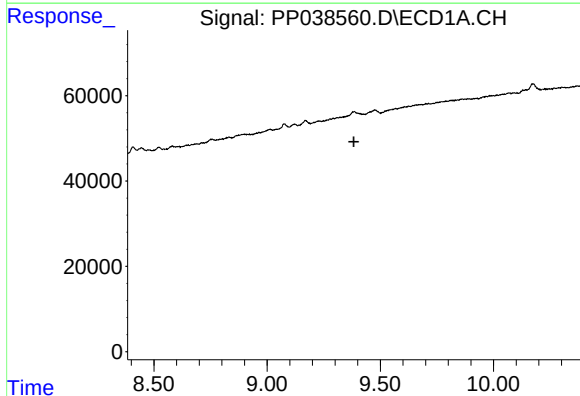


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 9.383 min
Response: 0
Conc: N.D.

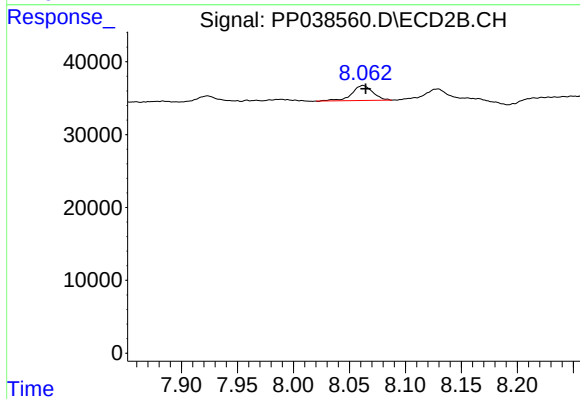

#38 AR-1262-3


R.T.: 8.062 min
Delta R.T.: -0.002 min
Response: 26967
Conc: 21.46 ng/ml

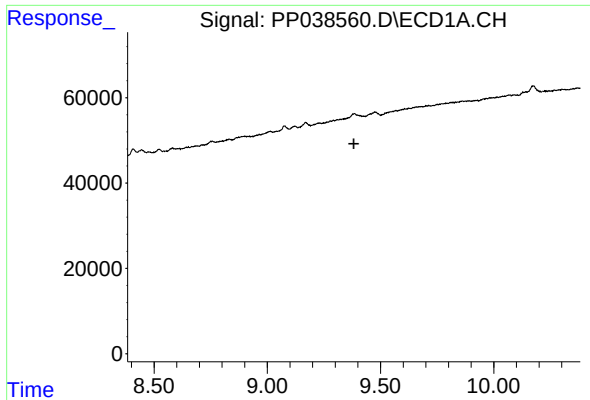

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

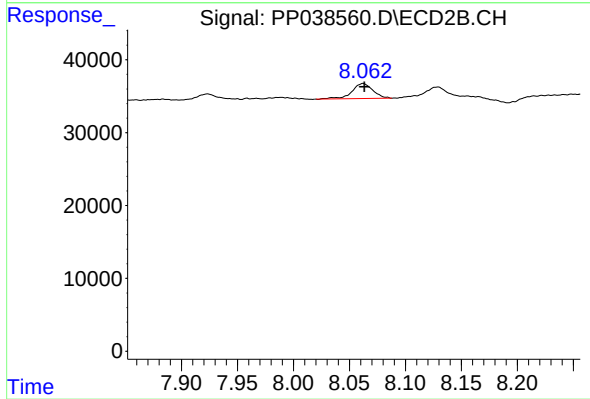

#41 AR-1268-1

R.T.: 8.062 min
Delta R.T.: -0.001 min
Response: 26967
Conc: 7.38 ng/ml