

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081822\
 Data File : PP050696.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2022 13:19
 Operator : YP\AJ
 Sample : N4232-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BU-01-081722

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/19/2022
 Supervised By :Ankita Jodhani 08/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 22:51:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Aug 09 11:38:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.345	3.591	32541847	64411053	20.217m	20.564
2) SA Decachlor...	10.099	8.556	30455866	26202988	17.296	17.025

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081822\
Data File : PP050696.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2022 13:19
Operator : YP\AJ
Sample : N4232-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BU-01-081722


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/19/2022
Supervised By :Ankita Jodhani 08/19/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 22:51:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080622.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Aug 09 11:38:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

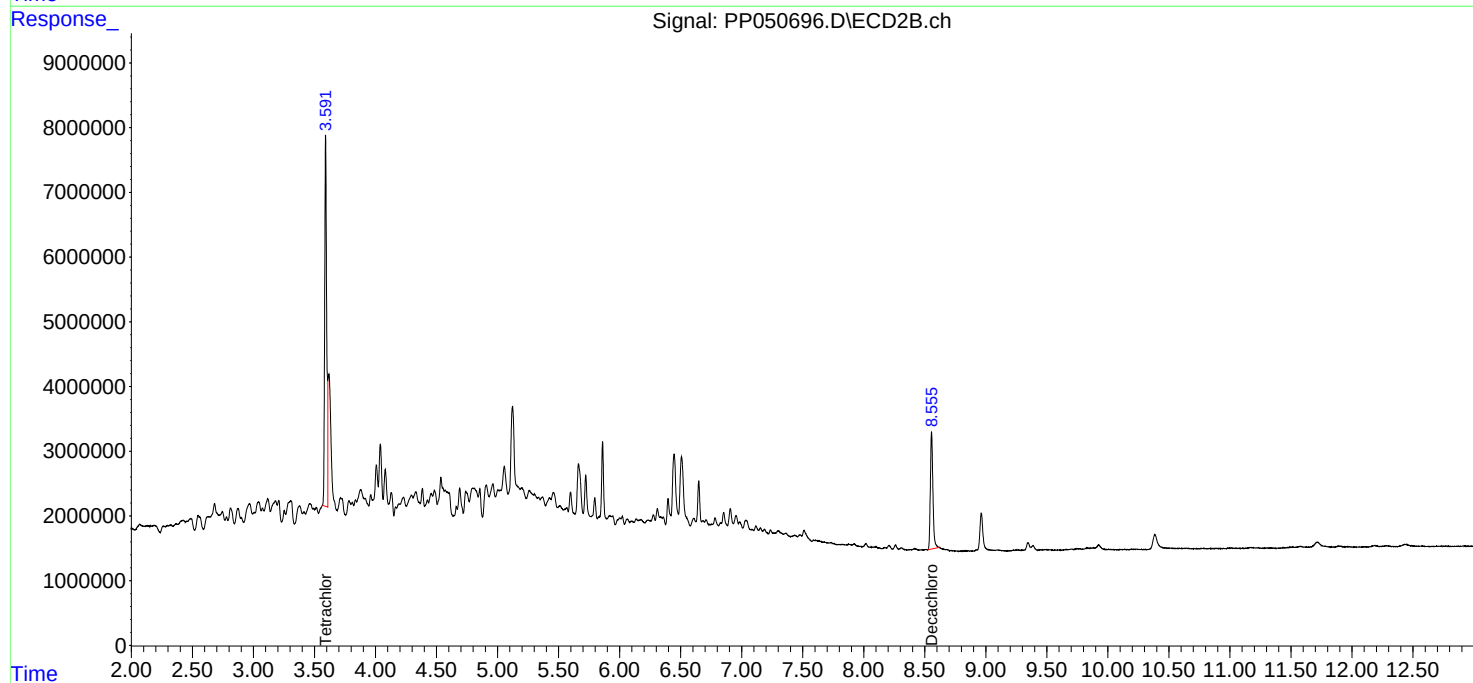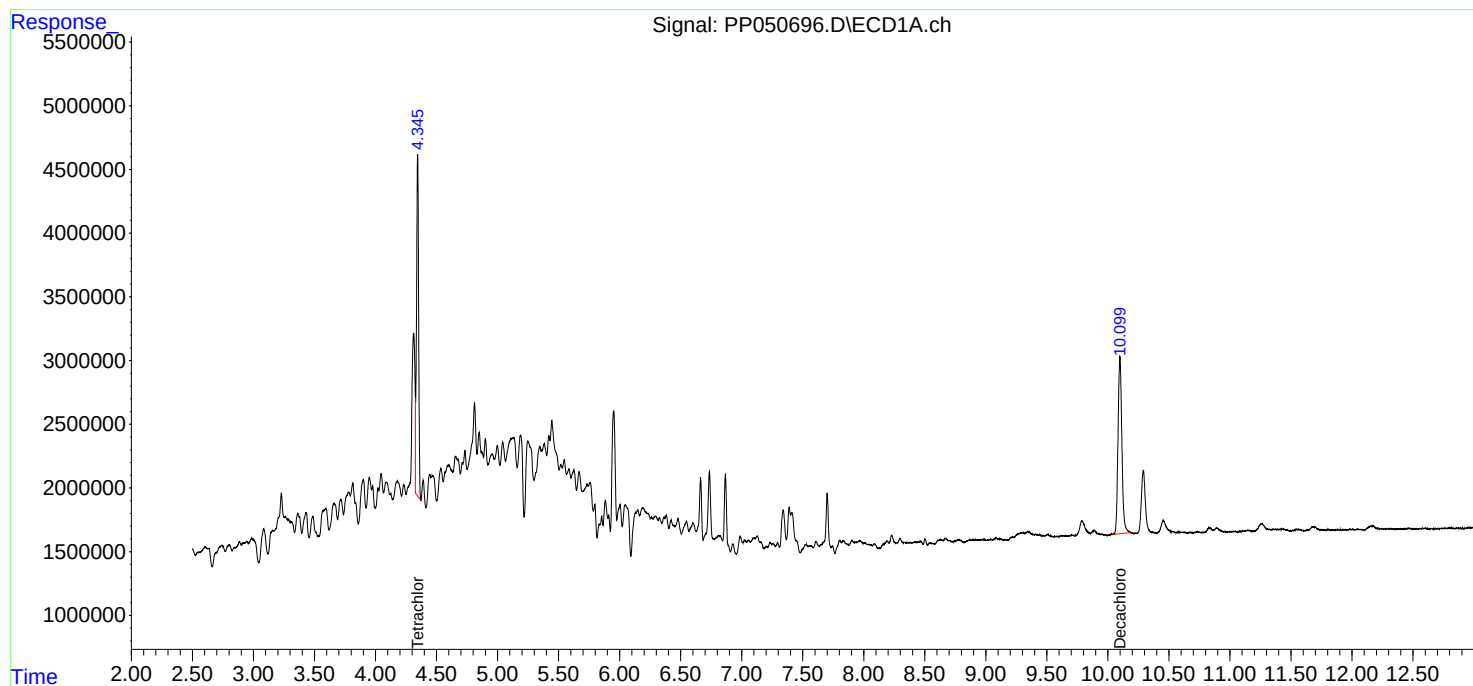

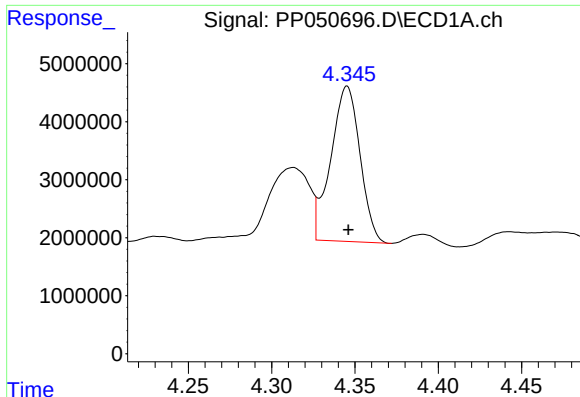


#1 Tetrachloro-m-xylene

R.T.: 4.345 min
Delta R.T.: -0.001 min
Response: 32541847
Conc: 20.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
BU-01-081722


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/19/2022
Supervised By :Ankita Jodhani 08/19/2022

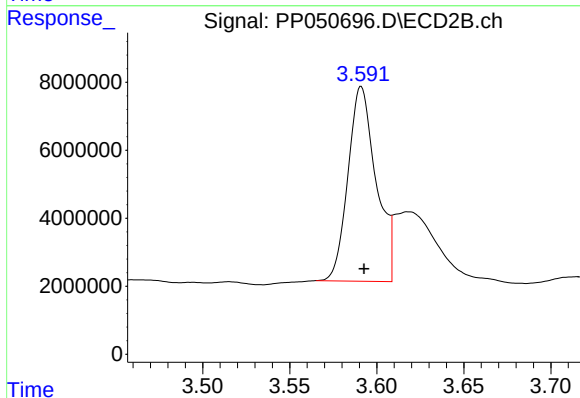


#1 Tetrachloro-m-xylene

R.T.: 3.591 min
Delta R.T.: -0.002 min
Response: 64411053
Conc: 20.56 ng/ml

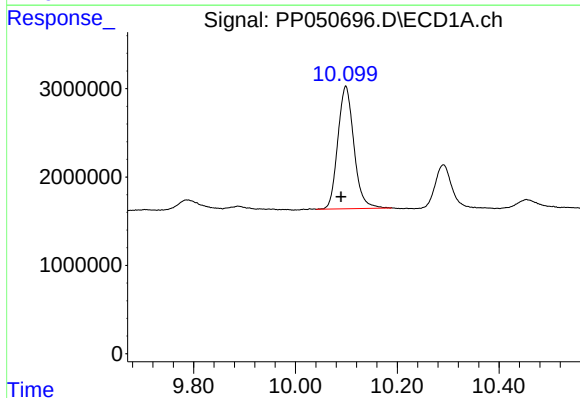

#2 Decachlorobiphenyl

R.T.: 10.099 min
Delta R.T.: 0.009 min
Response: 30455866
Conc: 17.30 ng/ml

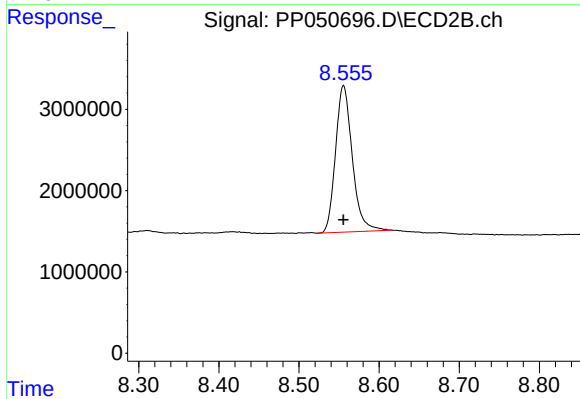

#2 Decachlorobiphenyl

R.T.: 8.556 min
Delta R.T.: 0.000 min
Response: 26202988
Conc: 17.03 ng/ml