

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081823\
 Data File : PP059420.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2023 17:48
 Operator : YP\AJ
 Sample : 04086-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 B-PP09B

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/21/2023
 Supervised By :Ankita Jodhani 08/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 00:29:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 09 02:30:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.414	3.642	29099038	49372317	23.715	24.368m
2) SA Decachlor...	10.204	8.677	14393406	23519644	18.858	16.718

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081823\
Data File : PP059420.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2023 17:48
Operator : YP\AJ
Sample : 04086-06
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
B-PP09B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/21/2023
Supervised By :Ankita Jodhani 08/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 00:29:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 09 02:30:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

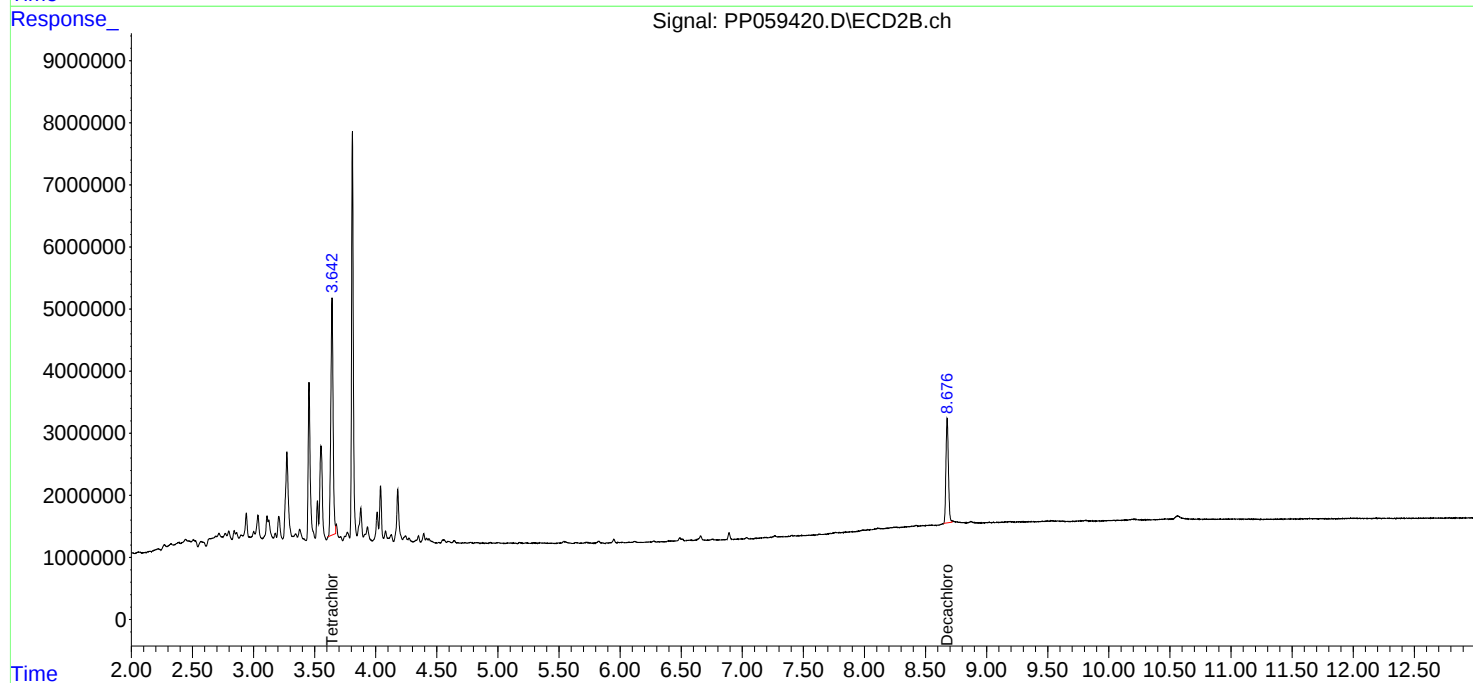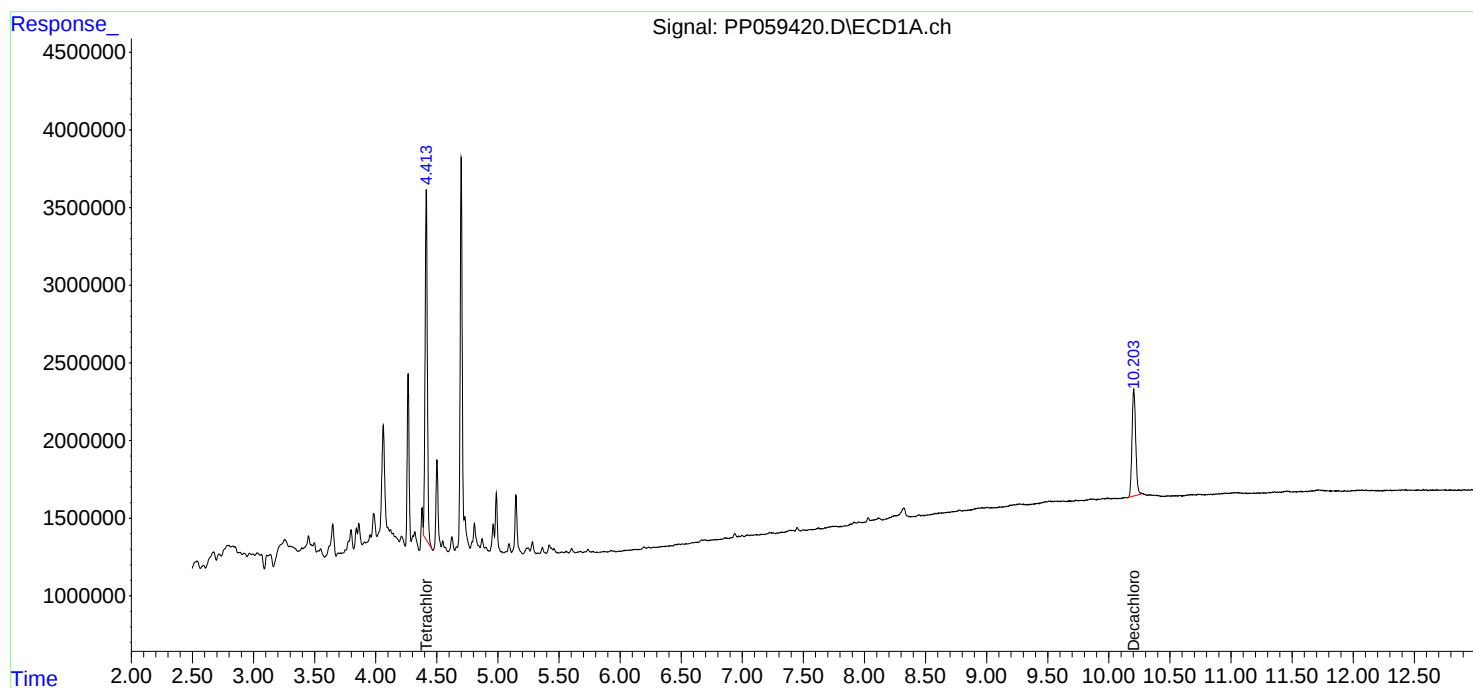

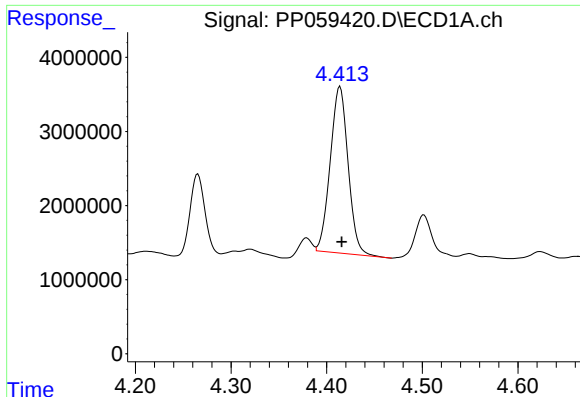


#1 Tetrachloro-m-xylene

R.T.: 4.414 min
Delta R.T.: -0.002 min
Response: 29099038
Conc: 23.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
B-PP09B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/21/2023
Supervised By :Ankita Jodhani 08/21/2023

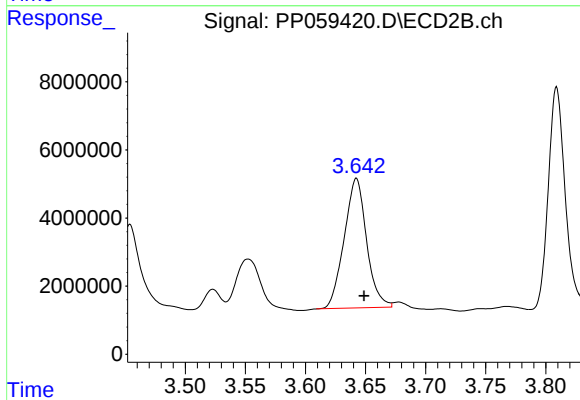


#1 Tetrachloro-m-xylene

R.T.: 3.642 min
Delta R.T.: -0.007 min
Response: 49372317
Conc: 24.37 ng/ml m

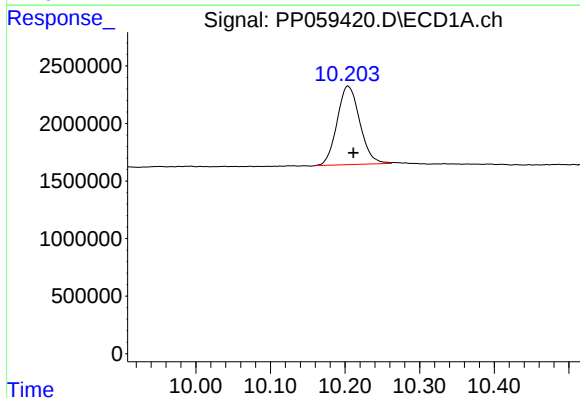

#2 Decachlorobiphenyl

R.T.: 10.204 min
Delta R.T.: -0.007 min
Response: 14393406
Conc: 18.86 ng/ml

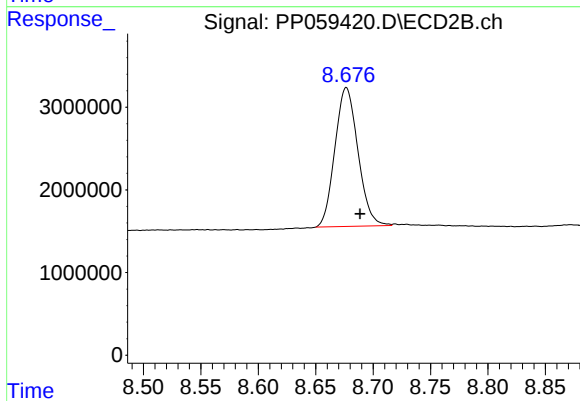

#2 Decachlorobiphenyl

R.T.: 8.677 min
Delta R.T.: -0.012 min
Response: 23519644
Conc: 16.72 ng/ml