

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081921\
 Data File : PP038607.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Aug 2021 20:12
 Operator : AJ\MA
 Sample : M3449-23
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CON-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 01:39:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 18 04:51:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.885	3.870	854346	522154	21.169	21.789
2) SA Decachlor...	10.873	9.131	568323	565540	23.099	23.220

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081921\
Data File : PP038607.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Aug 2021 20:12
Operator : AJ\MA
Sample : M3449-23
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
CON-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 01:39:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 18 04:51:26 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

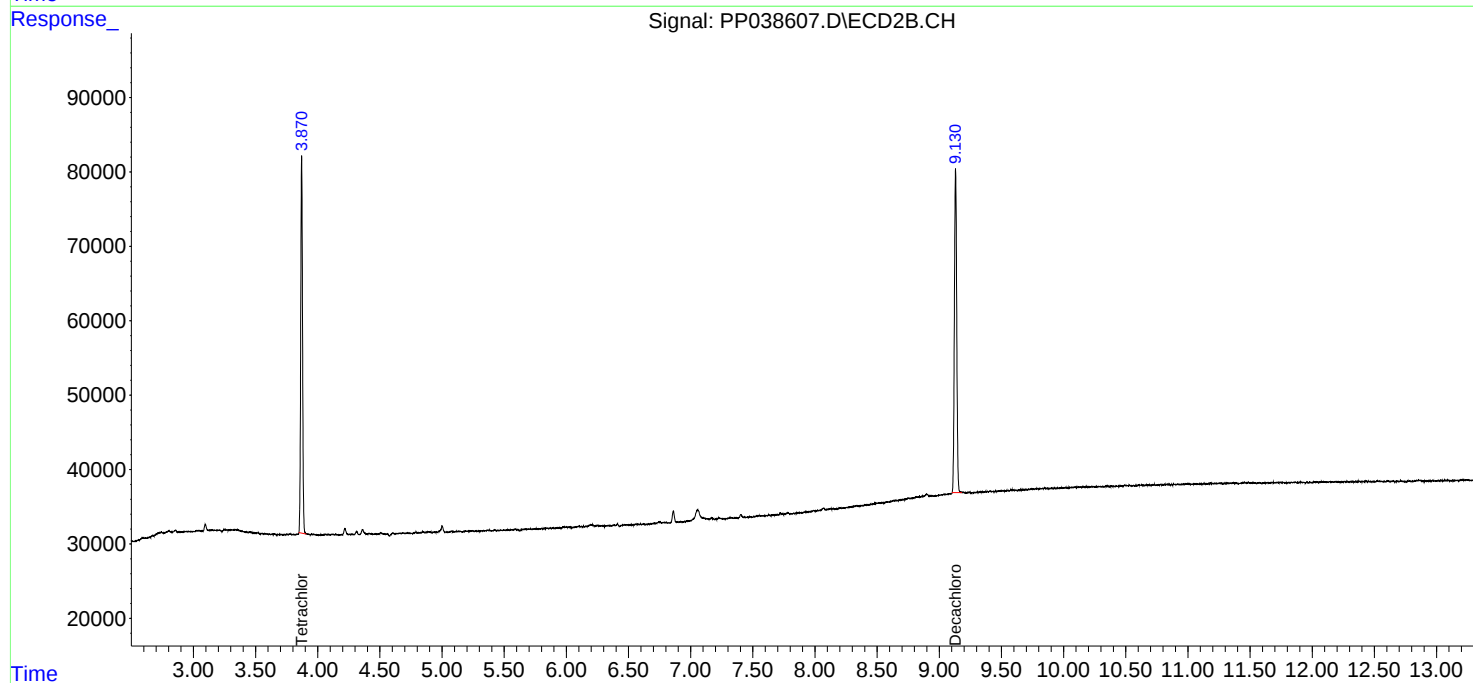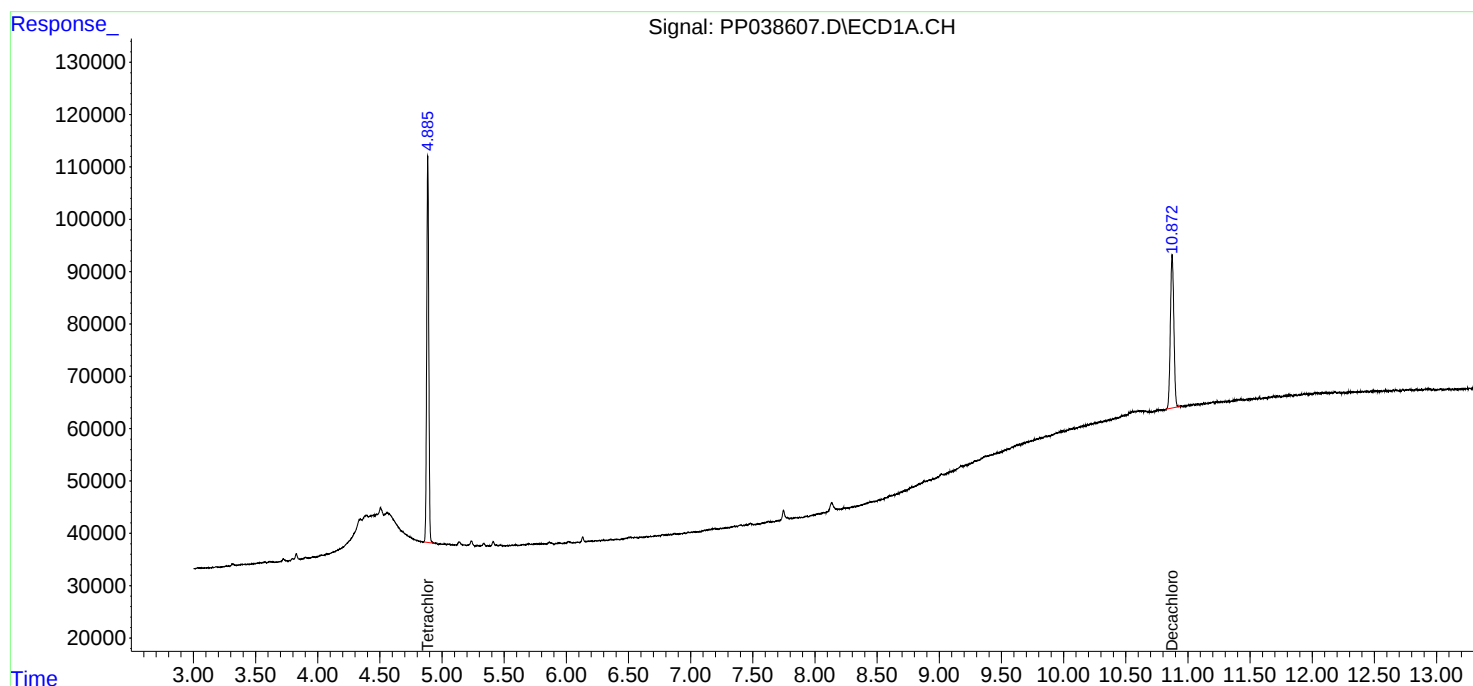


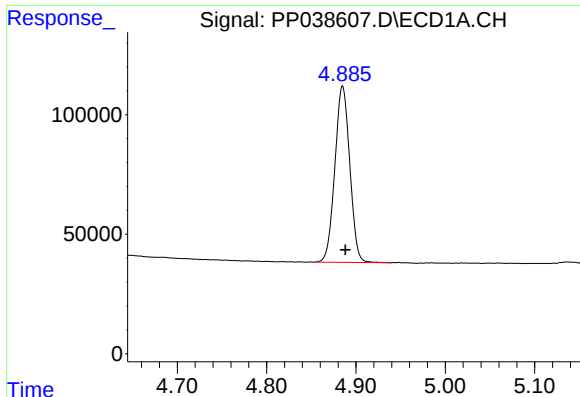

#1 Tetrachloro-m-xylene


R.T.: 4.885 min
Delta R.T.: -0.003 min
Response: 854346
Conc: 21.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
CON-3

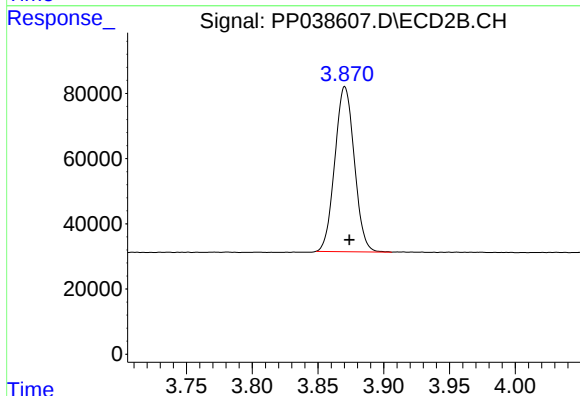


#1 Tetrachloro-m-xylene

R.T.: 3.870 min
Delta R.T.: -0.004 min
Response: 522154
Conc: 21.79 ng/ml

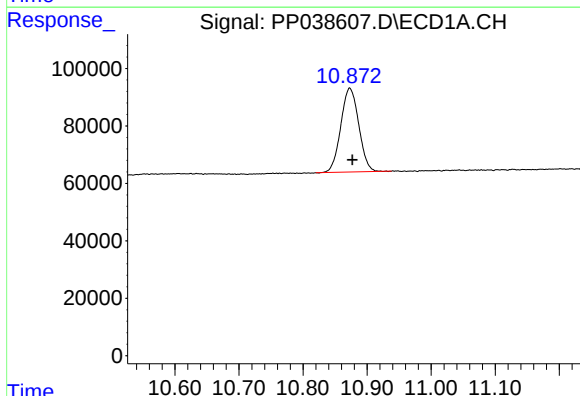

#2 Decachlorobiphenyl

R.T.: 10.873 min
Delta R.T.: -0.004 min
Response: 568323
Conc: 23.10 ng/ml

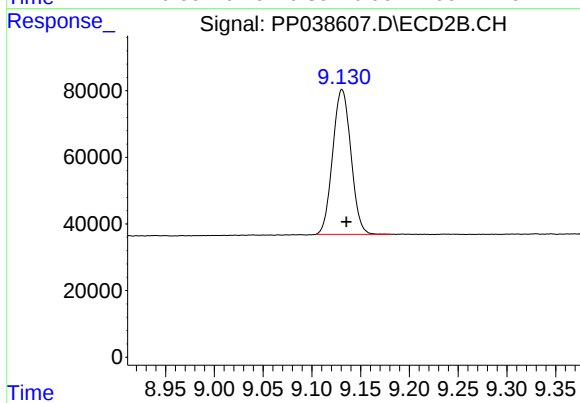

#2 Decachlorobiphenyl

R.T.: 9.131 min
Delta R.T.: -0.005 min
Response: 565540
Conc: 23.22 ng/ml