

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081925\
 Data File : PP074524.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2025 21:55
 Operator : YP\AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 06:25:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.689f	3.803	237002	169987	0.194	0.035 #
2)	SA Decachlor...	0.000	8.803	0	1280957	N.D.	0.171 #
Target Compounds							
3)	L1 AR-1016-1	5.784	4.903	336830	686777	7.640	1.348 #
4)	L1 AR-1016-2	5.823	4.951	198723	1240948	3.162	5.214 #
5)	L1 AR-1016-3	5.911	5.088	1228605	1110900	27.355	8.056 #
6)	L1 AR-1016-4	5.934f	5.139	1778920	2166559	50.564	15.497 #
7)	L1 AR-1016-5	0.000	5.336	0	968354	N.D.	5.831 #
8)	L2 AR-1221-1	4.852	3.999	56772	159472	3.227	2.578
9)	L2 AR-1221-2	4.921	4.096	322122	204568	24.116	4.525 #
10)	L2 AR-1221-3	5.069f	4.172	82161	174718	2.167	1.063 #
11)	L3 AR-1232-1	5.069f	4.172	82161	174718	2.705	1.364 #
12)	L3 AR-1232-2	5.599f	4.903	587999	686777	37.314	2.963 #
13)	L3 AR-1232-3	5.823	5.088	198723	1110900	6.506	18.497 #
14)	L3 AR-1232-4	5.934f	5.170	1778920	2446130	103.011	33.187 #
15)	L3 AR-1232-5	6.082	5.336	846980	968354	65.248	15.598 #
16)	L4 AR-1242-1	5.823	4.903	198723	686777	5.192	1.628 #
17)	L4 AR-1242-2	5.823	4.951	198723	1240948	3.518	6.196 #
18)	L4 AR-1242-3	5.911	5.088	1228605	1110900	30.259	9.391 #
19)	L4 AR-1242-4	5.934f	5.170	1778920	2446130	56.043	14.292 #
20)	L4 AR-1242-5	6.750	5.667	1433953	2302076	39.754	12.433 #
21)	L5 AR-1248-1	5.823	4.903	198723	686777	6.575	2.487 #
22)	L5 AR-1248-2	6.082	5.139	846980	2166559	19.653	12.257 #
23)	L5 AR-1248-3	0.000	5.170	0	2446130	N.D.	10.766 #
24)	L5 AR-1248-4	6.651	5.336	1815290	968354	33.005	4.442 #
25)	L5 AR-1248-5	6.750	5.702	1433953	5684171	25.851	15.475 #
26)	L6 AR-1254-1	6.651	5.702	1815290	5684171	31.153	11.924 #
27)	L6 AR-1254-2	6.865	5.819	2082611	882996	25.517	2.508 #
28)	L6 AR-1254-3	7.228	6.246	4938148	24602108	55.356	39.693 #
29)	L6 AR-1254-4	7.561f	6.450	2478680	1133594	37.605	2.419 #
30)	L6 AR-1254-5	7.948	6.874	521.4E6	3914.4E6	6274.939	7980.352 #
31)	L7 AR-1260-1	7.399	6.362	36885	2333152	0.638	6.218 #
32)	L7 AR-1260-2	7.634	6.547	571.8E6	2821126	8297.188	5.335 #
33)	L7 AR-1260-3	7.948f	0.000	521.4E6	0	10048.193	N.D. #
34)	L7 AR-1260-4	8.173f	7.177	174857	153087	2.741	0.401 #
35)	L7 AR-1260-5	8.564	7.407	162218	358204	1.430	0.357 #
36)	L8 AR-1262-1	8.173f	6.874f	174857	3914.4E6	2.270	5534.566 #
37)	L8 AR-1262-2	8.564	7.177	162218	153087	1.225	0.294 #
38)	L8 AR-1262-3	8.860	7.701	17824	7497577	0.183	16.079 #
39)	L8 AR-1262-4	0.000	7.800f	0	967974	N.D.	1.178 #
40)	L8 AR-1262-5	9.604f	8.265	3002114	342356	49.250	0.955 #
41)	L9 AR-1268-1	8.860	7.701	17824	7497577	0.110	5.316 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081925\
 Data File : PP074524.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2025 21:55
 Operator : YP\AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 06:25:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	7.720f	0	14890679	N.D.	10.922 #
43) L9	AR-1268-3	9.245	7.971	270087	139504	2.185	0.134 #
44) L9	AR-1268-4	9.604f	8.241	3002114	200233	44.633	0.523 #
45) L9	AR-1268-5	0.000	8.562	0	1205036	N.D.	0.384 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081925\
Data File : PP074524.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2025 21:55
Operator : YP\AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 06:25:01 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

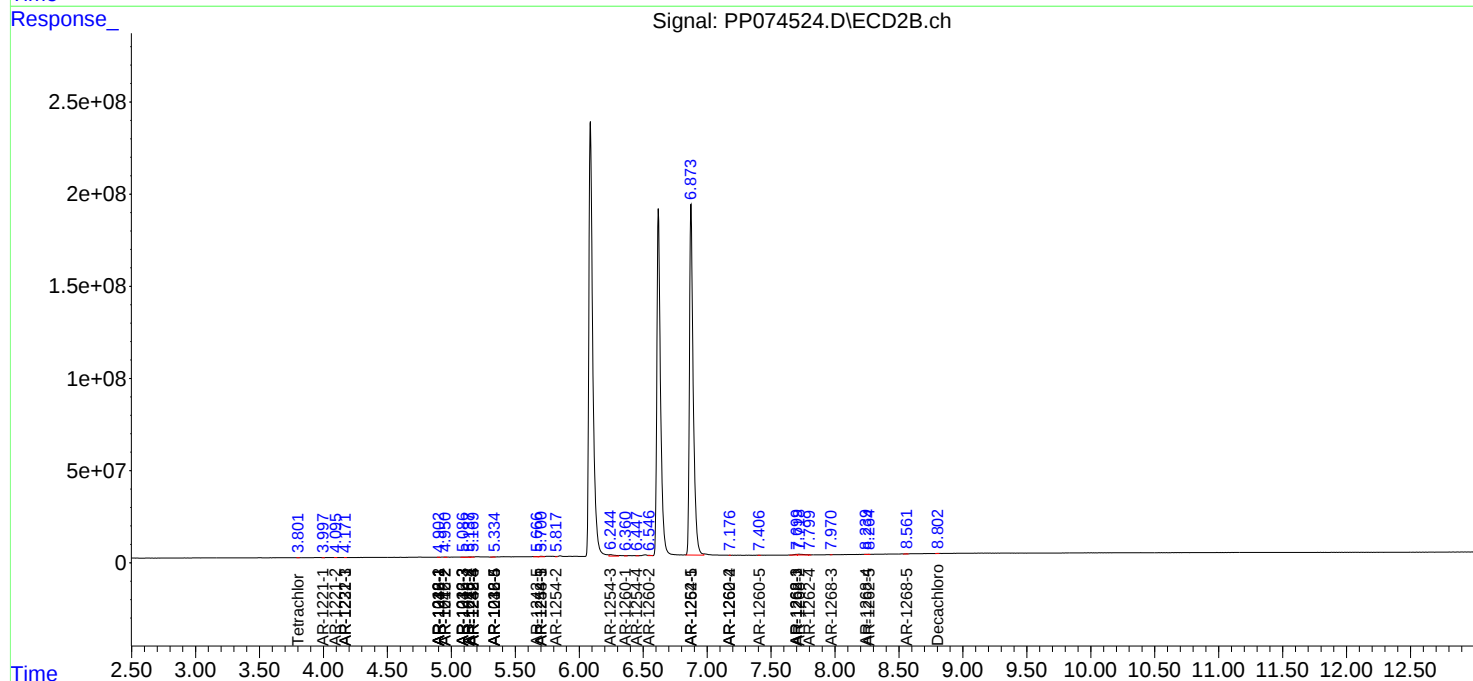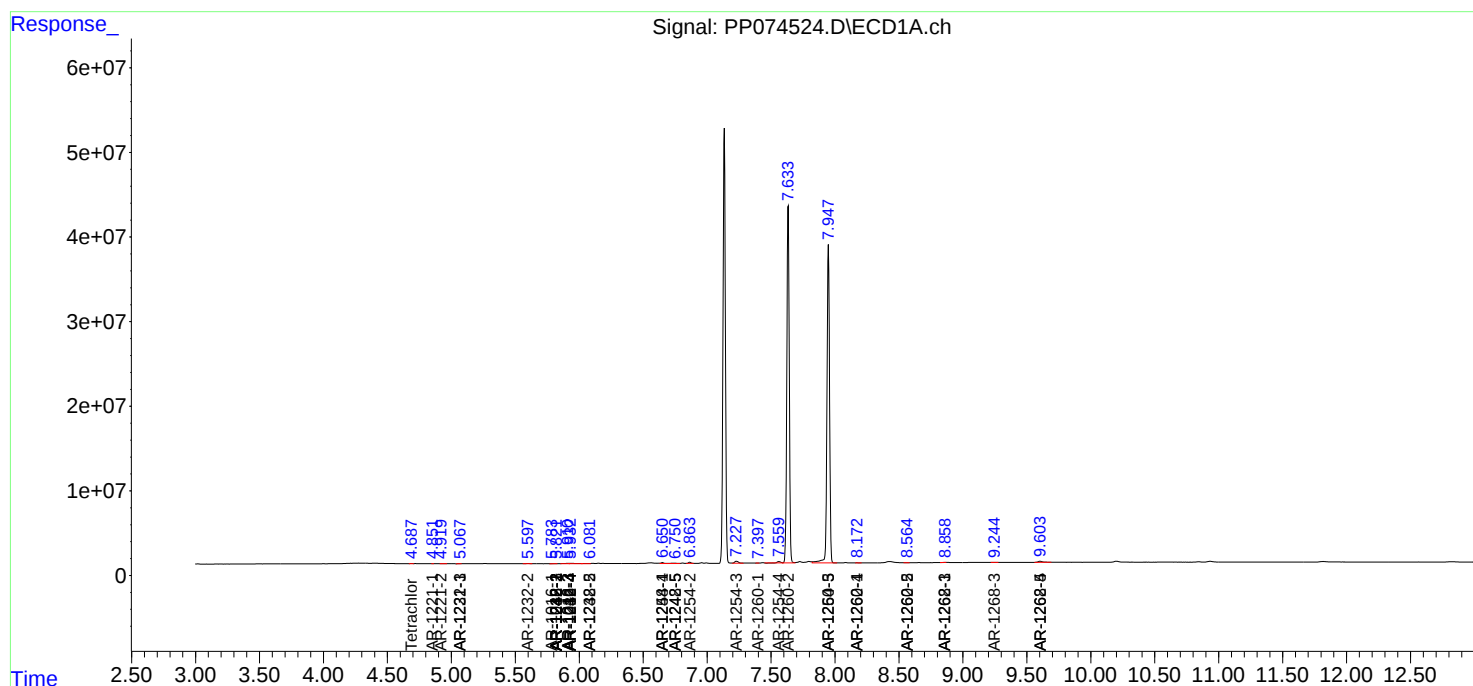


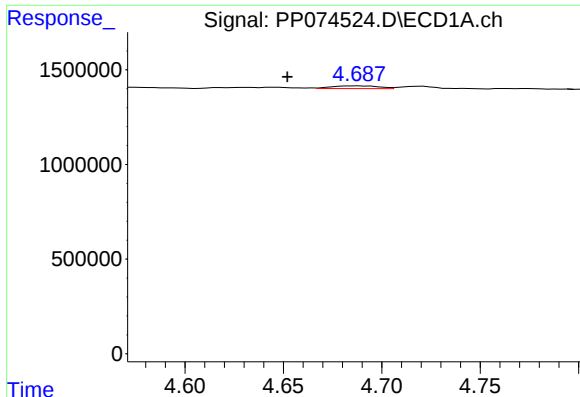

#1 Tetrachloro-m-xylene


R.T.: 4.689 min
Delta R.T.: 0.037 min
Response: 237002
Conc: 0.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

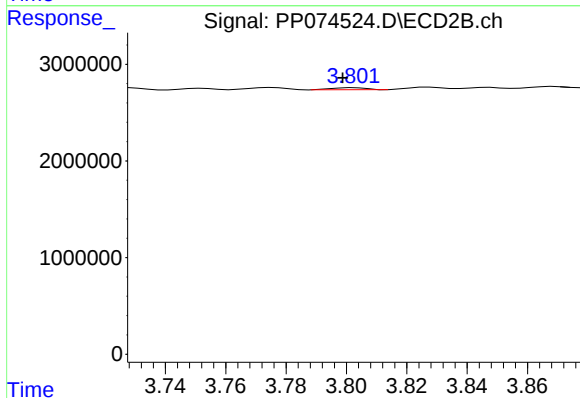


#1 Tetrachloro-m-xylene

R.T.: 3.803 min
Delta R.T.: 0.004 min
Response: 169987
Conc: 0.04 ng/ml

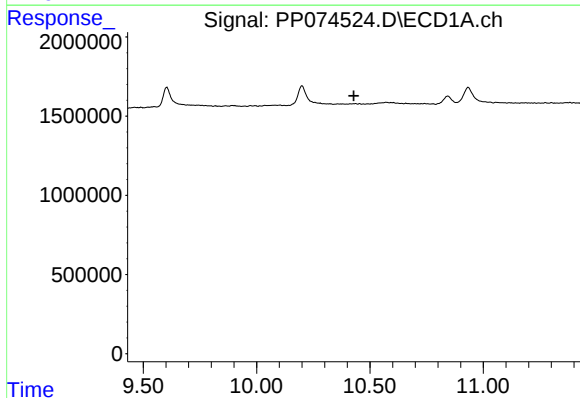


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.428 min
Response: 0
Conc: N.D.

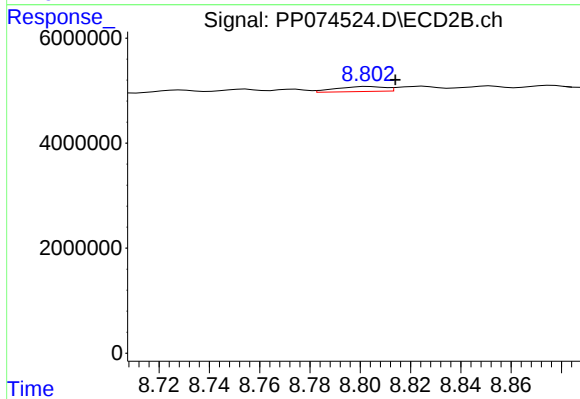

#2 Decachlorobiphenyl


R.T.: 8.803 min
Delta R.T.: -0.010 min
Response: 1280957
Conc: 0.17 ng/ml

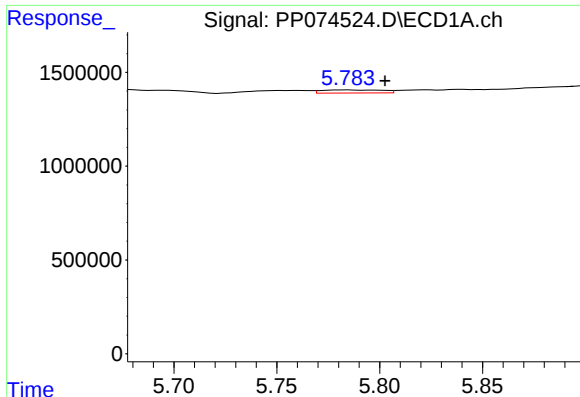

#3 AR-1016-1


R.T.: 5.784 min
Delta R.T.: -0.018 min
Response: 336830
Conc: 7.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

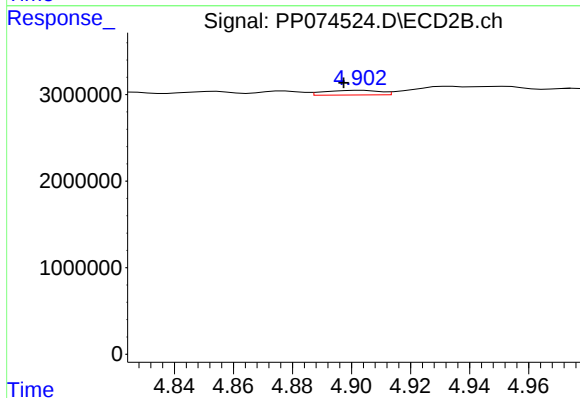


#3 AR-1016-1

R.T.: 4.903 min
Delta R.T.: 0.006 min
Response: 686777
Conc: 1.35 ng/ml

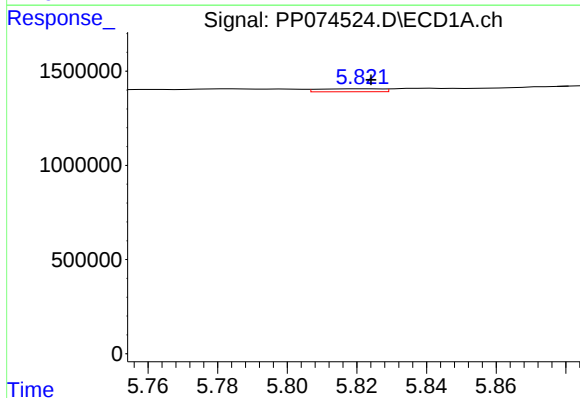


#4 AR-1016-2

R.T.: 5.823 min
Delta R.T.: -0.001 min
Response: 198723
Conc: 3.16 ng/ml

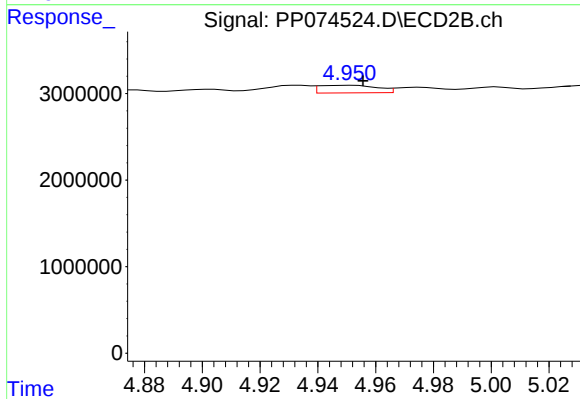

#4 AR-1016-2


R.T.: 4.951 min
Delta R.T.: -0.004 min
Response: 1240948
Conc: 5.21 ng/ml

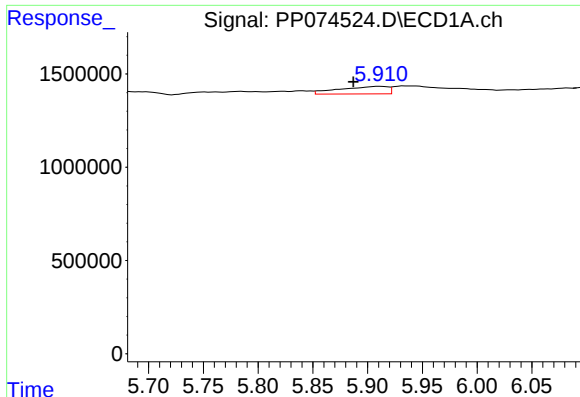

#5 AR-1016-3


R.T.: 5.911 min
Delta R.T.: 0.024 min
Response: 1228605
Conc: 27.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

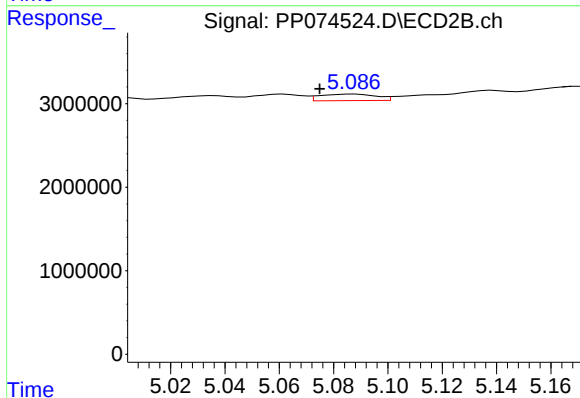


#5 AR-1016-3

R.T.: 5.088 min
Delta R.T.: 0.013 min
Response: 1110900
Conc: 8.06 ng/ml

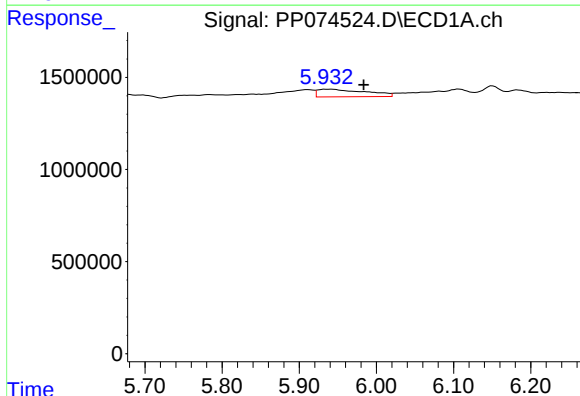


#6 AR-1016-4

R.T.: 5.934 min
Delta R.T.: -0.050 min
Response: 1778920
Conc: 50.56 ng/ml

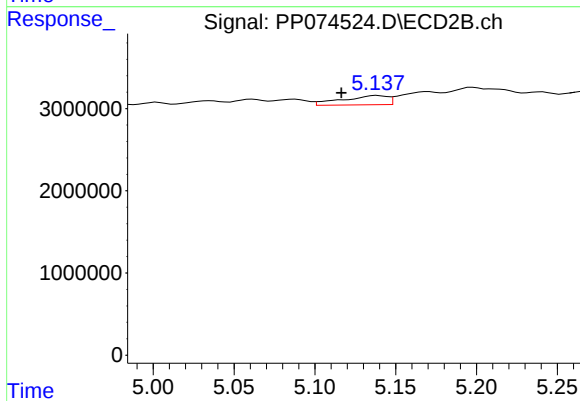

#6 AR-1016-4


R.T.: 5.139 min
Delta R.T.: 0.022 min
Response: 2166559
Conc: 15.50 ng/ml

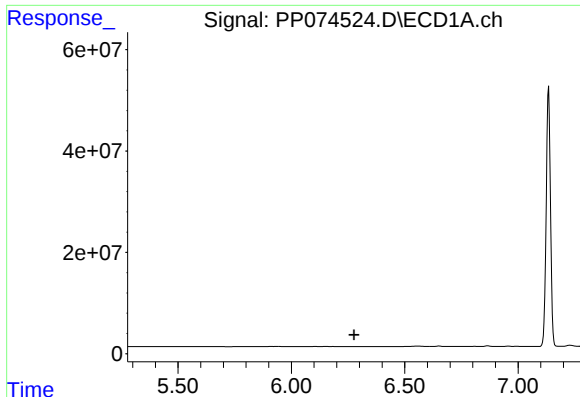

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

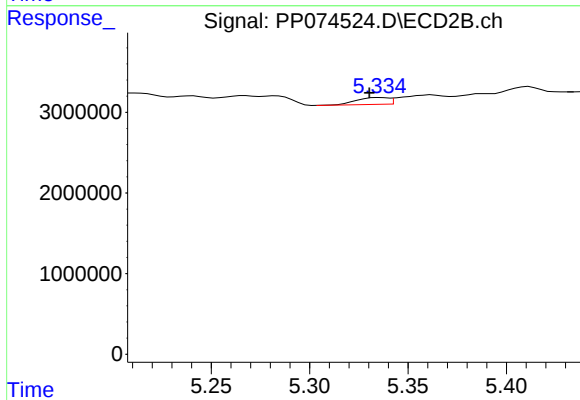


#7 AR-1016-5

R.T.: 5.336 min
Delta R.T.: 0.006 min
Response: 968354
Conc: 5.83 ng/ml

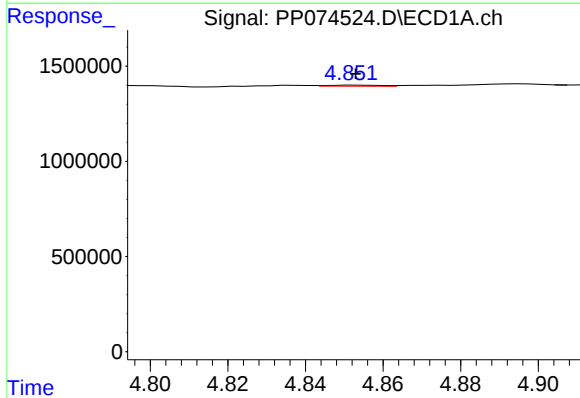


#8 AR-1221-1

R.T.: 4.852 min
Delta R.T.: 0.000 min
Response: 56772
Conc: 3.23 ng/ml

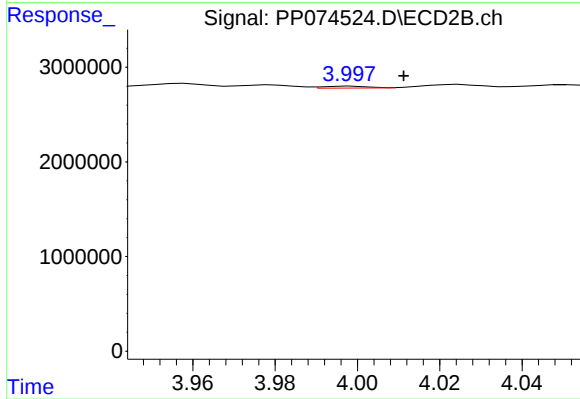

#8 AR-1221-1


R.T.: 3.999 min
Delta R.T.: -0.013 min
Response: 159472
Conc: 2.58 ng/ml

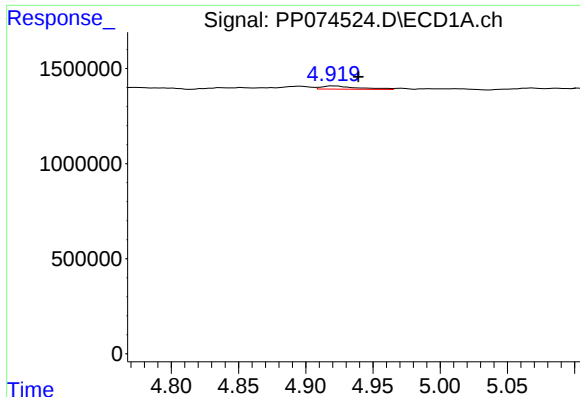

#9 AR-1221-2


R.T.: 4.921 min
Delta R.T.: -0.018 min
Response: 322122
Conc: 24.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

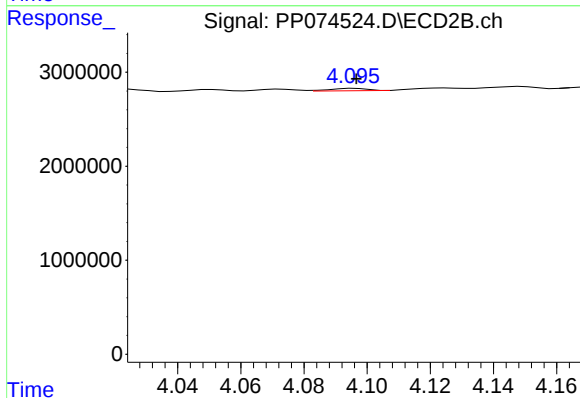


#9 AR-1221-2

R.T.: 4.096 min
Delta R.T.: 0.000 min
Response: 204568
Conc: 4.52 ng/ml

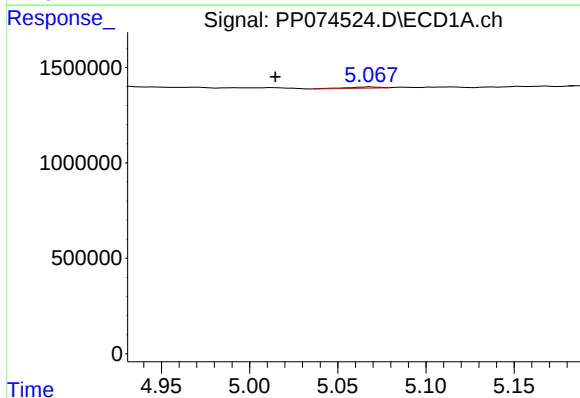


#10 AR-1221-3

R.T.: 5.069 min
Delta R.T.: 0.054 min
Response: 82161
Conc: 2.17 ng/ml

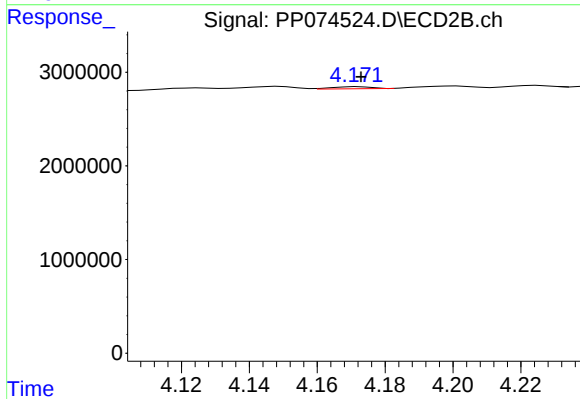

#10 AR-1221-3


R.T.: 4.172 min
Delta R.T.: 0.000 min
Response: 174718
Conc: 1.06 ng/ml

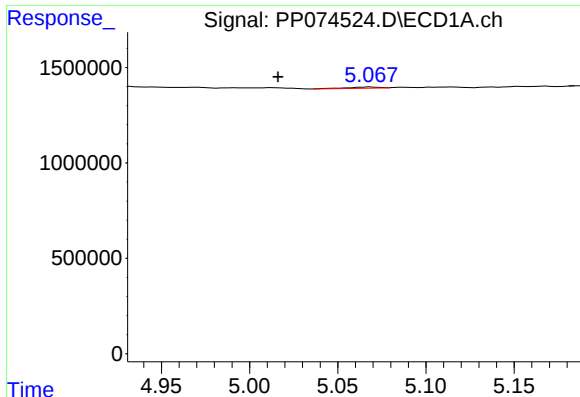

#11 AR-1232-1


R.T.: 5.069 min
Delta R.T.: 0.053 min
Response: 82161
Conc: 2.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

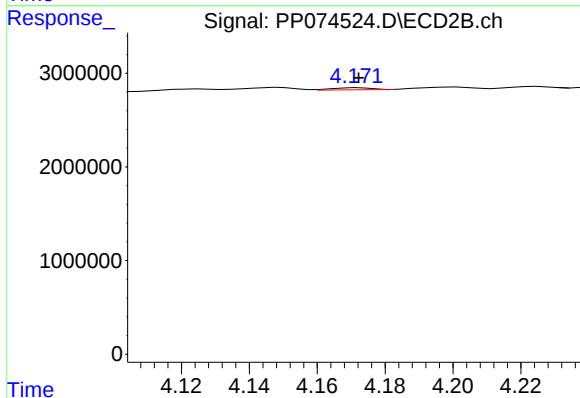


#11 AR-1232-1

R.T.: 4.172 min
Delta R.T.: 0.000 min
Response: 174718
Conc: 1.36 ng/ml

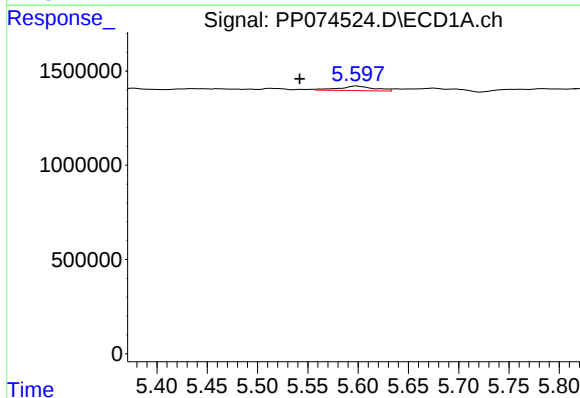


#12 AR-1232-2

R.T.: 5.599 min
Delta R.T.: 0.057 min
Response: 587999
Conc: 37.31 ng/ml

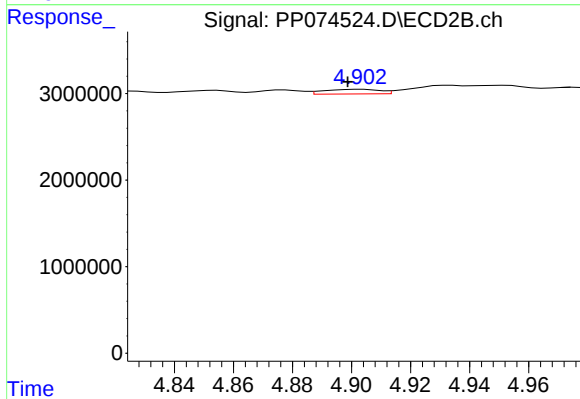

#12 AR-1232-2


R.T.: 4.903 min
Delta R.T.: 0.005 min
Response: 686777
Conc: 2.96 ng/ml

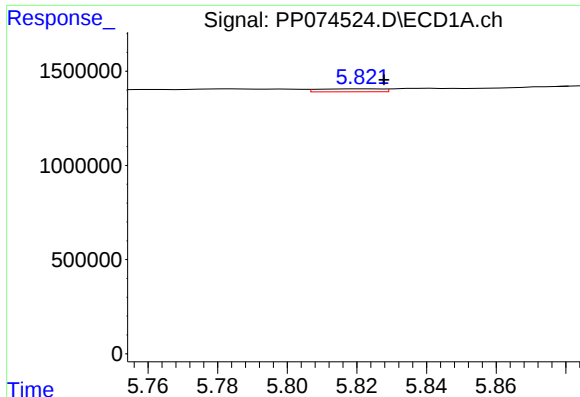

#13 AR-1232-3


R.T.: 5.823 min
Delta R.T.: -0.005 min
Response: 198723
Conc: 6.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

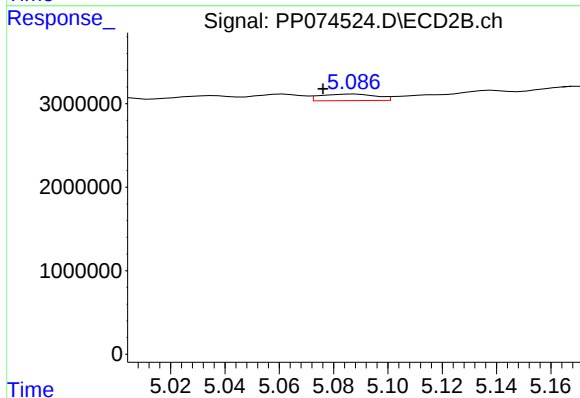


#13 AR-1232-3

R.T.: 5.088 min
Delta R.T.: 0.012 min
Response: 1110900
Conc: 18.50 ng/ml

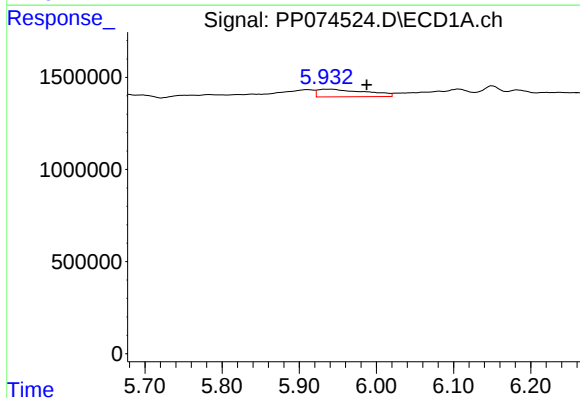


#14 AR-1232-4

R.T.: 5.934 min
Delta R.T.: -0.054 min
Response: 1778920
Conc: 103.01 ng/ml

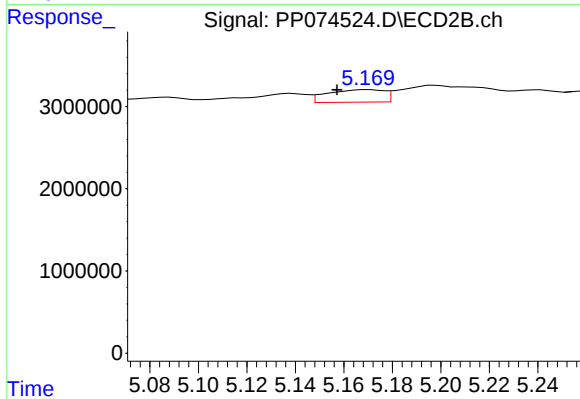

#14 AR-1232-4


R.T.: 5.170 min
Delta R.T.: 0.013 min
Response: 2446130
Conc: 33.19 ng/ml

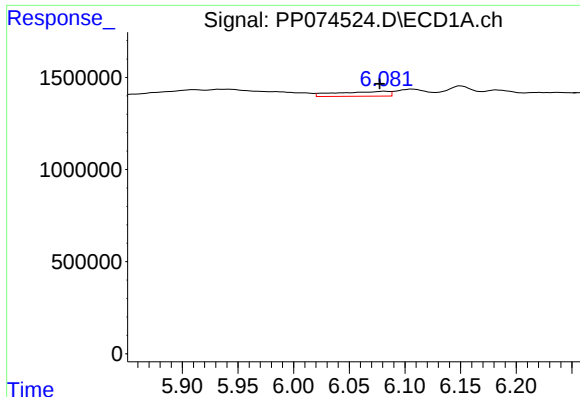

#15 AR-1232-5


R.T.: 6.082 min
Delta R.T.: 0.005 min
Response: 846980
Conc: 65.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

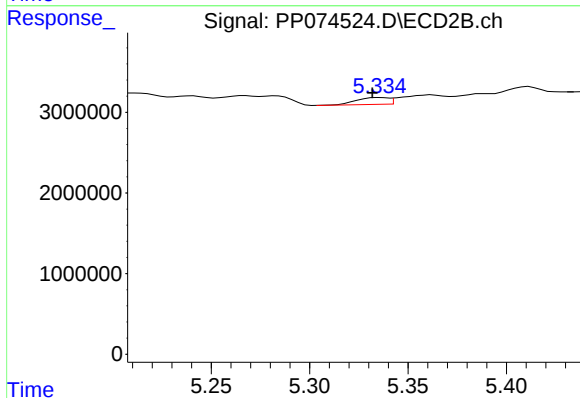


#15 AR-1232-5

R.T.: 5.336 min
Delta R.T.: 0.004 min
Response: 968354
Conc: 15.60 ng/ml

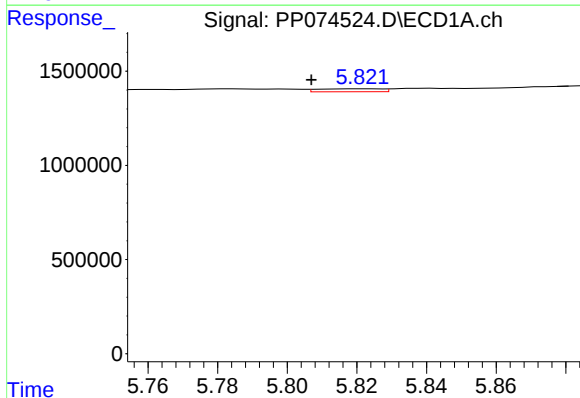


#16 AR-1242-1

R.T.: 5.823 min
Delta R.T.: 0.016 min
Response: 198723
Conc: 5.19 ng/ml

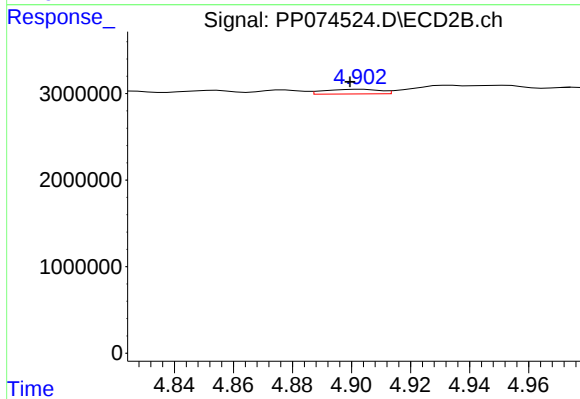

#16 AR-1242-1


R.T.: 4.903 min
Delta R.T.: 0.004 min
Response: 686777
Conc: 1.63 ng/ml

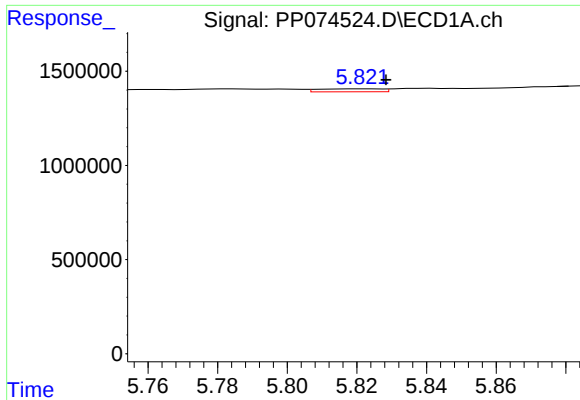

#17 AR-1242-2


R.T.: 5.823 min
Delta R.T.: -0.005 min
Response: 198723
Conc: 3.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

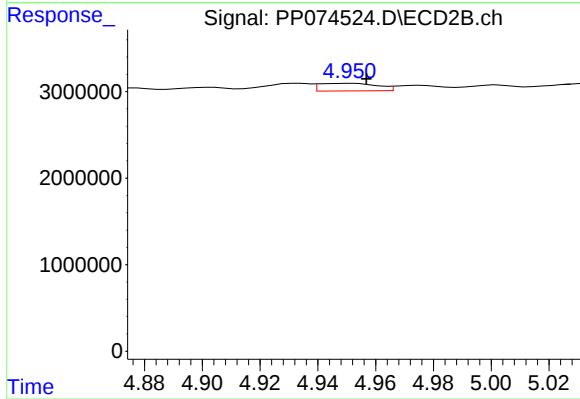


#17 AR-1242-2

R.T.: 4.951 min
Delta R.T.: -0.006 min
Response: 1240948
Conc: 6.20 ng/ml

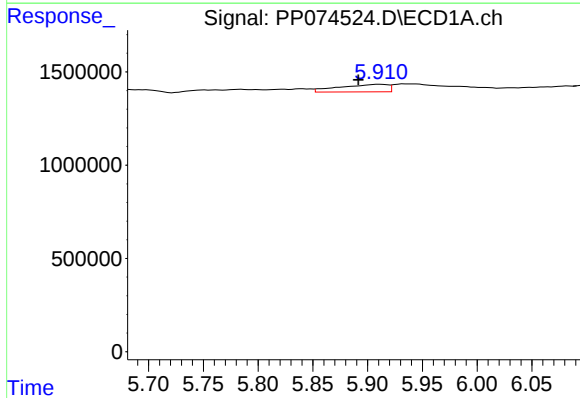


#18 AR-1242-3

R.T.: 5.911 min
Delta R.T.: 0.020 min
Response: 1228605
Conc: 30.26 ng/ml

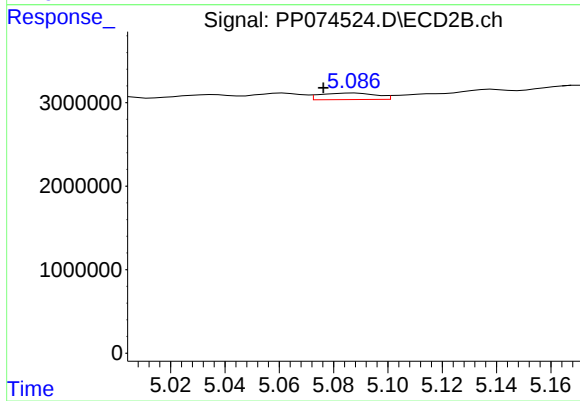

#18 AR-1242-3


R.T.: 5.088 min
Delta R.T.: 0.011 min
Response: 1110900
Conc: 9.39 ng/ml

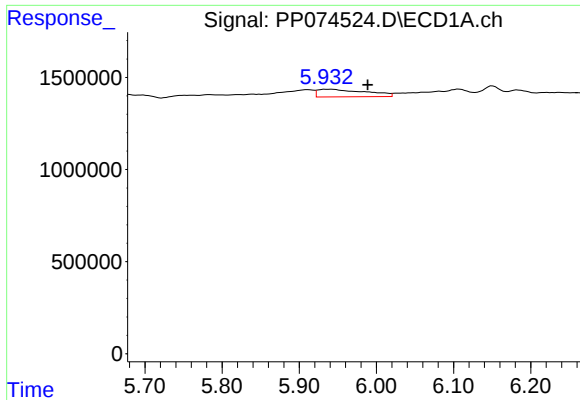

#19 AR-1242-4


R.T.: 5.934 min
Delta R.T.: -0.055 min
Response: 1778920
Conc: 56.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

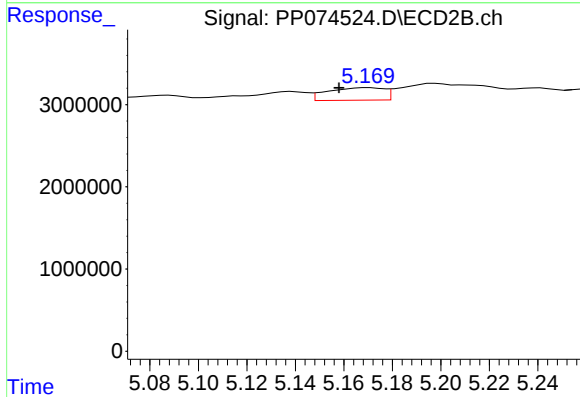


#19 AR-1242-4

R.T.: 5.170 min
Delta R.T.: 0.012 min
Response: 2446130
Conc: 14.29 ng/ml

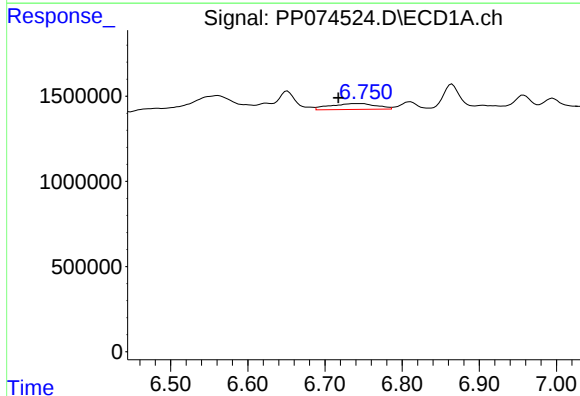


#20 AR-1242-5

R.T.: 6.750 min
Delta R.T.: 0.032 min
Response: 1433953
Conc: 39.75 ng/ml

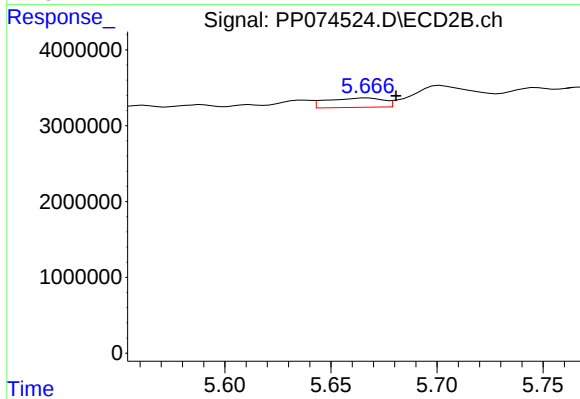

#20 AR-1242-5


R.T.: 5.667 min
Delta R.T.: -0.014 min
Response: 2302076
Conc: 12.43 ng/ml

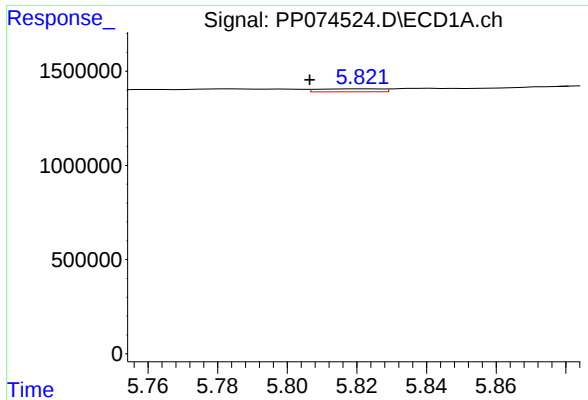

#21 AR-1248-1


R.T.: 5.823 min
Delta R.T.: 0.017 min
Response: 198723
Conc: 6.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

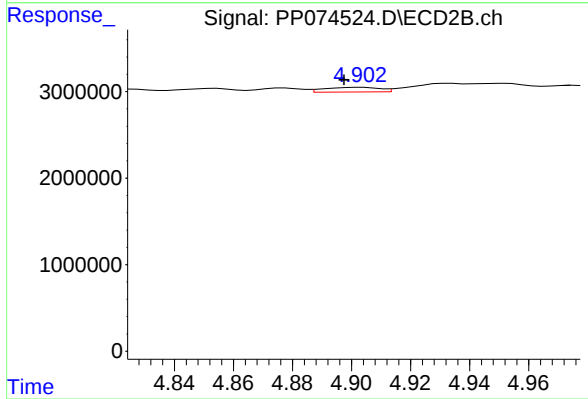


#21 AR-1248-1

R.T.: 4.903 min
Delta R.T.: 0.006 min
Response: 686777
Conc: 2.49 ng/ml

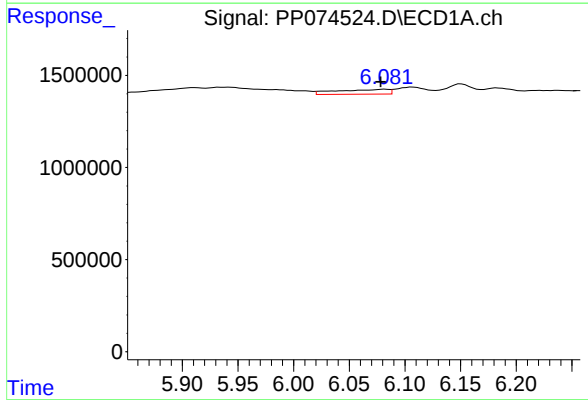


#22 AR-1248-2

R.T.: 6.082 min
Delta R.T.: 0.004 min
Response: 846980
Conc: 19.65 ng/ml

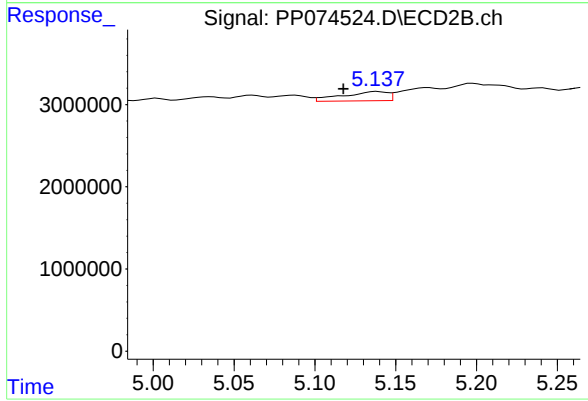

#22 AR-1248-2


R.T.: 5.139 min
Delta R.T.: 0.021 min
Response: 2166559
Conc: 12.26 ng/ml

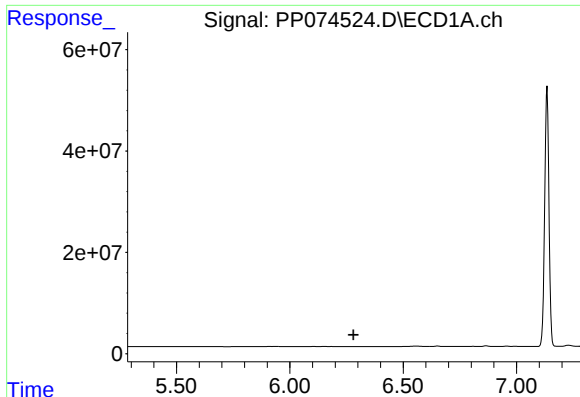

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 6.281 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

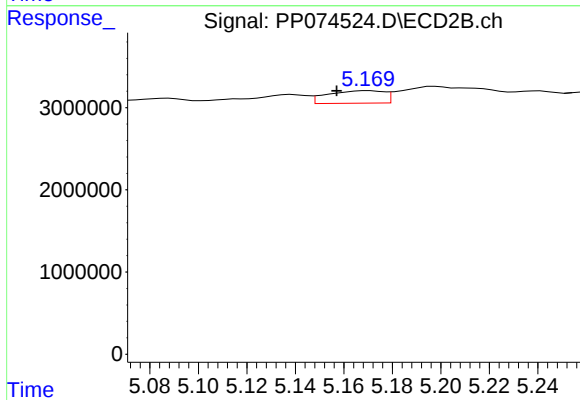


#23 AR-1248-3

R.T.: 5.170 min
Delta R.T.: 0.013 min
Response: 2446130
Conc: 10.77 ng/ml

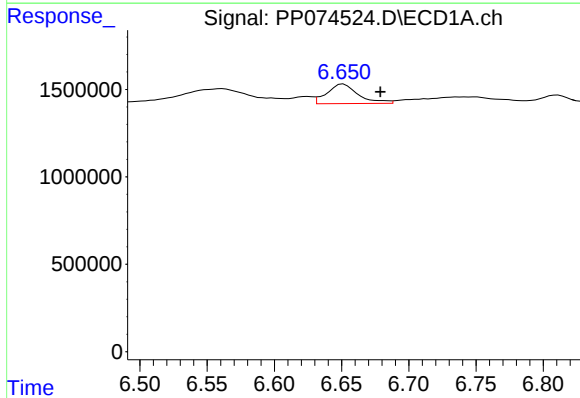


#24 AR-1248-4

R.T.: 6.651 min
Delta R.T.: -0.027 min
Response: 1815290
Conc: 33.00 ng/ml

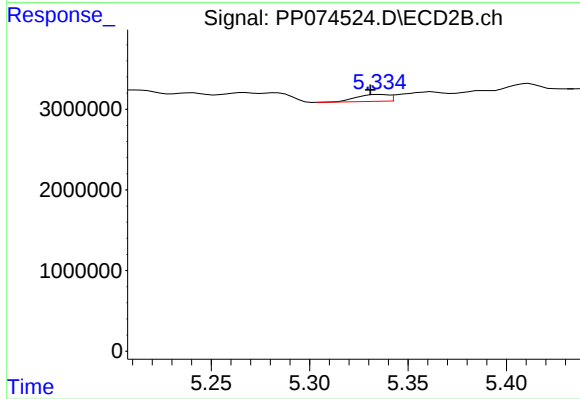

#24 AR-1248-4


R.T.: 5.336 min
Delta R.T.: 0.005 min
Response: 968354
Conc: 4.44 ng/ml

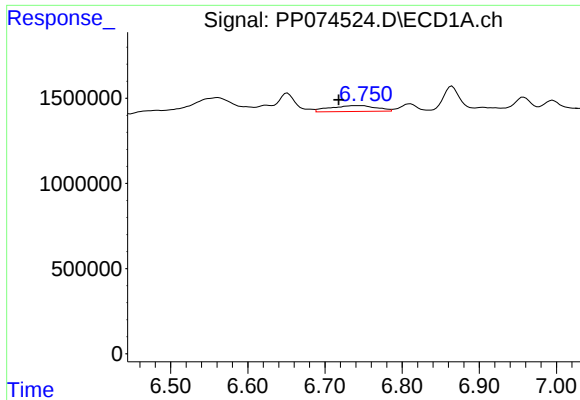

#25 AR-1248-5


R.T.: 6.750 min
Delta R.T.: 0.032 min
Response: 1433953
Conc: 25.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

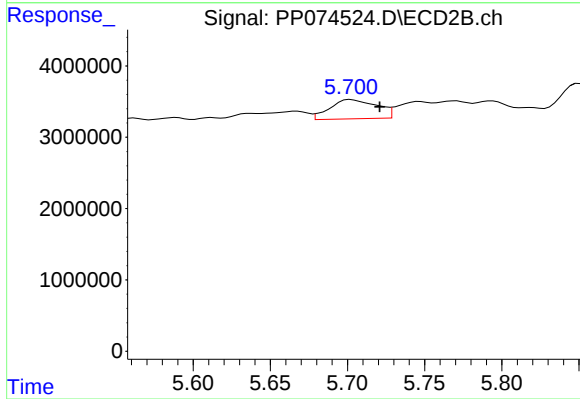


#25 AR-1248-5

R.T.: 5.702 min
Delta R.T.: -0.019 min
Response: 5684171
Conc: 15.47 ng/ml

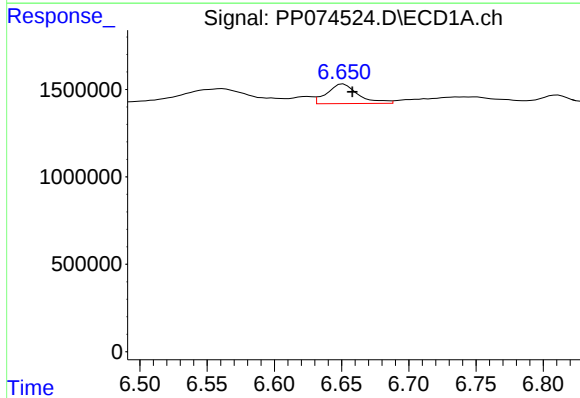


#26 AR-1254-1

R.T.: 6.651 min
Delta R.T.: -0.007 min
Response: 1815290
Conc: 31.15 ng/ml

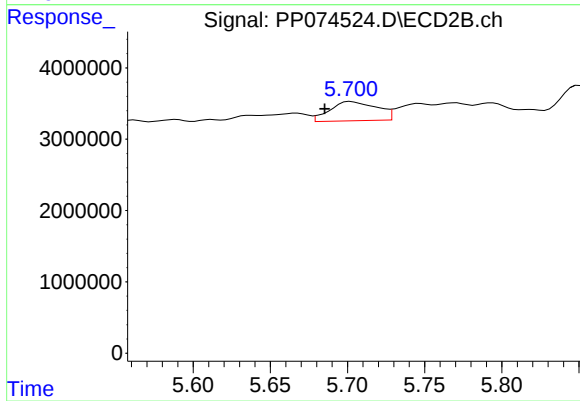

#26 AR-1254-1


R.T.: 5.702 min
Delta R.T.: 0.017 min
Response: 5684171
Conc: 11.92 ng/ml

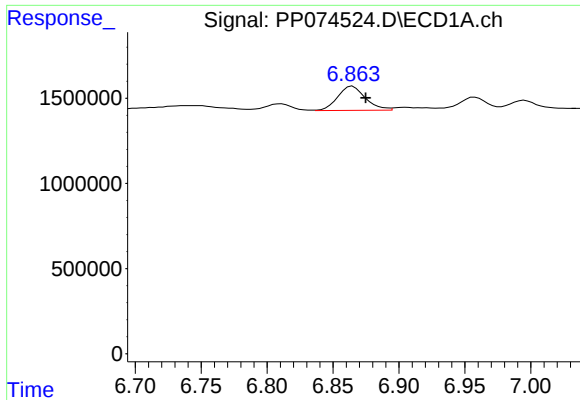

#27 AR-1254-2


R.T.: 6.865 min
Delta R.T.: -0.010 min
Response: 2082611
Conc: 25.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

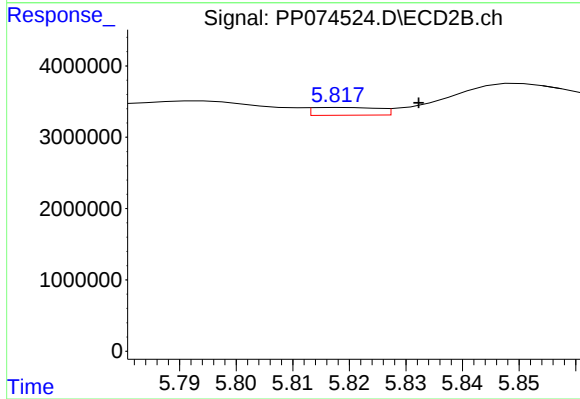


#27 AR-1254-2

R.T.: 5.819 min
Delta R.T.: -0.013 min
Response: 882996
Conc: 2.51 ng/ml

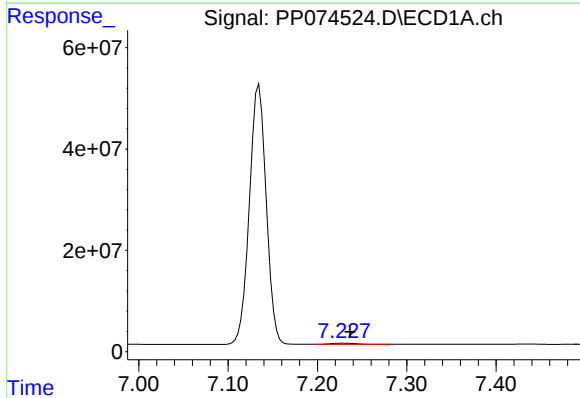


#28 AR-1254-3

R.T.: 7.228 min
Delta R.T.: -0.008 min
Response: 4938148
Conc: 55.36 ng/ml

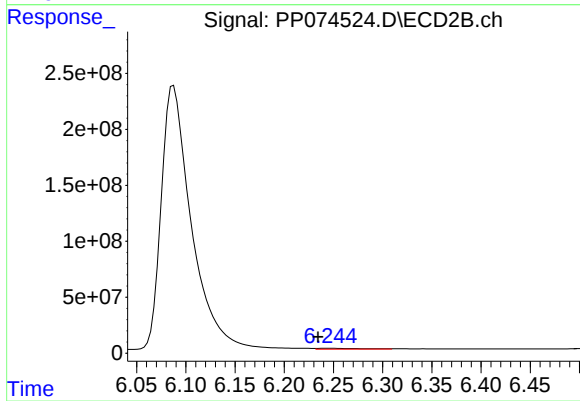

#28 AR-1254-3


R.T.: 6.246 min
Delta R.T.: 0.011 min
Response: 24602108
Conc: 39.69 ng/ml

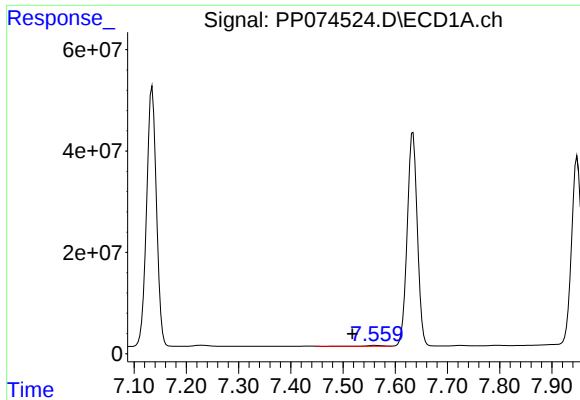

#29 AR-1254-4


R.T.: 7.561 min
Delta R.T.: 0.043 min
Response: 2478680
Conc: 37.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

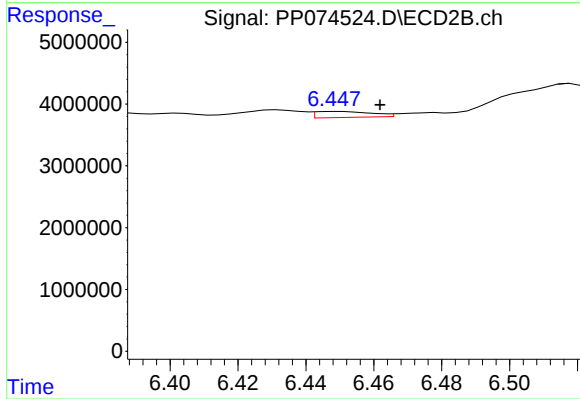


#29 AR-1254-4

R.T.: 6.450 min
Delta R.T.: -0.012 min
Response: 1133594
Conc: 2.42 ng/ml

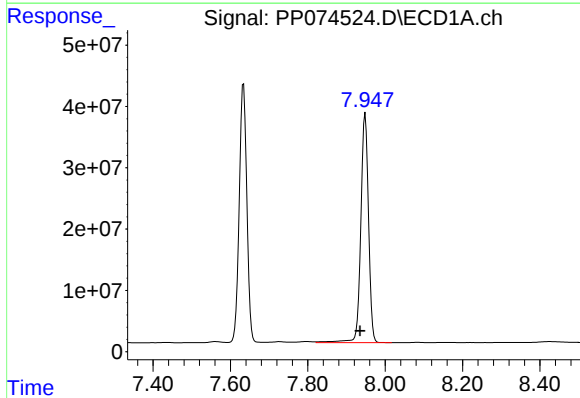


#30 AR-1254-5

R.T.: 7.948 min
Delta R.T.: 0.014 min
Response: 521353320
Conc: 6274.94 ng/ml

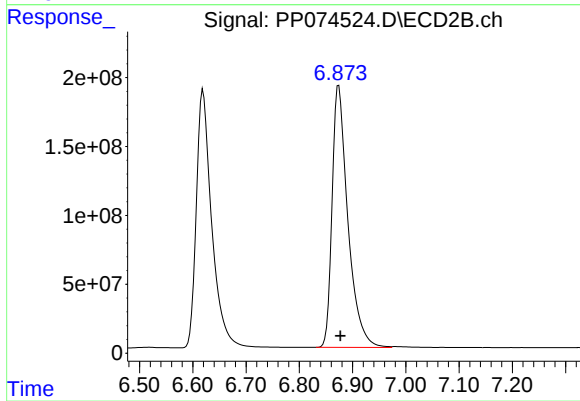

#30 AR-1254-5


R.T.: 6.874 min
Delta R.T.: -0.003 min
Response: 3914372370
Conc: 7980.35 ng/ml

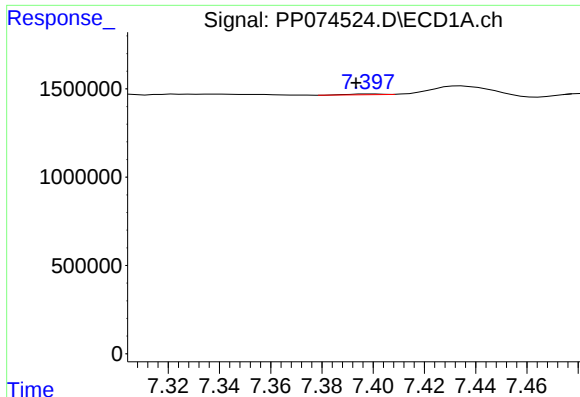

#31 AR-1260-1


R.T.: 7.399 min
Delta R.T.: 0.005 min
Response: 36885
Conc: 0.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

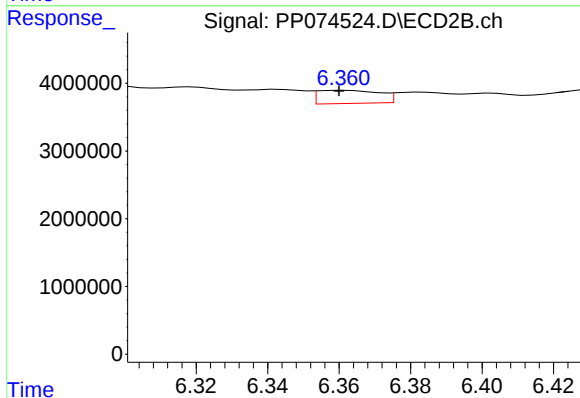


#31 AR-1260-1

R.T.: 6.362 min
Delta R.T.: 0.002 min
Response: 2333152
Conc: 6.22 ng/ml

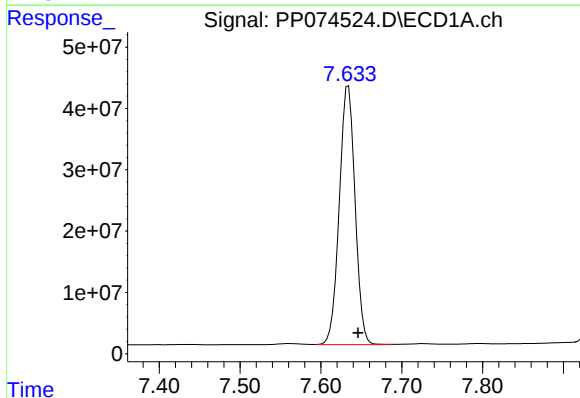


#32 AR-1260-2

R.T.: 7.634 min
Delta R.T.: -0.012 min
Response: 571821250
Conc: 8297.19 ng/ml

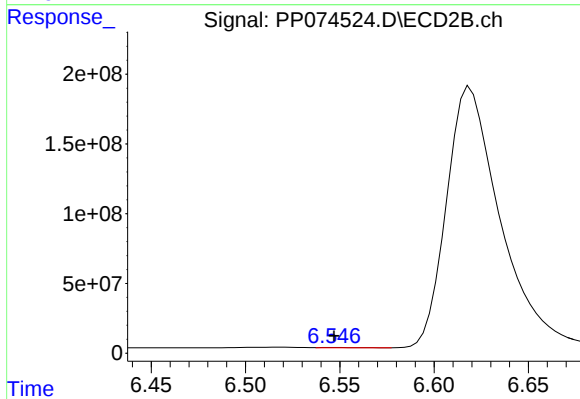

#32 AR-1260-2


R.T.: 6.547 min
Delta R.T.: 0.000 min
Response: 2821126
Conc: 5.33 ng/ml

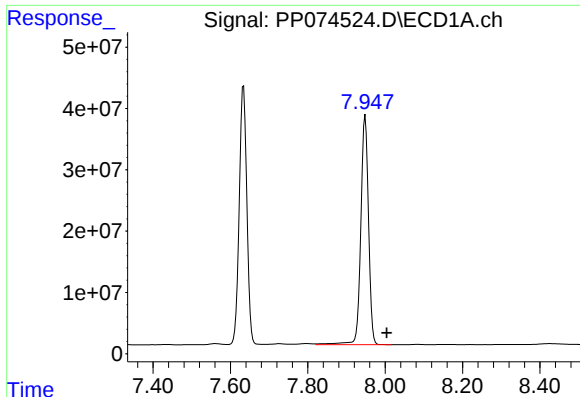

#33 AR-1260-3


R.T.: 7.948 min
Delta R.T.: -0.056 min
Response: 521353320
Conc: 10048.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

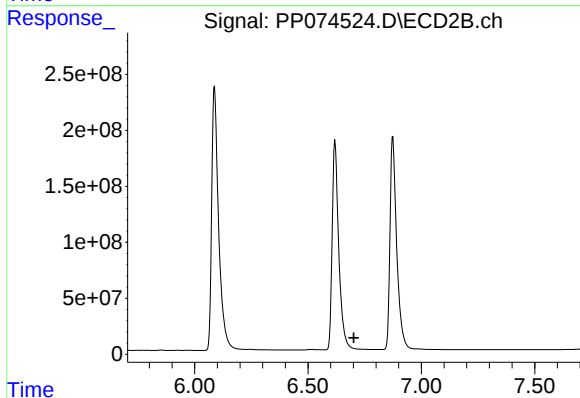


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.702 min
Response: 0
Conc: N.D.

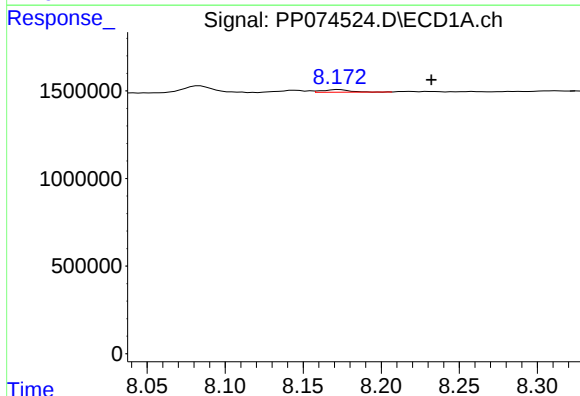


#34 AR-1260-4

R.T.: 8.173 min
Delta R.T.: -0.059 min
Response: 174857
Conc: 2.74 ng/ml

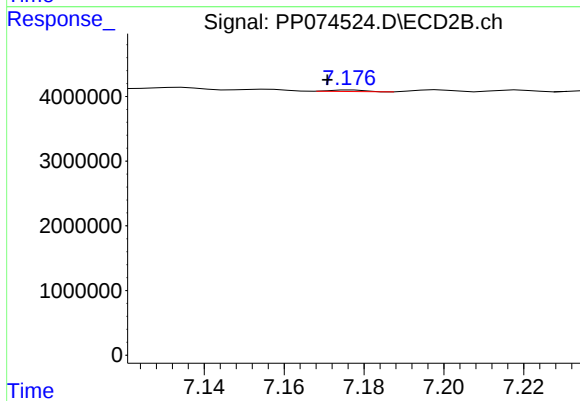

#34 AR-1260-4


R.T.: 7.177 min
Delta R.T.: 0.006 min
Response: 153087
Conc: 0.40 ng/ml

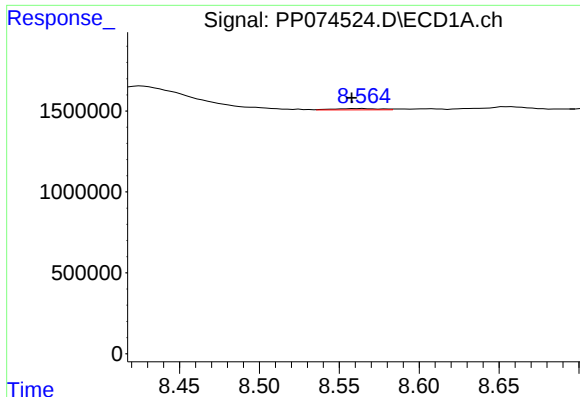

#35 AR-1260-5


R.T.: 8.564 min
Delta R.T.: 0.007 min
Response: 162218
Conc: 1.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

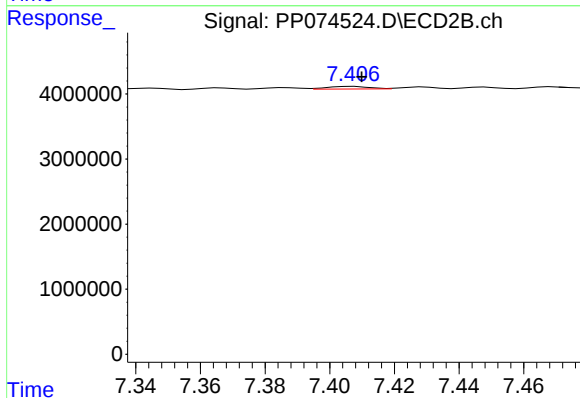


#35 AR-1260-5

R.T.: 7.407 min
Delta R.T.: -0.003 min
Response: 358204
Conc: 0.36 ng/ml

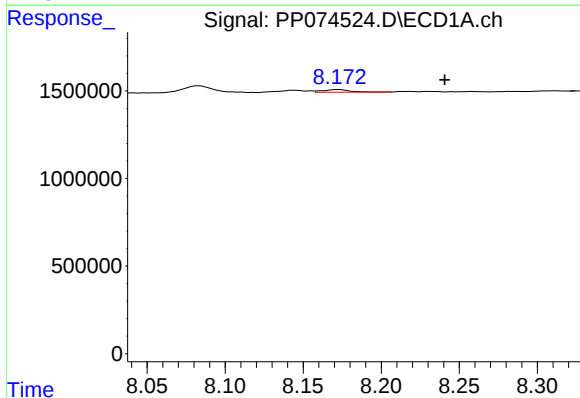


#36 AR-1262-1

R.T.: 8.173 min
Delta R.T.: -0.068 min
Response: 174857
Conc: 2.27 ng/ml

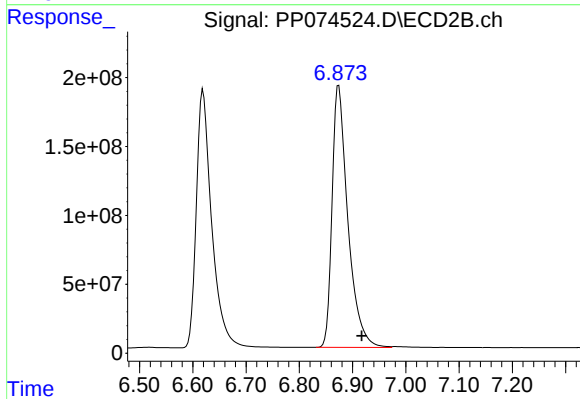

#36 AR-1262-1


R.T.: 6.874 min
Delta R.T.: -0.043 min
Response: 3914372370
Conc: 5534.57 ng/ml

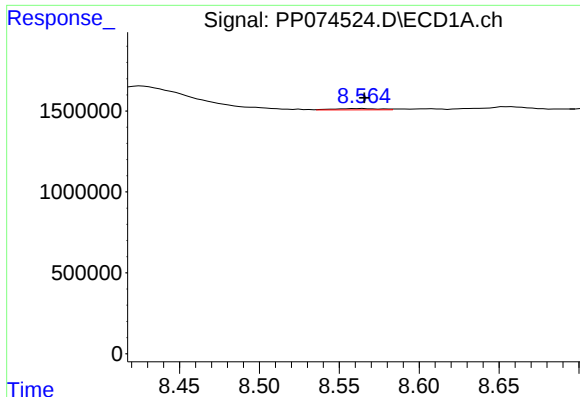

#37 AR-1262-2


R.T.: 8.564 min
Delta R.T.: -0.001 min
Response: 162218
Conc: 1.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

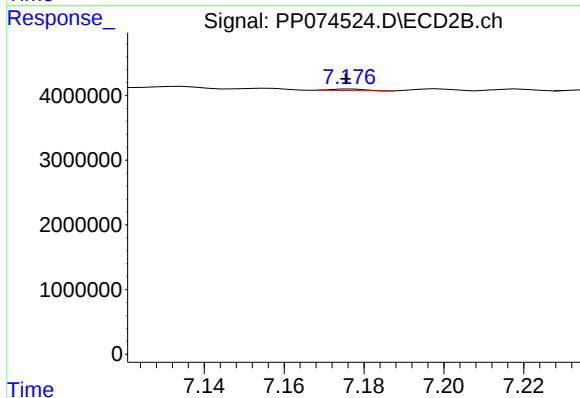


#37 AR-1262-2

R.T.: 7.177 min
Delta R.T.: 0.002 min
Response: 153087
Conc: 0.29 ng/ml

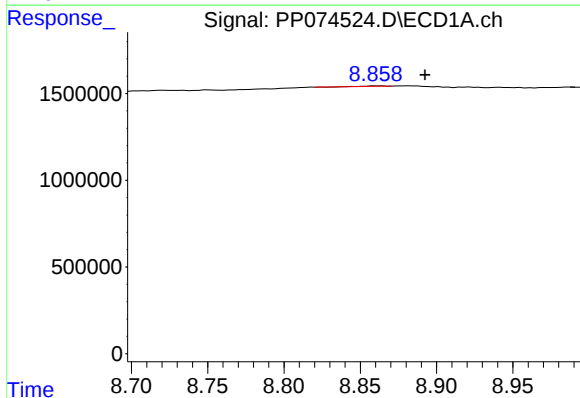


#38 AR-1262-3

R.T.: 8.860 min
Delta R.T.: -0.032 min
Response: 17824
Conc: 0.18 ng/ml

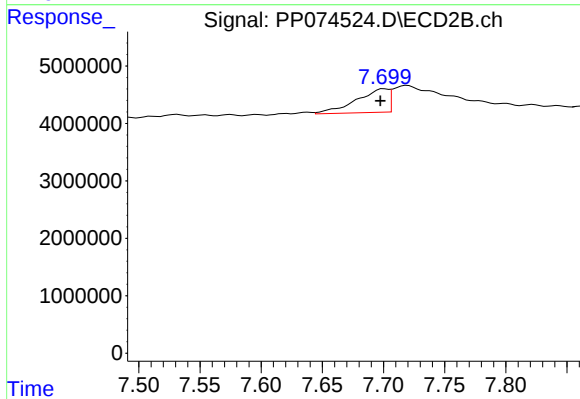

#38 AR-1262-3


R.T.: 7.701 min
Delta R.T.: 0.003 min
Response: 7497577
Conc: 16.08 ng/ml

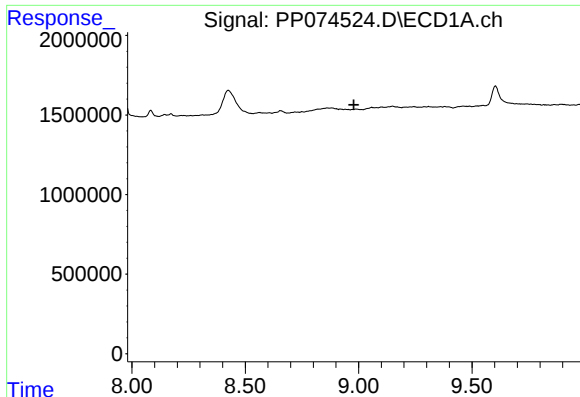

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

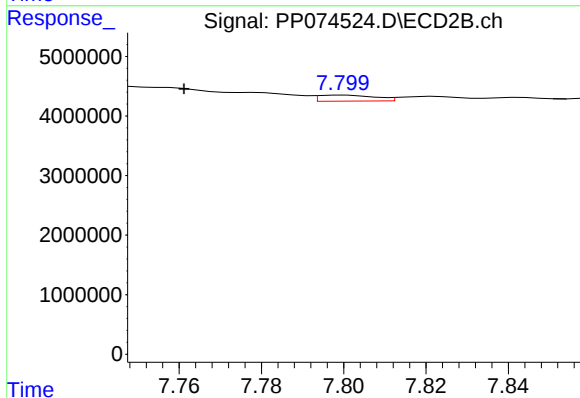


#39 AR-1262-4

R.T.: 7.800 min
Delta R.T.: 0.039 min
Response: 967974
Conc: 1.18 ng/ml

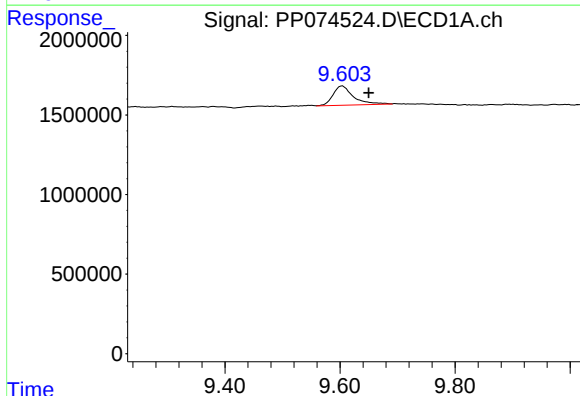


#40 AR-1262-5

R.T.: 9.604 min
Delta R.T.: -0.045 min
Response: 3002114
Conc: 49.25 ng/ml

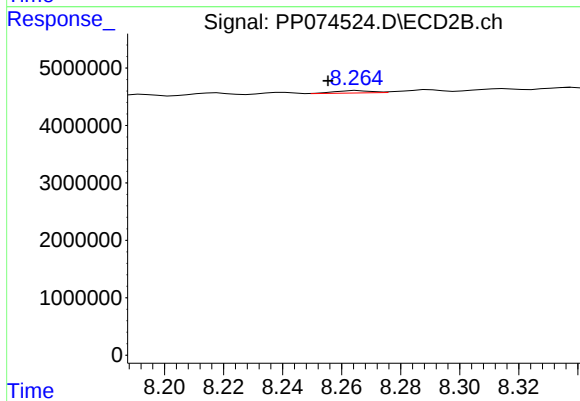

#40 AR-1262-5


R.T.: 8.265 min
Delta R.T.: 0.010 min
Response: 342356
Conc: 0.96 ng/ml

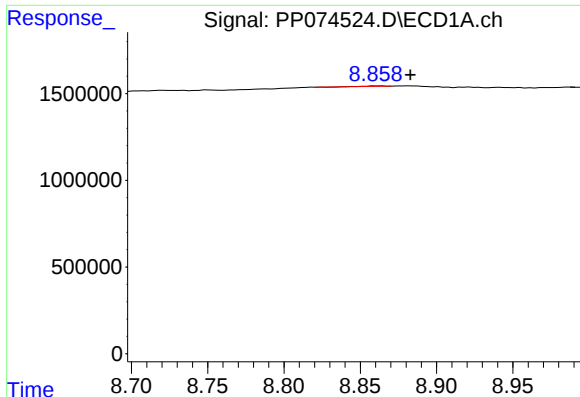

#41 AR-1268-1


R.T.: 8.860 min
Delta R.T.: -0.023 min
Response: 17824
Conc: 0.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

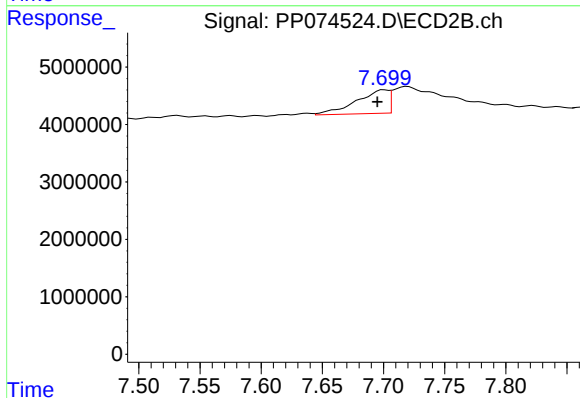


#41 AR-1268-1

R.T.: 7.701 min
Delta R.T.: 0.006 min
Response: 7497577
Conc: 5.32 ng/ml

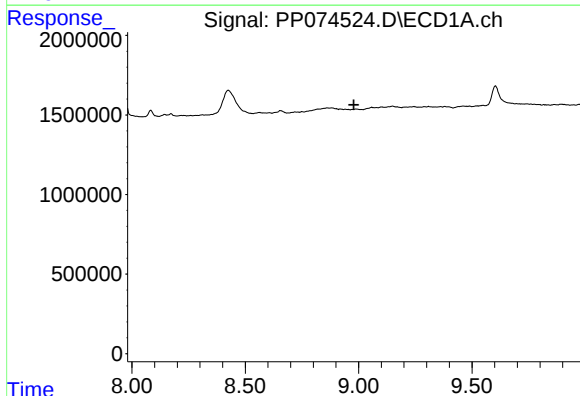


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.978 min
Response: 0
Conc: N.D.

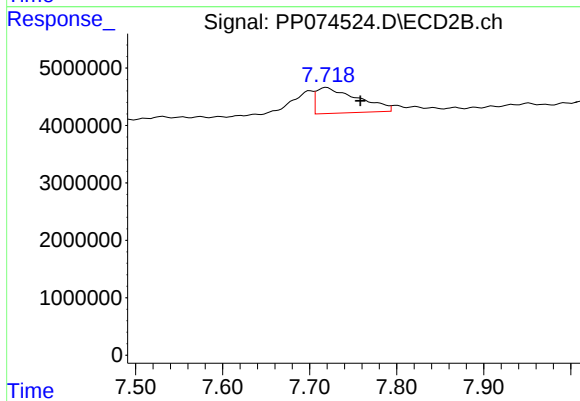

#42 AR-1268-2


R.T.: 7.720 min
Delta R.T.: -0.039 min
Response: 14890679
Conc: 10.92 ng/ml

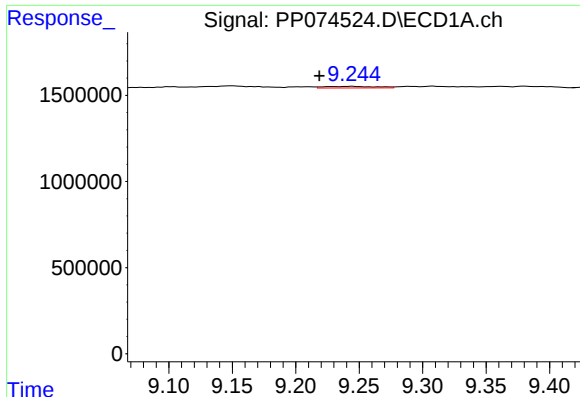

#43 AR-1268-3


R.T.: 9.245 min
Delta R.T.: 0.027 min
Response: 270087
Conc: 2.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

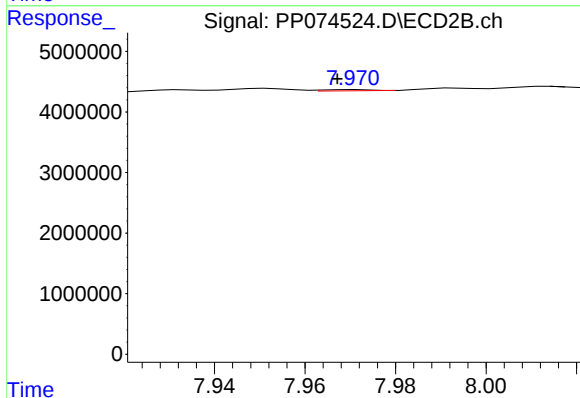


#43 AR-1268-3

R.T.: 7.971 min
Delta R.T.: 0.004 min
Response: 139504
Conc: 0.13 ng/ml

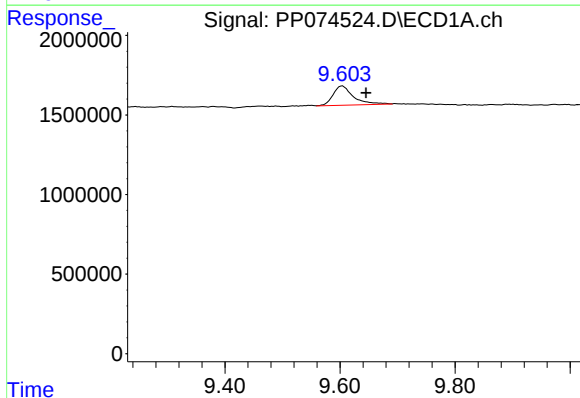


#44 AR-1268-4

R.T.: 9.604 min
Delta R.T.: -0.041 min
Response: 3002114
Conc: 44.63 ng/ml

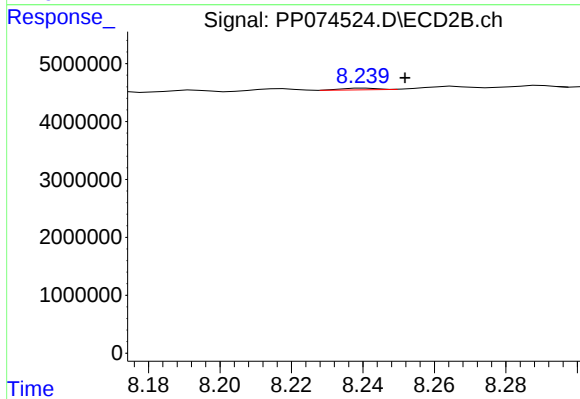

#44 AR-1268-4


R.T.: 8.241 min
Delta R.T.: -0.011 min
Response: 200233
Conc: 0.52 ng/ml

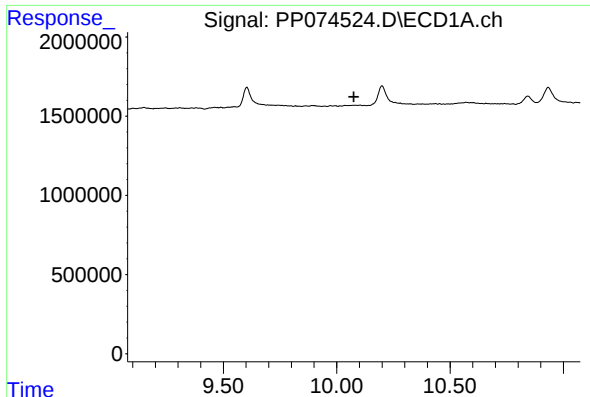

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.076 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

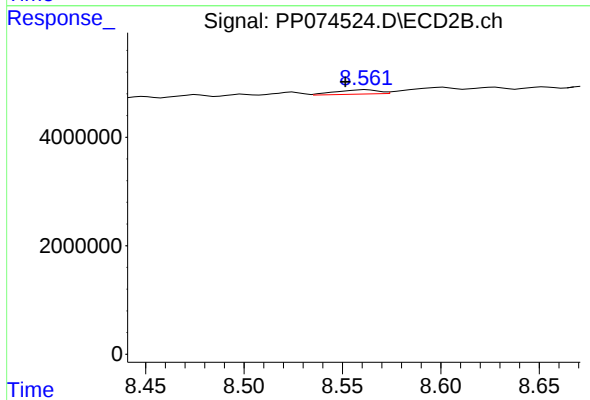

#45 AR-1268-5

R.T.: 8.562 min
Delta R.T.: 0.011 min
Response: 1205036
Conc: 0.38 ng/ml