

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082019\
 Data File : PP030408.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Aug 2019 13:29
 Operator : SM\AJ
 Sample : K4387-26
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 05:22:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081419.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 15 11:48:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	10.919	11.051	189.4E6	104.0E6	552.829	464.439
Target Compounds							
6) T	MCP	11.558	11.621	53483798	7319065	72.162	17.961 #
9) T	2,4-D	12.795	0.000	276.2E6	0	651.538	N.D. #
15) T	Picloram	16.338	0.000	20622065	0	6.721	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082019\
Data File : PP030408.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Aug 2019 13:29
Operator : SM\AJ
Sample : K4387-26
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 05:22:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081419.M
Quant Title : 8080.M
QLast Update : Thu Aug 15 11:48:40 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

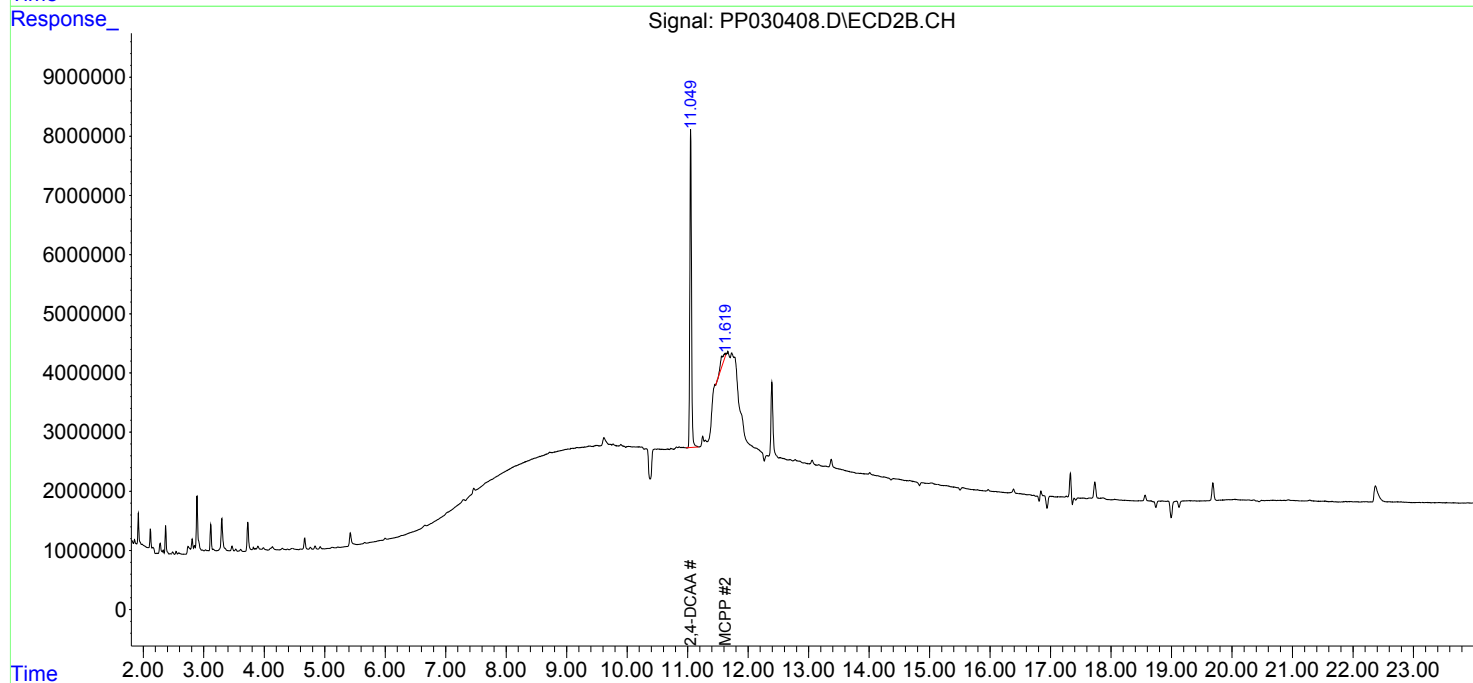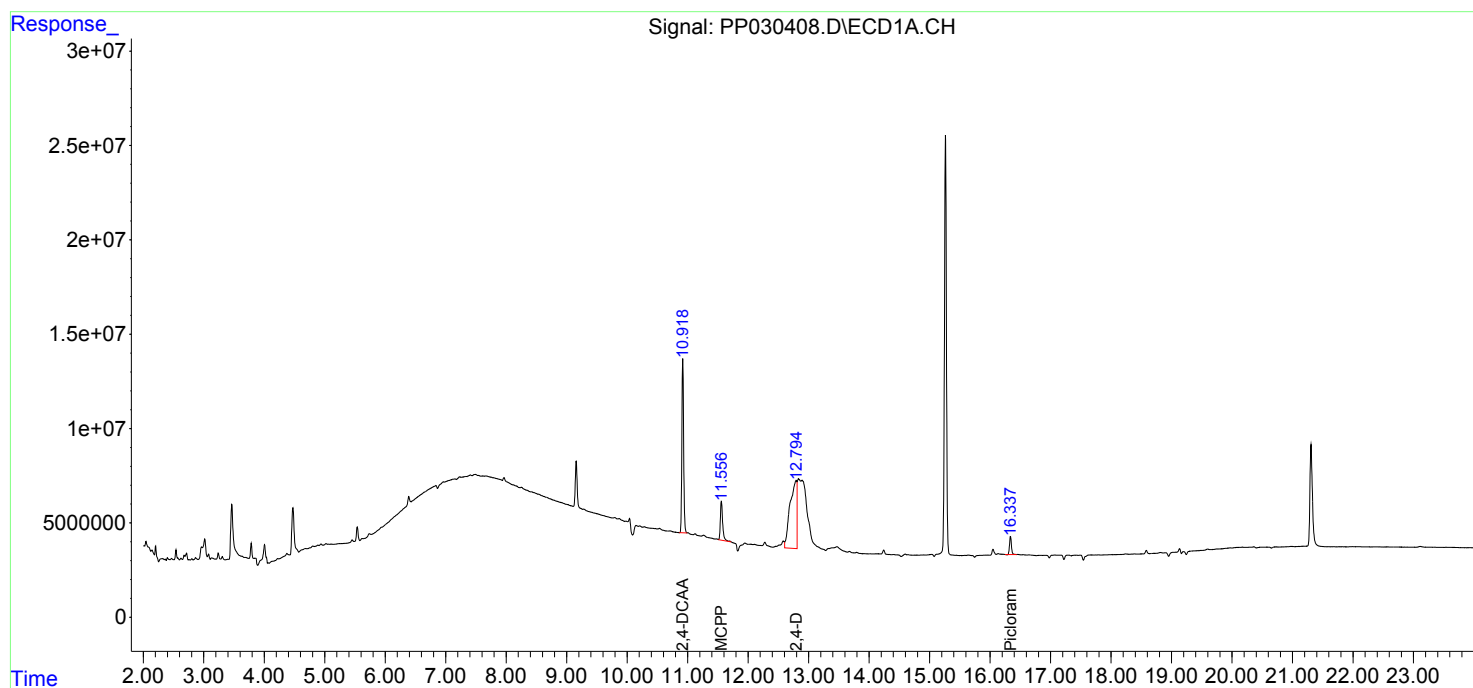


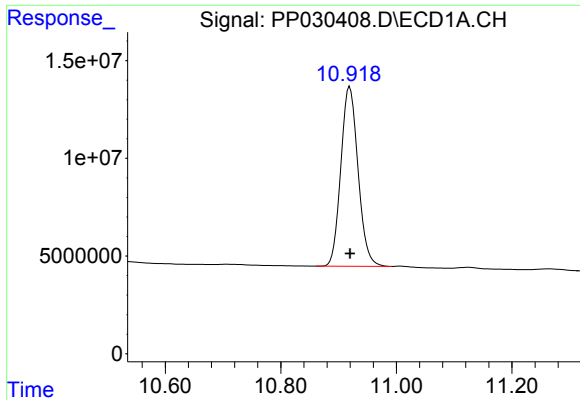

#4 2,4-DCAA


R.T.: 10.919 min
Delta R.T.: 0.000 min
Response: 189425728
Conc: 552.83 ng/ml

Instrument :
ECD_P
ClientSampleId :

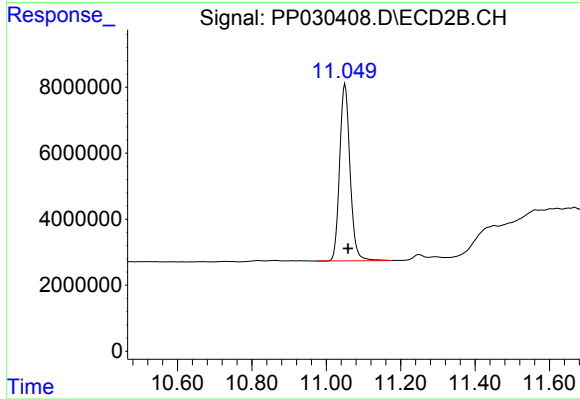


#4 2,4-DCAA

R.T.: 11.051 min
Delta R.T.: -0.008 min
Response: 104038241
Conc: 464.44 ng/ml

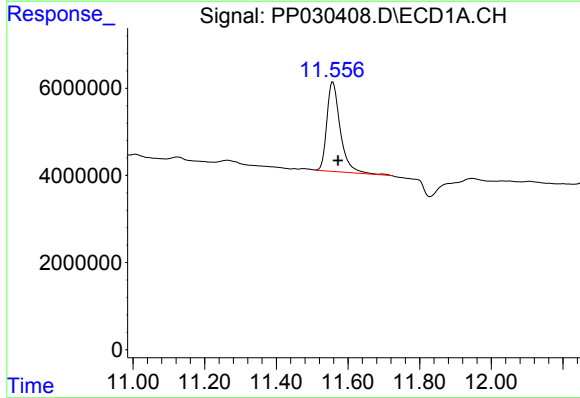


#6 MCP

R.T.: 11.558 min
Delta R.T.: -0.015 min
Response: 53483798
Conc: 72.16 ug/ml

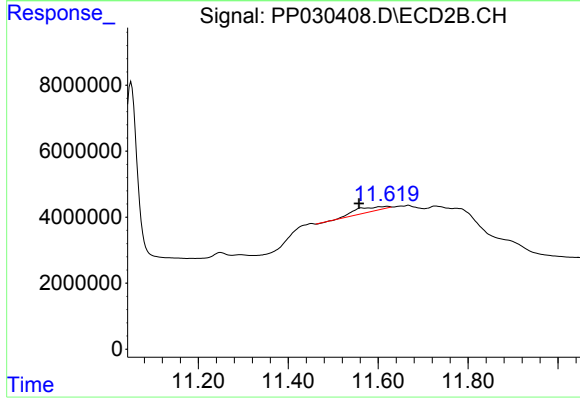

#6 MCP


R.T.: 11.621 min
Delta R.T.: 0.063 min
Response: 7319065
Conc: 17.96 ug/ml

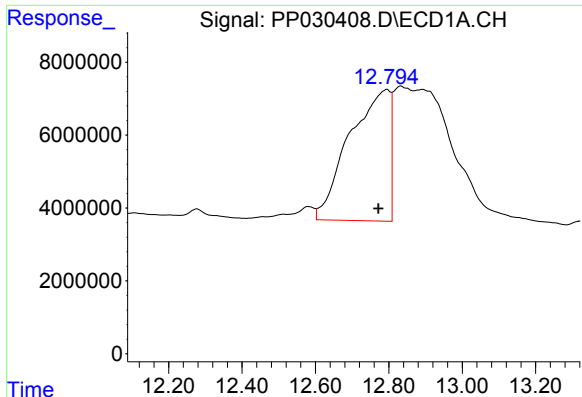

#9 2,4-D


R.T.: 12.795 min
Delta R.T.: 0.023 min
Response: 276226862
Conc: 651.54 ng/ml

Instrument :
ECD_P
ClientSampleId :

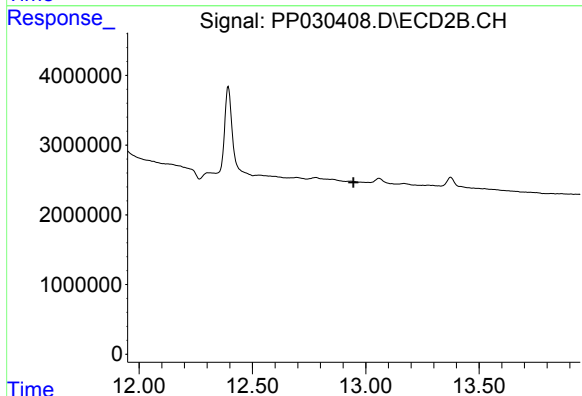


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 12.947 min
Response: 0
Conc: N.D.

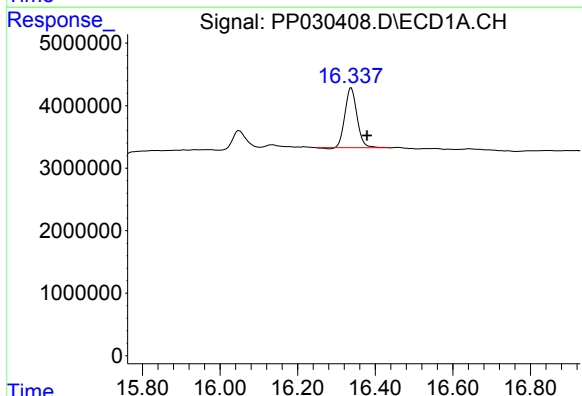

#15 Picloram

R.T.: 16.338 min
Delta R.T.: -0.041 min
Response: 20622065
Conc: 6.72 ng/ml

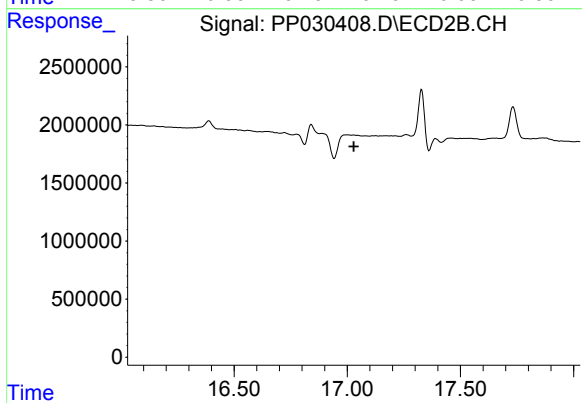

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.029 min
Response: 0
Conc: N.D.