

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082021\
 Data File : PP038699.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Aug 2021 5:57
 Operator : AJ\MA
 Sample : M3463-25
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SWCS-23-0002

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 02:09:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 18 04:51:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.883	3.869	754586	471427	18.697	19.672
2)	SA Decachlor...	10.869	9.128	351569	345622	14.289	14.191
Target Compounds							
8)	L2 AR-1221-1	5.136	0.000	33775	0	72.223	N.D. #
28)	L6 AR-1254-3	7.744f	0.000	22815	0	12.709	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082021\
Data File : PP038699.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Aug 2021 5:57
Operator : AJ\MA
Sample : M3463-25
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SWCS-23-0002

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 02:09:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 18 04:51:26 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

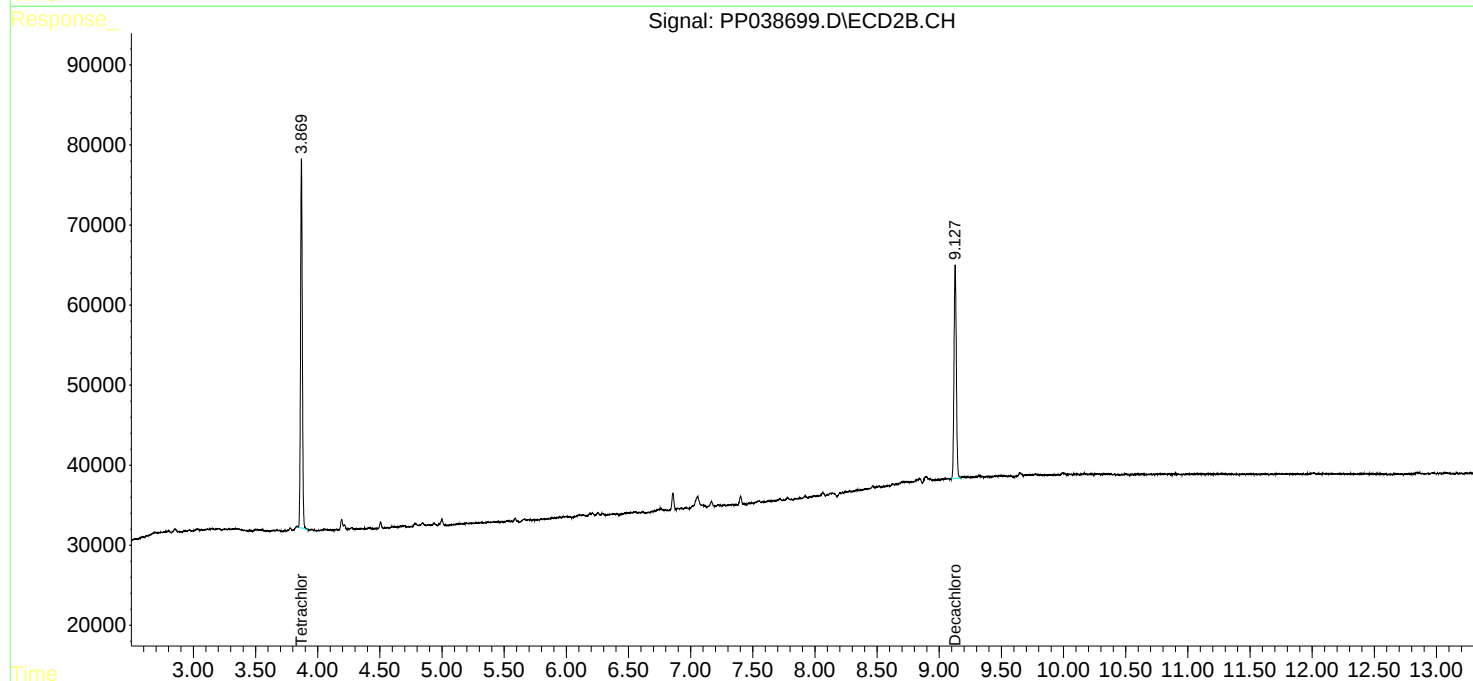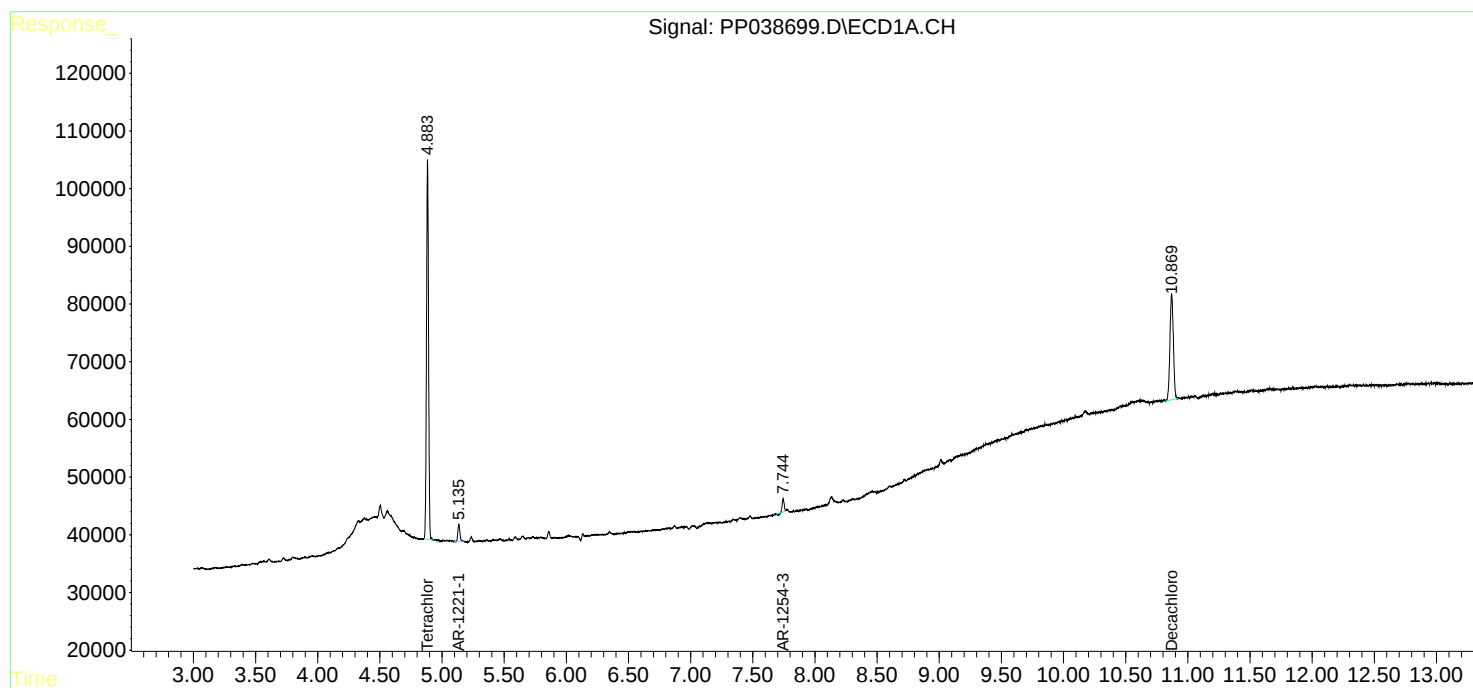


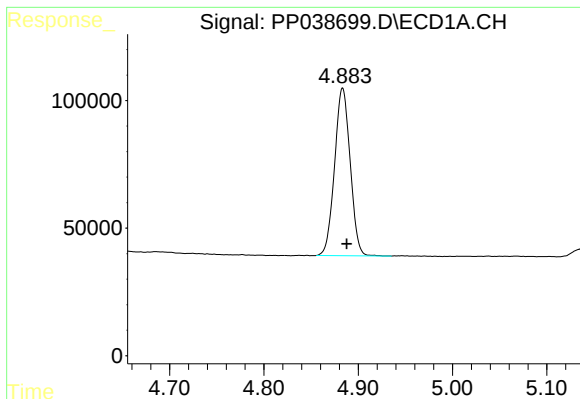

#1 Tetrachloro-m-xylene


R.T.: 4.883 min
Delta R.T.: -0.005 min
Response: 754586
Conc: 18.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
SWCS-23-0002

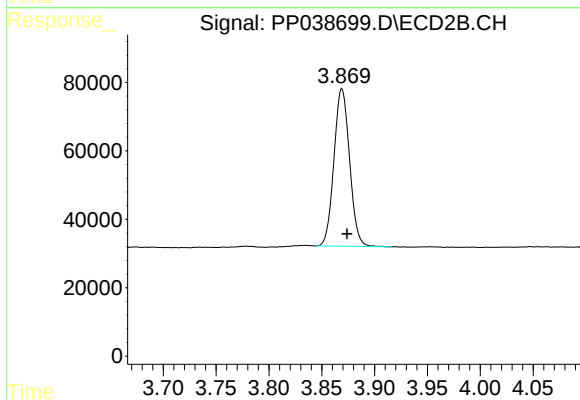


#1 Tetrachloro-m-xylene

R.T.: 3.869 min
Delta R.T.: -0.005 min
Response: 471427
Conc: 19.67 ng/ml

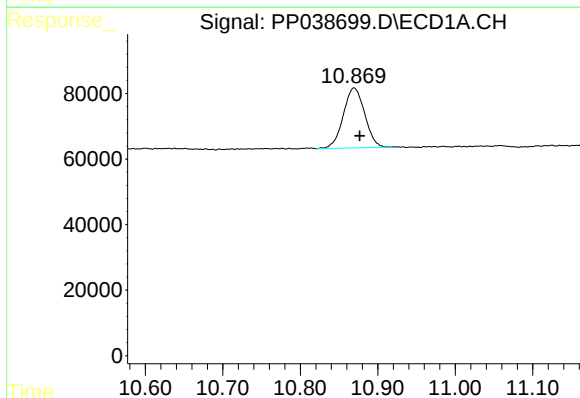


#2 Decachlorobiphenyl

R.T.: 10.869 min
Delta R.T.: -0.007 min
Response: 351569
Conc: 14.29 ng/ml

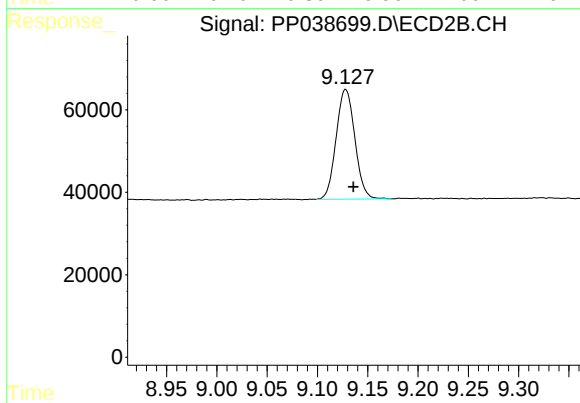

#2 Decachlorobiphenyl


R.T.: 9.128 min
Delta R.T.: -0.008 min
Response: 345622
Conc: 14.19 ng/ml

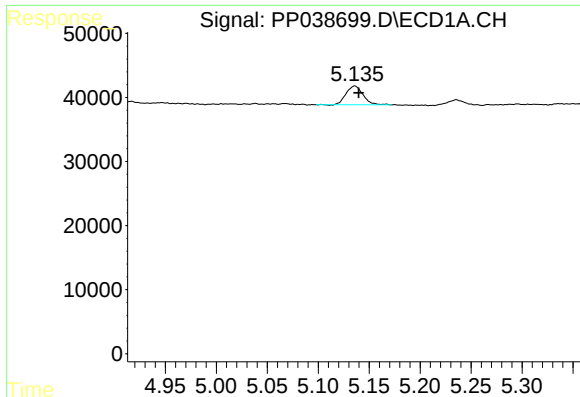

#8 AR-1221-1


R.T.: 5.136 min
Delta R.T.: -0.004 min
Response: 33775
Conc: 72.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
SWCS-23-0002

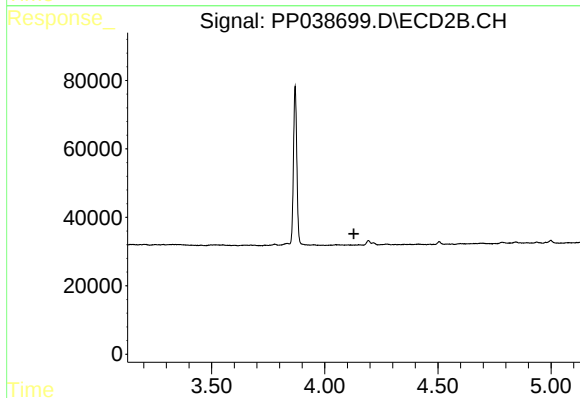


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.129 min
Response: 0
Conc: N.D.

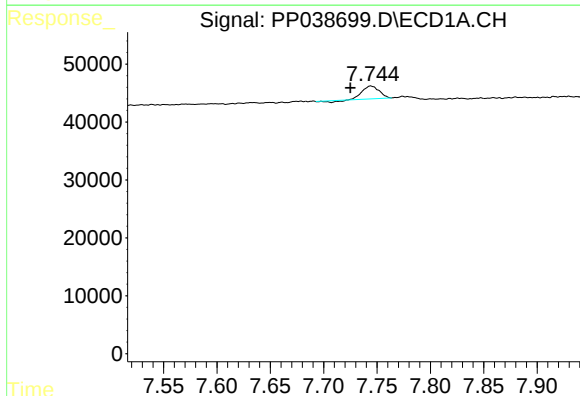

#28 AR-1254-3

R.T.: 7.744 min
Delta R.T.: 0.019 min
Response: 22815
Conc: 12.71 ng/ml

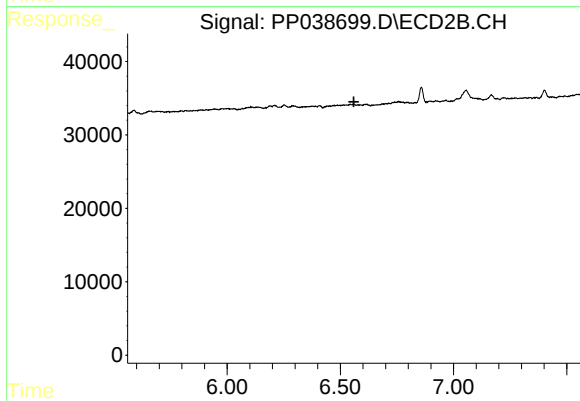

#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.560 min
Response: 0
Conc: N.D.