

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082021\
 Data File : PP038702.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Aug 2021 6:48
 Operator : AJ\MA
 Sample : M3463-31
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 02:10:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 18 04:51:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.883	3.869	779590	490262	19.317	20.458
2)	SA Decachlor...	10.868	9.128	352275	349765	14.318	14.361
Target Compounds							
8)	L2 AR-1221-1	5.136	0.000	26078	0	55.763	N.D. #
27)	L6 AR-1254-2	7.342	0.000	22337	0	12.935	N.D. #
28)	L6 AR-1254-3	7.744f	0.000	32650	0	18.188	N.D. #
29)	L6 AR-1254-4	8.019	0.000	23333	0	18.083	N.D. #
30)	L6 AR-1254-5	8.447	0.000	101301	0	81.905	N.D. #
32)	L7 AR-1260-2	8.154	0.000	54822	0	37.365	N.D. #
34)	L7 AR-1260-4	8.754	0.000	5936	0	5.220	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082021\
Data File : PP038702.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Aug 2021 6:48
Operator : AJ\MA
Sample : M3463-31
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 02:10:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 18 04:51:26 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

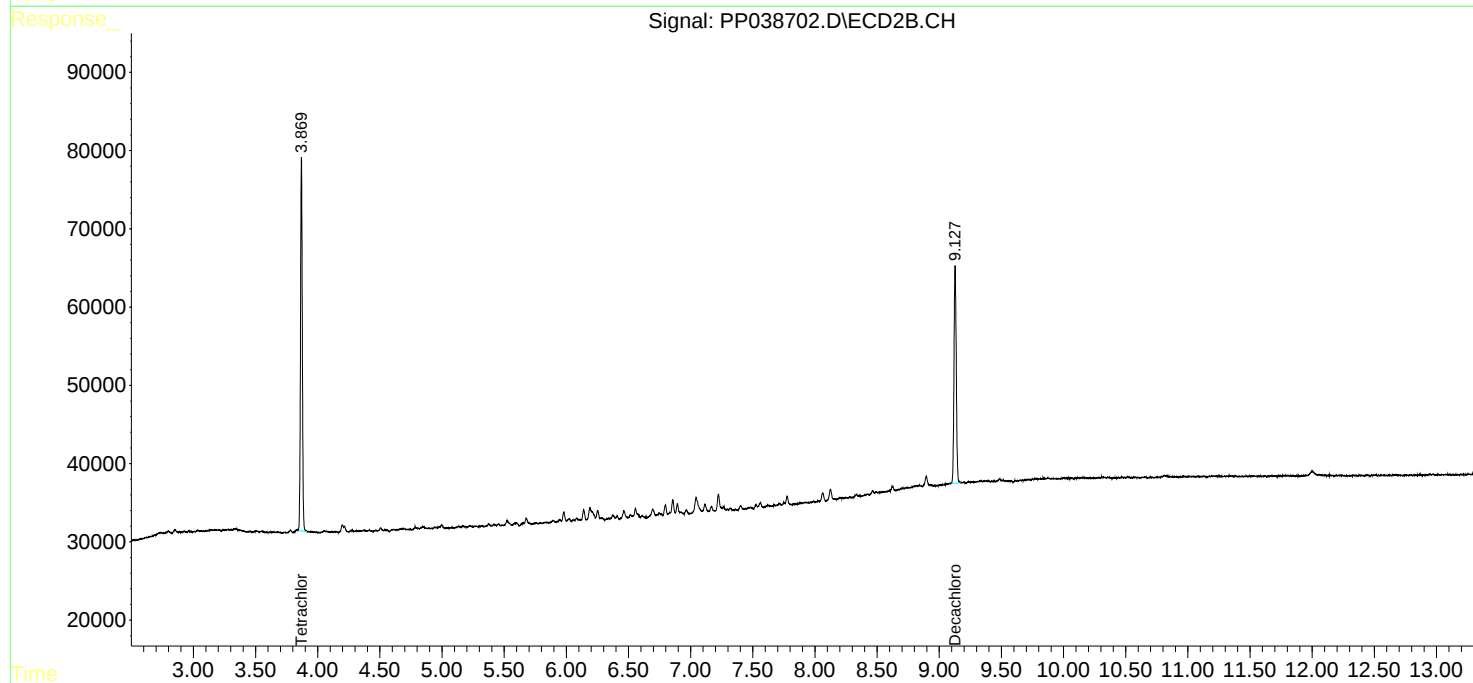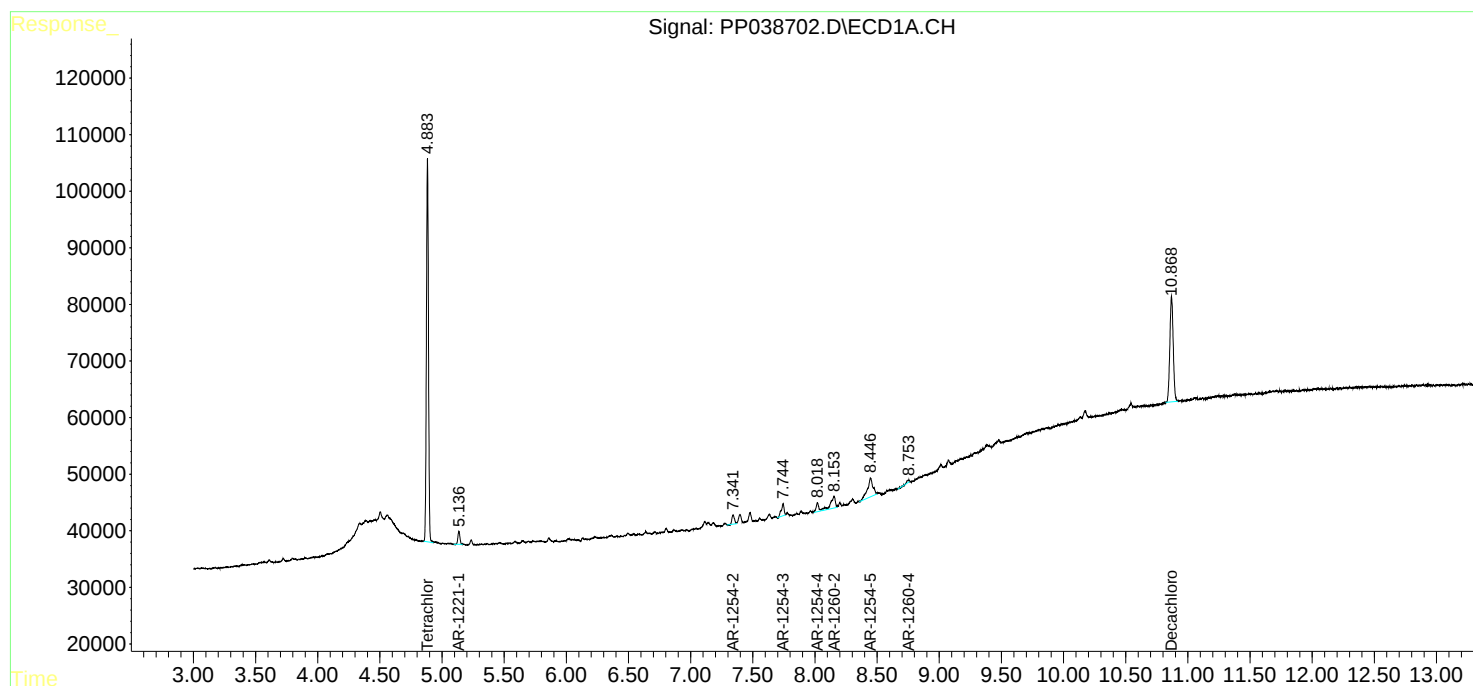


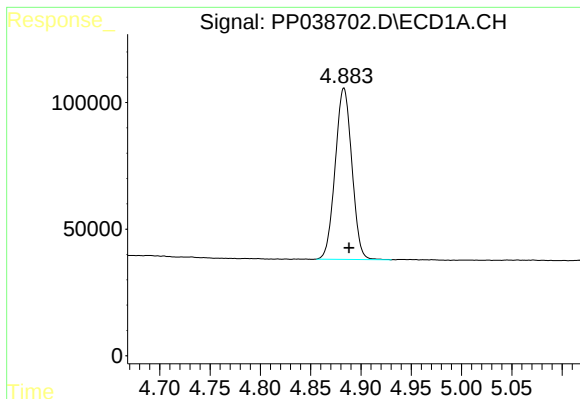

#1 Tetrachloro-m-xylene


R.T.: 4.883 min
Delta R.T.: -0.005 min
Response: 779590
Conc: 19.32 ng/ml

Instrument :
ECD_P
ClientSampleId :

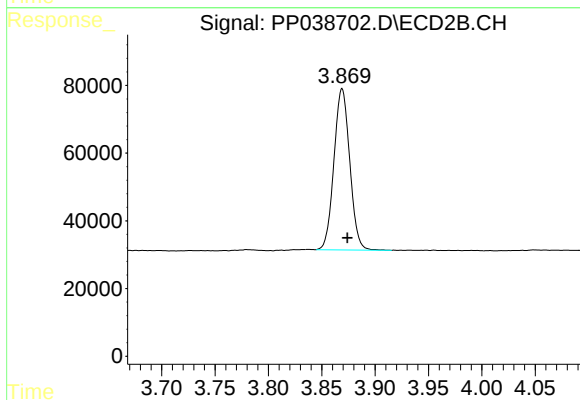


#1 Tetrachloro-m-xylene

R.T.: 3.869 min
Delta R.T.: -0.005 min
Response: 490262
Conc: 20.46 ng/ml

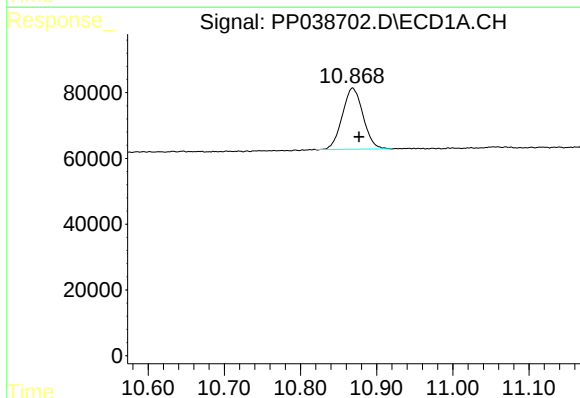


#2 Decachlorobiphenyl

R.T.: 10.868 min
Delta R.T.: -0.008 min
Response: 352275
Conc: 14.32 ng/ml

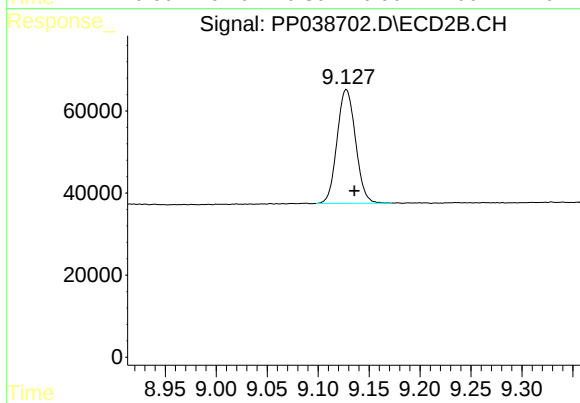

#2 Decachlorobiphenyl


R.T.: 9.128 min
Delta R.T.: -0.008 min
Response: 349765
Conc: 14.36 ng/ml

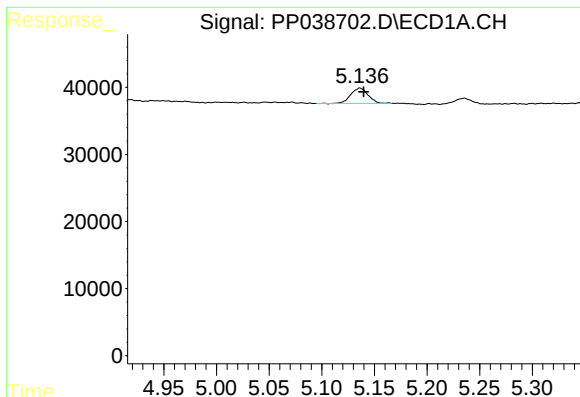

#8 AR-1221-1


R.T.: 5.136 min
Delta R.T.: -0.004 min
Response: 26078
Conc: 55.76 ng/ml

Instrument :
ECD_P
ClientSampleId :

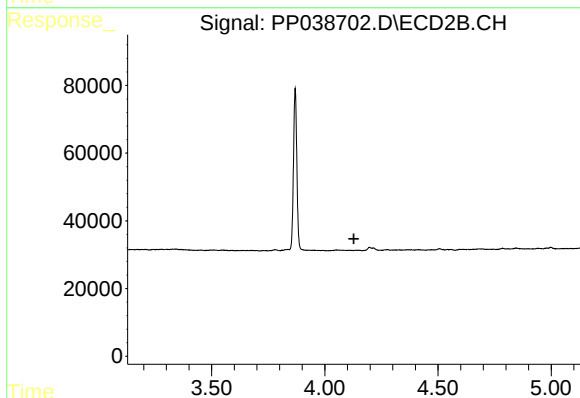


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.129 min
Response: 0
Conc: N.D.

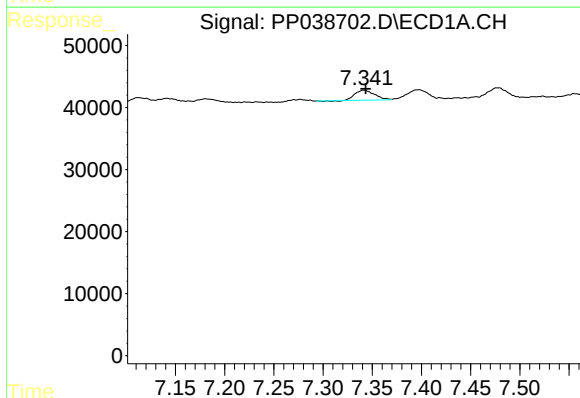


#27 AR-1254-2

R.T.: 7.342 min
Delta R.T.: -0.002 min
Response: 22337
Conc: 12.94 ng/ml

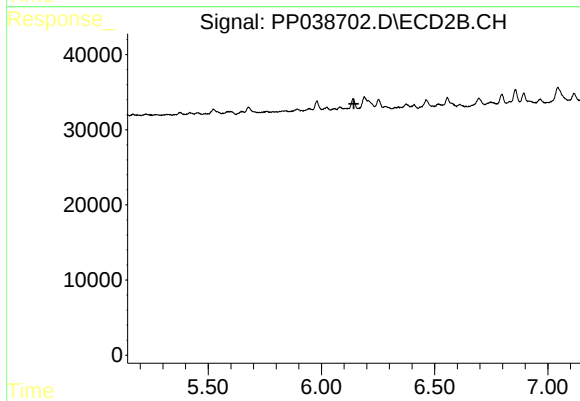

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T. : 6.144 min
Response: 0
Conc: N.D.

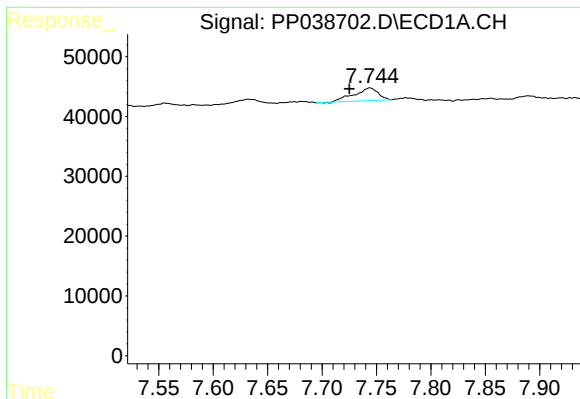

#28 AR-1254-3


R.T.: 7.744 min
Delta R.T.: 0.019 min
Response: 32650
Conc: 18.19 ng/ml

Instrument :
ECD_P
ClientSampleId :

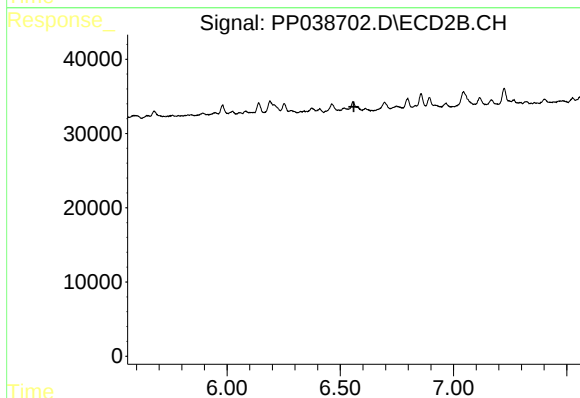


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.560 min
Response: 0
Conc: N.D.

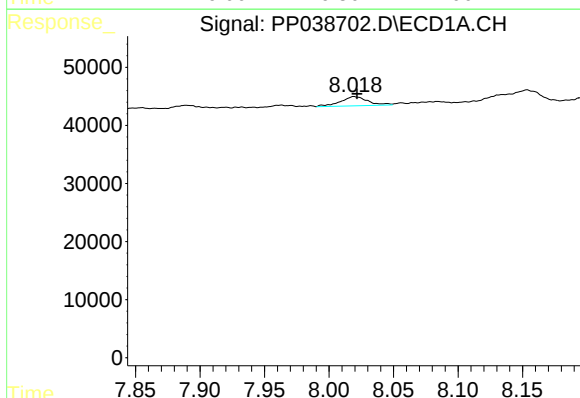


#29 AR-1254-4

R.T.: 8.019 min
Delta R.T.: -0.003 min
Response: 23333
Conc: 18.08 ng/ml

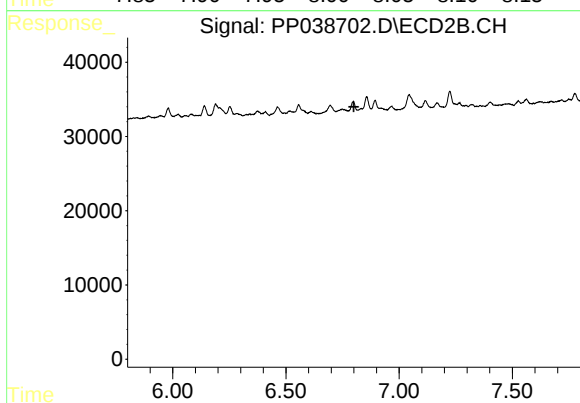

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.800 min
Response: 0
Conc: N.D.

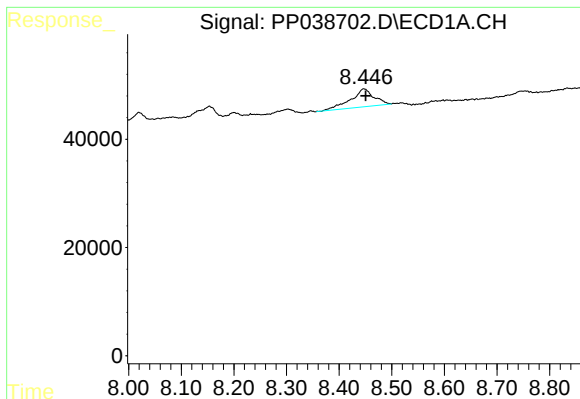

#30 AR-1254-5


R.T.: 8.447 min
Delta R.T.: -0.004 min
Response: 101301
Conc: 81.91 ng/ml

Instrument :
ECD_P
ClientSampleId :

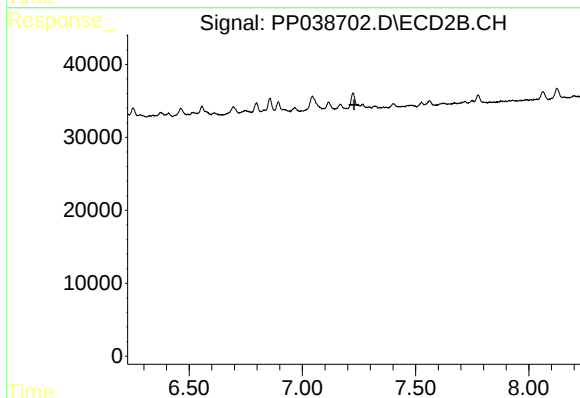


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.228 min
Response: 0
Conc: N.D.

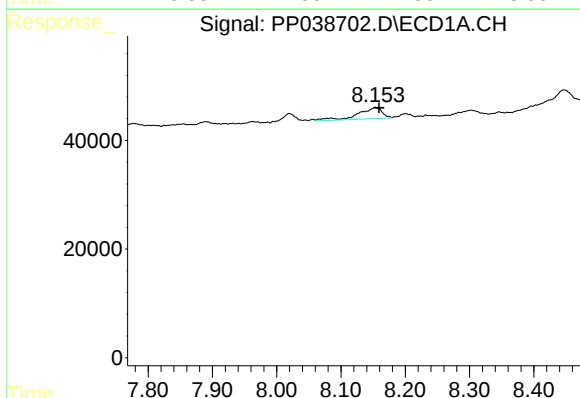


#32 AR-1260-2

R.T.: 8.154 min
Delta R.T.: -0.006 min
Response: 54822
Conc: 37.37 ng/ml

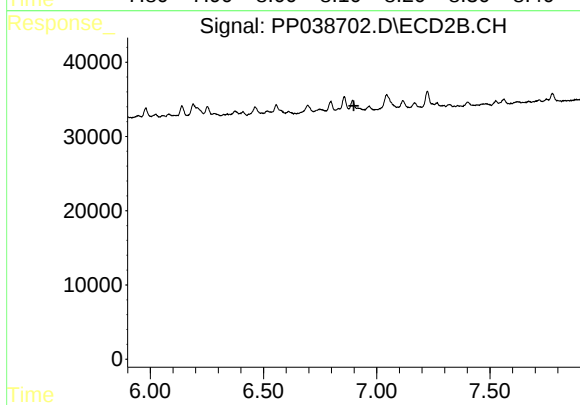

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.899 min
Response: 0
Conc: N.D.

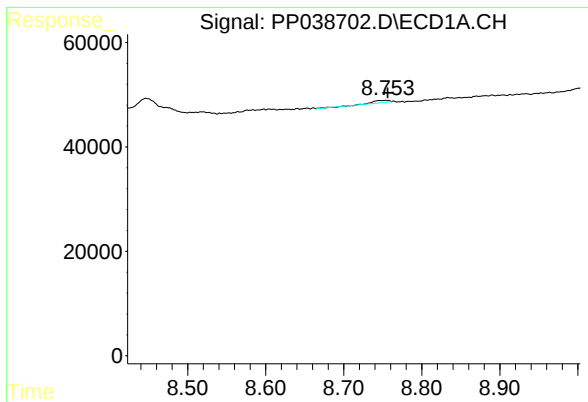

#34 AR-1260-4

R.T.: 8.754 min
Delta R.T.: -0.003 min
Response: 5936
Conc: 5.22 ng/ml

Instrument :
ECD_P
ClientSampleId :

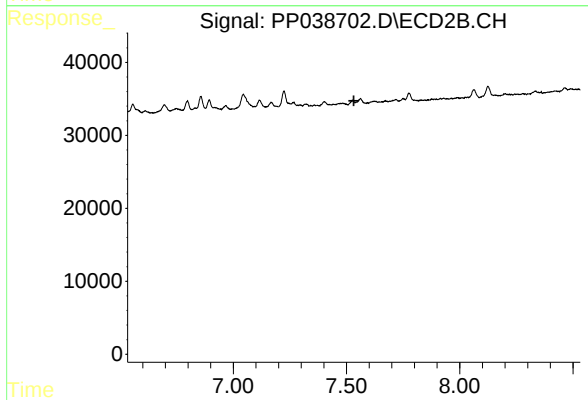

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.533 min
Response: 0
Conc: N.D.