

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082021\
 Data File : PP038757.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Aug 2021 22:22
 Operator : AJ\MA
 Sample : M3475-01
 Misc :
 ALS Vial : 88 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 N5868-N34145

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 02:31:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 18 04:51:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.883	3.869	780090	491685	19.329	20.518
2)	SA Decachlor...	10.867	9.126	427603	421523	17.380	17.307
Target Compounds							
8)	L2 AR-1221-1	5.135	0.000	60793	0	129.995	N.D. #
20)	L4 AR-1242-5	7.181	0.000	721755	0	1009.506	N.D. #
25)	L5 AR-1248-5	7.181	0.000	721755	0	590.308	N.D. #
28)	L6 AR-1254-3	7.744f	0.000	17963	0	10.006	N.D. #
32)	L7 AR-1260-2	8.136f	0.000	26843	0	18.296	N.D. #
35)	L7 AR-1260-5	9.093	0.000	20717	0	9.232	N.D. #
37)	L8 AR-1262-2	9.093f	0.000	20717	0	7.781	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP082021\
Data File : PP038757.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Aug 2021 22:22
Operator : AJ\MA
Sample : M3475-01
Misc :
ALS Vial : 88 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
N5868-N34145

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 02:31:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081721.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 18 04:51:26 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

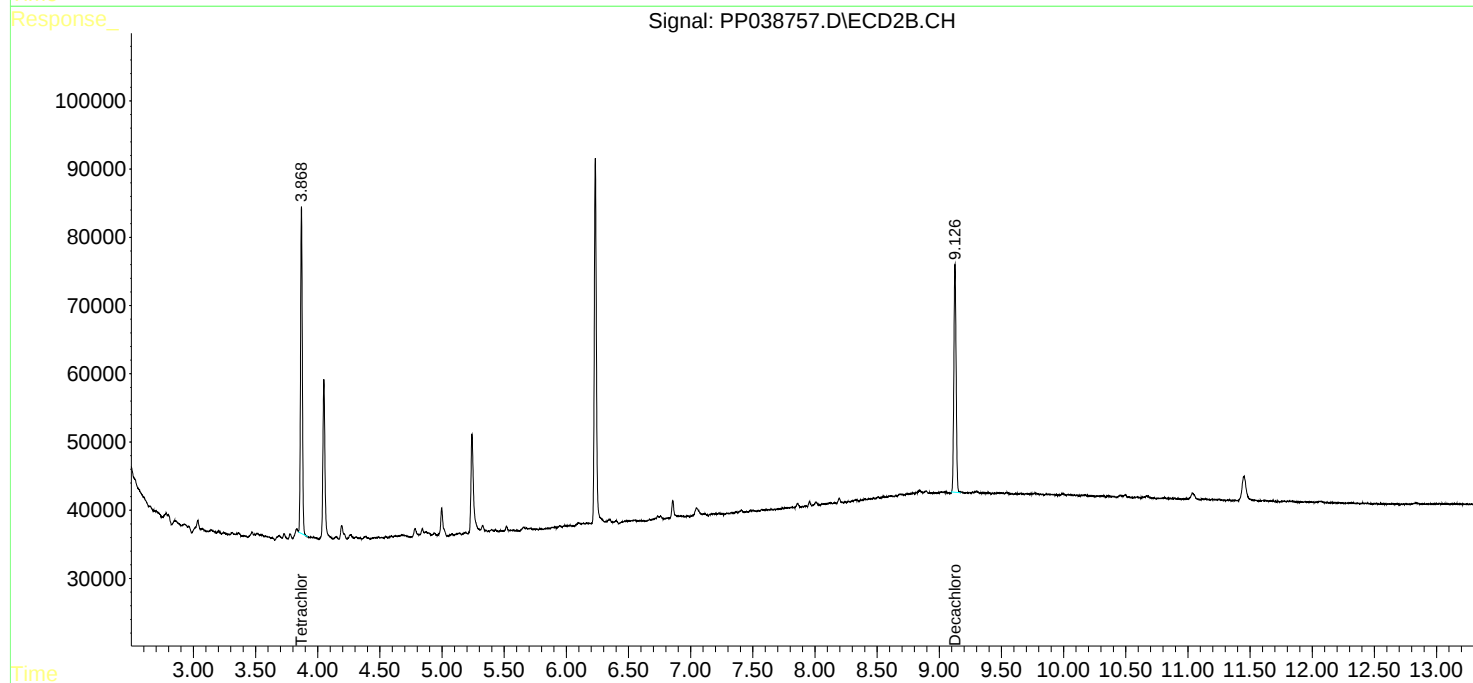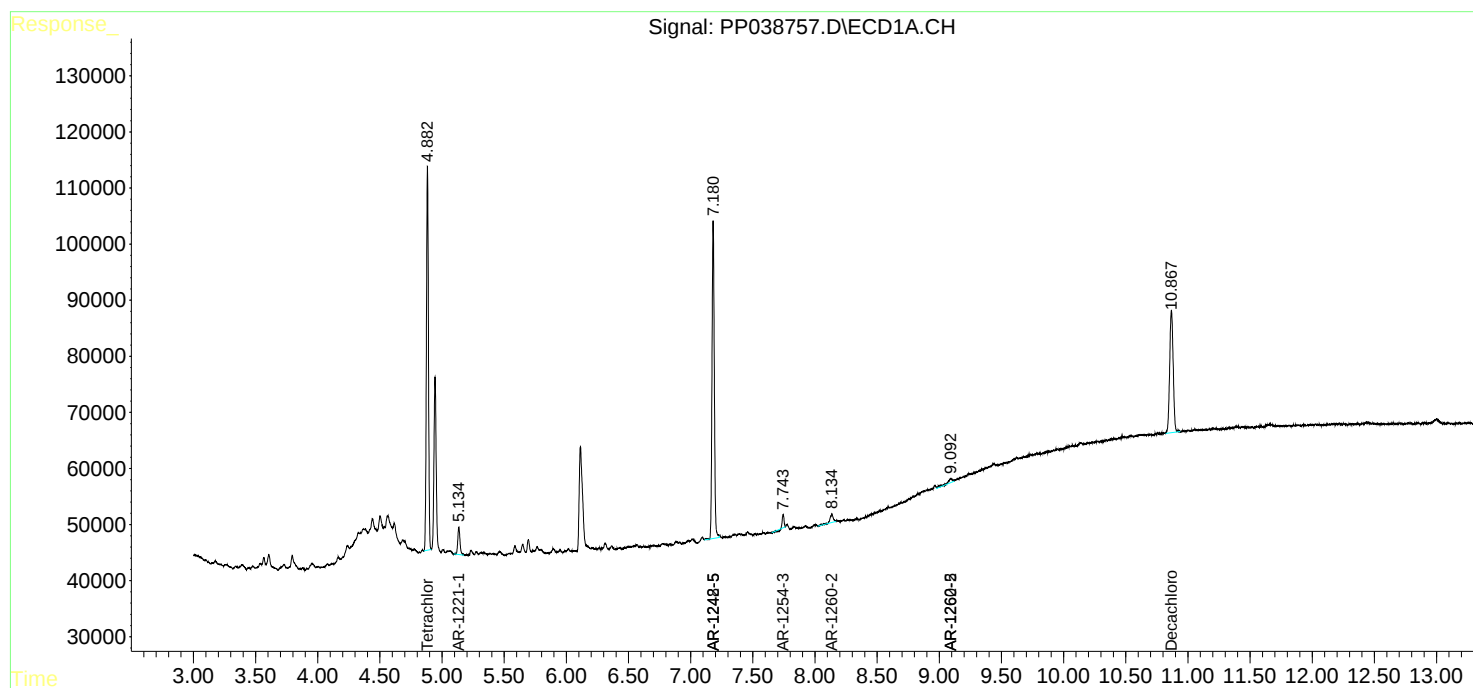


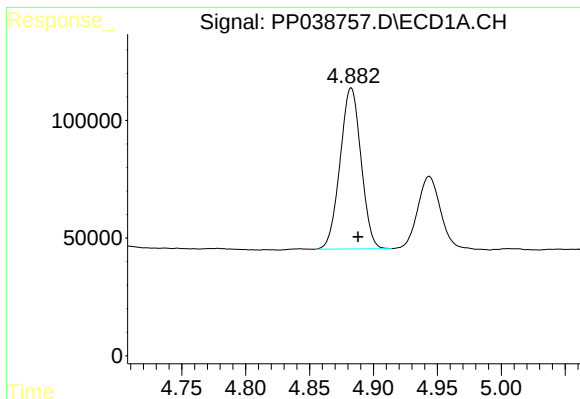

#1 Tetrachloro-m-xylene


R.T.: 4.883 min
Delta R.T.: -0.005 min
Response: 780090
Conc: 19.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
N5868-N34145

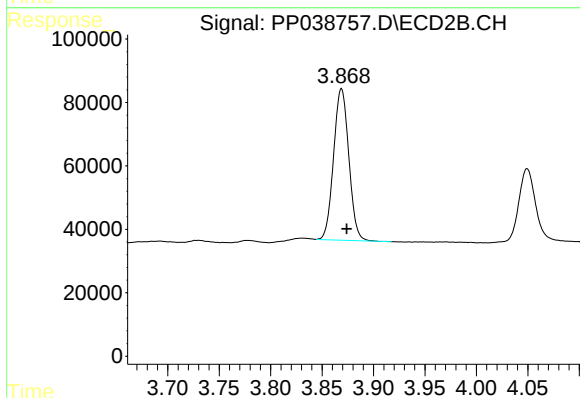


#1 Tetrachloro-m-xylene

R.T.: 3.869 min
Delta R.T.: -0.005 min
Response: 491685
Conc: 20.52 ng/ml

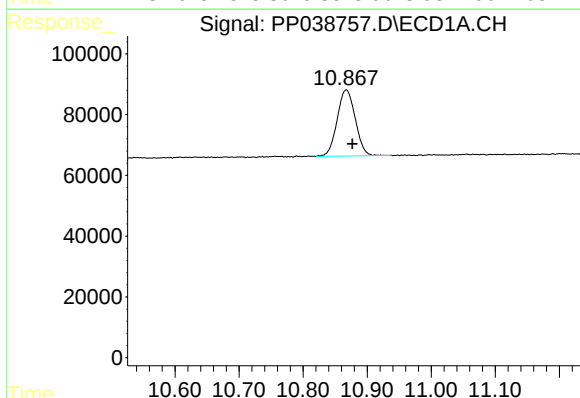


#2 Decachlorobiphenyl

R.T.: 10.867 min
Delta R.T.: -0.009 min
Response: 427603
Conc: 17.38 ng/ml

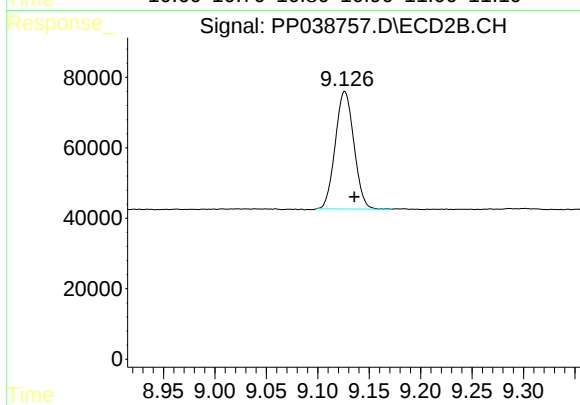

#2 Decachlorobiphenyl


R.T.: 9.126 min
Delta R.T.: -0.009 min
Response: 421523
Conc: 17.31 ng/ml

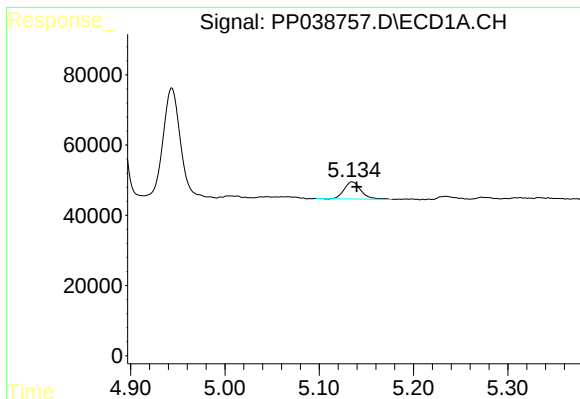

#8 AR-1221-1


R.T.: 5.135 min
Delta R.T.: -0.005 min
Response: 60793
Conc: 129.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
N5868-N34145

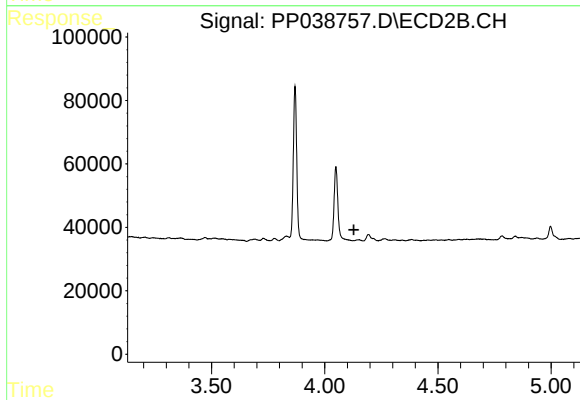


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.129 min
Response: 0
Conc: N.D.

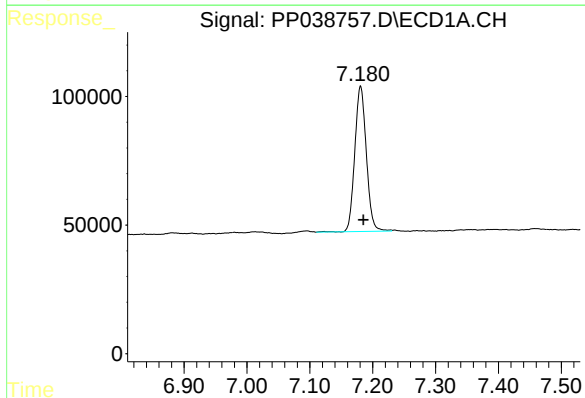


#20 AR-1242-5

R.T.: 7.181 min
Delta R.T.: -0.004 min
Response: 721755
Conc: 1009.51 ng/ml

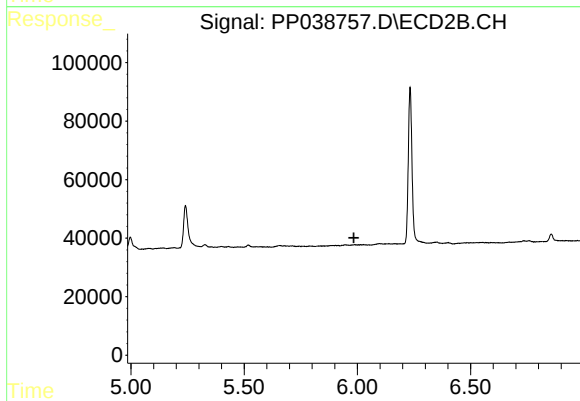

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 5.985 min
Response: 0
Conc: N.D.

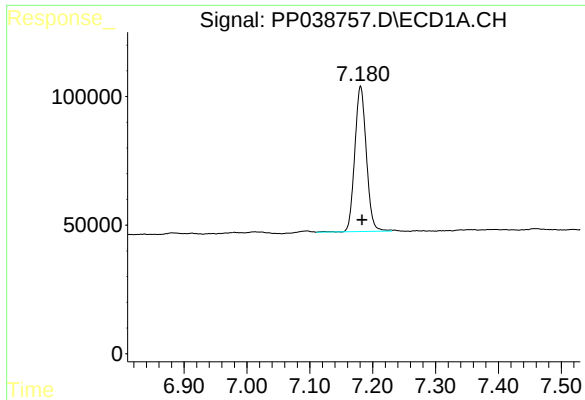

#25 AR-1248-5


R.T.: 7.181 min
Delta R.T.: -0.003 min
Response: 721755
Conc: 590.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
N5868-N34145

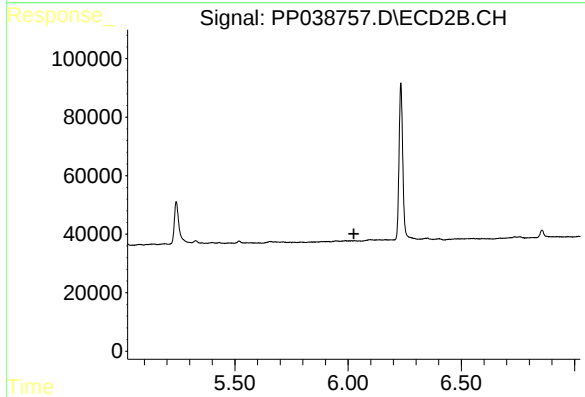


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 6.025 min
Response: 0
Conc: N.D.

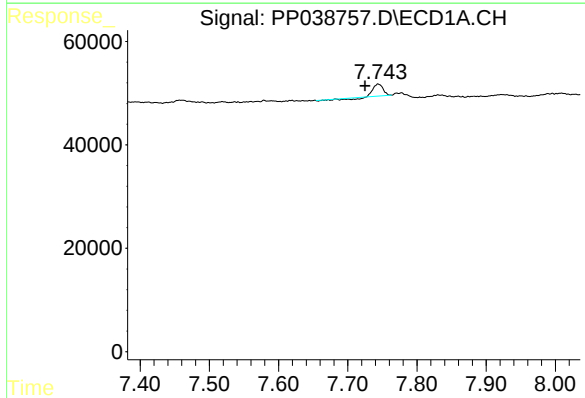


#28 AR-1254-3

R.T.: 7.744 min
Delta R.T.: 0.019 min
Response: 17963
Conc: 10.01 ng/ml

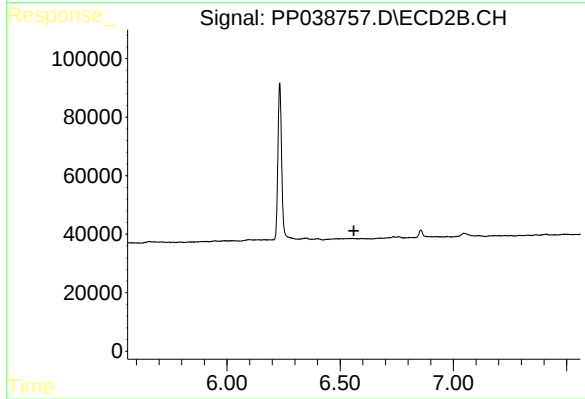

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.560 min
Response: 0
Conc: N.D.

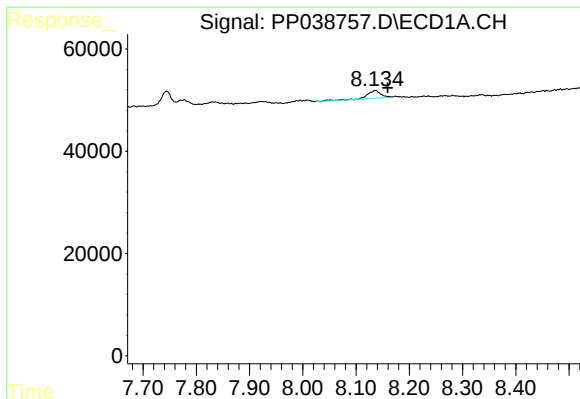

#32 AR-1260-2


R.T.: 8.136 min
Delta R.T.: -0.024 min
Response: 26843
Conc: 18.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
N5868-N34145

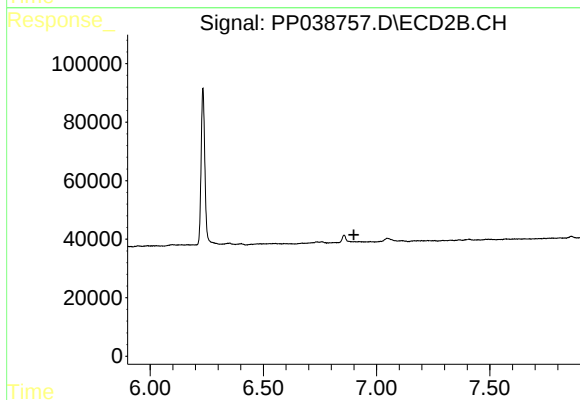


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.899 min
Response: 0
Conc: N.D.

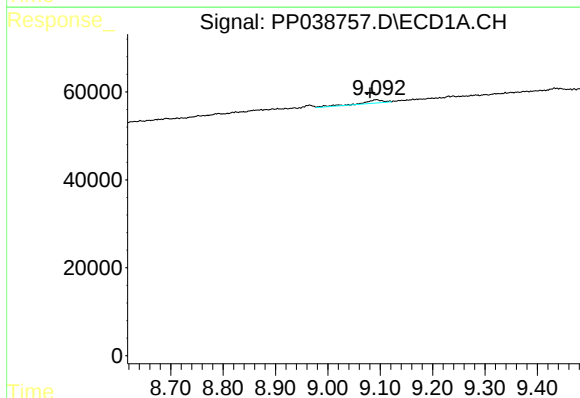


#35 AR-1260-5

R.T.: 9.093 min
Delta R.T.: 0.012 min
Response: 20717
Conc: 9.23 ng/ml

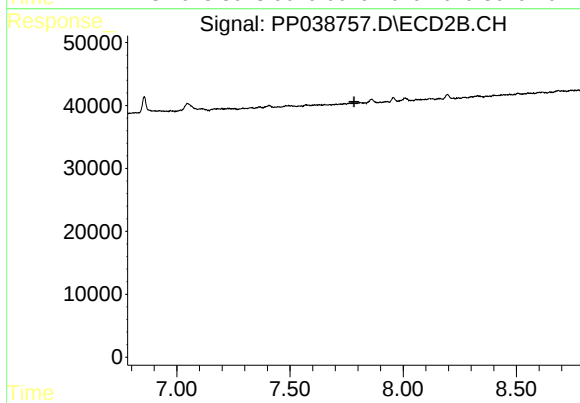

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.783 min
Response: 0
Conc: N.D.

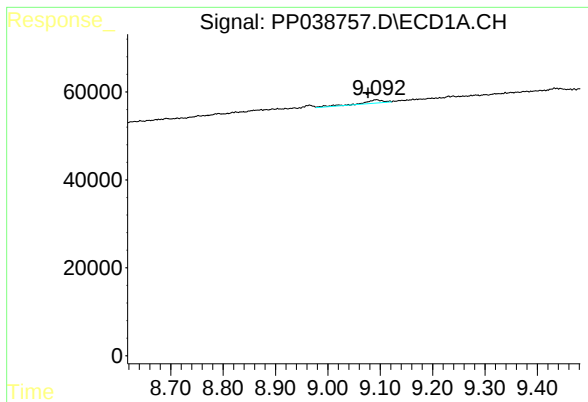

#37 AR-1262-2

R.T.: 9.093 min
Delta R.T.: 0.016 min
Response: 20717
Conc: 7.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
N5868-N34145

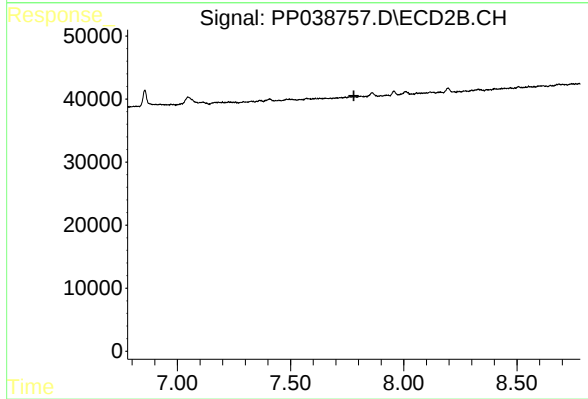

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.779 min
Response: 0
Conc: N.D.